

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094826.D
 Acq On : 22 Nov 2017 11:50
 Operator : SJ/JU
 Sample : PB104352BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK52

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:24:53 PM

Quant Time: Nov 23 01:05:33 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

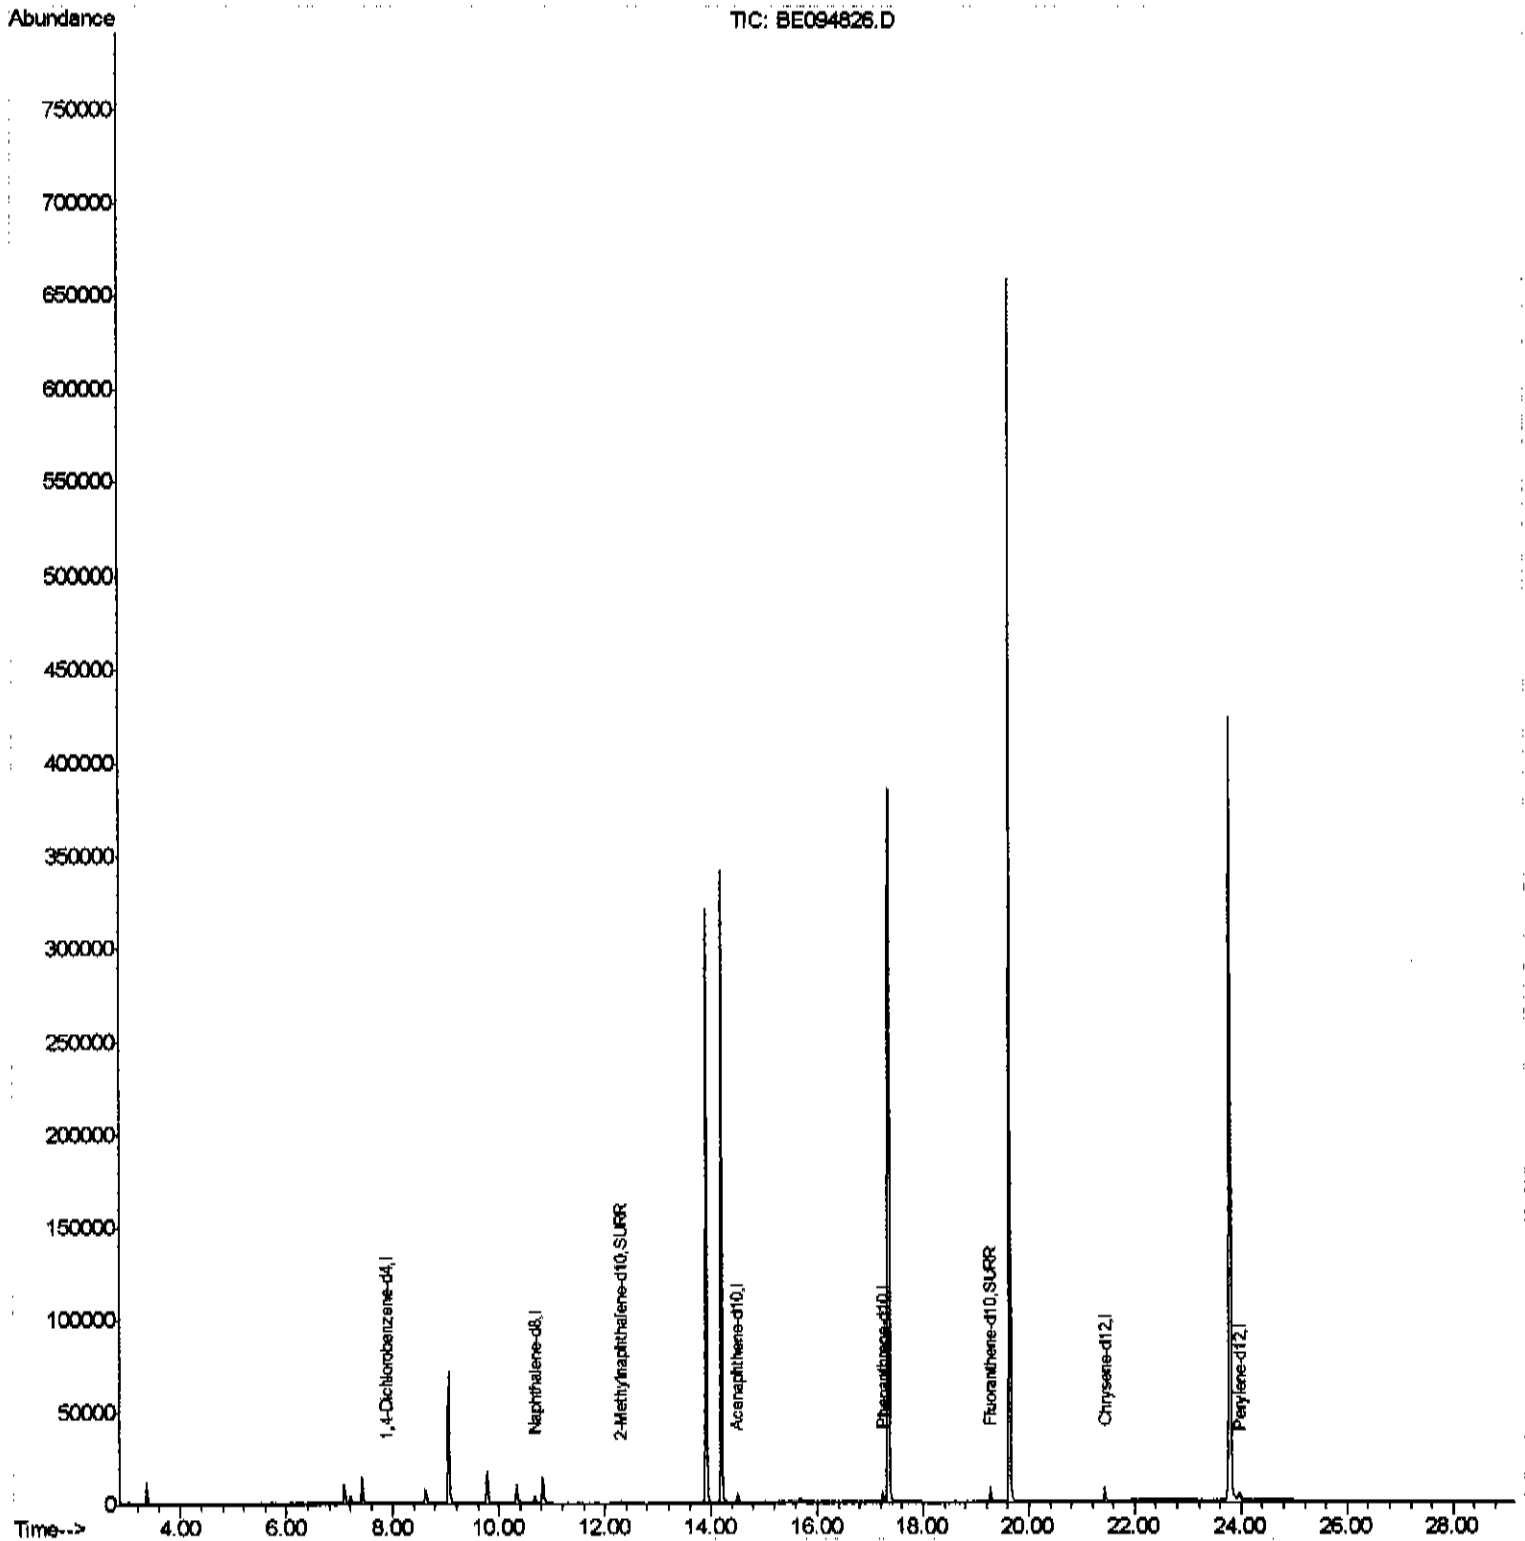

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094826.D
 Acq On : 22 Nov 2017 11:50
 Operator : SJ/JU
 Sample : PB104352BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK52

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:24:53 PM

Quant Time: Nov 23 00:56:58 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

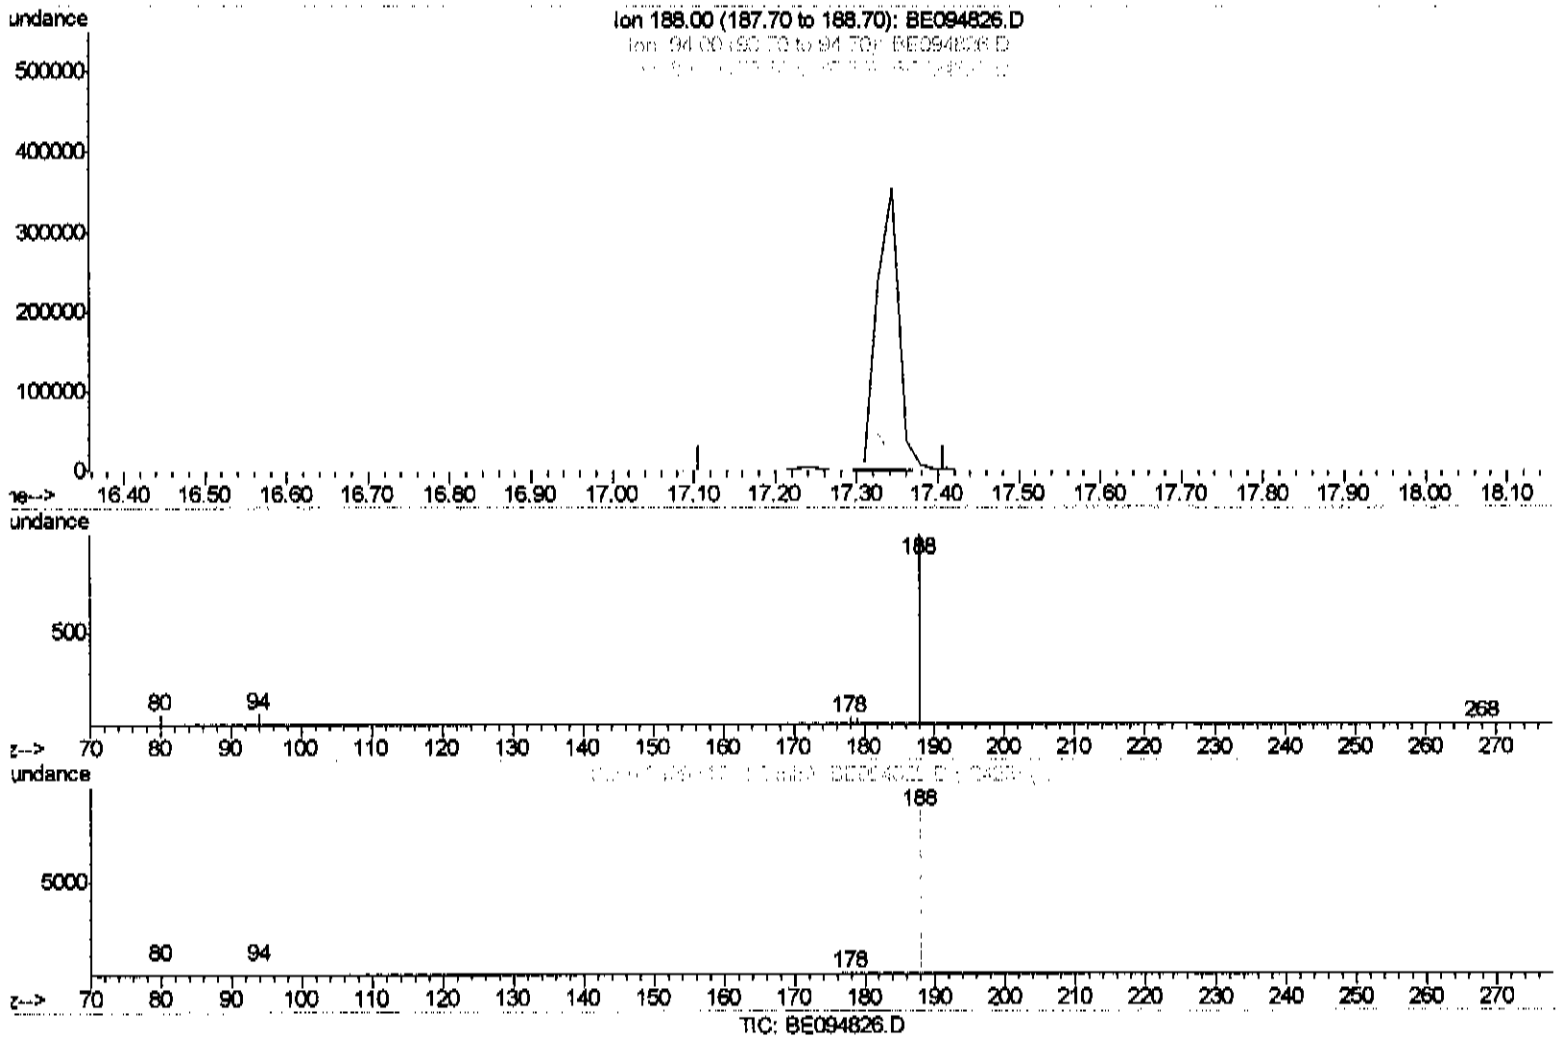

(10) Phenanthrene-d10 (I)

17.256min (-17.256) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094826.D
 Acq On : 22 Nov 2017 11:50
 Operator : SJ/JU
 Sample : PB104352BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK52

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:24:53 PM

Quant Time: Nov 23 00:56:58 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

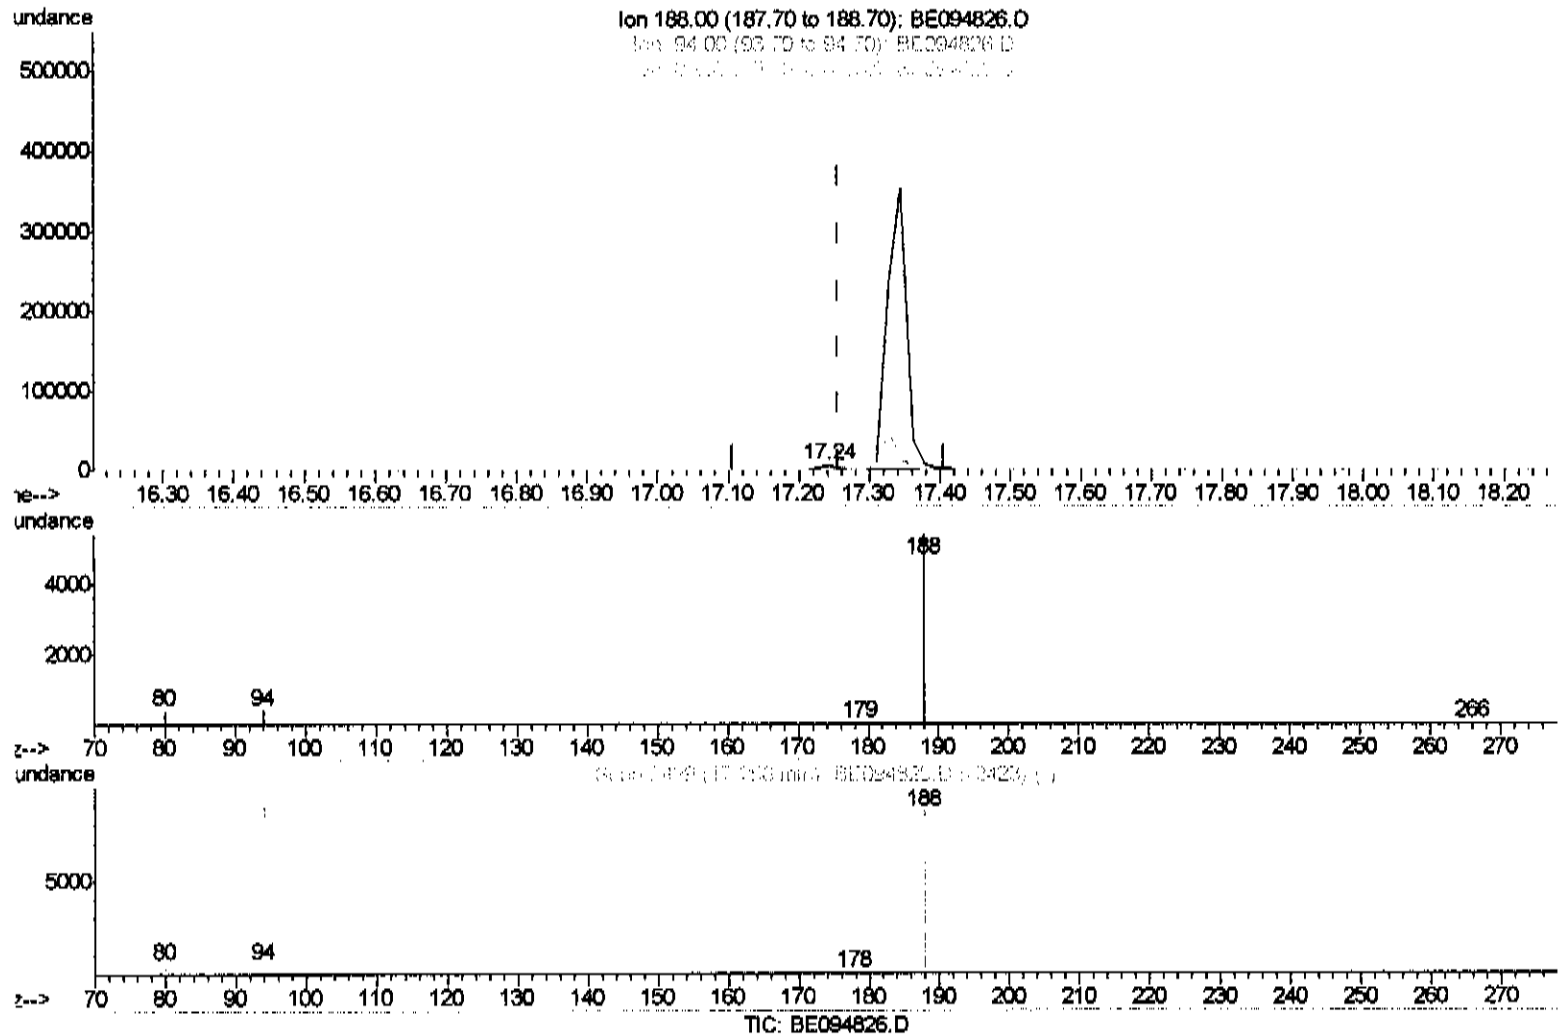

(10) Phenanthrene-d10 (I)

17.240min (-0.016) 0.40ng/ul m

SJ 11/27/17

response 7736

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.20#
80.00	11.80	7.95#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampled :
SBLK52

Manual Integrations
APPROVED

Sohil
11/27/2017 3:24:53 PM

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094826.D
Acq On : 22 Nov 2017 11:50
Operator : SJ/JU
Sample : PB104352BL
Disc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 23 01:05:33 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration

Internal Standards	R.T.	OIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	689	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.67	136	4401	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.50	164	3150	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	7736m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.44	240	8200	0.40	ng/ul	0.01
20) Perylene-d12	23.96	264	9488	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	OIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.30	152	2634	0.37	ng/ul	0.02
14) Fluoranthene-d10	19.27	212	8864	0.33	ng/ul	-0.01

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

1004/27/17