

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094832.D
 Acq On : 22 Nov 2017 15:22
 Operator : SJ/JU
 Sample : I6514-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC7

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:05 PM

Quant Time: Nov 23 01:31:44 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

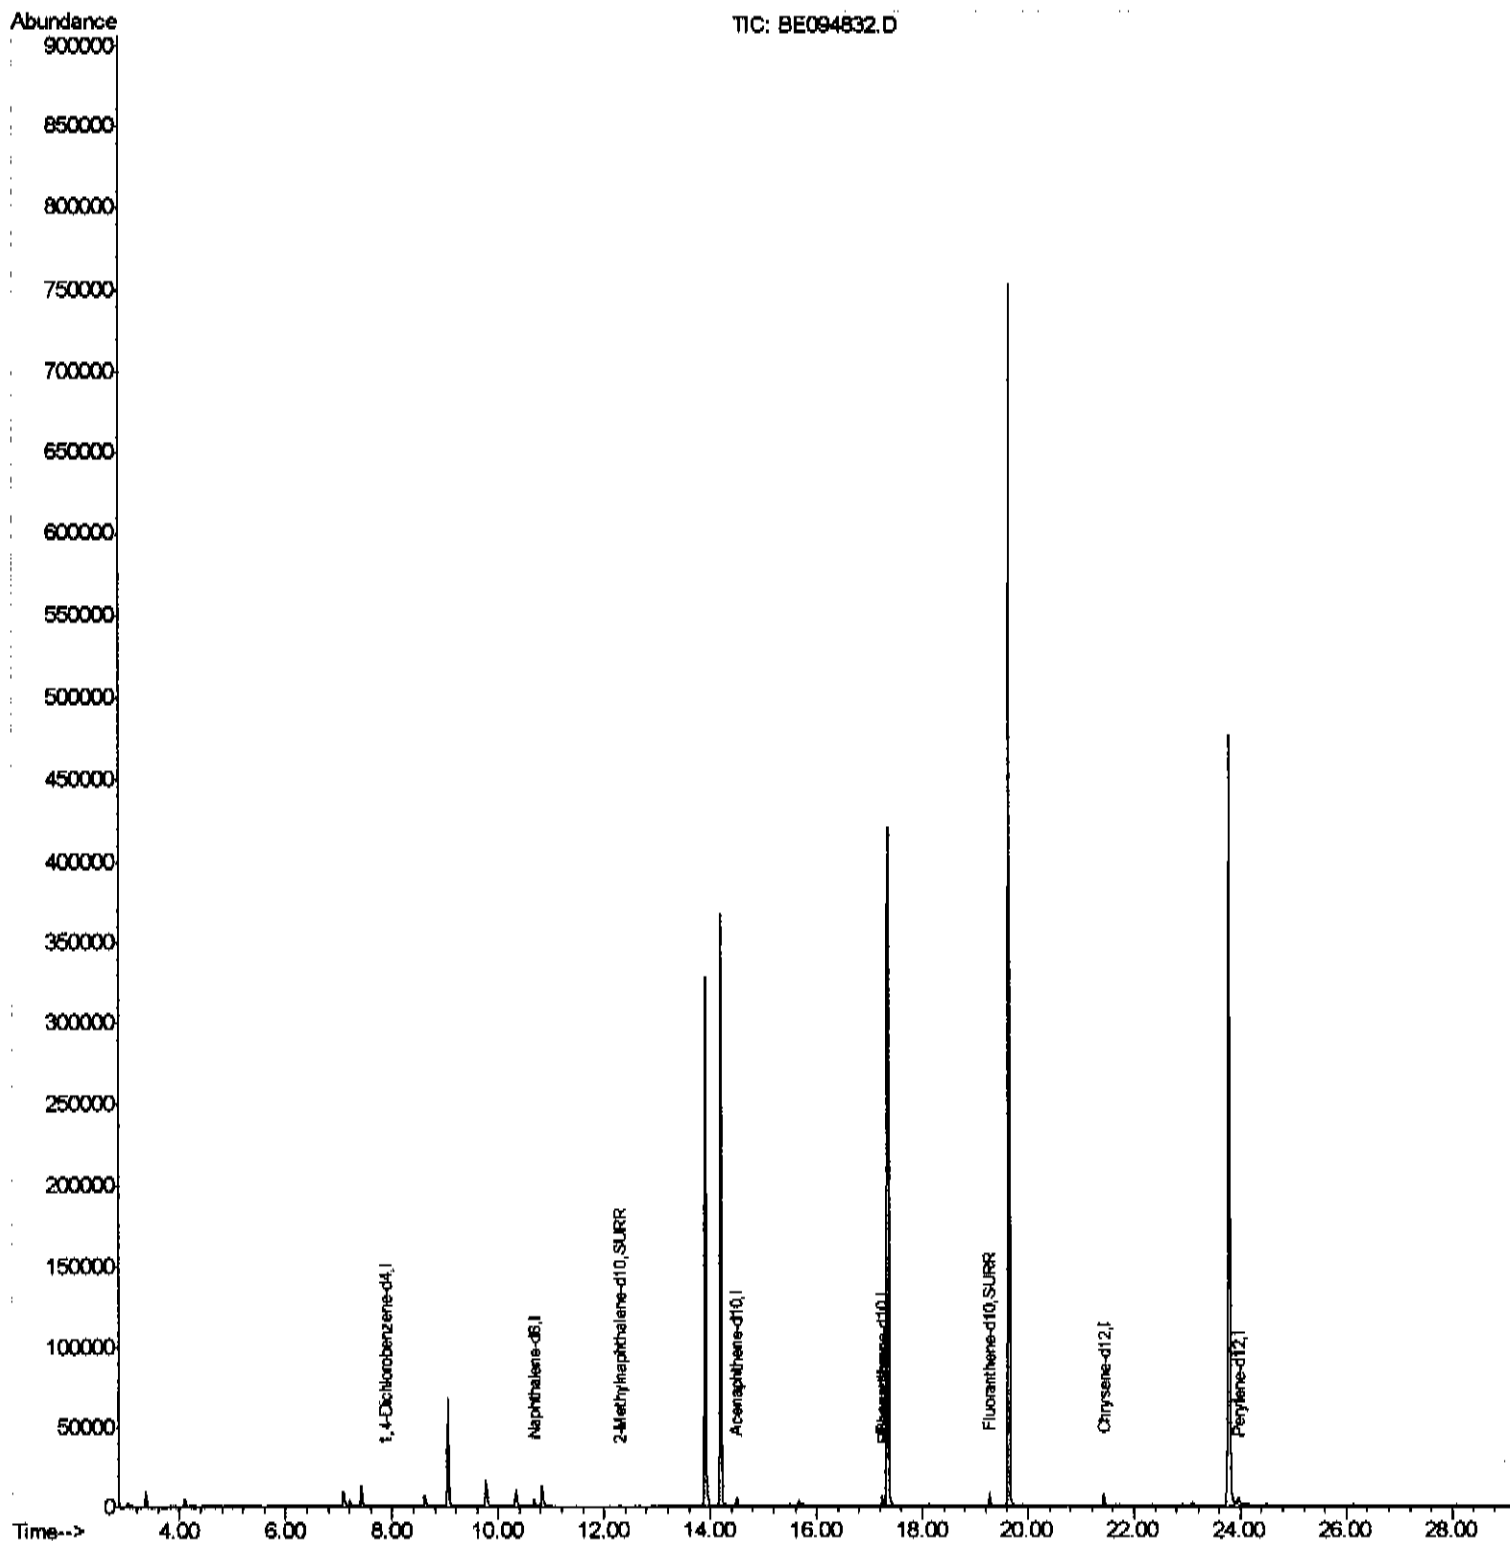

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094832.D
 Acq On : 22 Nov 2017 15:22
 Operator : SJ/JU
 Sample : I6514-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC7

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:05 PM

Quant Time: Nov 23 00:58:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

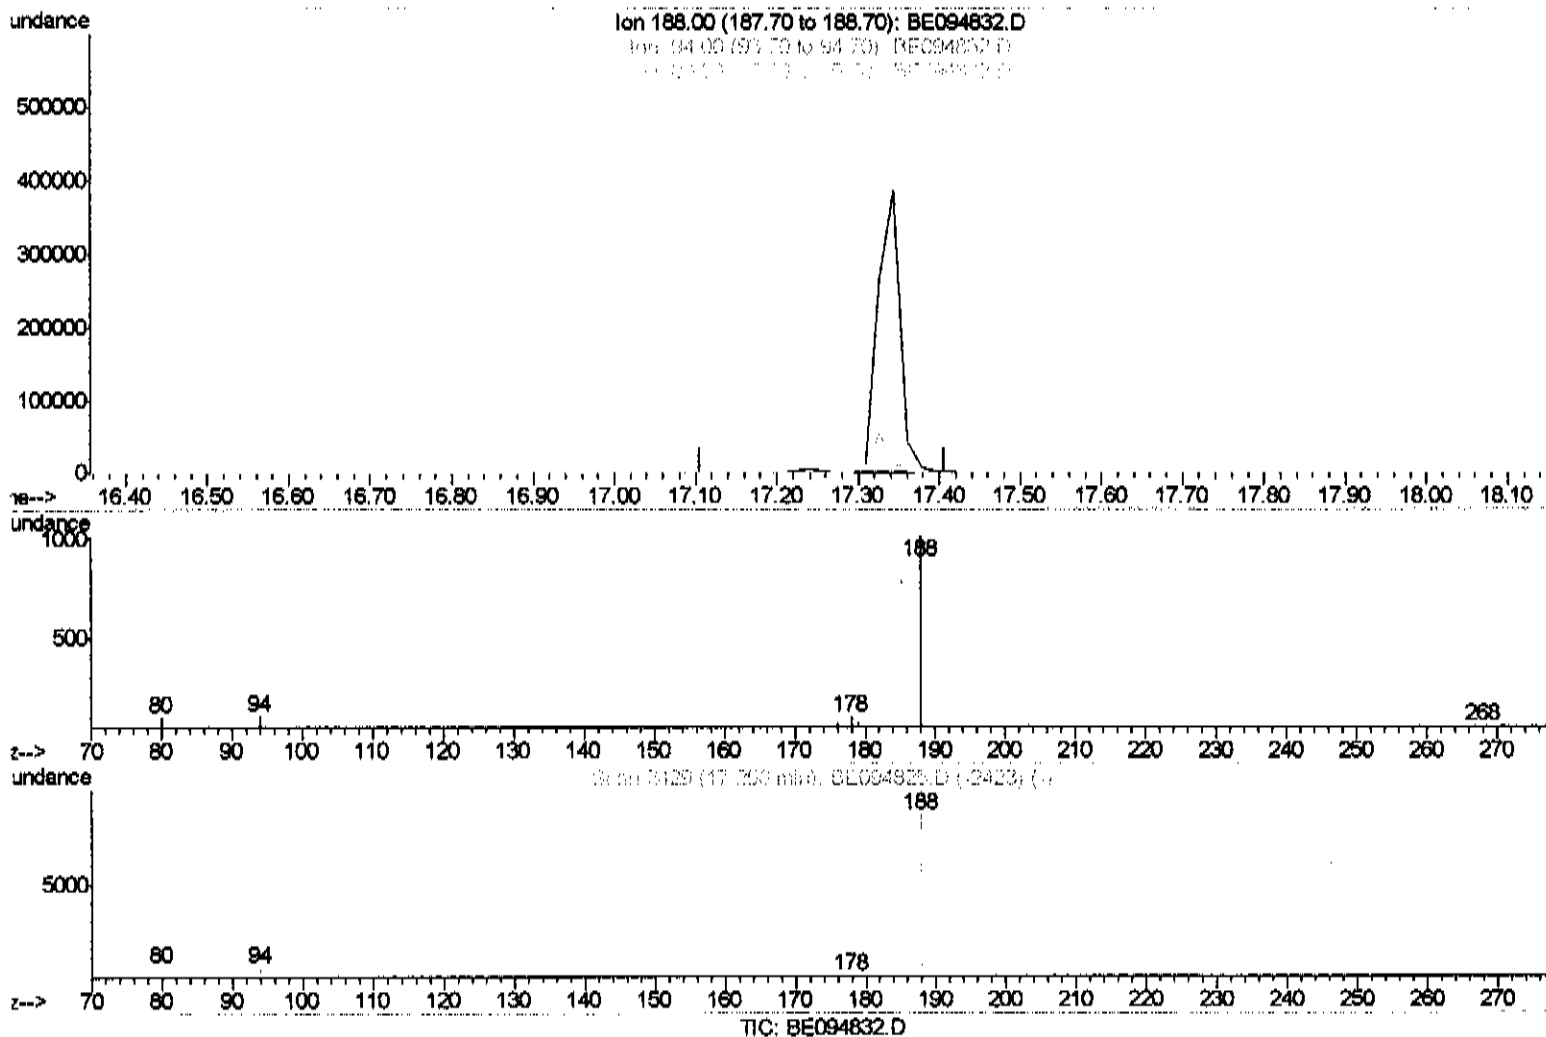

(10) Phenanthrene-d10 (I)

17.256min (-17.256) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094832.D
 Acq On : 22 Nov 2017 15:22
 Operator : SJ/JU
 Sample : I6514-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC7

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:05 PM

Quant Time: Nov 23 00:58:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

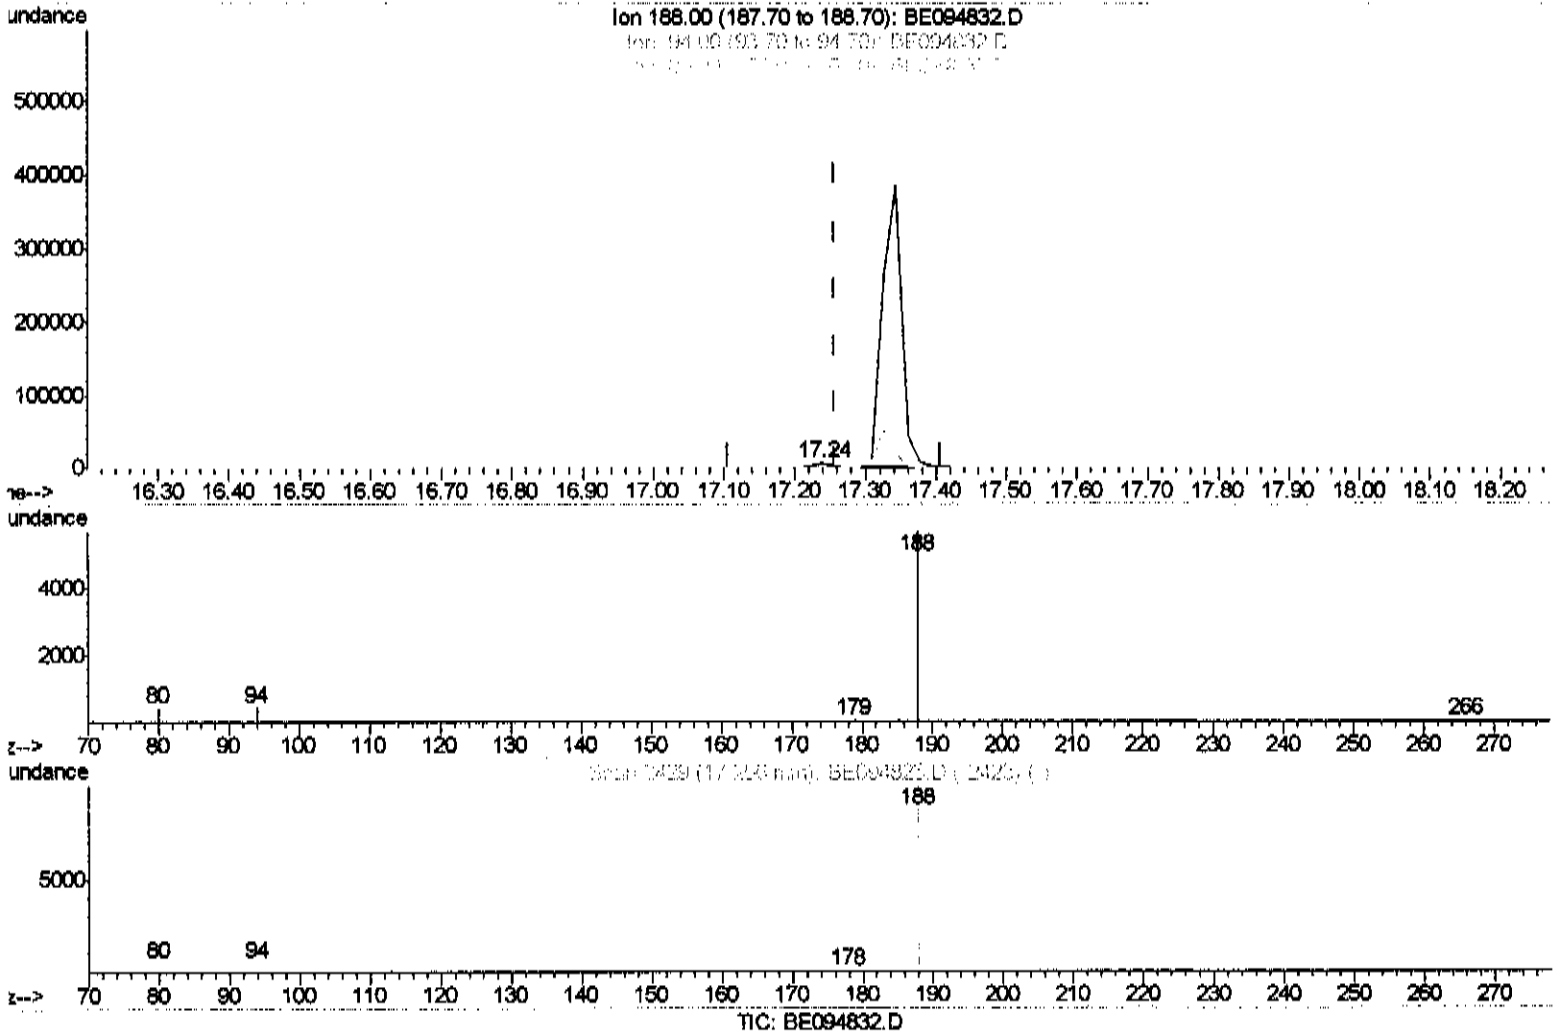

(10) Phenanthrene-d10 (I)

17.239min (-0.018) 0.40ng/ul m

SJ 11/27/17

response 8140

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.06#
80.00	11.80	7.73#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094832.D
 Acq On : 22 Nov 2017 15:22
 Operator : SJ/JU
 Sample : I6514-06
 Disc :
 Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 C0AC7

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:05 PM

Quant Time: Nov 23 01:31:44 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	693	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.67	136	4611	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.50	164	3384	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	8140m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	8475	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	9681	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	2678	0.36	ng/ul	0.02
14) Fluoranthene-d10	19.27	212	9950	0.36	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) Phenanthrene	17.27	178	566	0.03	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

- 30 u/27/17