

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:52:48 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 OLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

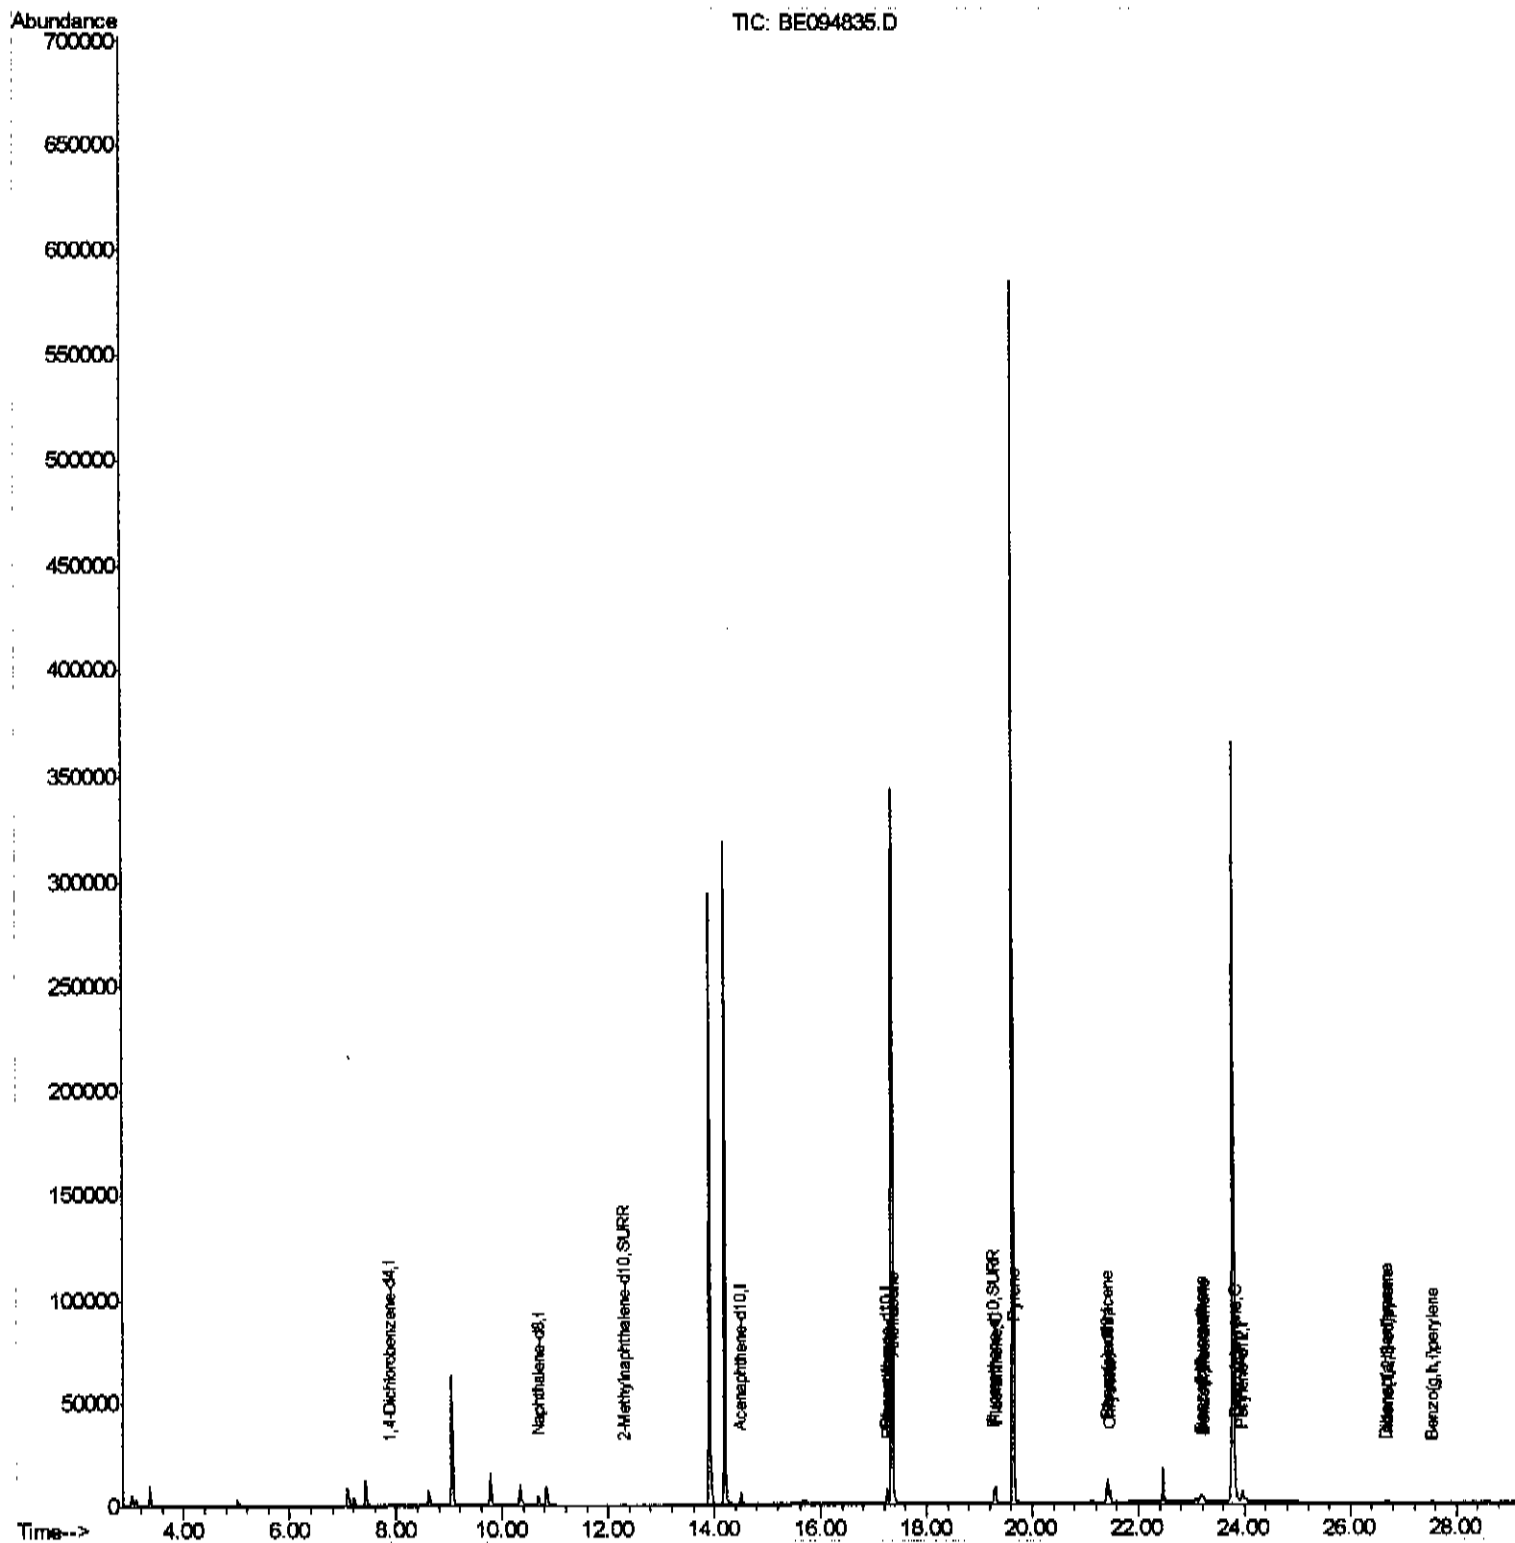

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 00:58:28 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

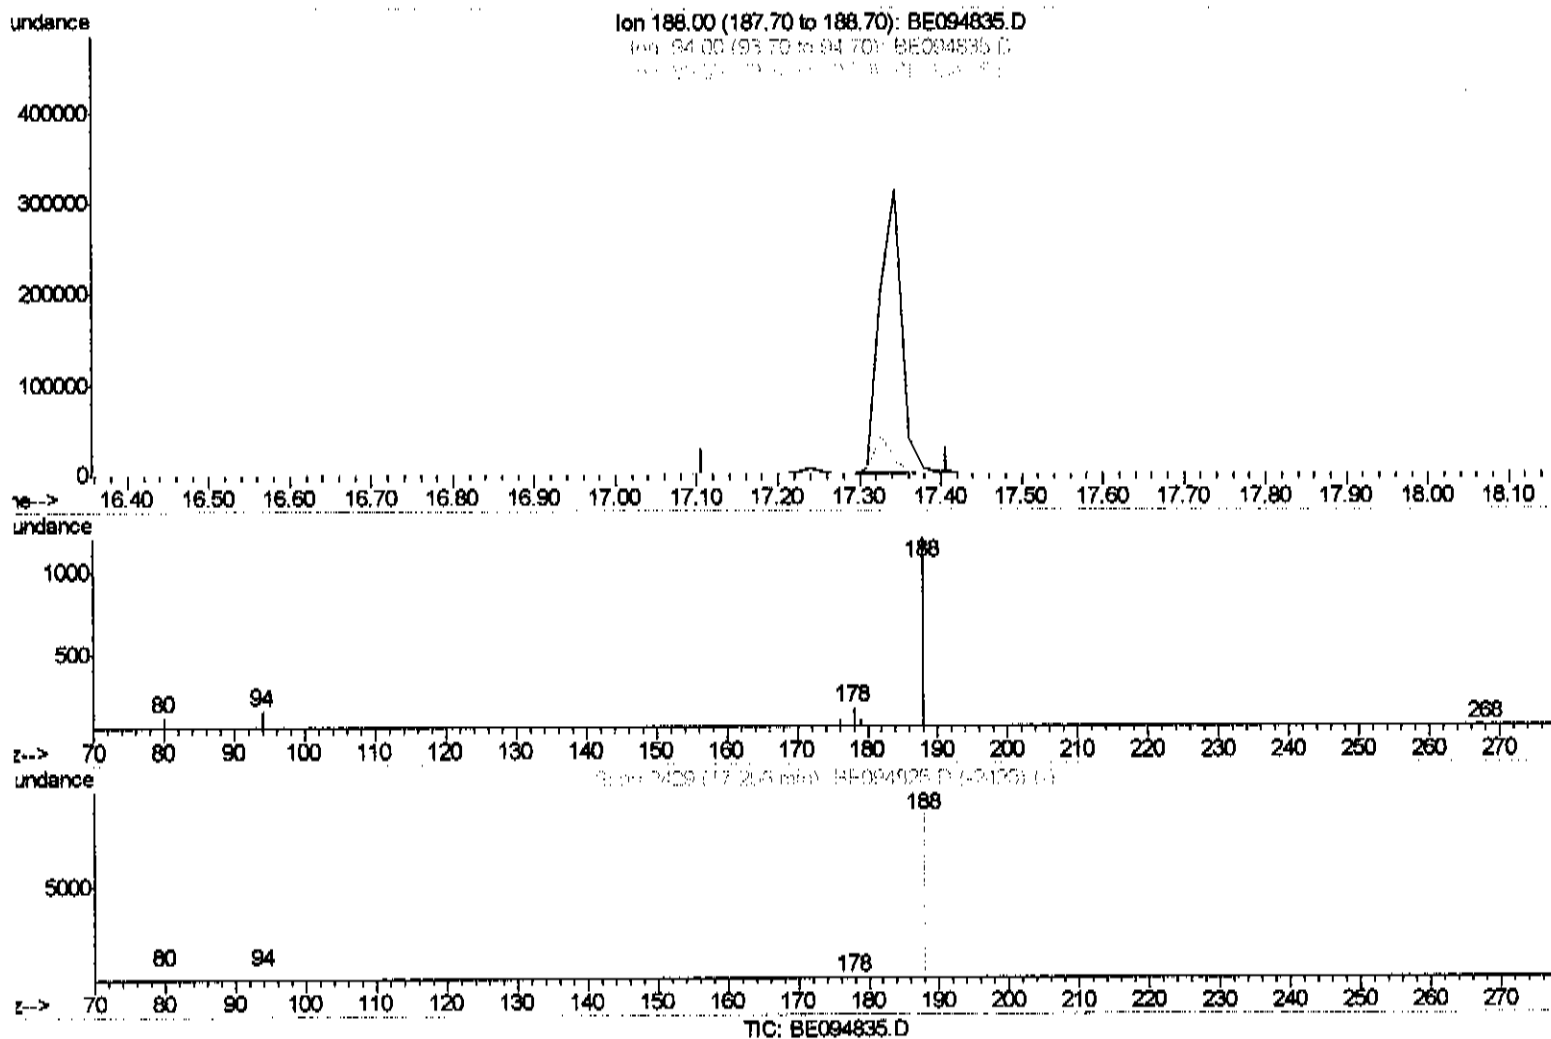

(10) Phenanthrene-d10 (I)

17.256min (-17.256) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 00:58:28 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

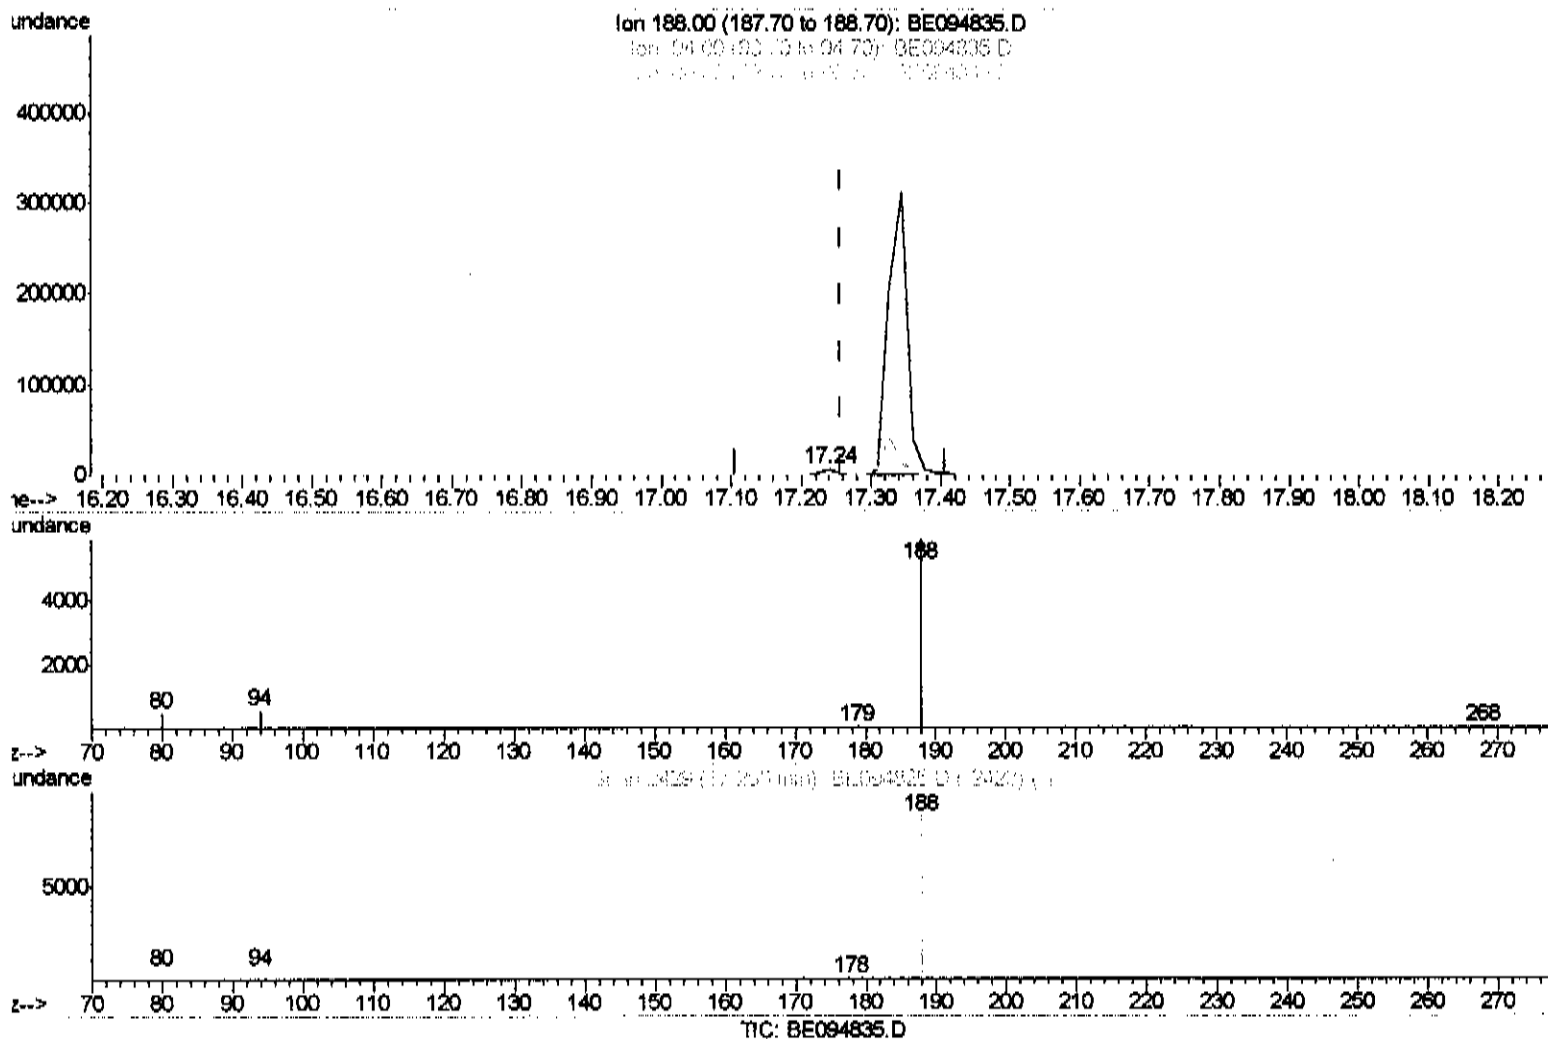

(10) Phenanthrene-d10 (I)

17.239min (-0.017) 0.40ng/ul m

10/11/27/17

response 8523

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.99
80.00	11.80	8.61#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:49:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

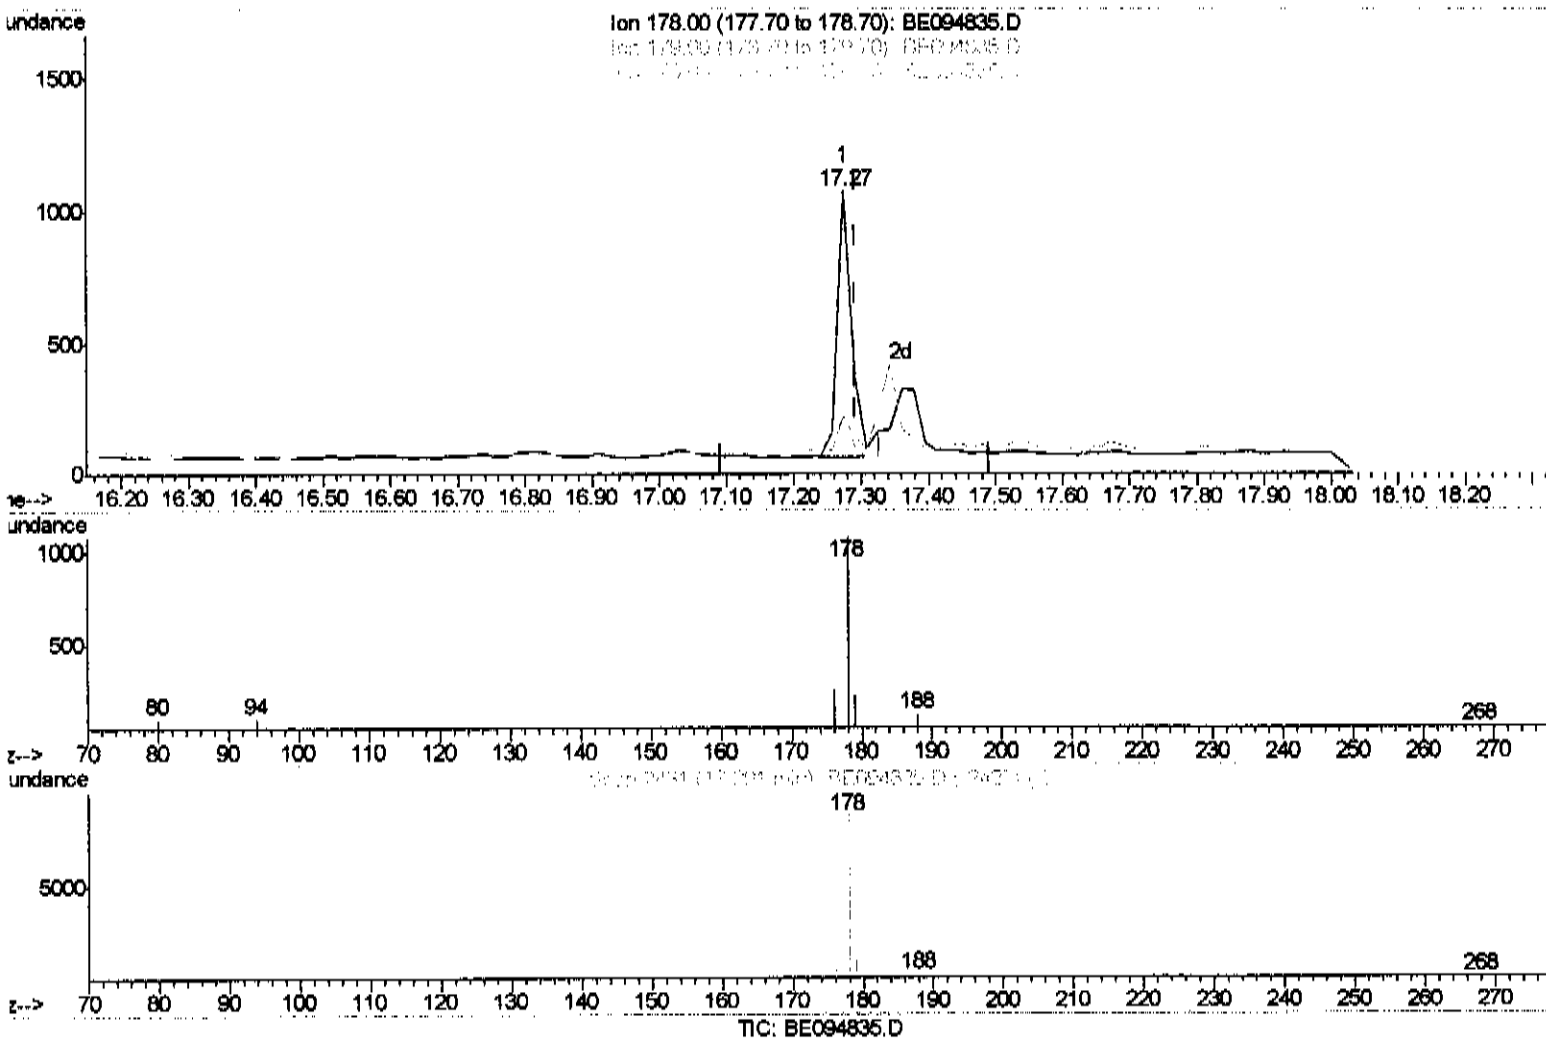

(12) Phenanthrene

17.274min (-0.017) 0.07ng/ul

response 1620

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	20.82
176.00	17.00	23.23#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:49:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

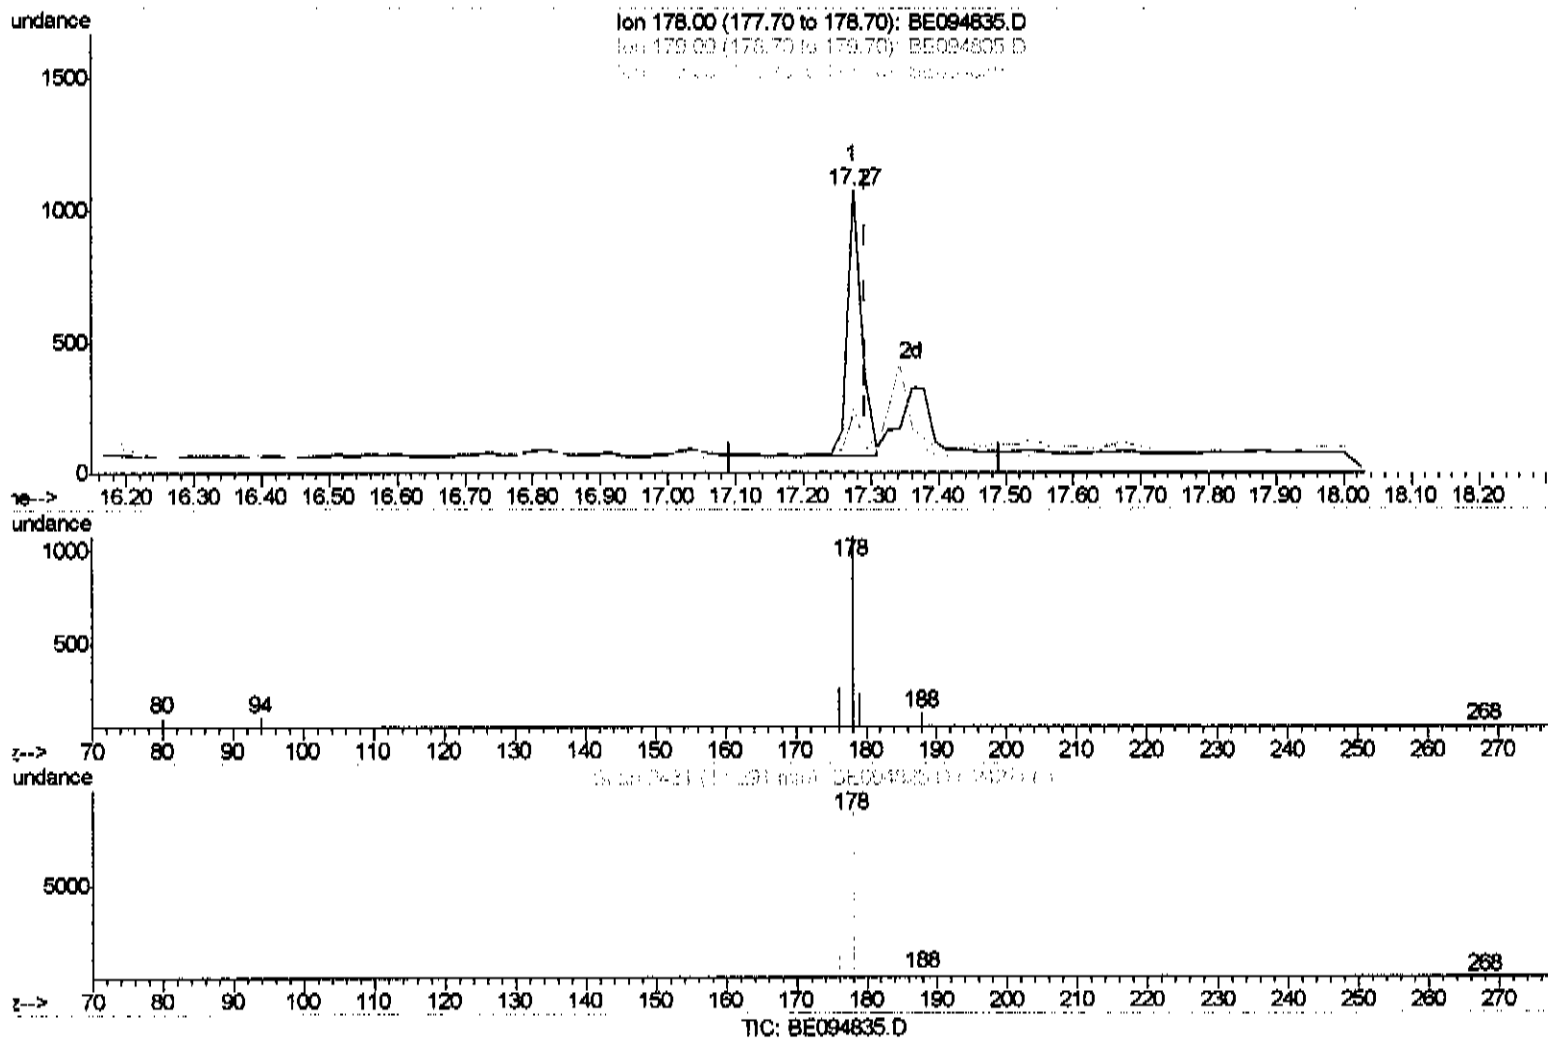

(12) Phenanthrene

17.274min (-0.017) 0.07ng/ul m

response 1524

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	20.82
176.00	17.00	23.23#
0.00	0.00	0.00

JO 11/27/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:49:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

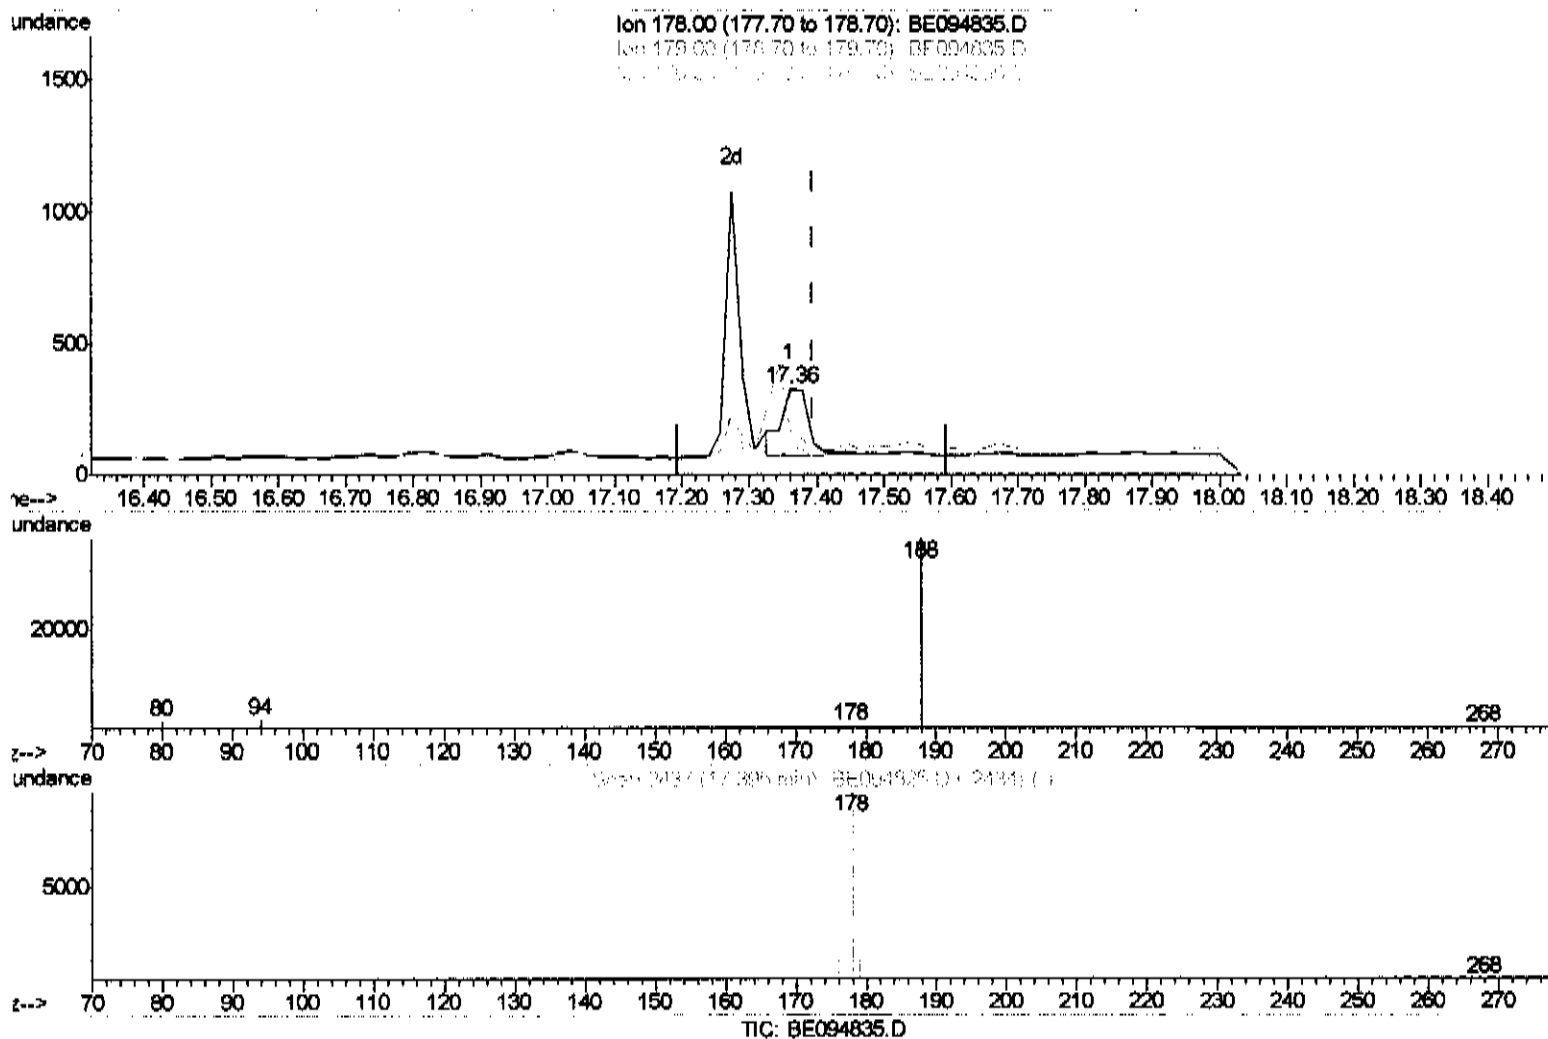

(13) Anthracene

17.360min (-0.035) 0.03ng/ul

response 713

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	51.82#
176.00	18.40	33.33#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:49:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

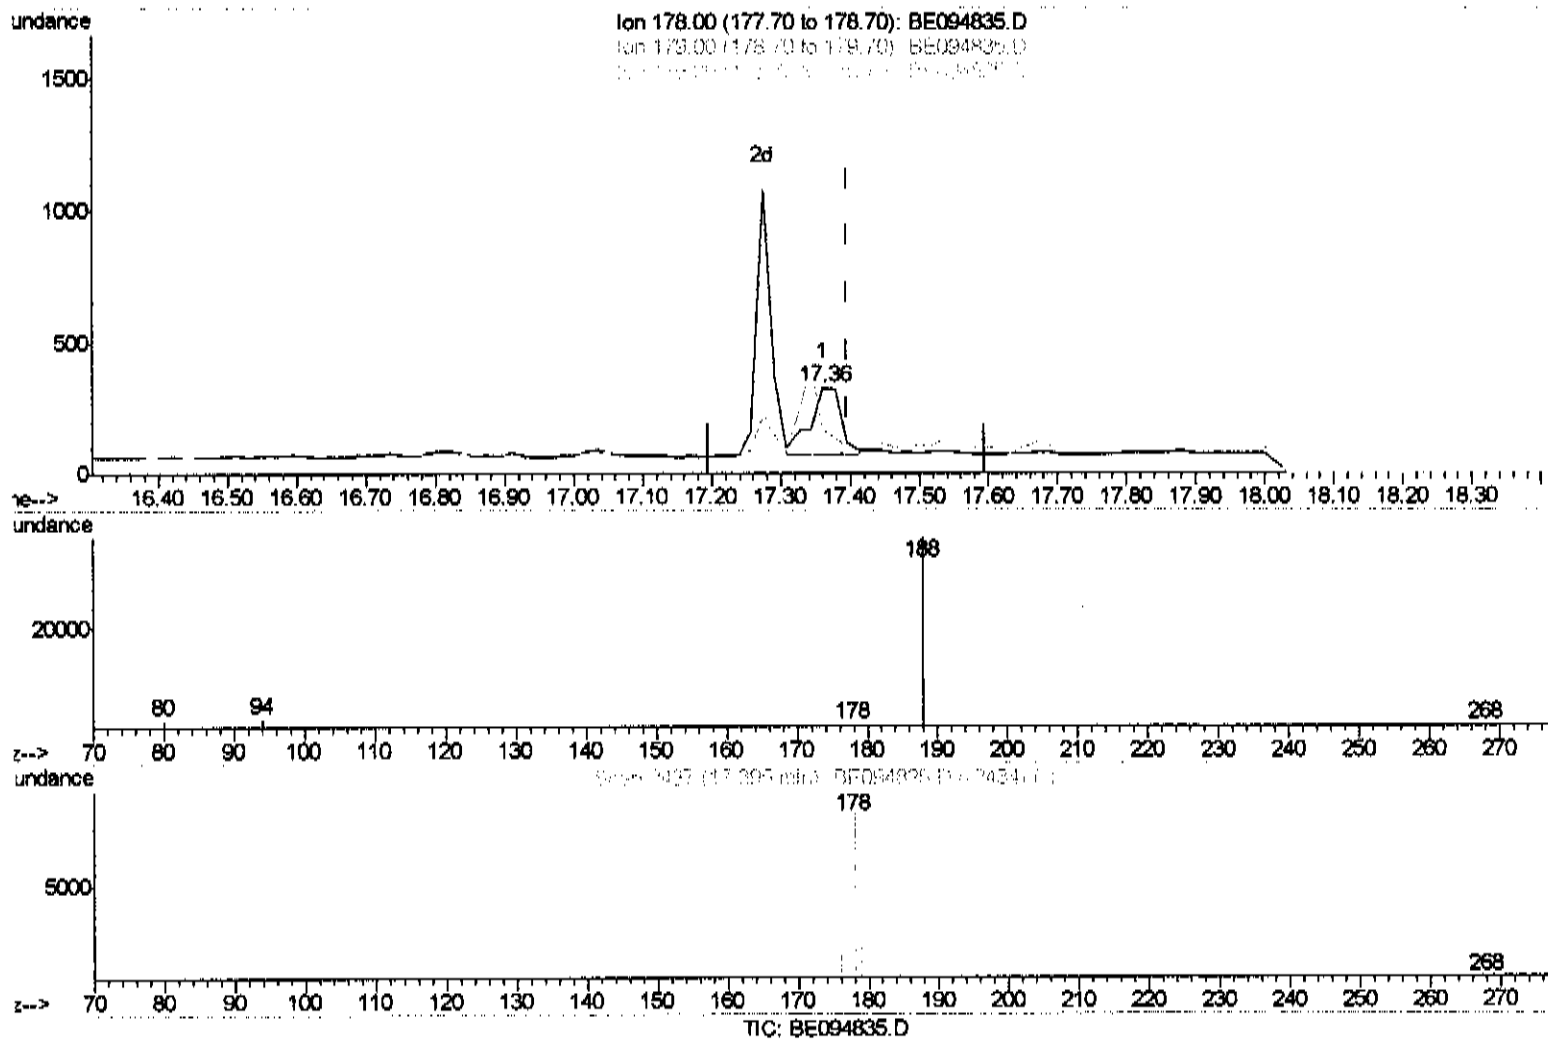

(13) Anthracene

17.360min (-0.035) 0.03ng/ul m

50 11/27/17

response 774

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	51.82#
176.00	18.40	33.33#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:49:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

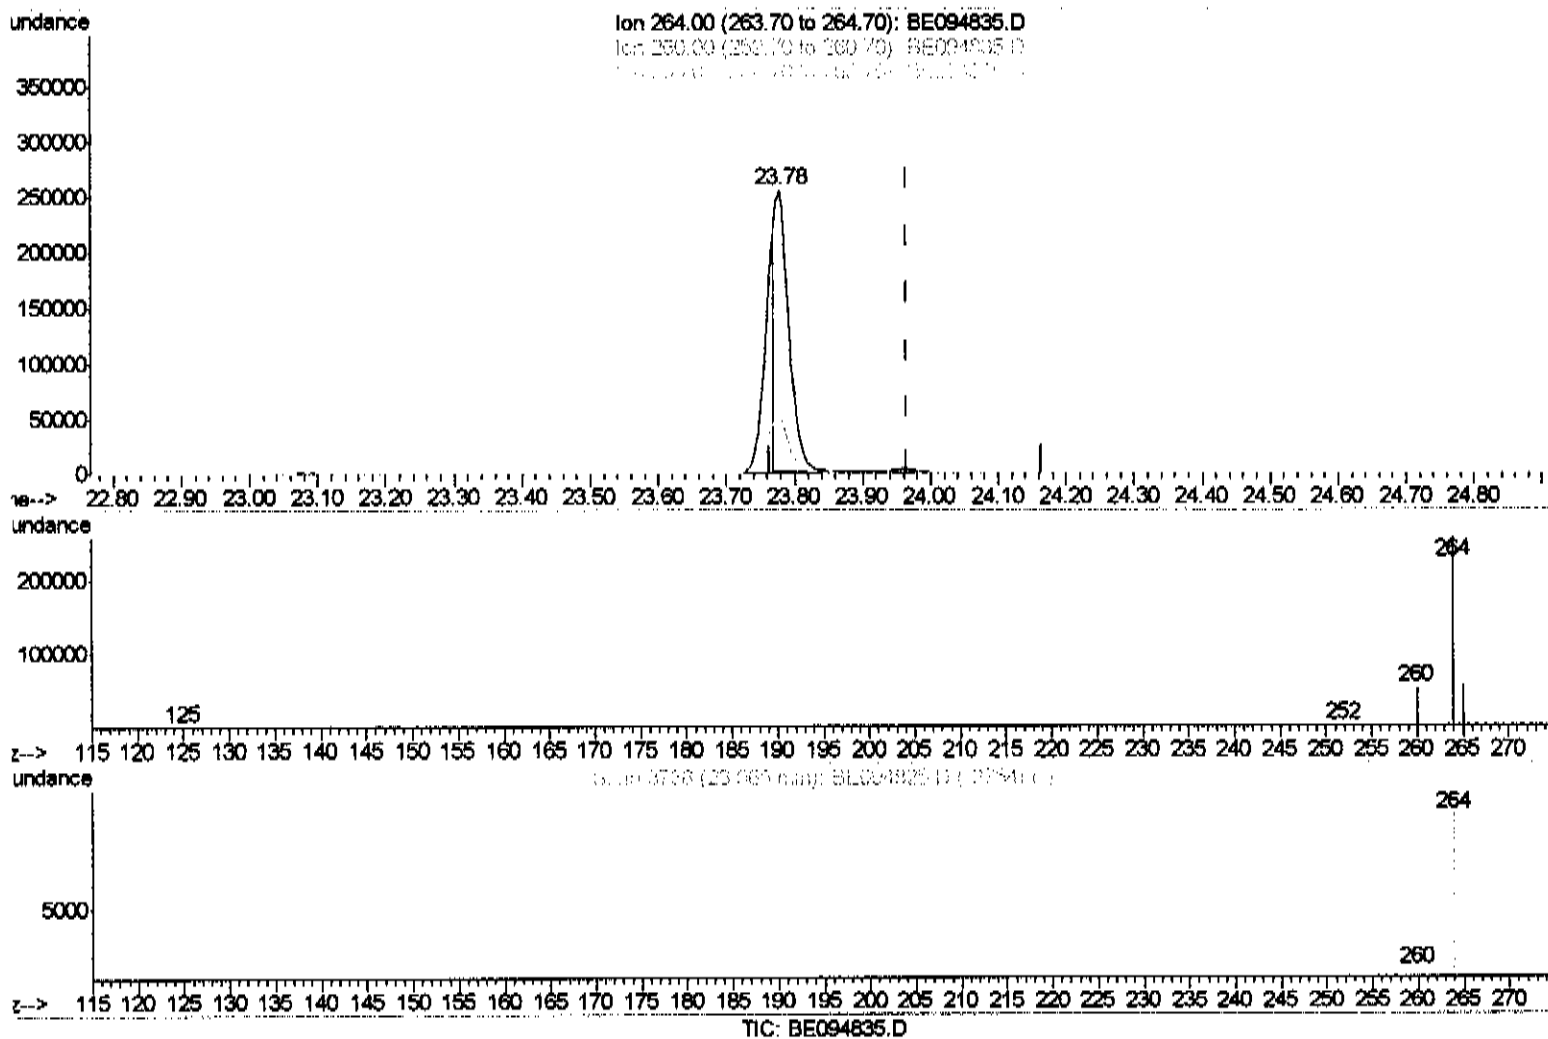

(20) Perylene-d12 (I)

23.778min (-0.187) 0.40ng/ul

response 368340

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.24#
265.00	103.50	21.94#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:49:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

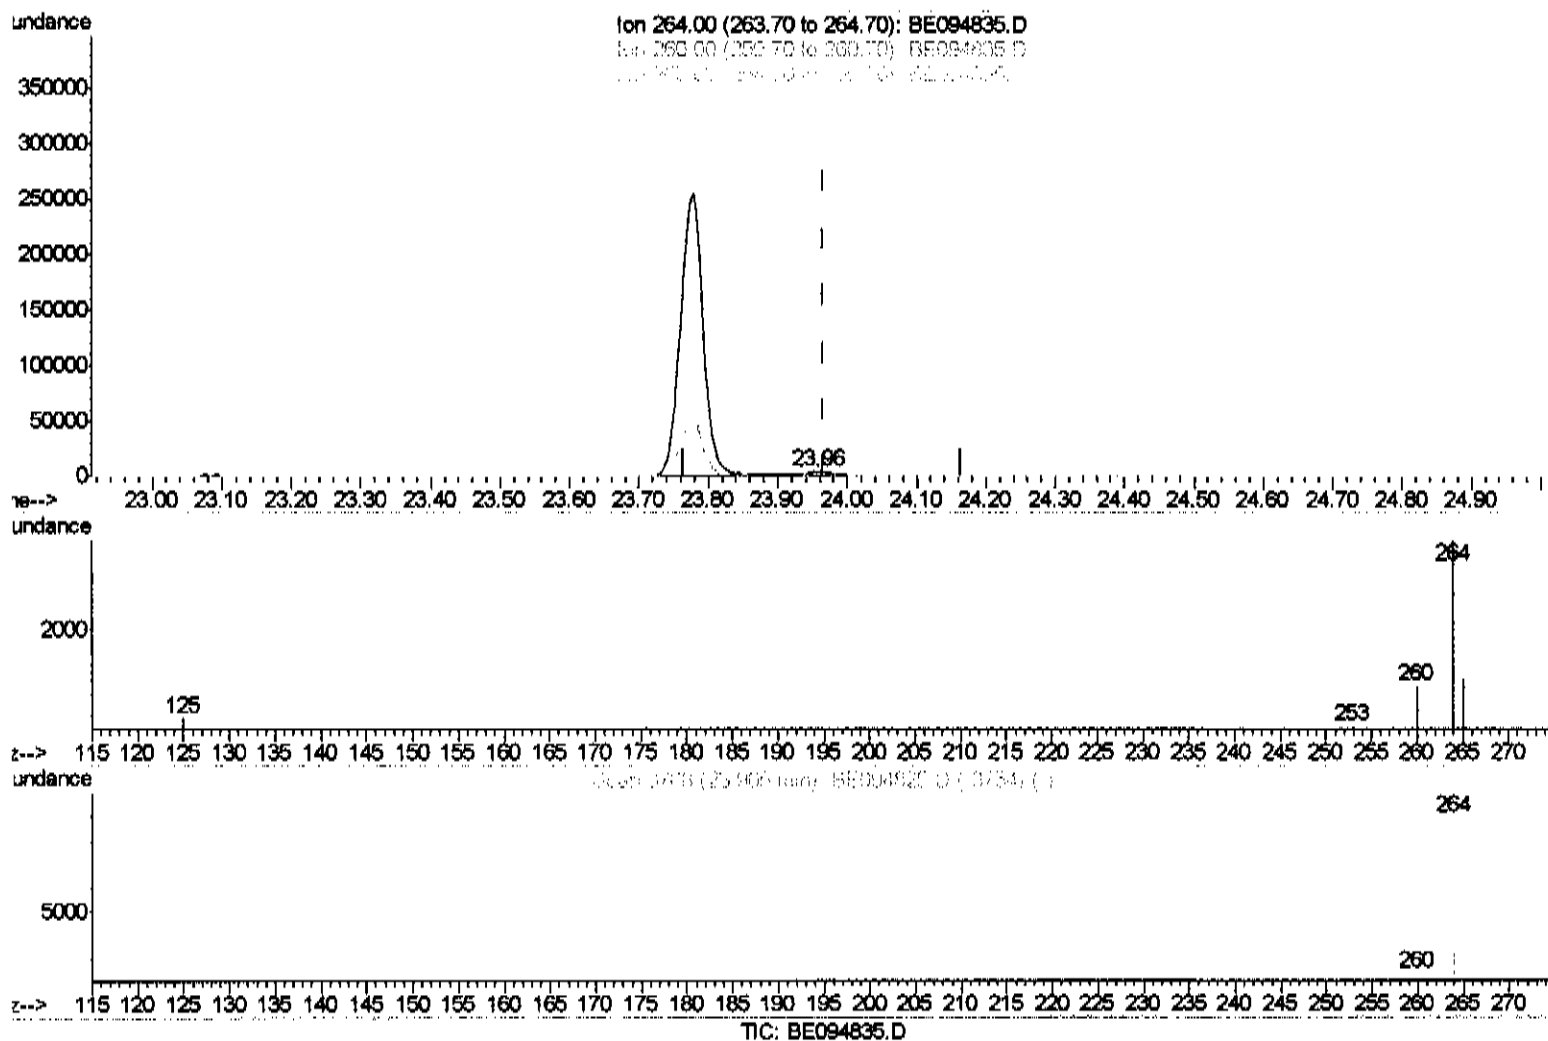

(20) Perylene-d12 (I)

23.955min (-0.010) 0.40ng/ul m

SJ 11/27/17

response 7478

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.65
265.00	103.50	29.49%
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

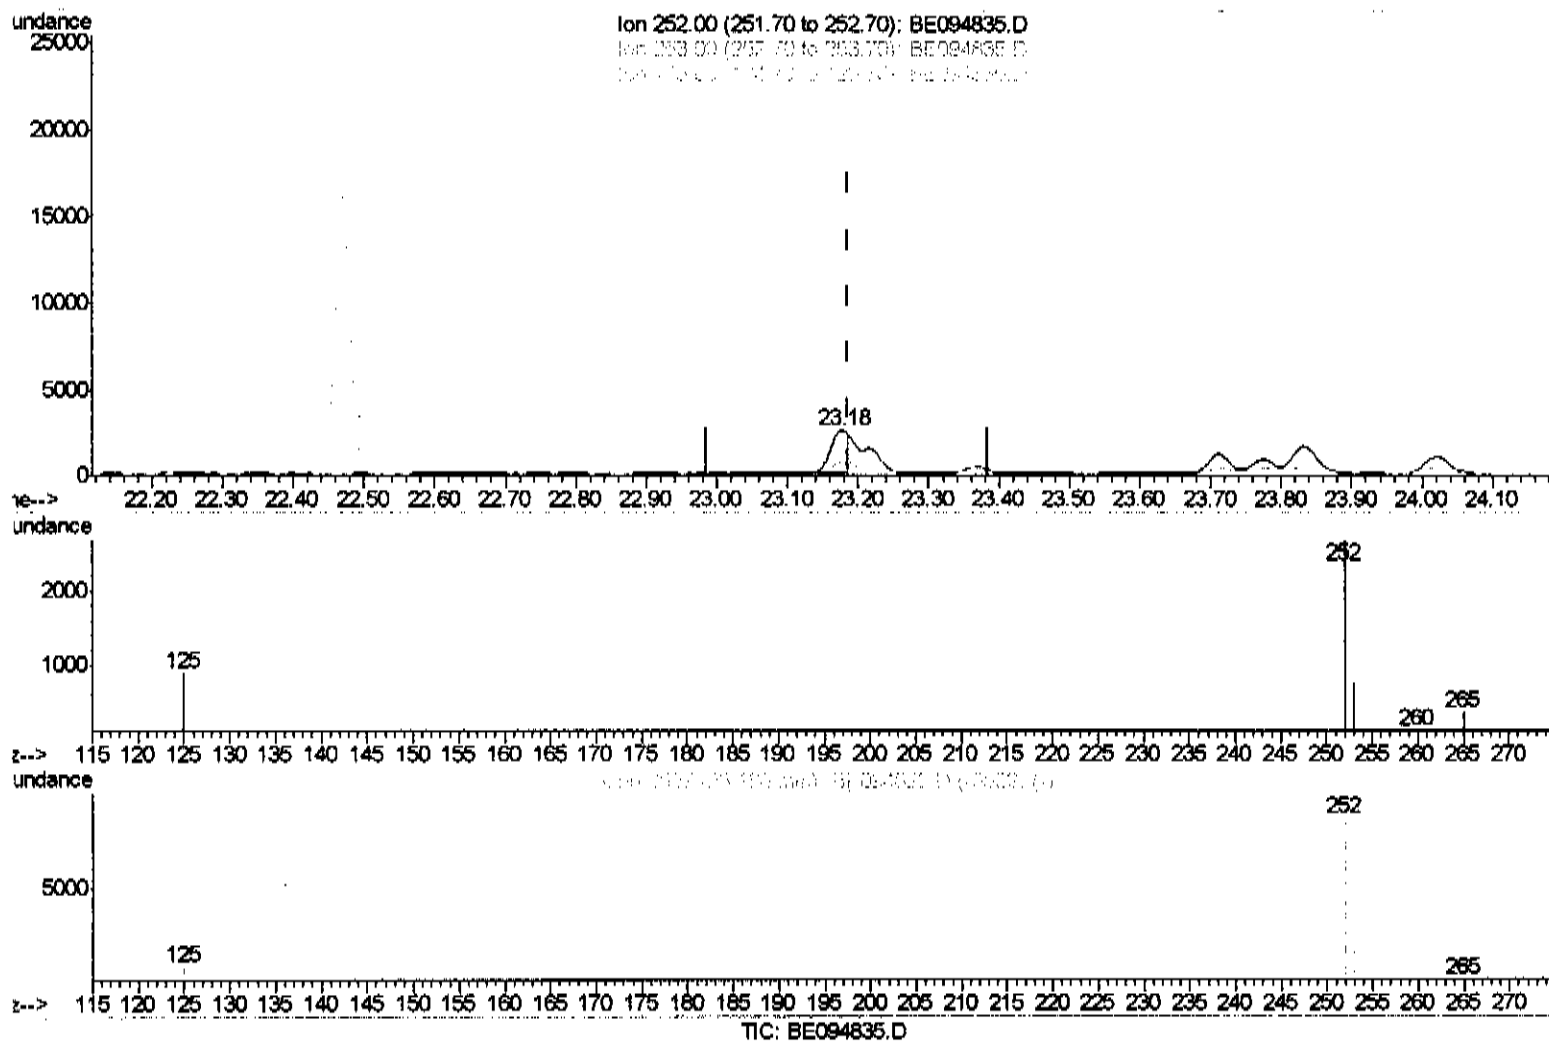

(21) Benzo(b)fluoranthene

23.176min (-0.010) 0.20ng/ul

response 4423

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.15
125.00	17.50	33.15
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

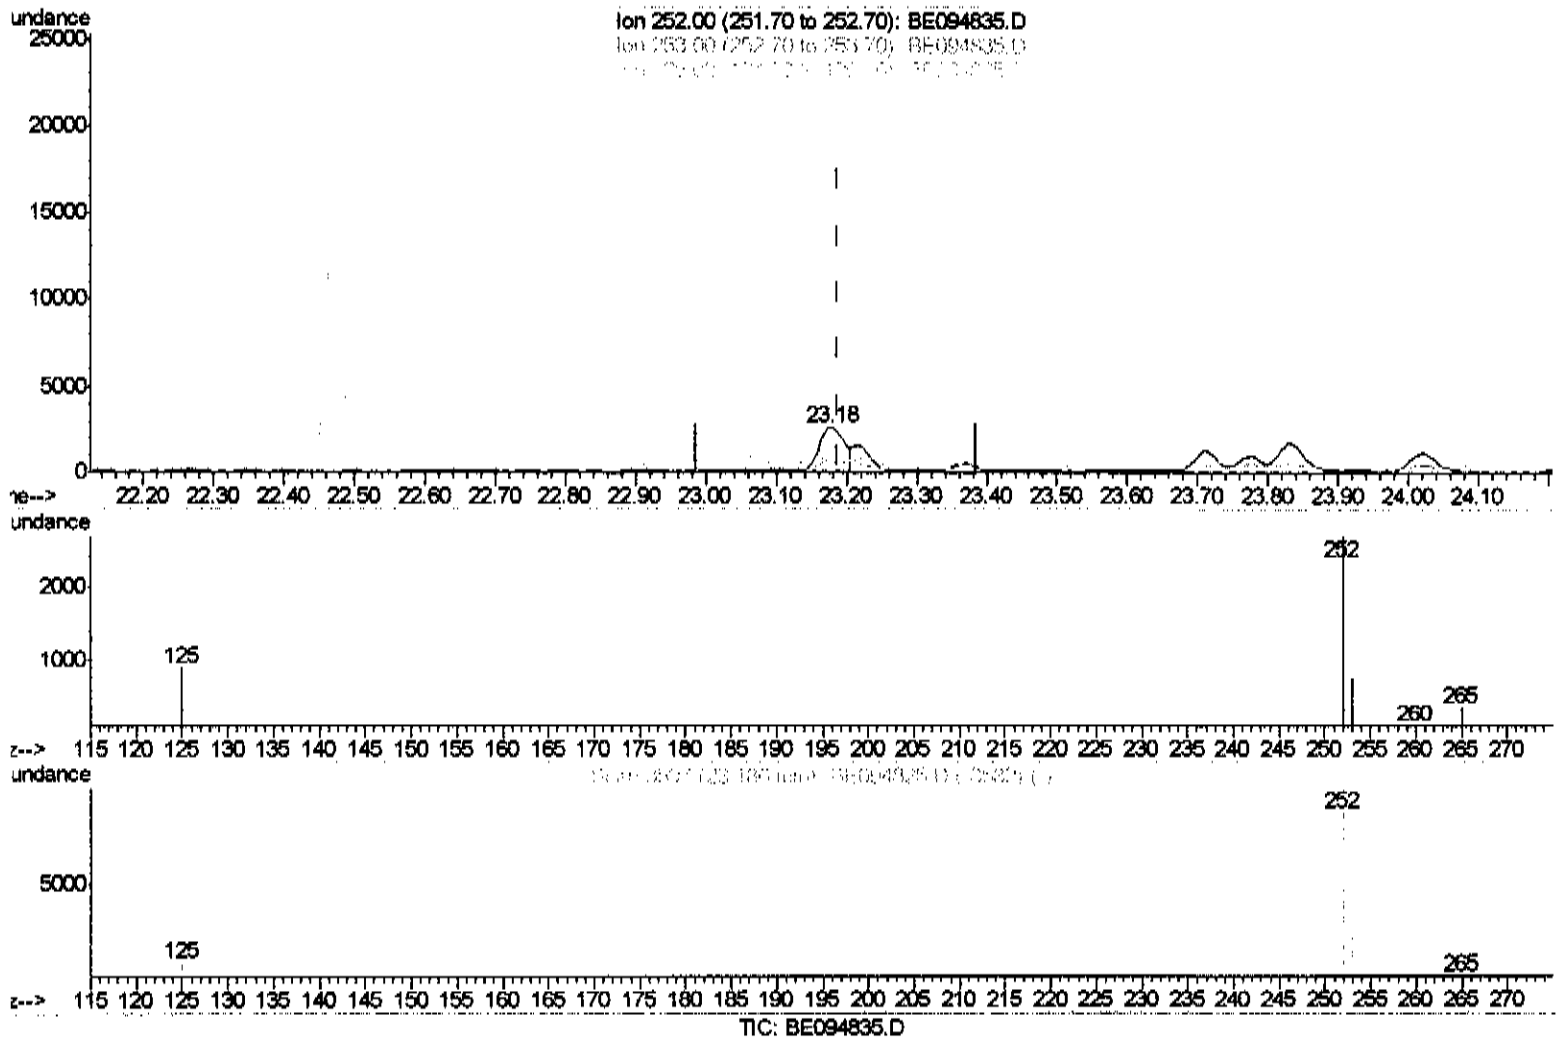

(21) Benzo(b)fluoranthene

23.176min (-0.010) 0.28ng/ul m

response 6239

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.15
125.00	17.50	33.15
0.00	0.00	0.00

SJ 11/27/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

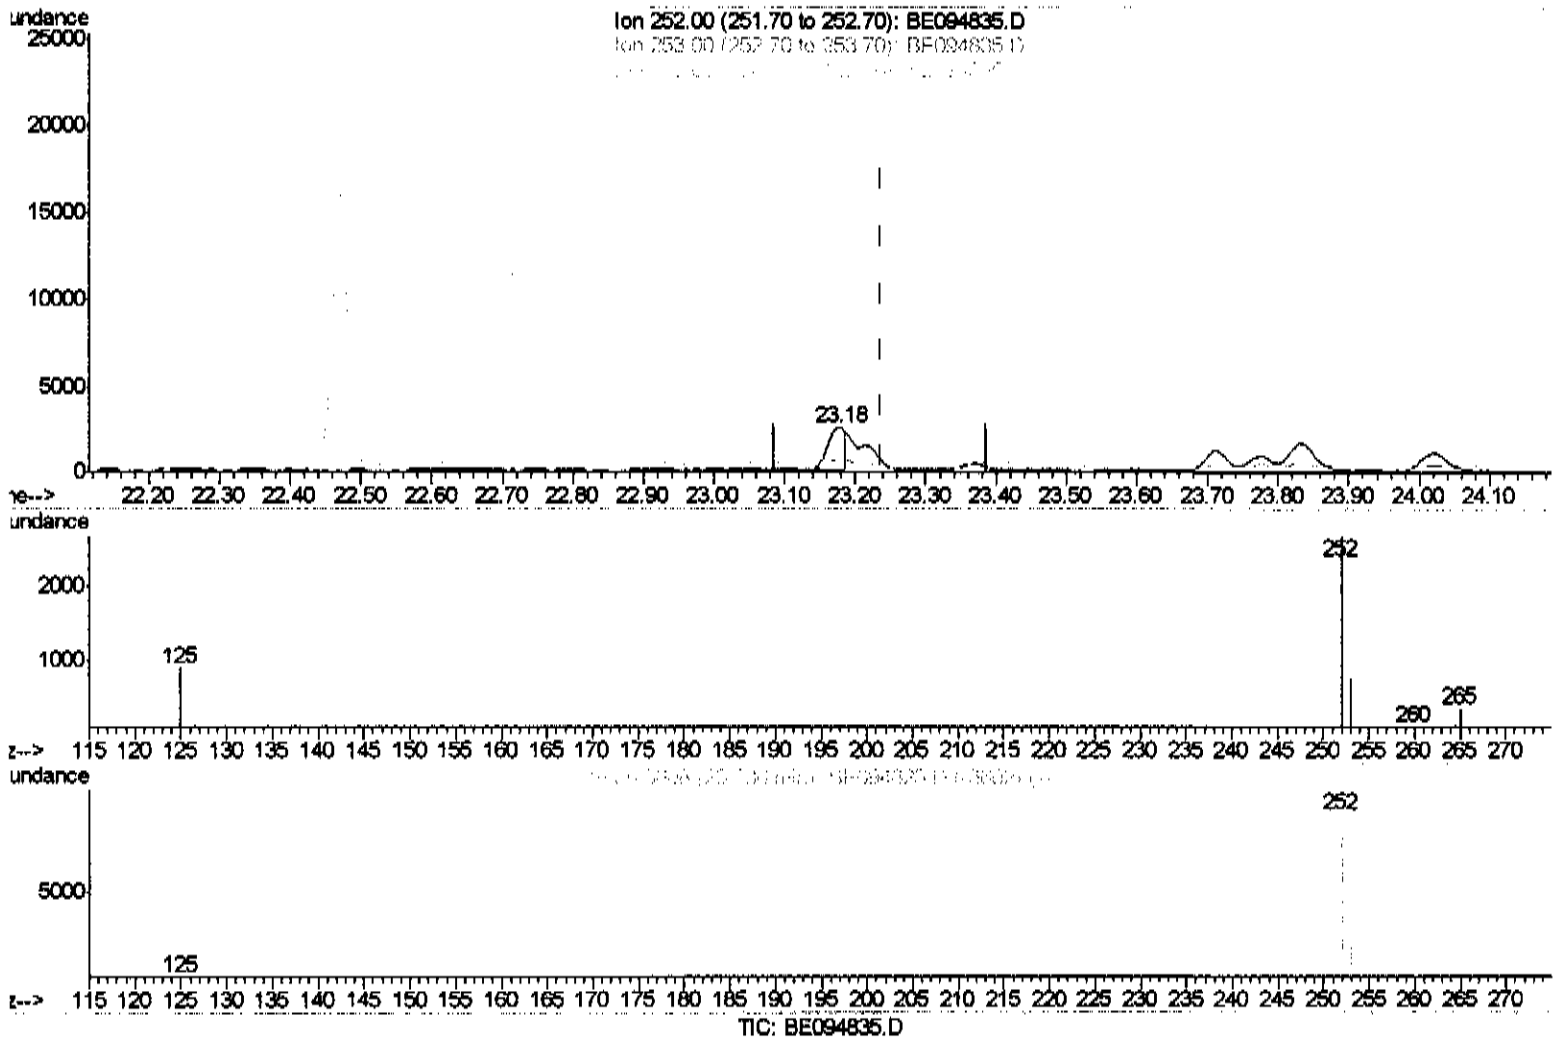

(22) Benzo(k)fluoranthene

23.176min (-0.060) 0.19ng/ul

response 4423

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	28.15
125.00	17.10	33.15#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

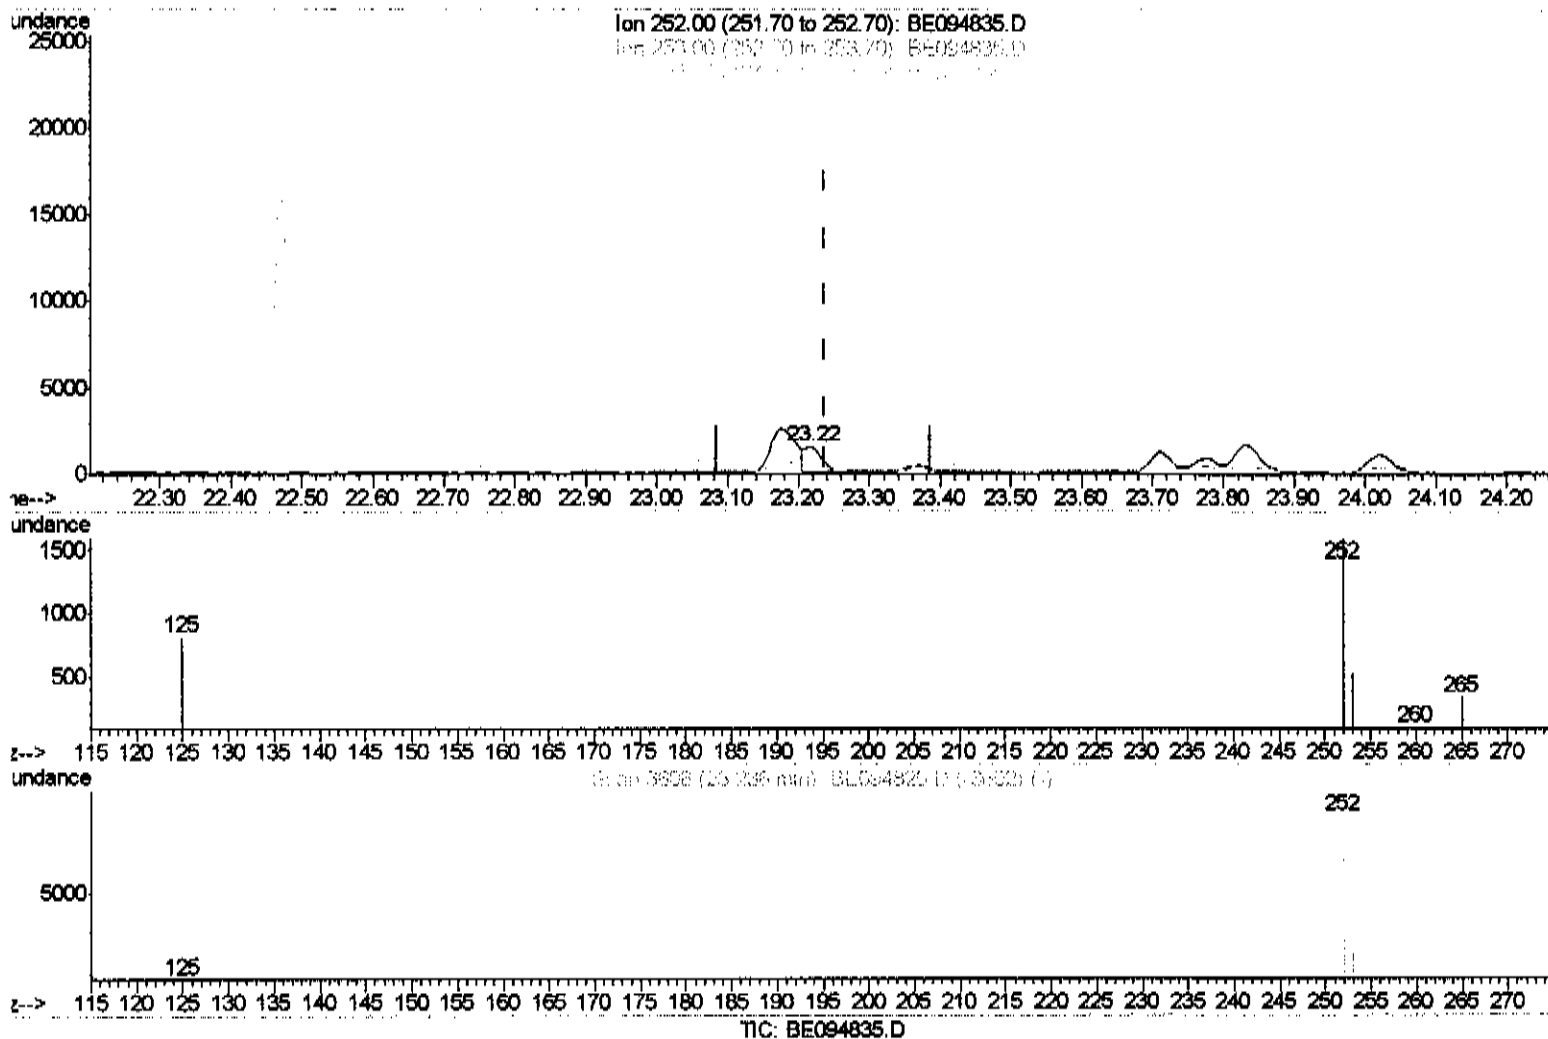

(22) Benzo(k)fluoranthene

23.217min (-0.019) 0.10ng/ul m

response 2455

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	32.64
125.00	17.10	51.08#
0.00	0.00	0.00

JU 11/27/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

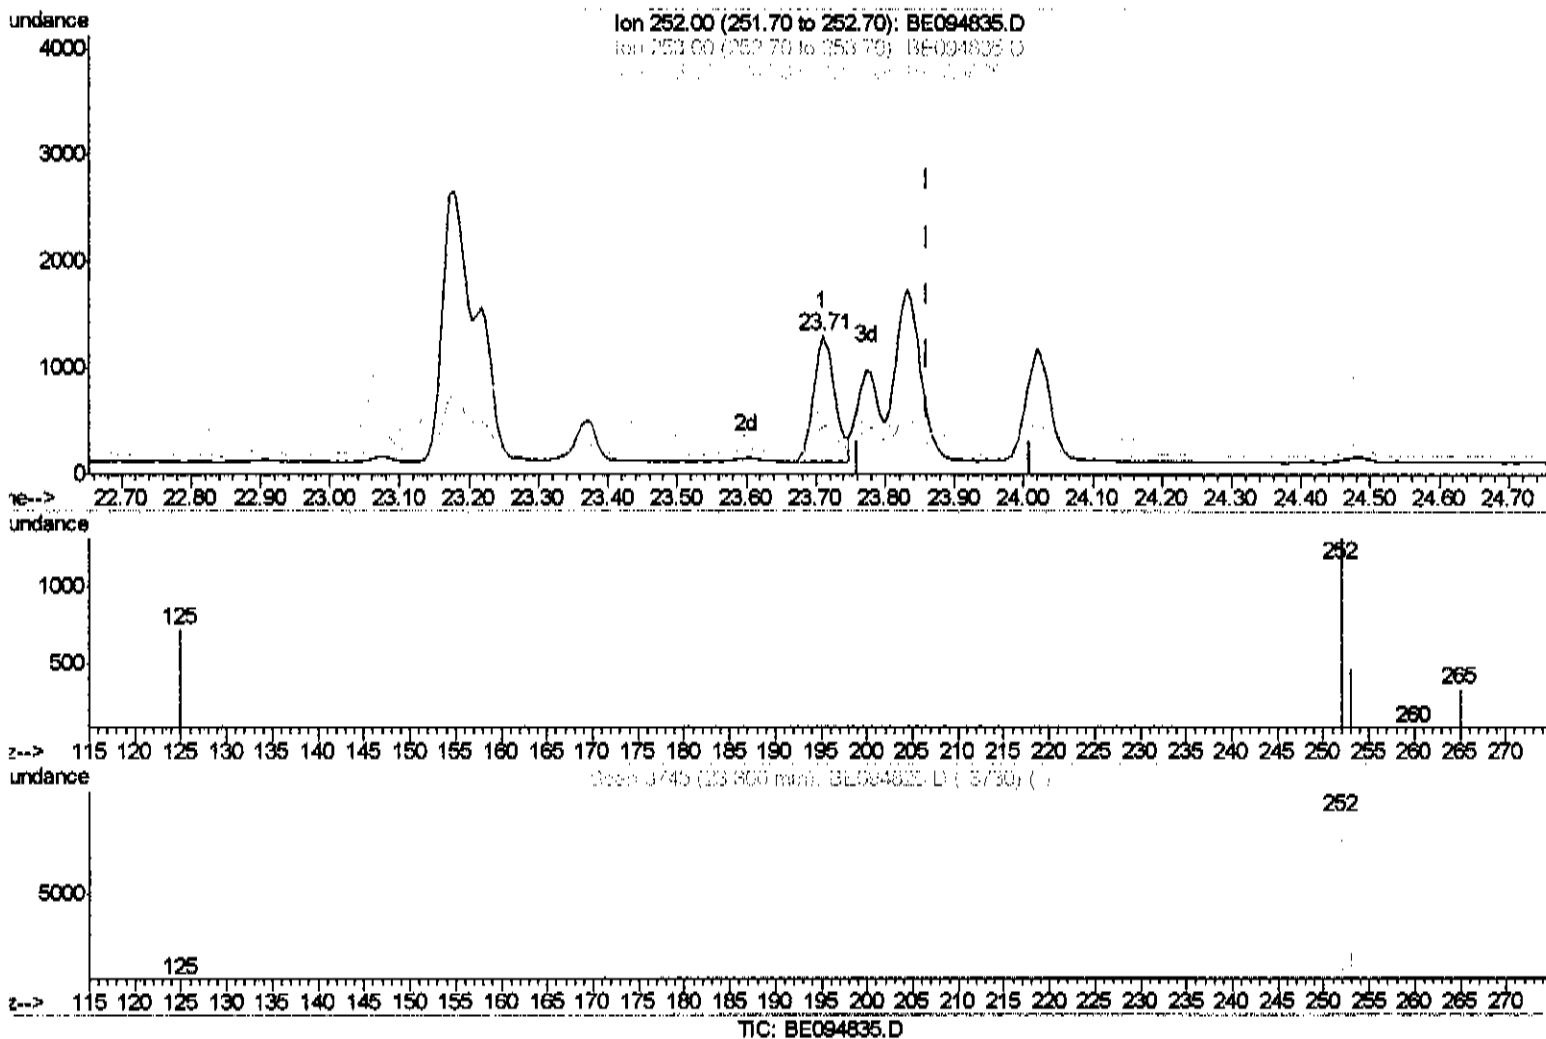

(23) Benzo(a)pyrene (C)

23.709min (-0.151) 0.11ng/ul

response 2530

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	34.89
125.00	22.60	54.96#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

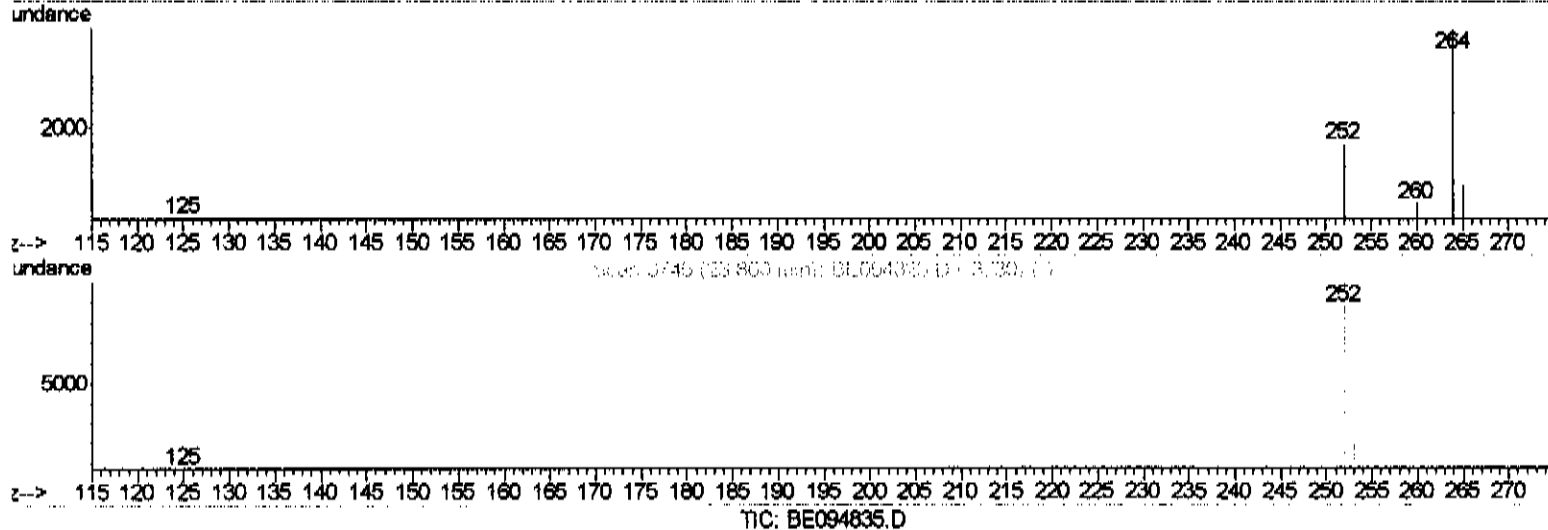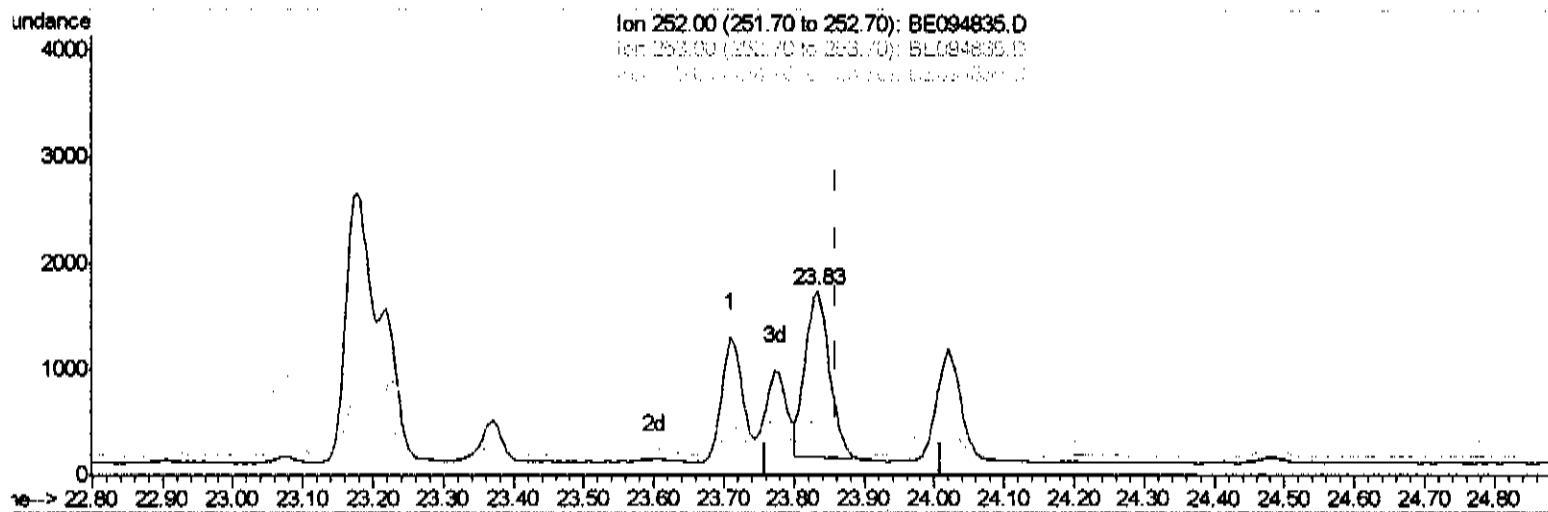

(23) Benzo(a)pyrene (C)

23.832min (-0.028) 0.17ng/ul m

response 3791

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	30.96
125.00	22.60	31.25#
0.00	0.00	0.00

JU 11/27/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

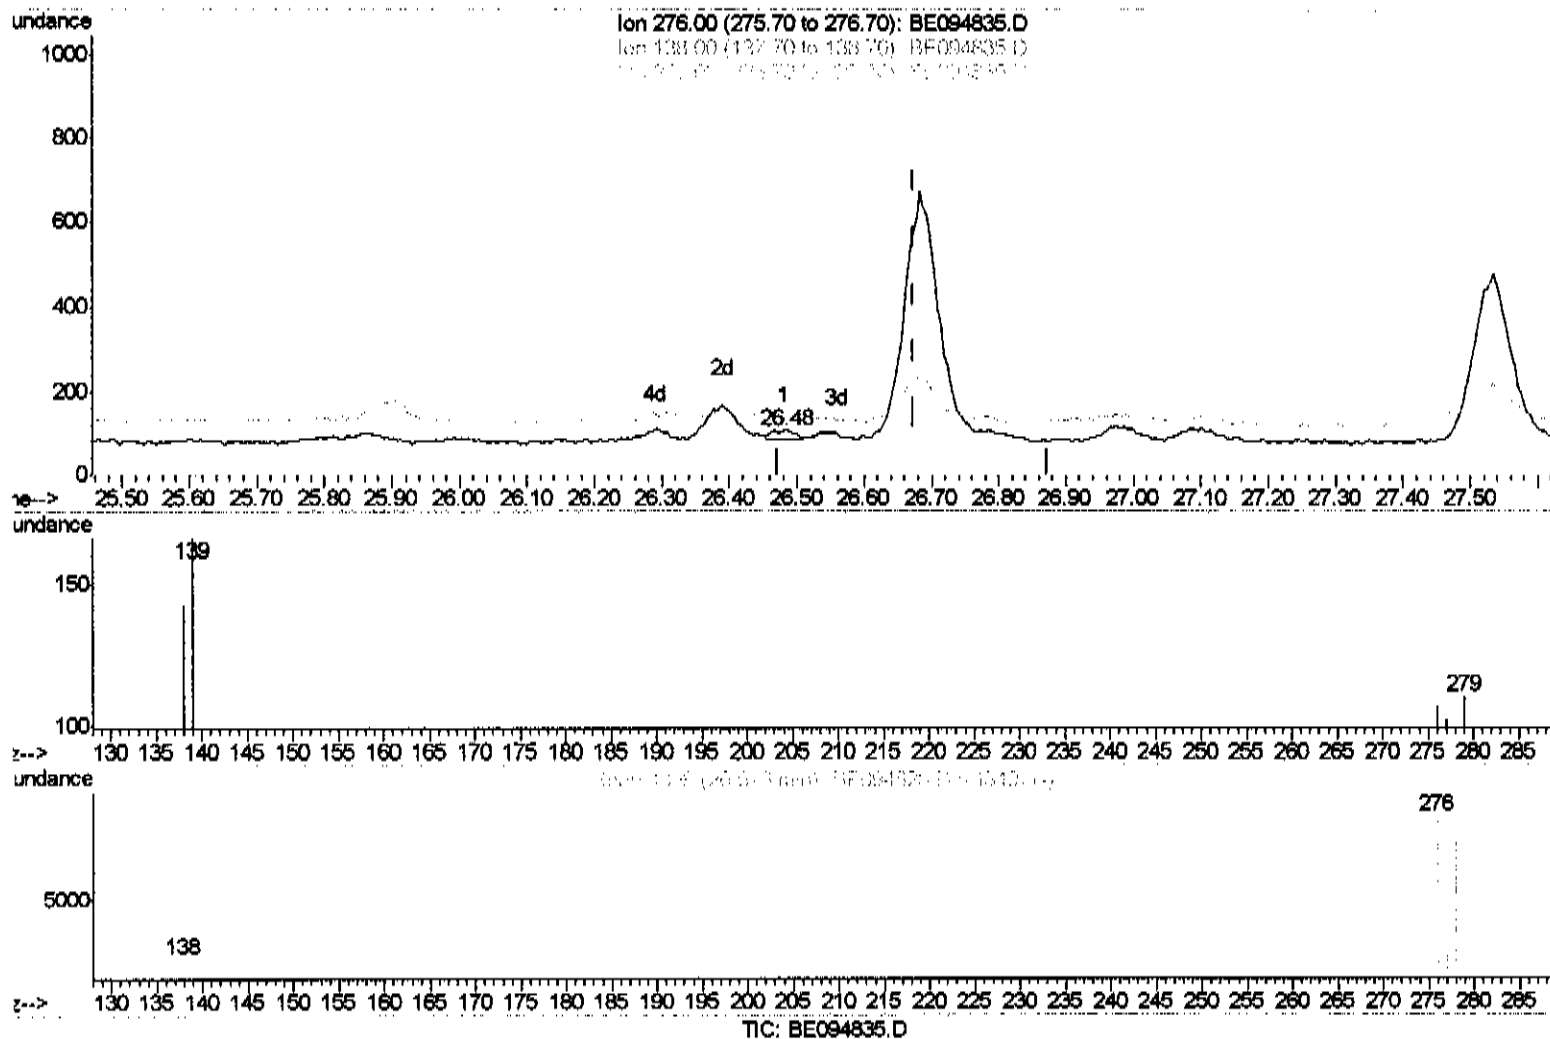

(24) Indeno(1,2,3-cd)pyrene

26.481min (-0.192) 0.00ng/ul

response 48

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	31.25
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

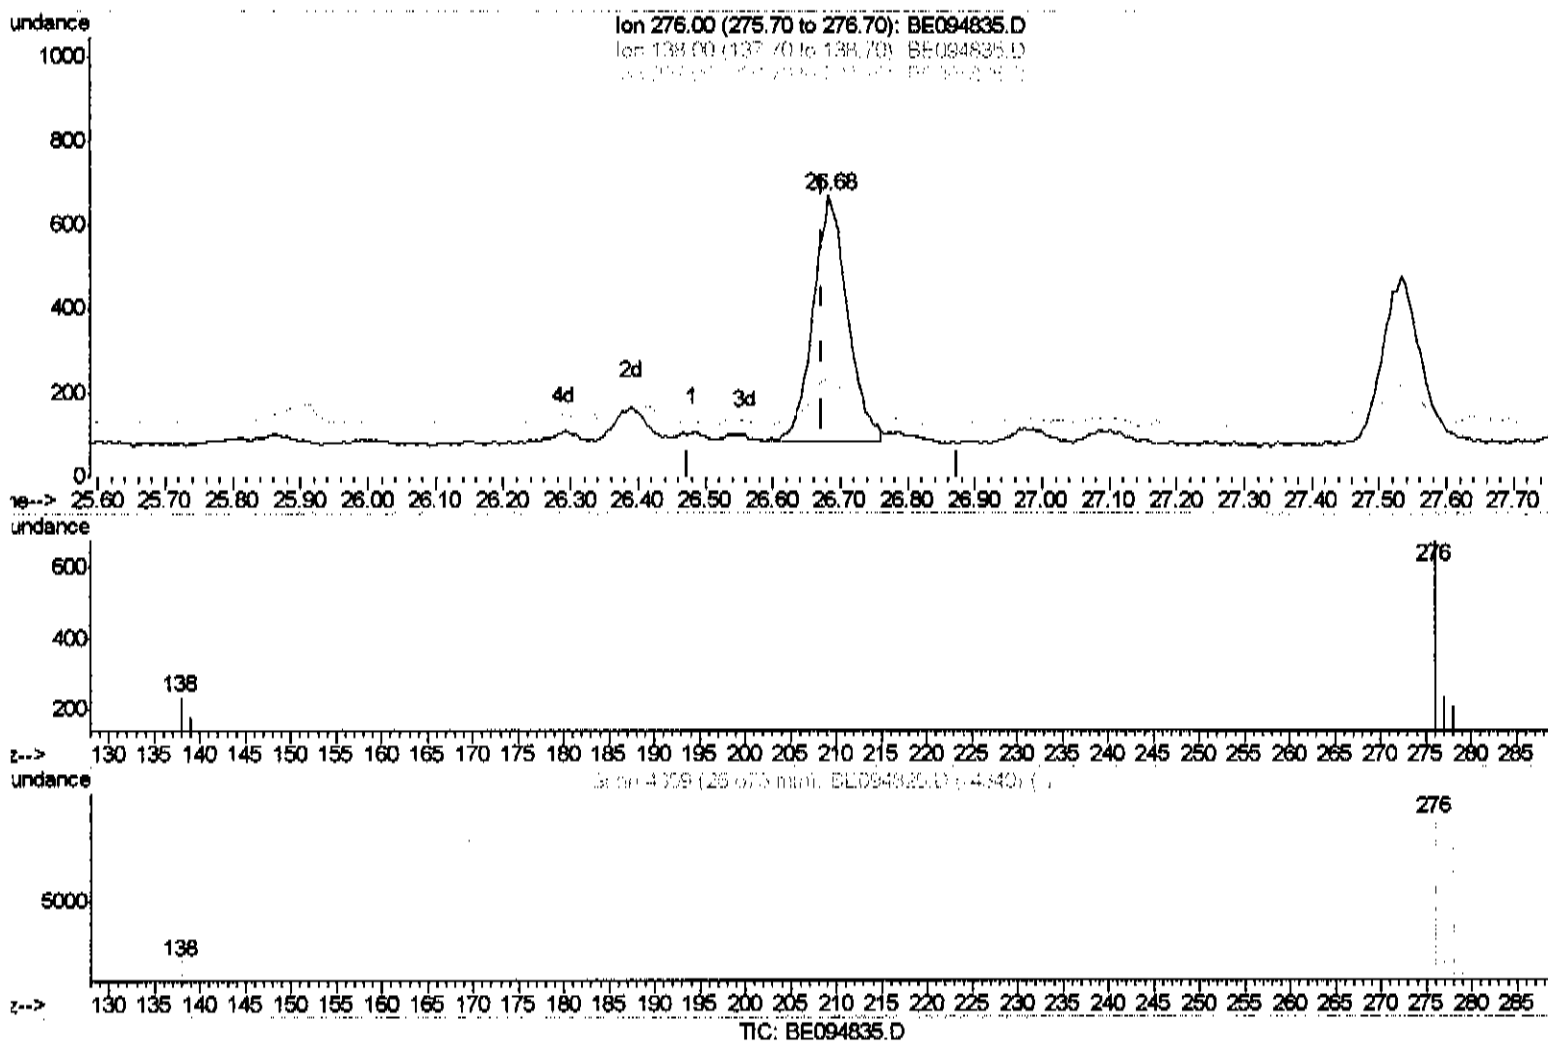

(24) Indeno(1,2,3-cd)pyrene

26.682min (+0.009) 0.09ng/ul m

response 2107

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	0.71#
227.00	10.00	0.00#
0.00	0.00	0.00

10/11/27/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

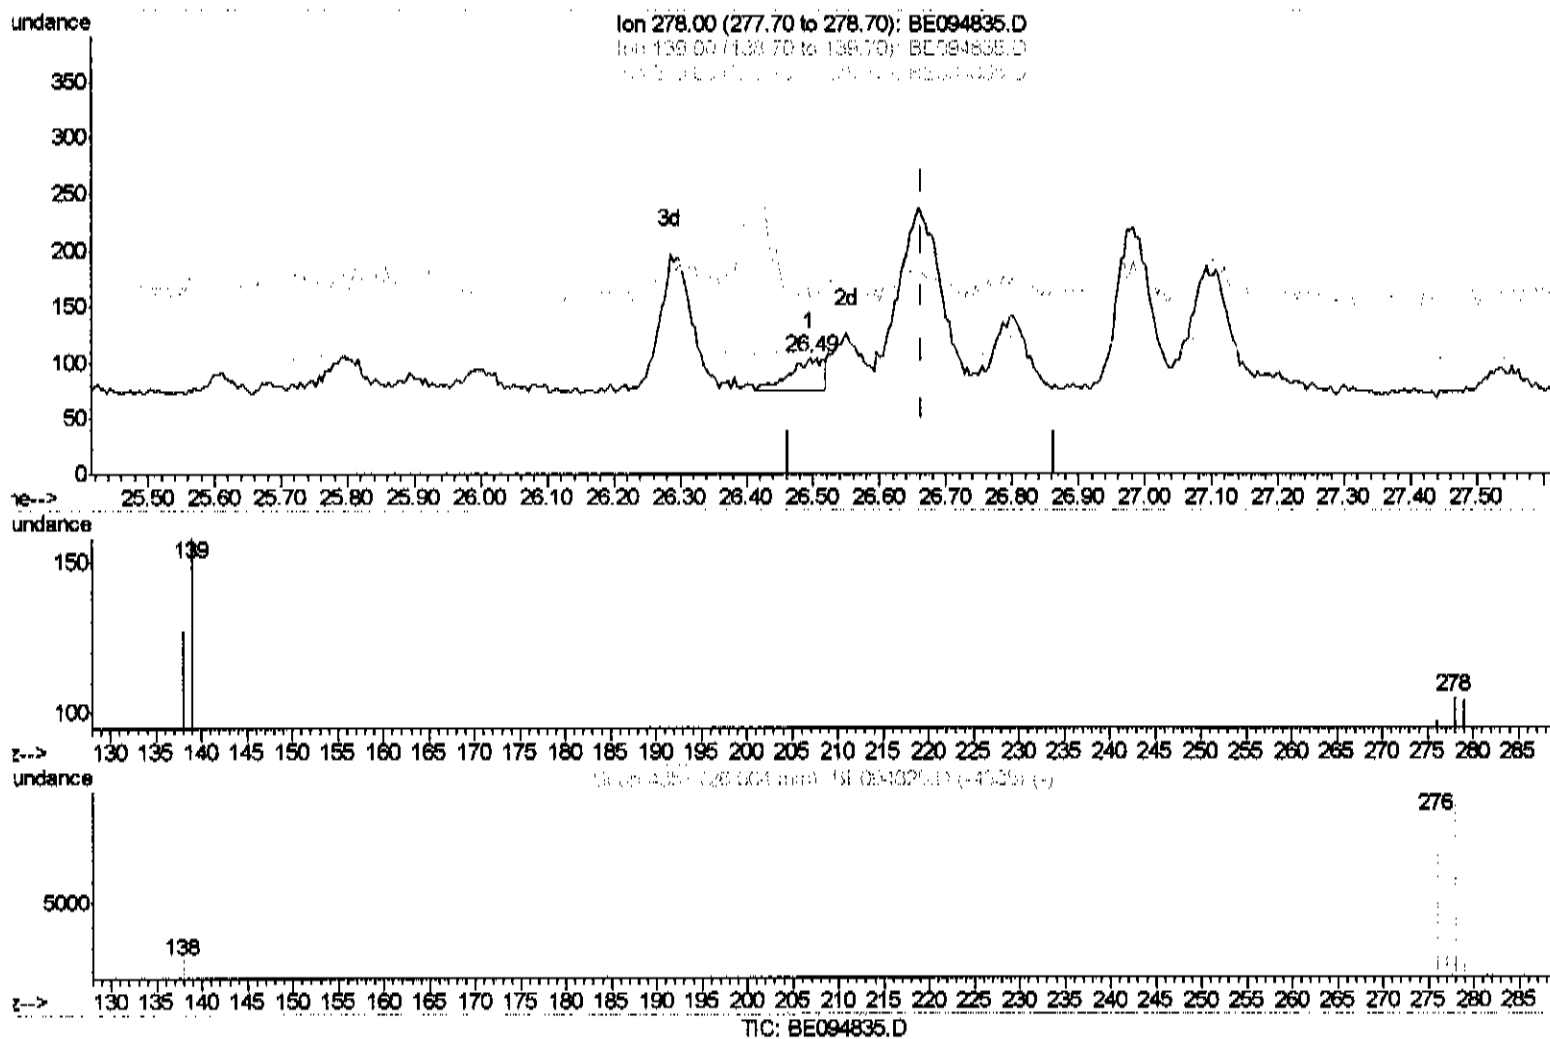

(25) Dibenzo(a,h)anthracene

26.495min (-0.169) 0.00ng/ul

response 96

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	150.48#
279.00	32.40	99.05#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

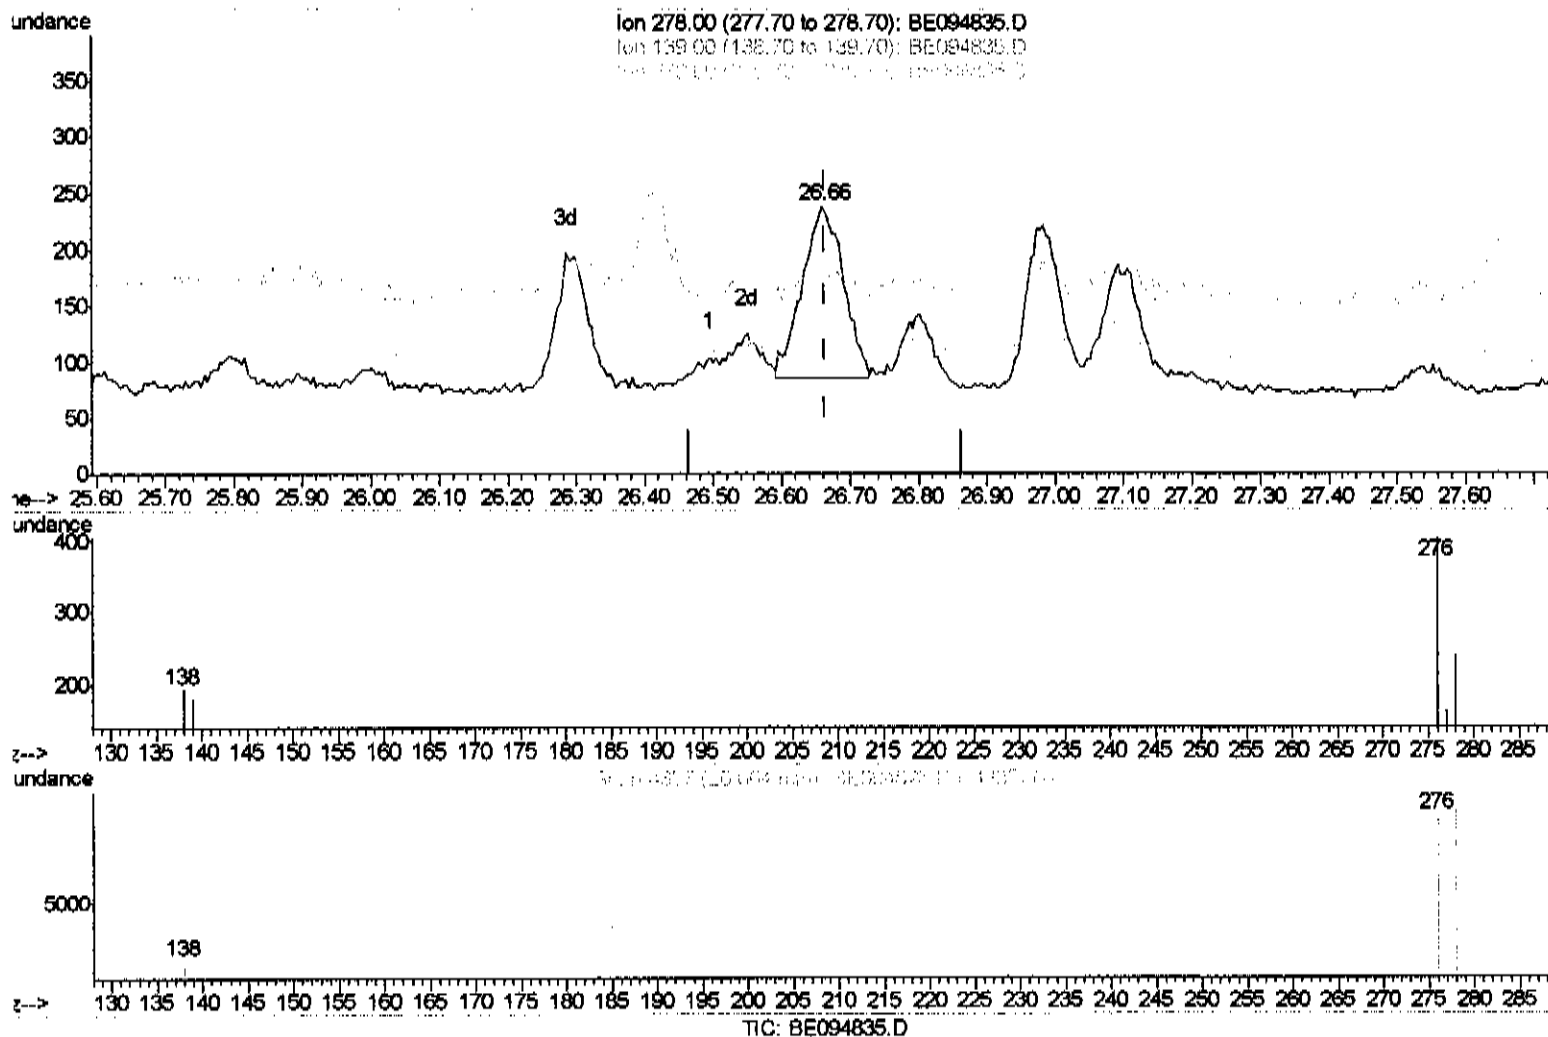

(25) Dibenzo(a,h)anthracene

26.659min (-0.005) 0.03ng/ul m

response 635

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	74.90#
279.00	32.40	58.58#
0.00	0.00	0.00

50 11/27/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

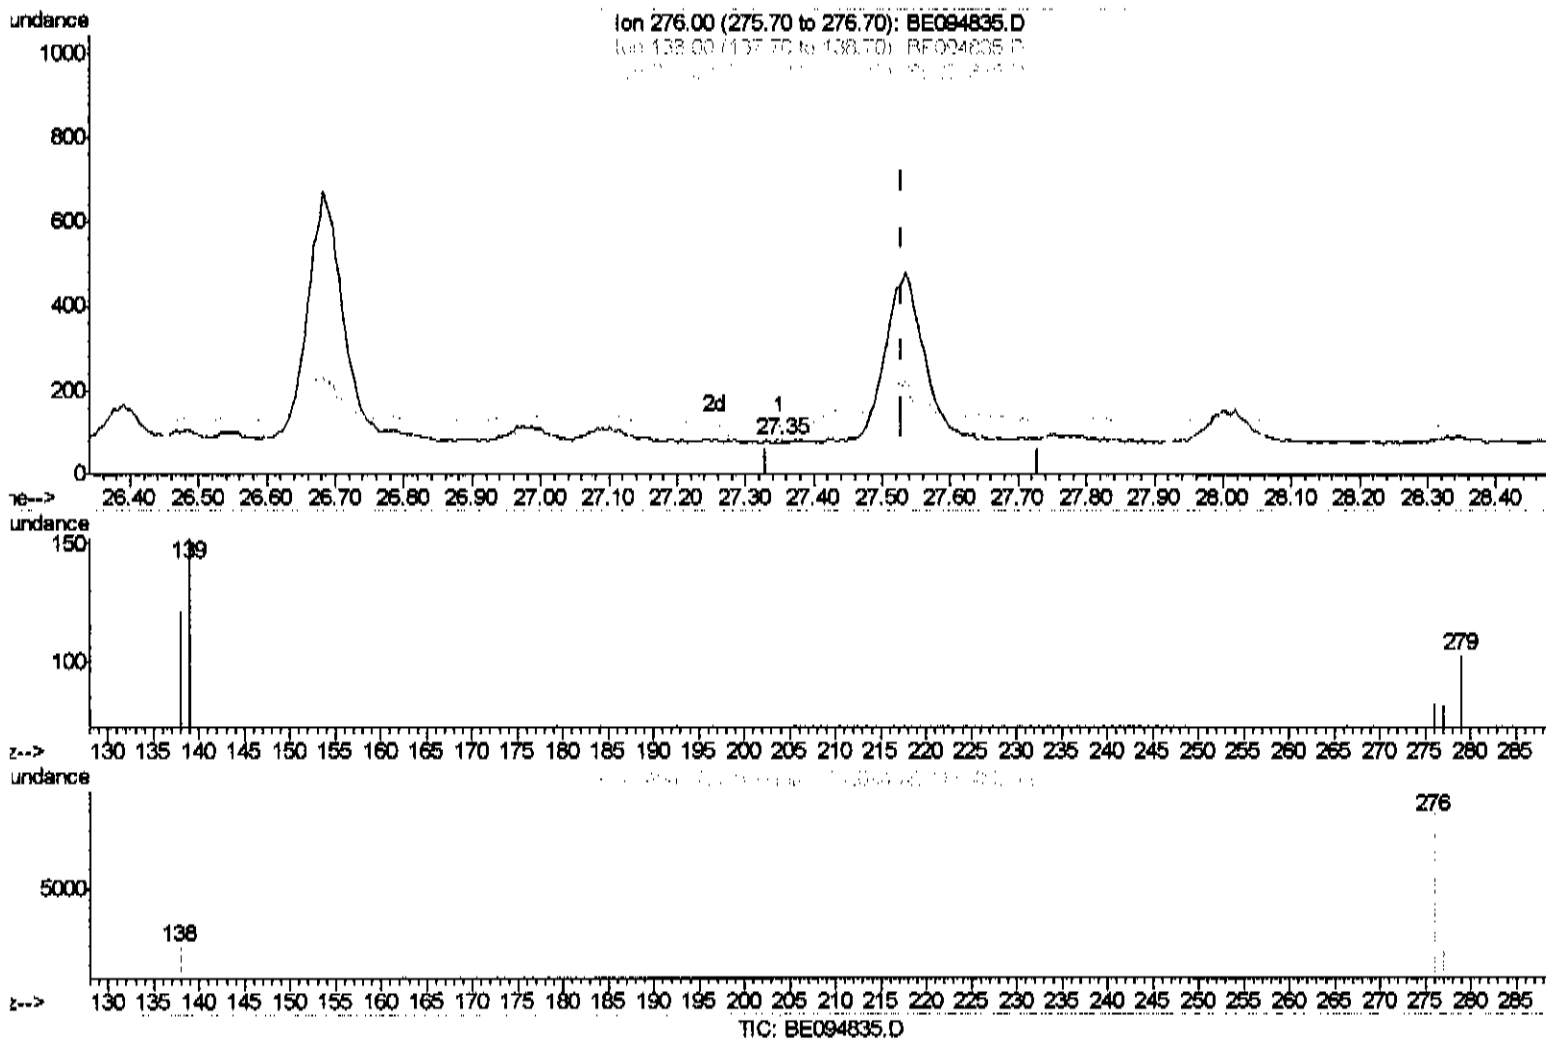

(26) Benzo(g,h,i)perylene

27.352min (-0.178) 0.00ng/ul

response 9

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	145.78#
277.00	25.60	98.80#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

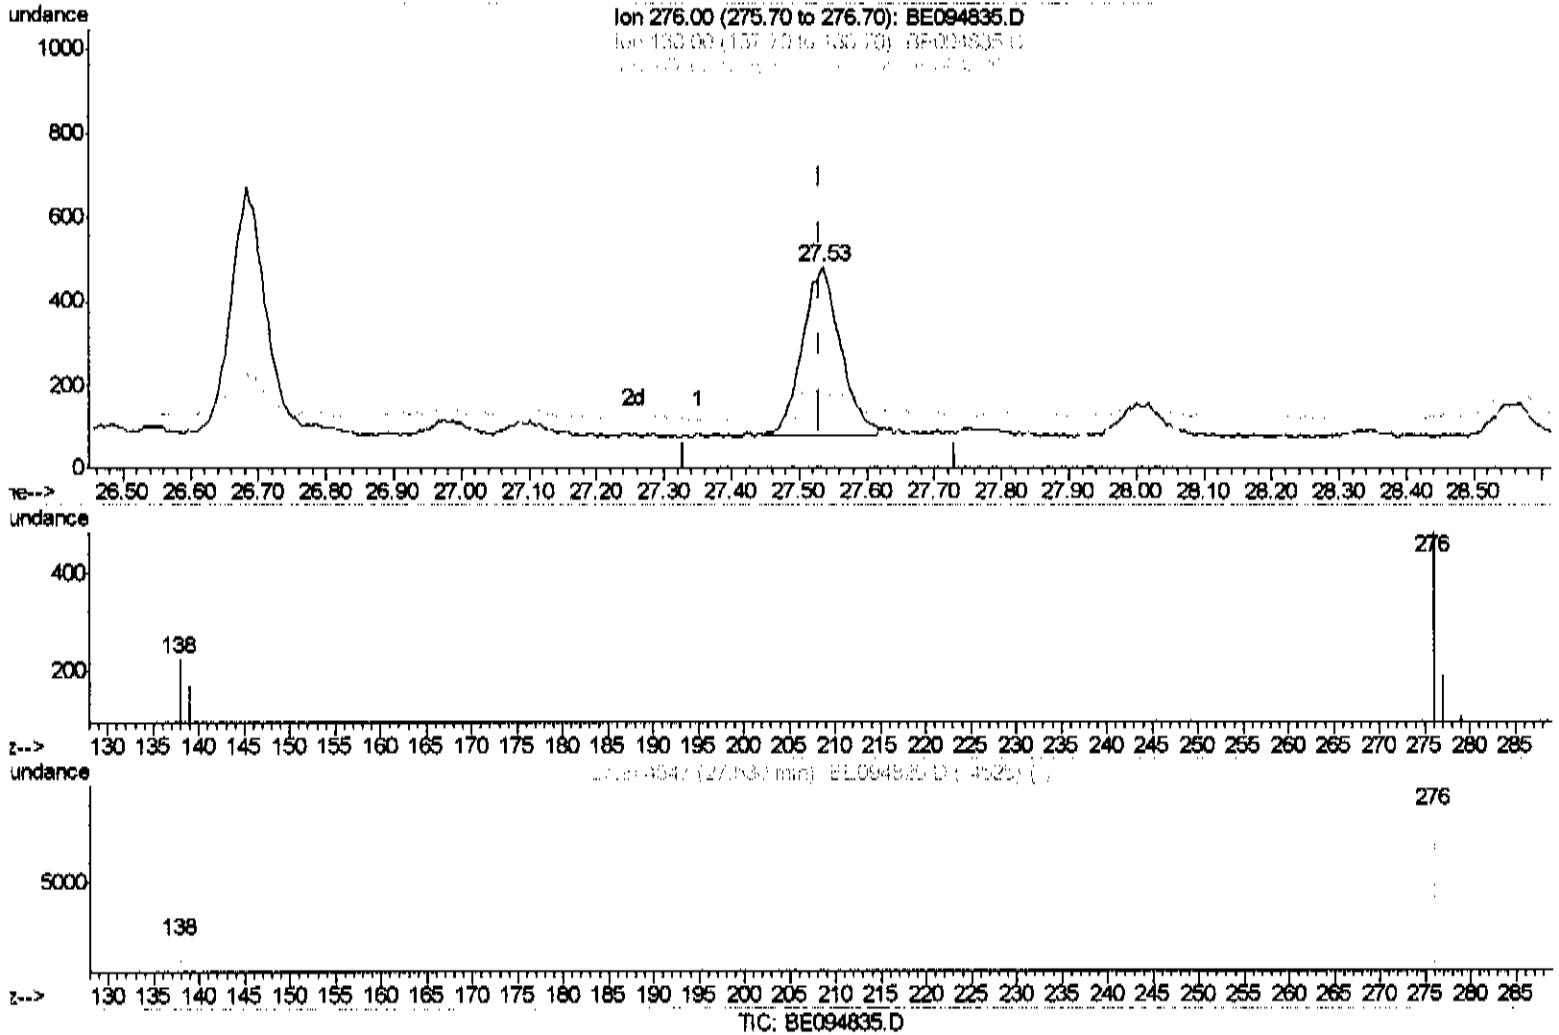

(26) Benzo(g,h,i)perylene

27.534min (+0.004) 0.08ng/ul m

response 1582

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	46.89#
277.00	25.60	39.63#
0.00	0.00	0.00

JU 11/27/17

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:11 PM

Quant Time: Nov 23 01:52:48 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	752	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.67	136	4893	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.50	164	3493	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	8523m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.42	240	8767	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	7478m	0.40	ng/ul	0.00

JU 11/27/17
 JU 11/27/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	2523	0.32	ng/ul	0.01
14) Fluoranthene-d10	19.27	212	7982	0.27	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) Phenanthrene	17.27	178	1524m	0.07	ng/ul	>
13) Anthracene	17.36	178	774m	0.03	ng/ul	>
15) Fluoranthene	19.30	202	10206	0.34	ng/ul	83
17) Pyrene	19.66	202	10308	0.38	ng/ul#	83
18) Benzo(a)anthracene	21.41	228	7046	0.26	ng/ul#	90
19) Chrysene	21.46	228	6548	0.25	ng/ul	96
21) Benzo(b)fluoranthene	23.18	252	6239m	0.28	ng/ul	
22) Benzo(k)fluoranthene	23.22	252	2455m	0.10	ng/ul	
23) Benzo(a)pyrene	23.83	252	3791m	0.17	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.68	276	2107m	0.09	ng/ul	
25) Dibenzo(a,h)anthracene	26.66	278	635m	0.03	ng/ul	
26) Benzo(a,h,i)perylene	27.53	276	1582m	0.08	ng/ul	

JU 11/27/17
 JU 11/27/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed