

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094836.D
Acq On : 22 Nov 2017 17:46
Operator : SJ/JU
Sample : PB104369BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 23 01:58:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration

Instrument :
BNA_E
Client Sampled :
SBLK69

Manual Integrations
APPROVED

Sohil
11/27/2017 3:25:13 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	668	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.67	136	4321	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.50	164	3169	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	7879m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.44	240	8069	0.40	ng/ul	0.01
20) Perylene-d12	23.97	264	9337	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	2542	0.36	ng/ul	0.03
14) Fluoranthene-d10	19.27	212	8489	0.31	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} JU 11/27/17


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094836.D
Acq On : 22 Nov 2017 17:46
Operator : SJ/JU
Sample : PB104869BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 23 01:58:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
SBLK69

Manual Integrations
APPROVED

Sohil
11/27/2017 3:25:13 PM

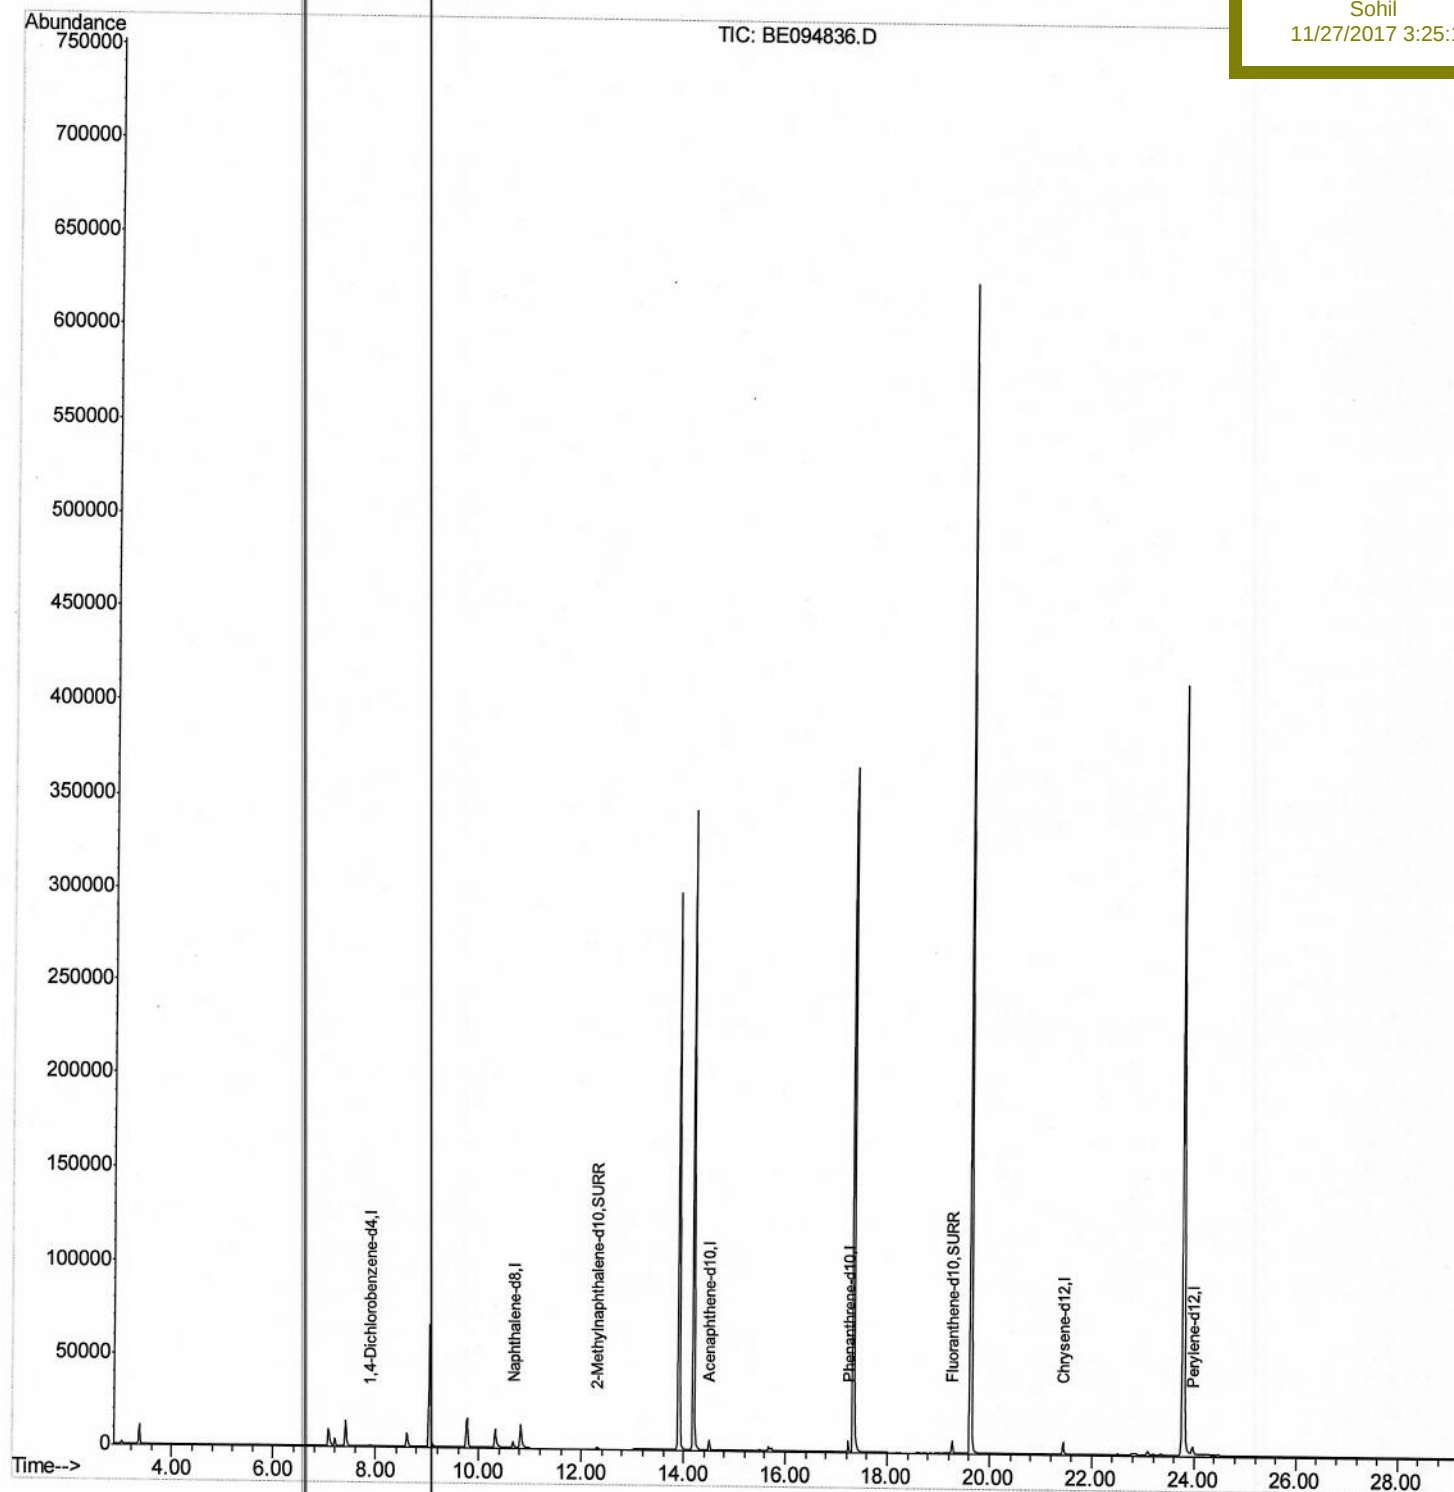

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094836.D
 Acq On : 22 Nov 2017 17:46
 Operator : SJ/JU
 Sample : PB104369BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 23 00:58:37 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK69

Manual Integrations
 APPROVED

Sohil
 11/27/2017 3:25:13 PM

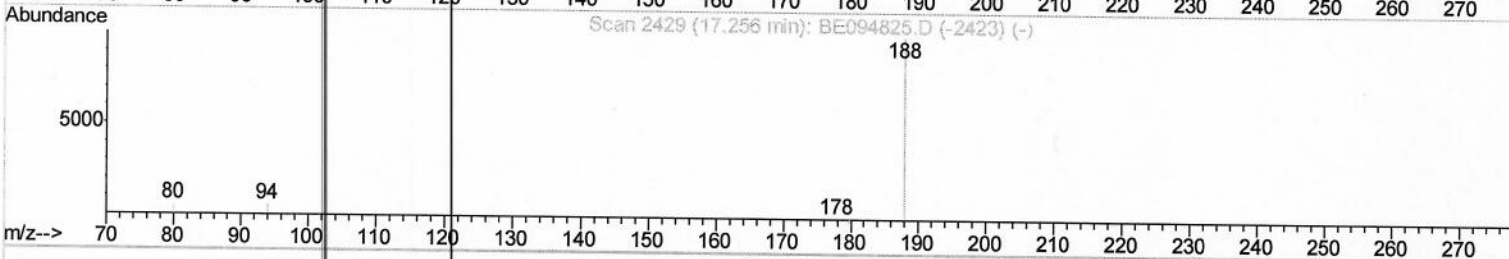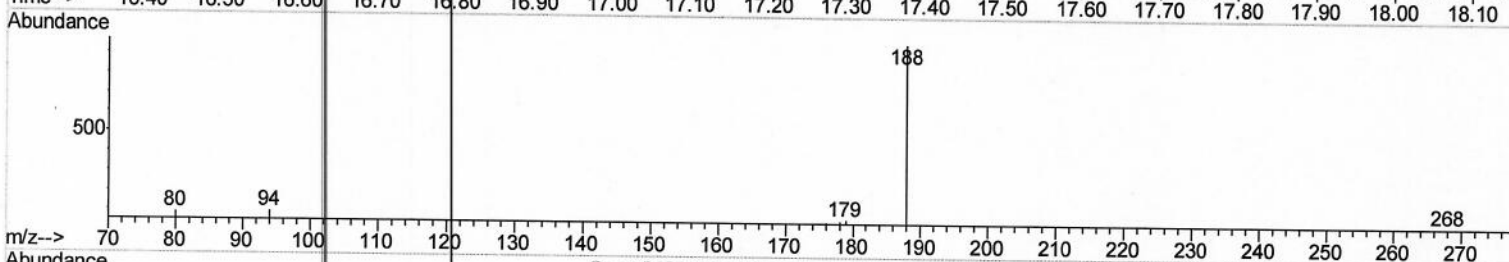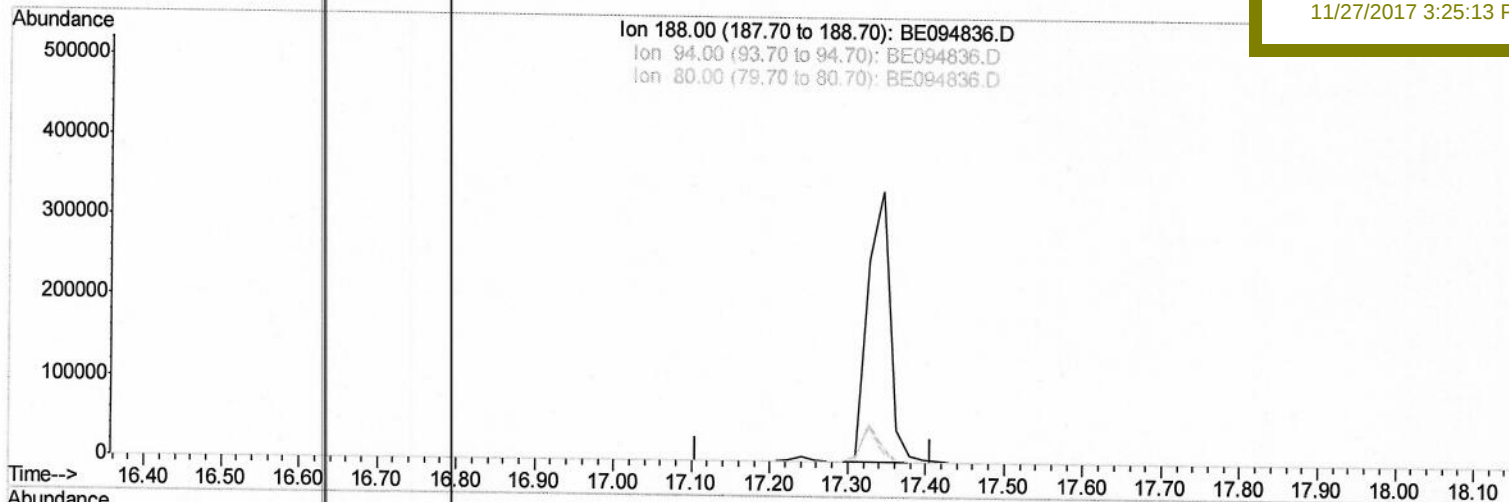

TIC: BE094836.D

(10) Phenanthrene-d10 (I)

17.256min (-17.256) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094836.D
 Acq On : 22 Nov 2017 17:46
 Operator : SJ/JU
 Sample : PB104369BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

SBLK69

Quant Time: Nov 23 00:58:37 2017

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




QLast Update : Thu Nov 23 00:56:52 2017

Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil

11/27/2017 3:25:13 PM

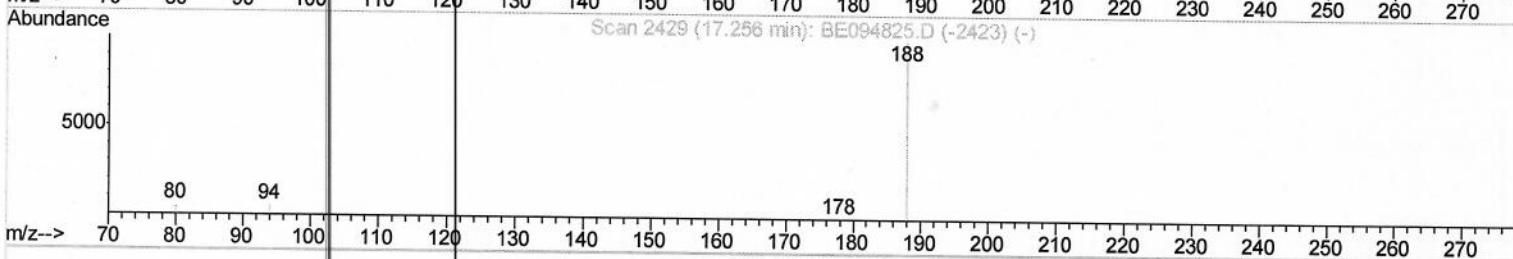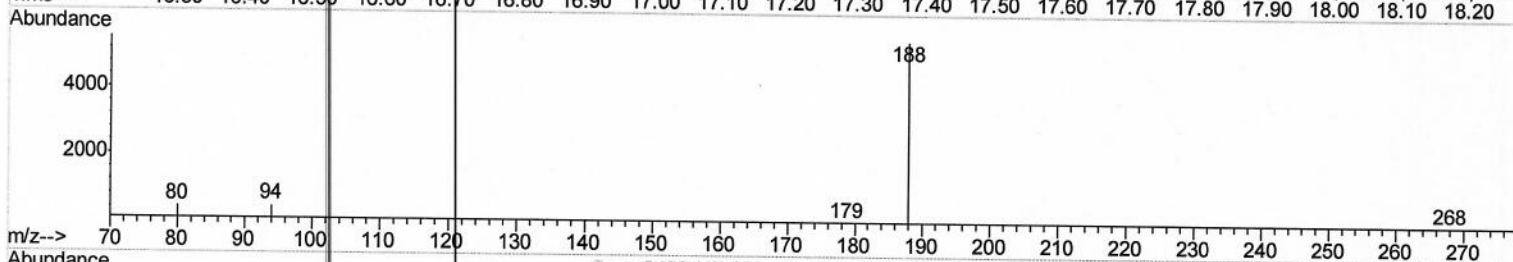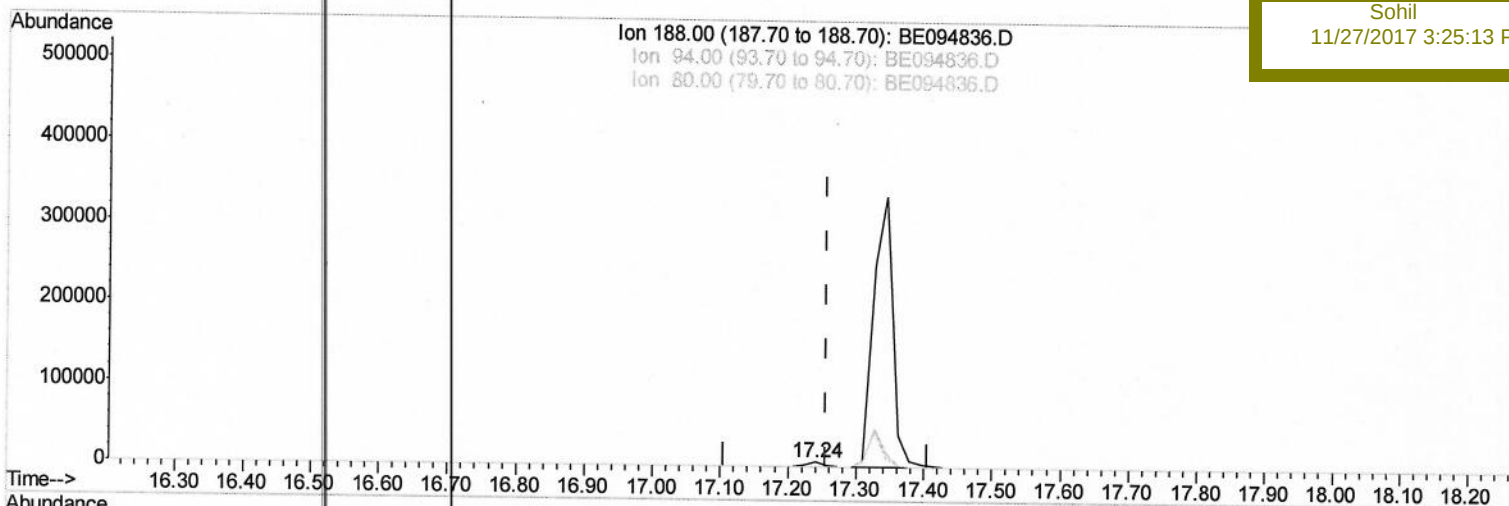

TIC: BE094836.D

(10) Phenanthrene-d10 (I)

17.240min (-0.016) 0.40ng/ul m

JUN 11/27/17

response 7879

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.84#
80.00	11.80	7.60#
0.00	0.00	0.00