

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094850.D
 Acq On : 23 Nov 2017 2:01
 Operator : SJ/JU
 Sample : I6496-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC1

Quant Time: Nov 23 03:23:00 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 02:50:08 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	745	0.40	ng/ul	-0.04
2) Naphthalene-d8	10.67	136	4998	0.40	ng/ul	-0.04
6) Acenaphthene-d10	14.50	164	3448	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.24	188	8073	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	8651	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	9772	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	1869	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	7201	0.26	ng/ul	-0.01
Target Compounds						
12) Phenanthrene	17.27	178	580	0.027	ng/ul#	Ovalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094850.D
Acq On : 23 Nov 2017 2:01
Operator : SJ/JU
Sample : I6496-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC1

Quant Time: Nov 23 03:23:00 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 02:50:08 2017
Response via : Initial Calibration

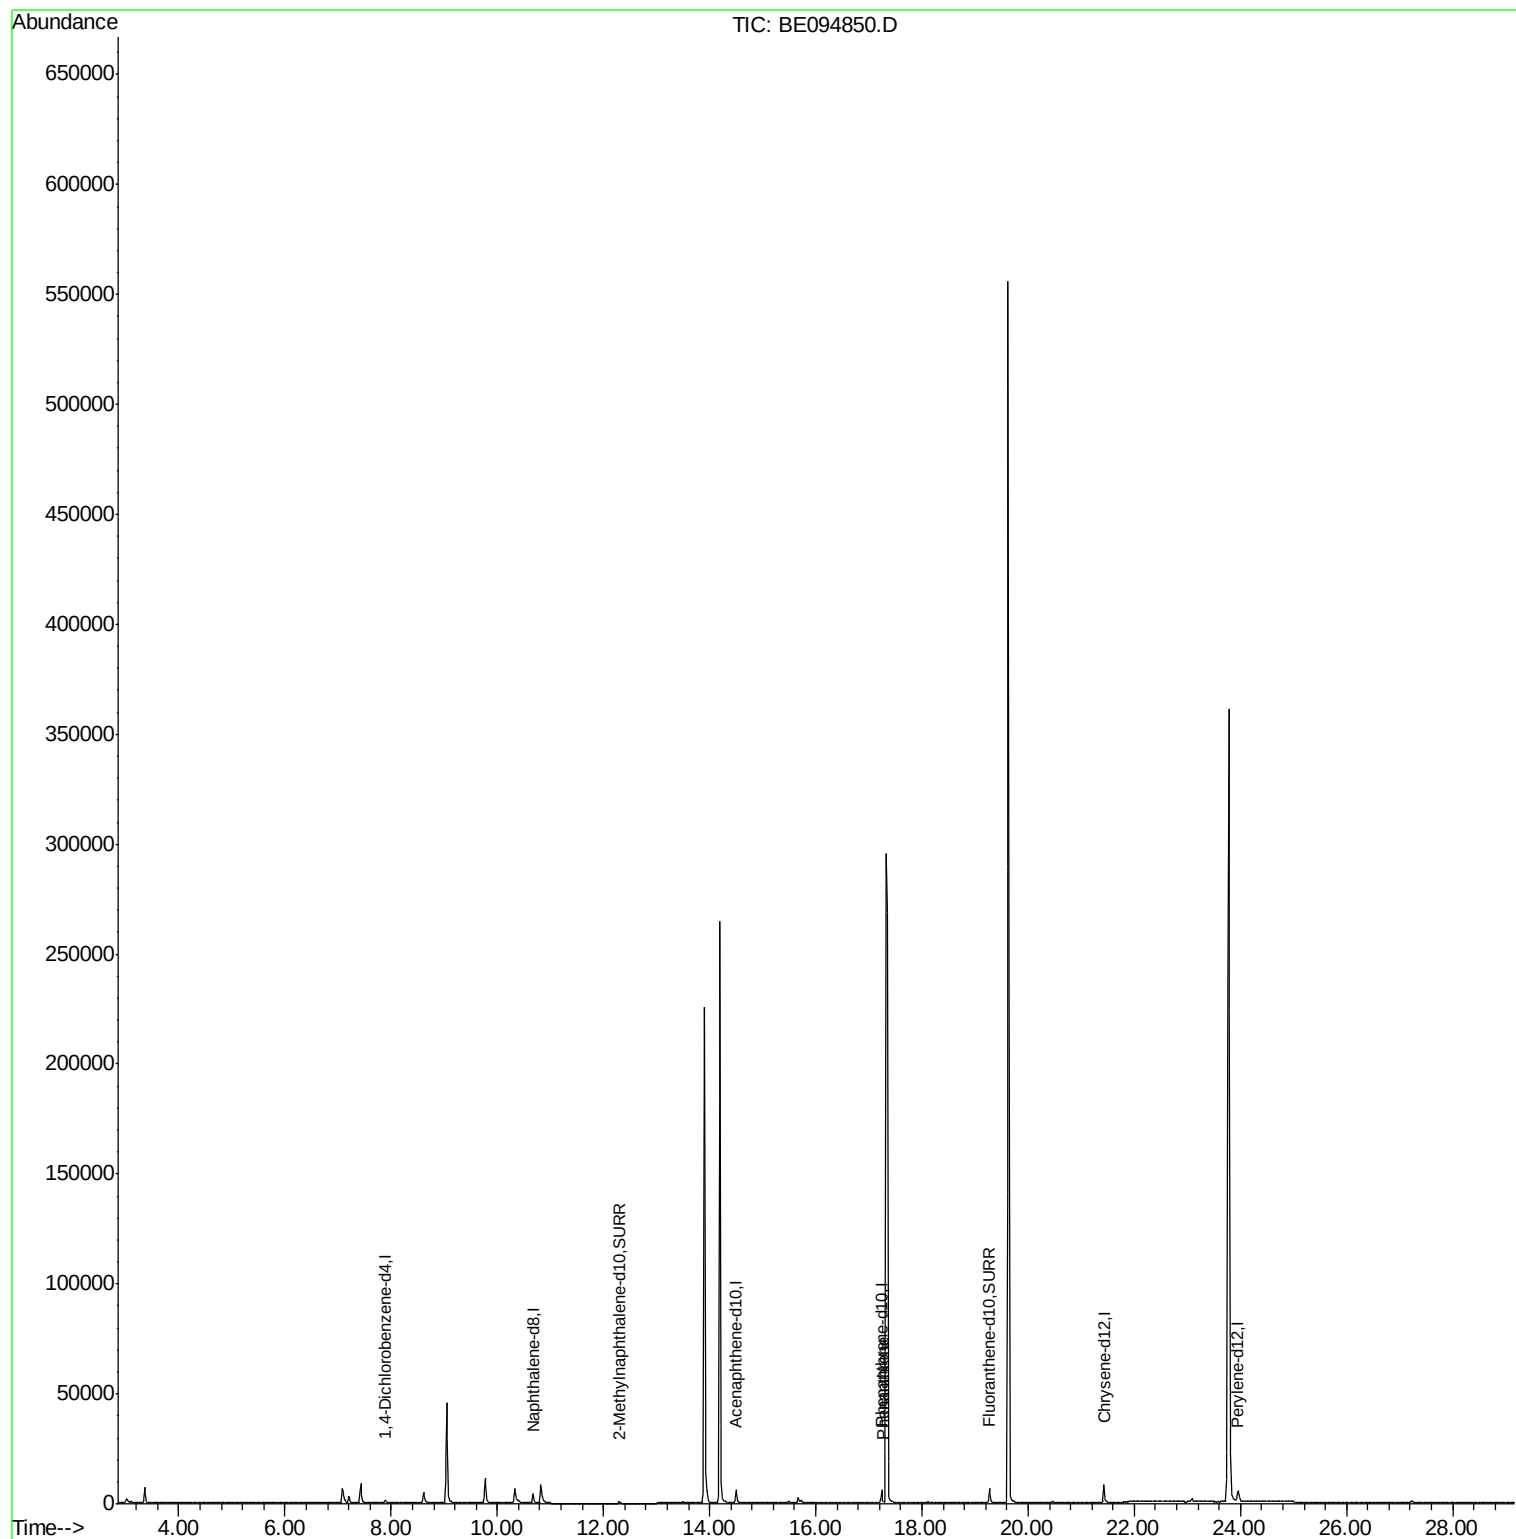

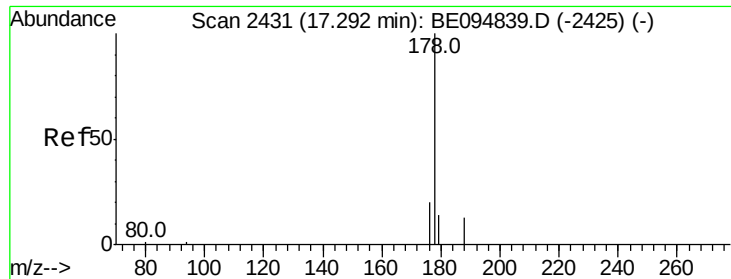

#12

Phenanthrene

Concen: 0.027 ng/ul

RT: 17.27 min Scan# 2430

Delta R.T. -0.02 min

Lab File: BE094850.D

Acq: 23 Nov 2017 2:01

Instrument :

BNA_E

ClientSampleId :

C0AC1


Tot Ion:178 Resp: 580

Ion Ratio Lower Upper

178 100

179 29.6 18.4 27.6#

176 28.9 13.6 20.4#

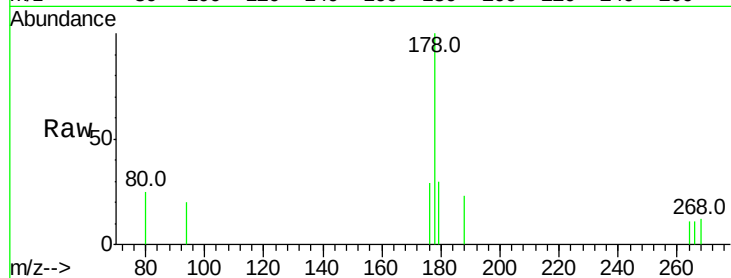

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

