

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE112315\
 Data File : BE091309.D
 Acq On : 23 Nov 2015 20:48
 Operator : UM/NP
 Sample : PB86831BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK31

Quant Time: Nov 24 02:53:26 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 24 02:51:08 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	2460	0.40	ng/ul	-0.03
4) Naphthalene-d8	9.54	136	11703	0.40	ng/ul	-0.02
8) Acenaphthene-d10	13.36	164	6104	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.16	188	1076824	0.40	ng/ul	0.07
18) Chrysene-d12	20.23	240	15217	0.40	ng/ul	0.00
22) Perylene-d12	21.98	264	1343373	0.40	ng/ul	-0.12
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.92	96	19436	10.98	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.07	152	3990	0.25	ng/ul	0.00
16) Fluoranthene-d10	18.07	212	10738	0.00	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Fluorene	14.34	166	1939	0.07	ng/ul#	11
19) Pyrene	18.45	202	9967	0.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE112315\
Data File : BE091309.D
Acq On : 23 Nov 2015 20:48
Operator : UM/NP
Sample : PB86831BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK31

Quant Time: Nov 24 02:53:26 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 02:51:08 2015
Response via : Initial Calibration

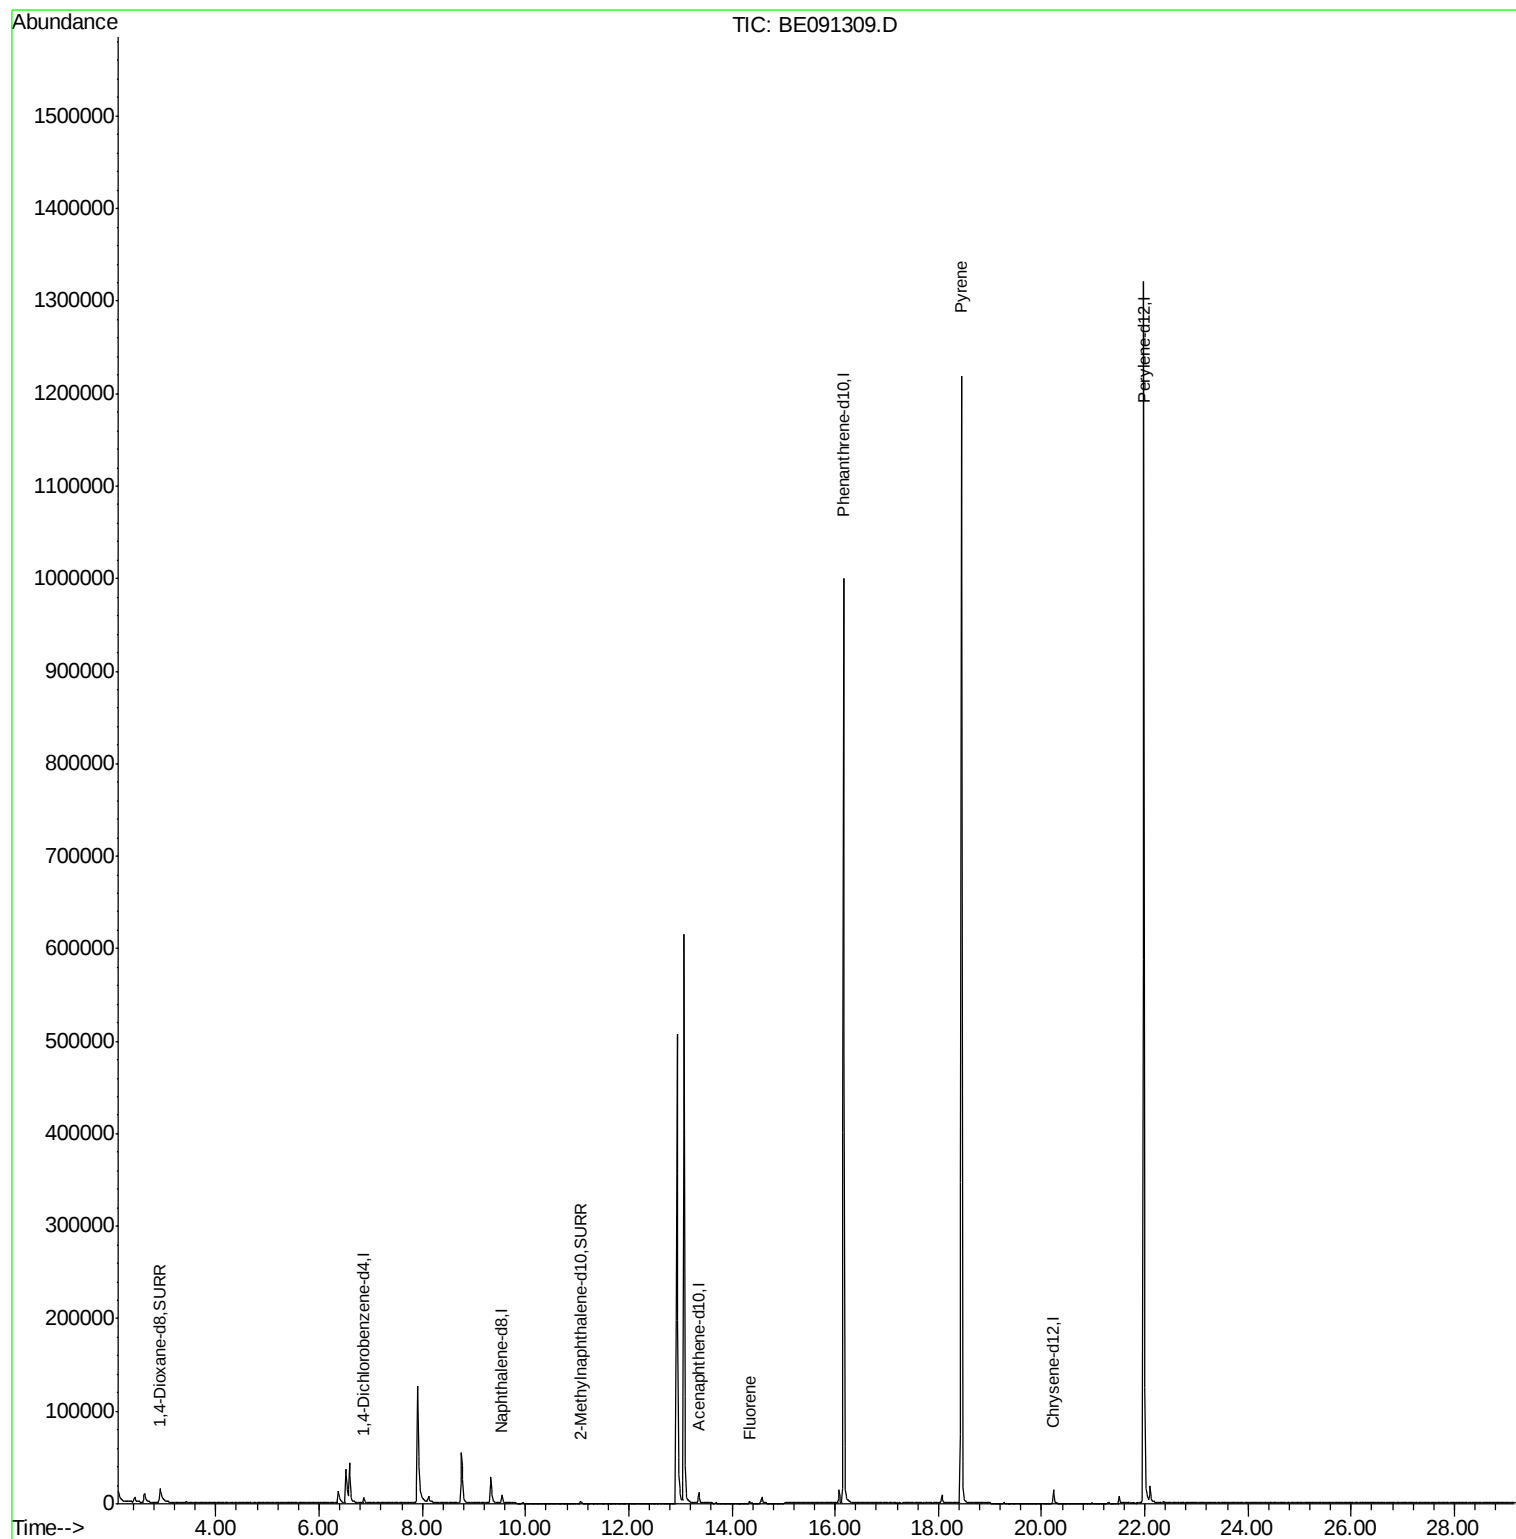

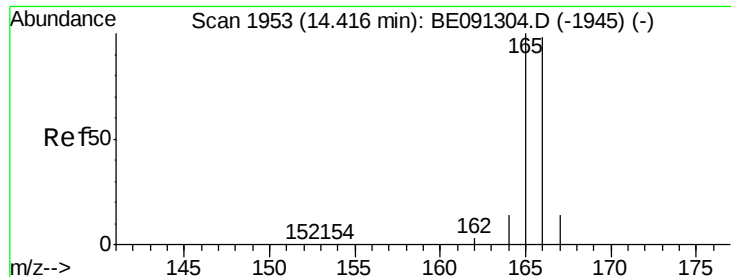

#11

Fluorene

Concen: 0.07 ng/ul

RT: 14.34 min Scan# 1943

Delta R.T. -0.07 min

Lab File: BE091309.D

Acq: 23 Nov 2015 20:48

Instrument :

BNA_E

ClientSampleId :

SBLK31





Tgt Ion:166 Resp: 1939

Ion Ratio Lower Upper

166 100

165 10.1 87.6 131.4#

167 33.9 11.1 16.7#

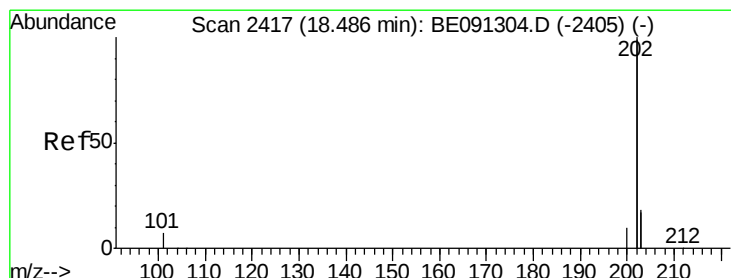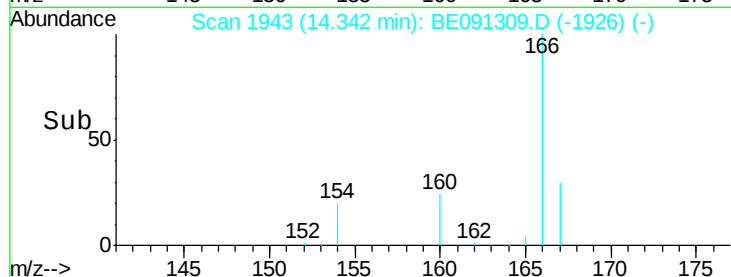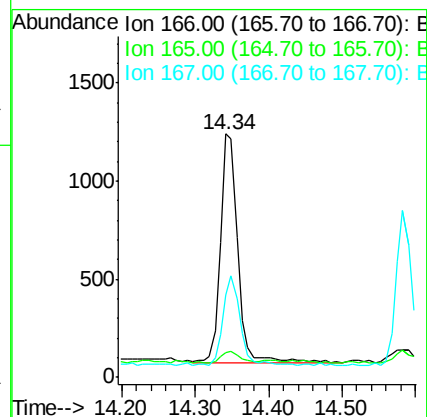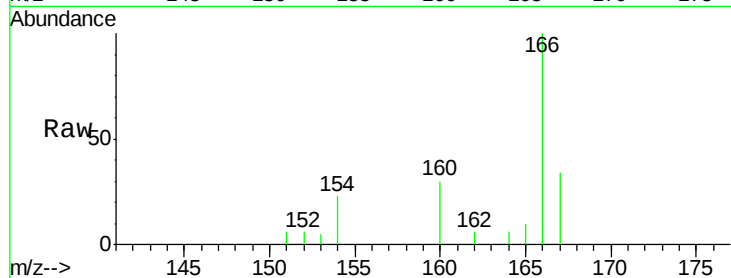

#19

Pyrene

Concen: 0.06 ng/ul

RT: 18.45 min Scan# 2411

Delta R.T. -0.04 min

Lab File: BE091309.D

Acq: 23 Nov 2015 20:48

Tgt Ion:202 Resp: 9967

Ion Ratio Lower Upper

202 100

200 1.9 18.0 27.0#

203 168.0 13.8 20.6#

