


Data Path : Z:\HPCHEM1\BNA_E\Data\BE112717\
 Data File : BE094862.D
 Acq On : 27 Nov 2017 8:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 22:40:47 2017

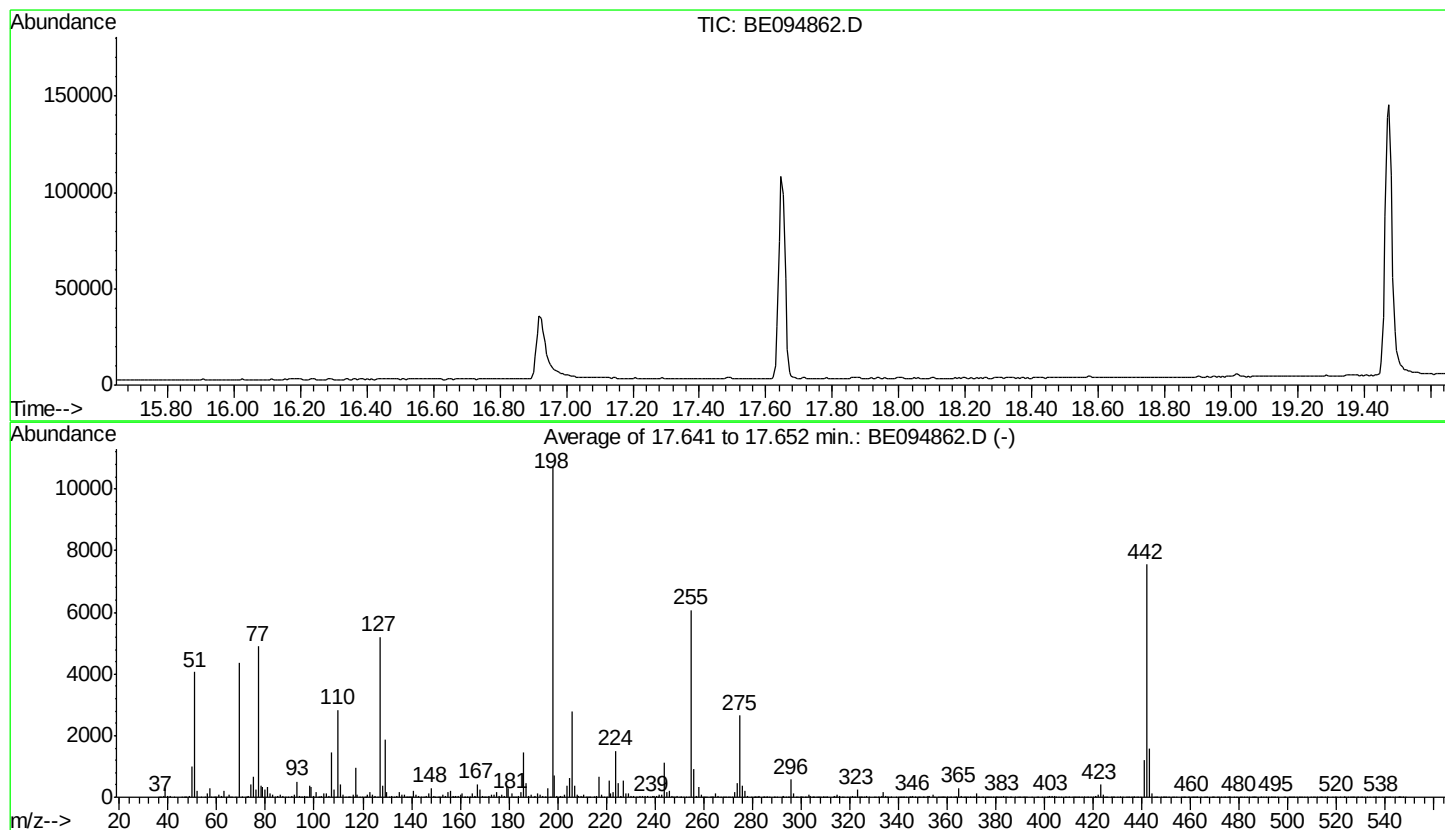

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	4064	PASS
68	69	0.00	2	0.1	4	PASS
69	198	0.00	100	40.4	4349	PASS
70	69	0.00	2	0.4	19	PASS
127	198	10	80	48.4	5210	PASS
197	198	0.00	2	0.2	20	PASS
198	198	100	100	100.0	10764	PASS
199	198	5	9	6.6	714	PASS
275	198	10	60	24.7	2655	PASS
365	198	1	100	2.7	293	PASS
441	442	0.01	24	15.8	1190	PASS
442	198	50	100	70.1	7546	PASS
443	442	15	24	20.9	1576	PASS