

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112817\
 Data File : BE094879.D
 Acq On : 28 Nov 2017 12:15
 Operator : SJ/JU
 Sample : I6496-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0B95

Quant Time: Nov 29 01:13:09 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 29 01:10:42 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	528	0.40	ng/ul	-0.05
2) Naphthalene-d8	10.68	136	3586	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.50	164	2669	0.40	ng/ul	-0.02
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.44	240	6215	0.40	ng/ul	0.01
20) Perylene-d12	23.96	264	7984	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.31	152	1976	0.34	ng/ul	0.01
14) Fluoranthene-d10	19.27	212	6244	0.00	ng/ul	-0.01
Target Compounds						
9) Fluorene	15.49	166	596	0.06	ng/ul#	24
17) Pyrene	19.63	202	772	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112817\
Data File : BE094879.D
Acq On : 28 Nov 2017 12:15
Operator : SJ/JU
Sample : I6496-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0B95

Quant Time: Nov 29 01:13:09 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 29 01:10:42 2017
Response via : Initial Calibration

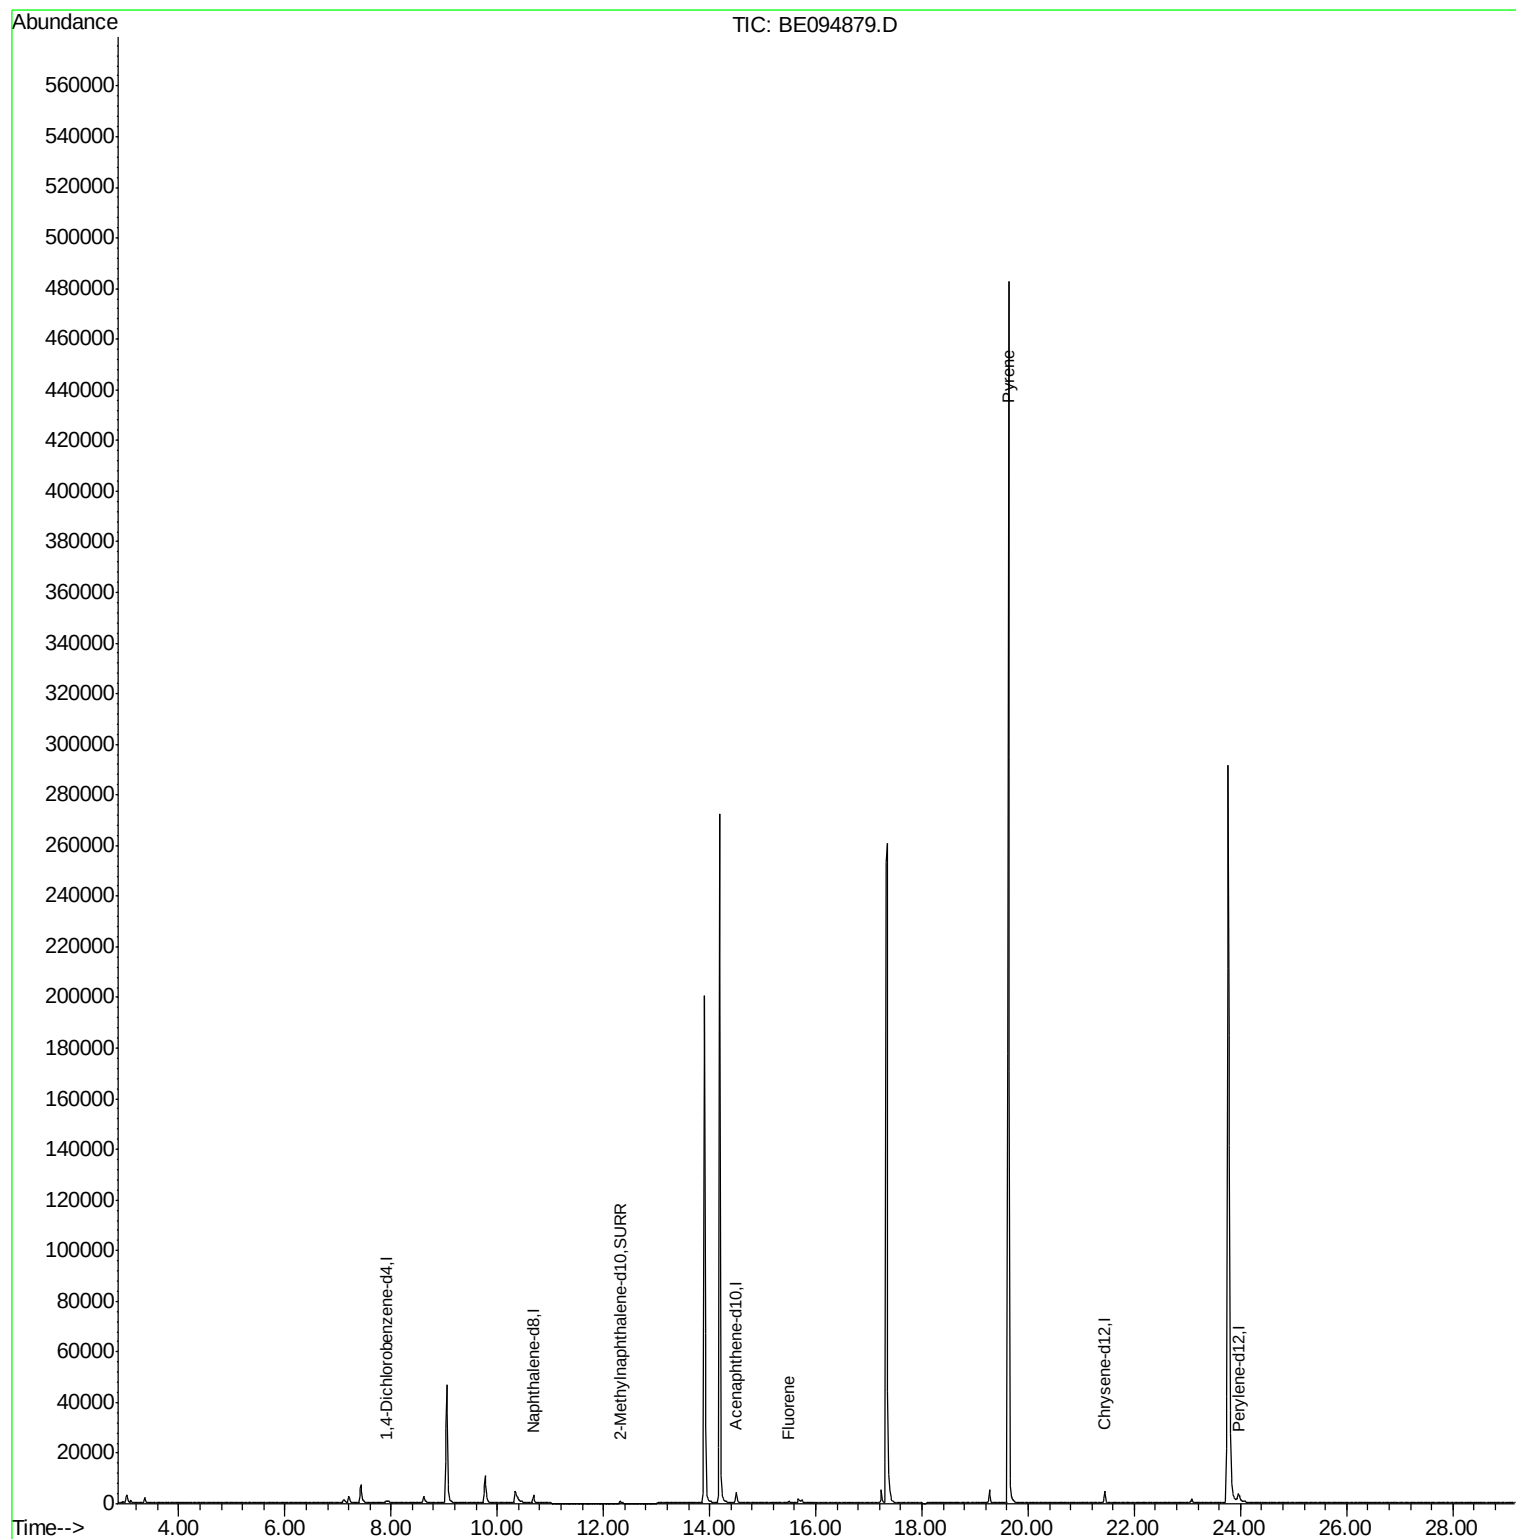

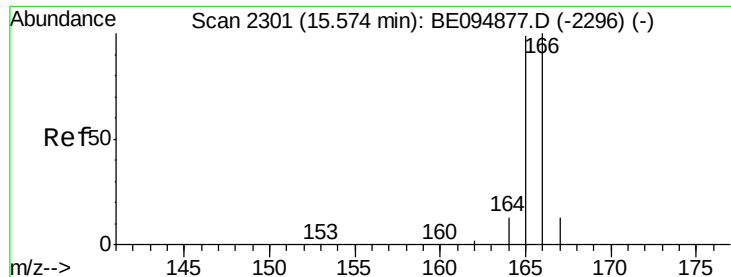

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.49 min Scan# 2290

Delta R.T. -0.08 min

Lab File: BE094879.D

Acq: 28 Nov 2017 12:15

Instrument :

BNA_E

ClientSampleId :

C0B95


Tot Ion:166 Resp: 596

Ion Ratio Lower Upper

166 100

165 14.5 73.4 110.2#


167 41.1 14.6 22.0#

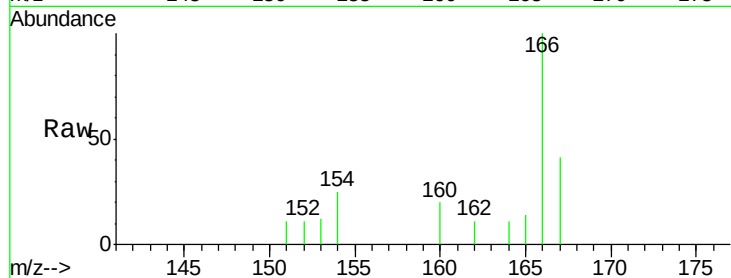



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

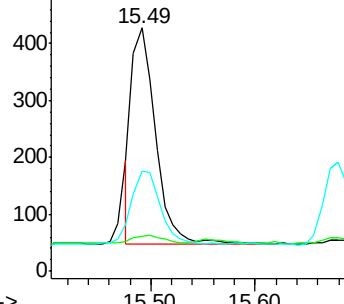

Time-->

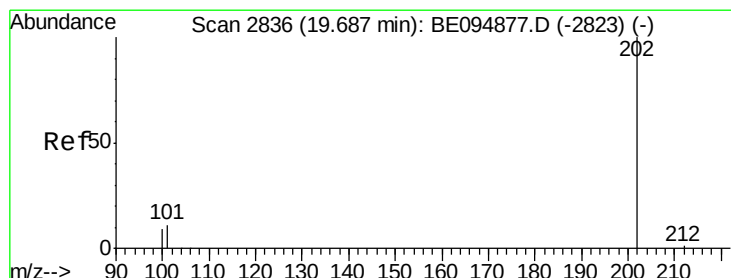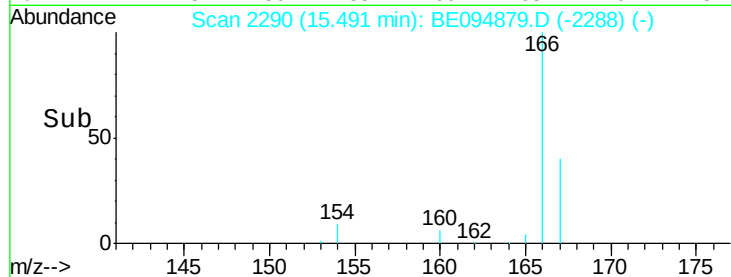

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.63 min Scan# 2823

Delta R.T. -0.06 min

Lab File: BE094879.D

Acq: 28 Nov 2017 12:15


Tgt Ion:202 Resp: 772

Ion Ratio Lower Upper

202 100

101 141.1 18.2 27.4#


100 761.8 15.6 23.4#

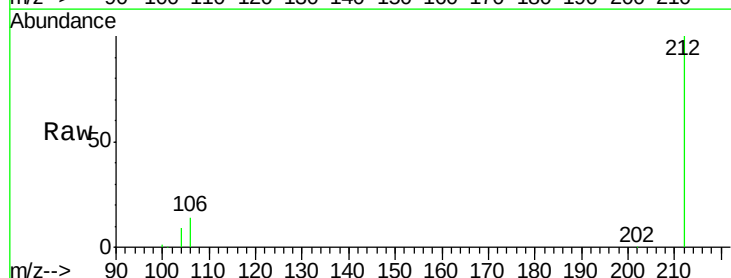

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

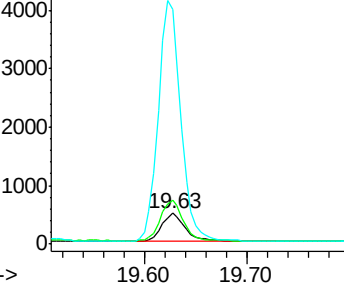

Time-->

