

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112817\
 Data File : BE094879.D
 Acq On : 28 Nov 2017 12:15
 Operator : SJ/JU
 Sample : I6496-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0B95

Manual Integrations
 APPROVED

Sohil
 11/29/2017 5:14:55 PM

Quant Time: Nov 29 01:21:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 29 01:10:42 2017
 Response via : Initial Calibration

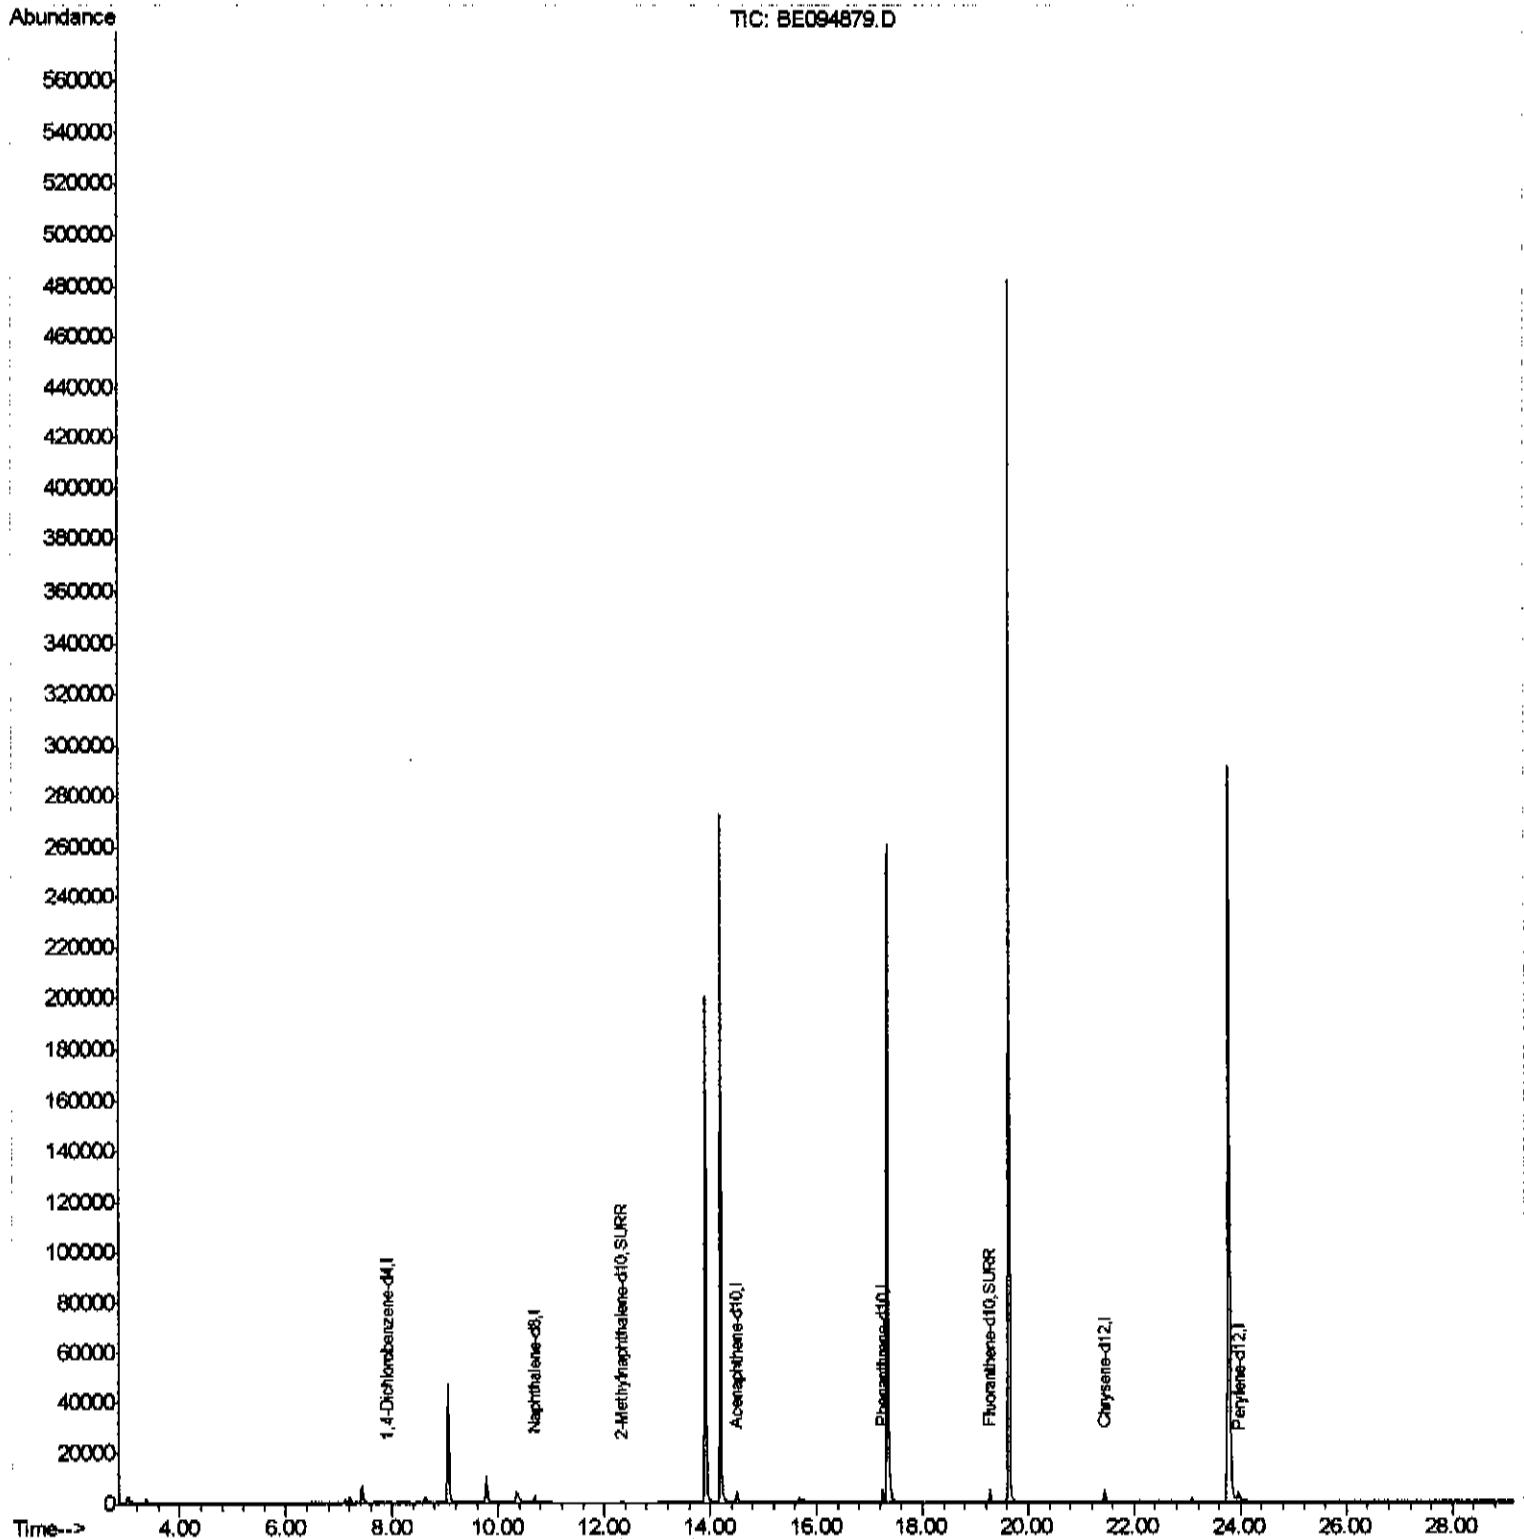

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112817\
 Data File : BE094879.D
 Acq On : 28 Nov 2017 12:15
 Operator : SJ/JU
 Sample : I6496-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0B95

Manual Integrations
 APPROVED

Sohil
 11/29/2017 5:14:55 PM

Quant Time: Nov 29 01:13:09 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 29 01:10:42 2017
 Response via : Initial Calibration

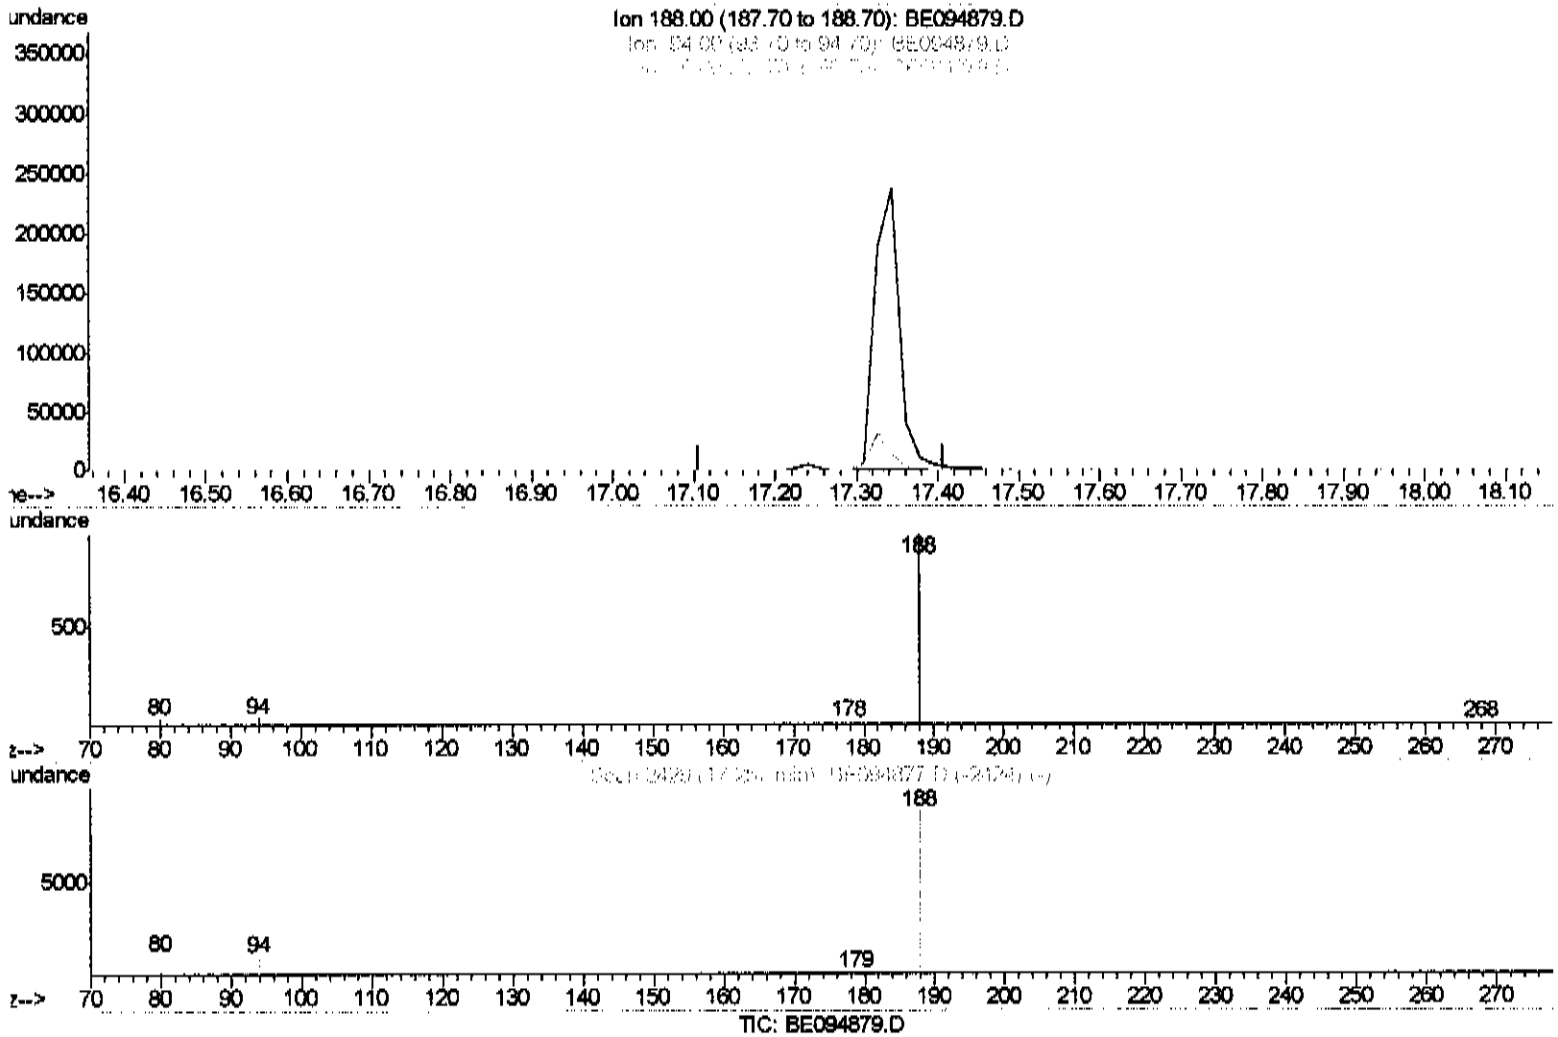

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112817\
 Data File : BE094879.D
 Acq On : 28 Nov 2017 12:15
 Operator : SJ/JU
 Sample : I6496-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0B95

Manual Integrations
 APPROVED

Sohil
 11/29/2017 5:14:55 PM

Quant Time: Nov 29 01:13:09 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 29 01:10:42 2017
 Response via : Initial Calibration

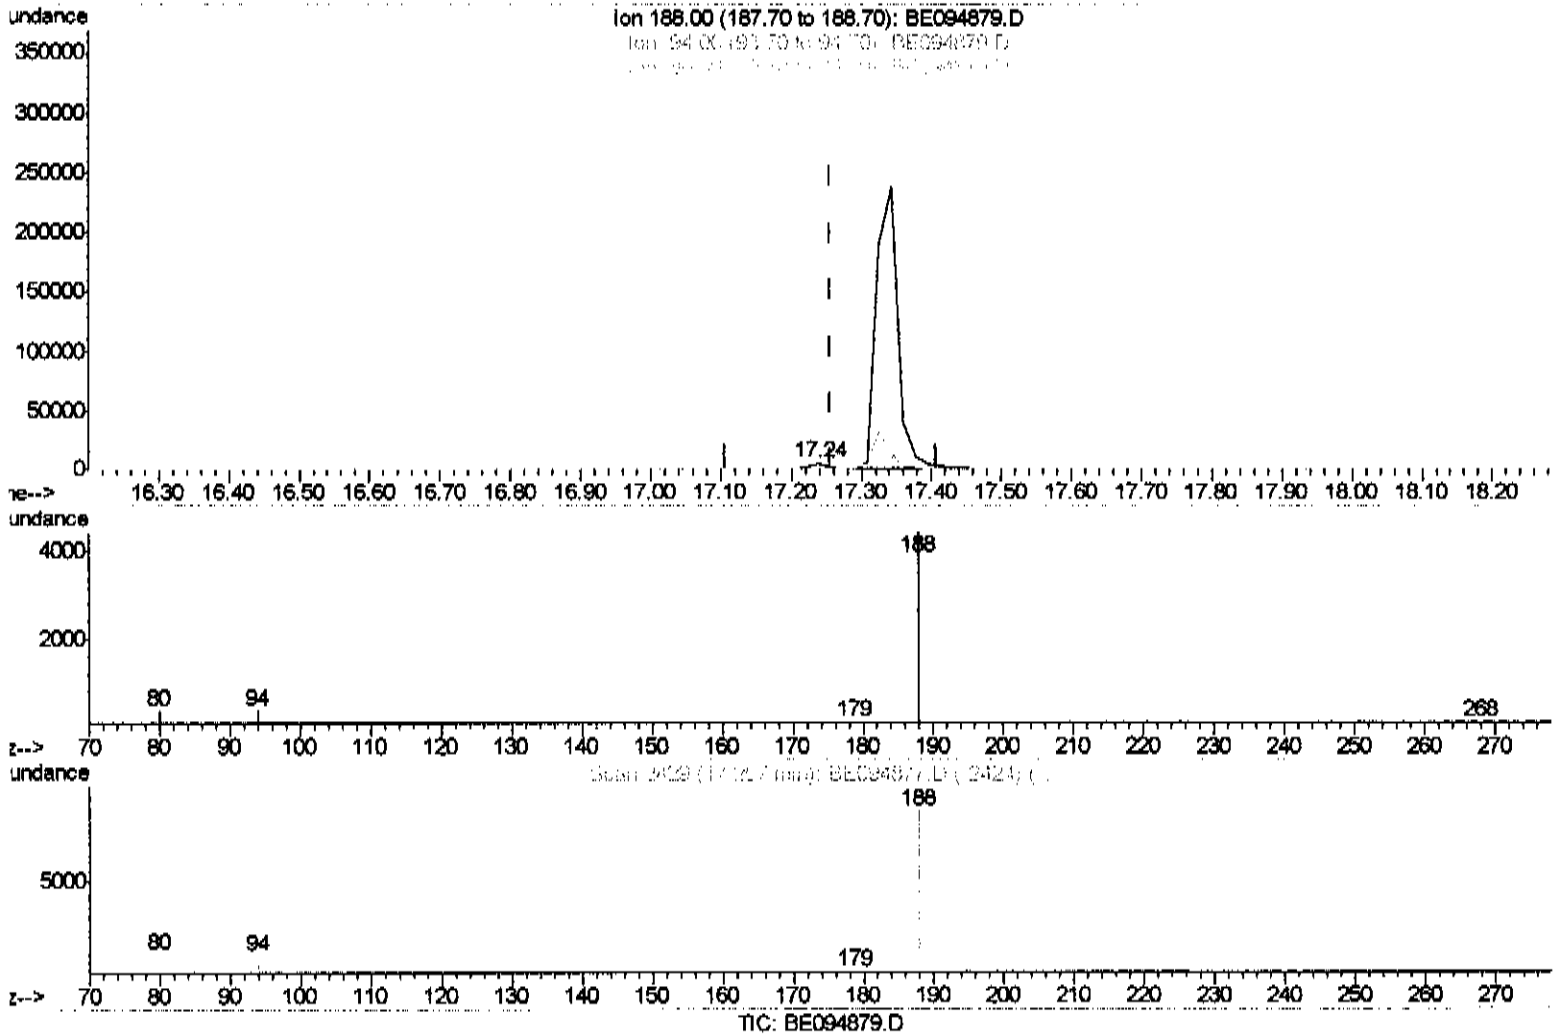

(10) Phenanthrene-d10 (I)

17.239min (-0.018) 0.40ng/ul m *SJ 11/29/17*

response 6318

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.55#
80.00	11.80	7.49#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112817\
 Data File : BE094879.D
 Acq On : 28 Nov 2017 12:15
 Operator : SJ/JU
 Sample : I6496-12
 Disc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 C0B95

Manual Integrations
 APPROVED

Sohil
 11/29/2017 5:14:55 PM

Quant Time: Nov 29 01:21:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 29 01:10:42 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	528	0.40	ng/ul	-0.05
2) Naphthalene-d8	10.68	136	3586	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.50	164	2669	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.24	188	6318m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.44	240	6215	0.40	ng/ul	0.01
20) Perylene-d12	23.96	264	7984	0.40	ng/ul	0.00

50 ng/29/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.31	152	1976	0.34	ng/ul	0.01
14) Fluoranthene-d10	19.27	212	6244	0.29	ng/ul	-0.01

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed