


Data Path : Z:\HPCHEM1\BNA E\DATA\BE113017\
 Data File : BE094887.D
 Acq On : 30 Nov 2017 12:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 01 13:33:28 2017

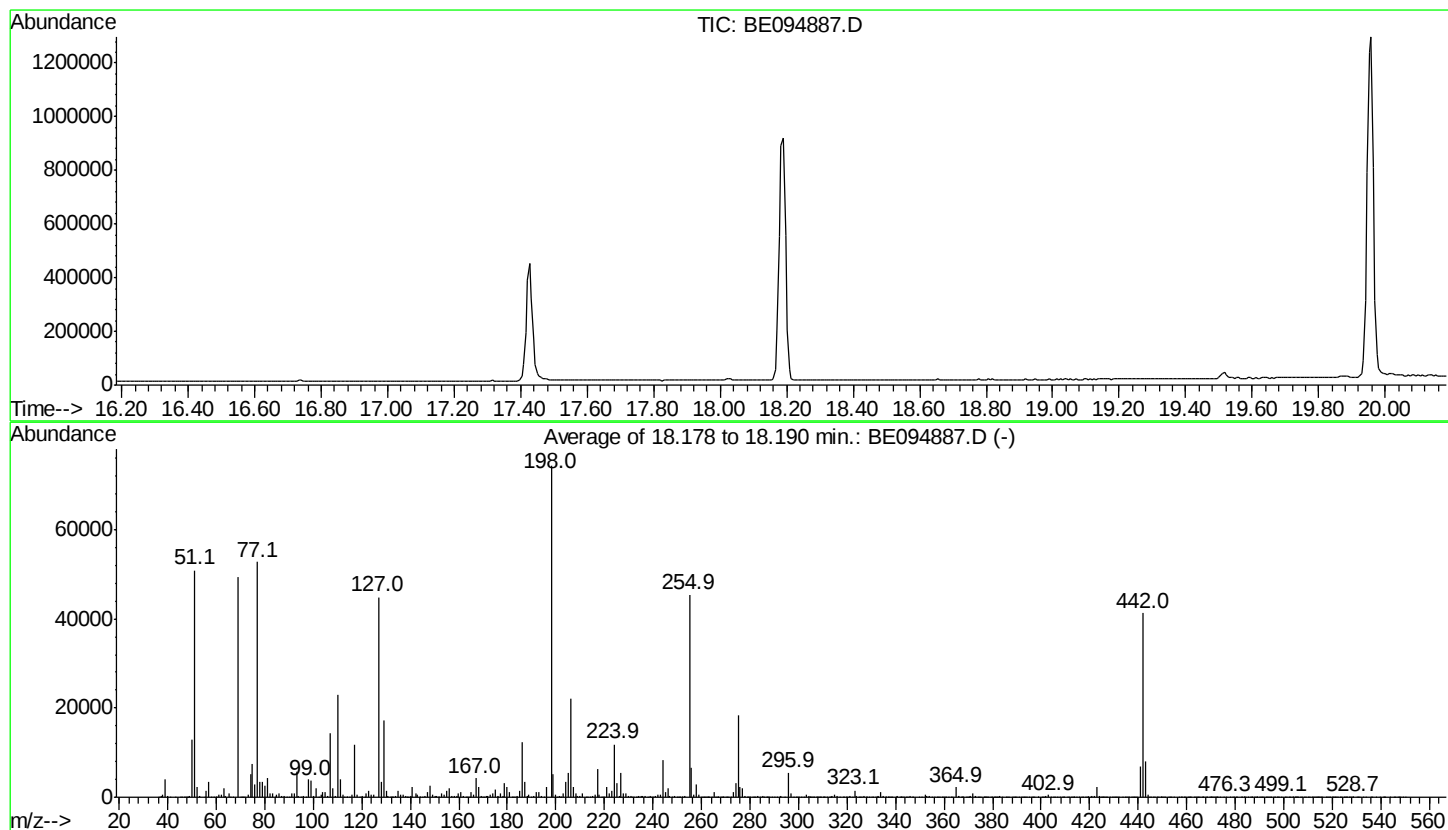

AutoFind: Scans 2653, 2654, 2655; Background Corrected with Scan 2643

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.4	50871	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	66.5	49427	PASS
70	69	0.00	2	0.3	138	PASS
127	198	10	80	60.4	44886	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74336	PASS
199	198	5	9	7.0	5227	PASS
275	198	10	60	24.8	18465	PASS
365	198	1	100	3.0	2193	PASS
441	442	0.01	24	16.8	6928	PASS
442	198	50	100	55.5	41239	PASS
443	442	15	24	19.6	8093	PASS