
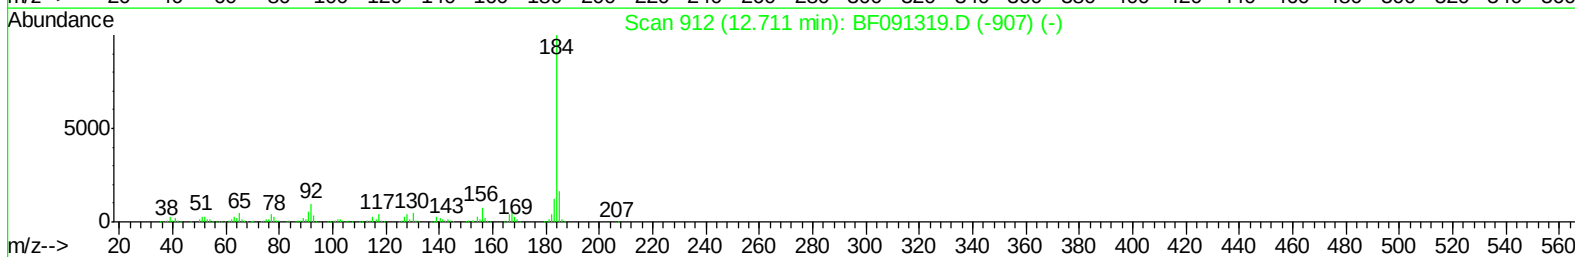
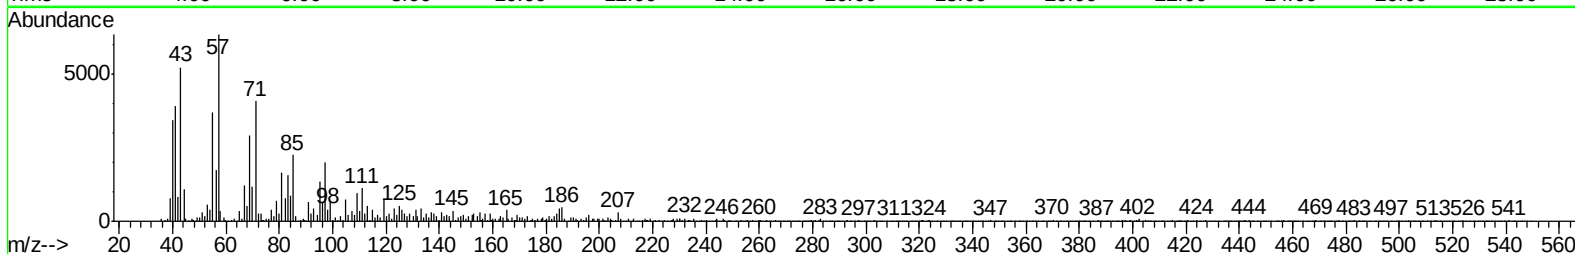


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120116\
Data File : BE092579.D
Acq On : 1 Dec 2016 8:56
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 02:16:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

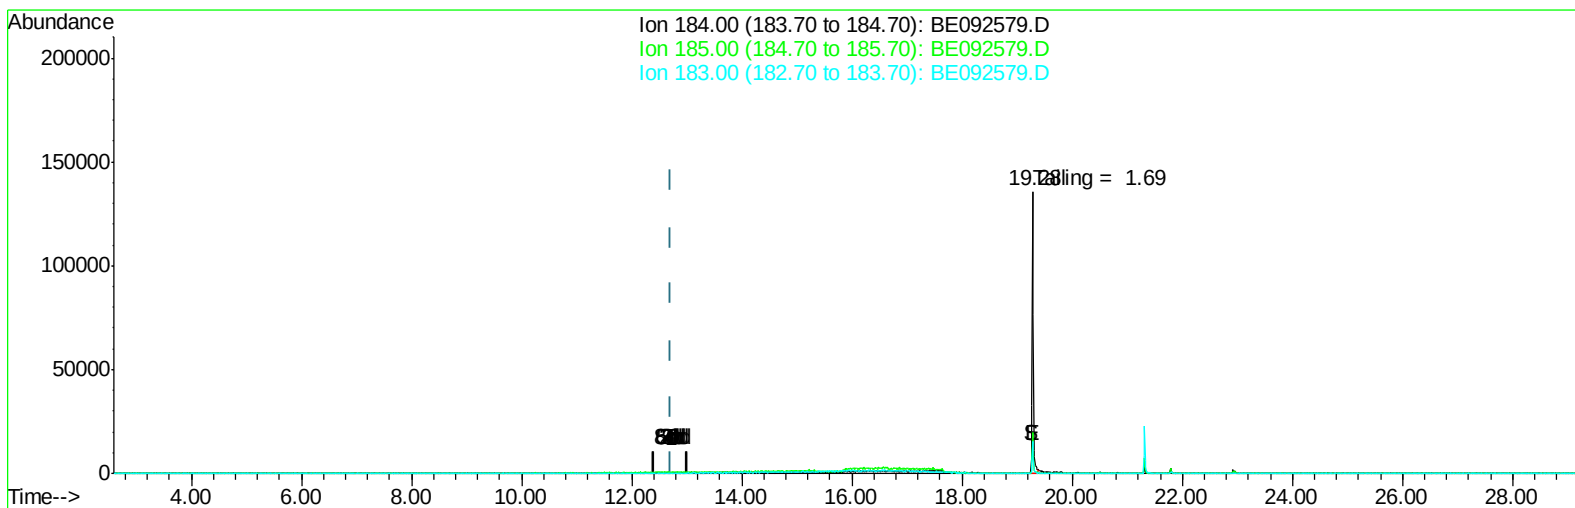

TIC: BE092579.D

(76) Benzidine




12.740min (+0.013) 47.47ng

response 85

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	172.61#
183.00	11.10	66.39#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120116\
Data File : BE092579.D
Acq On : 1 Dec 2016 8:56
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 02:16:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

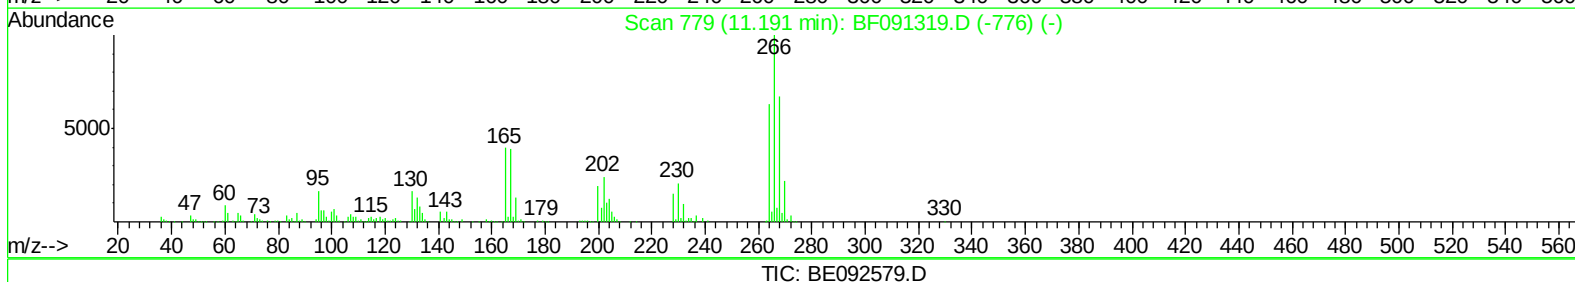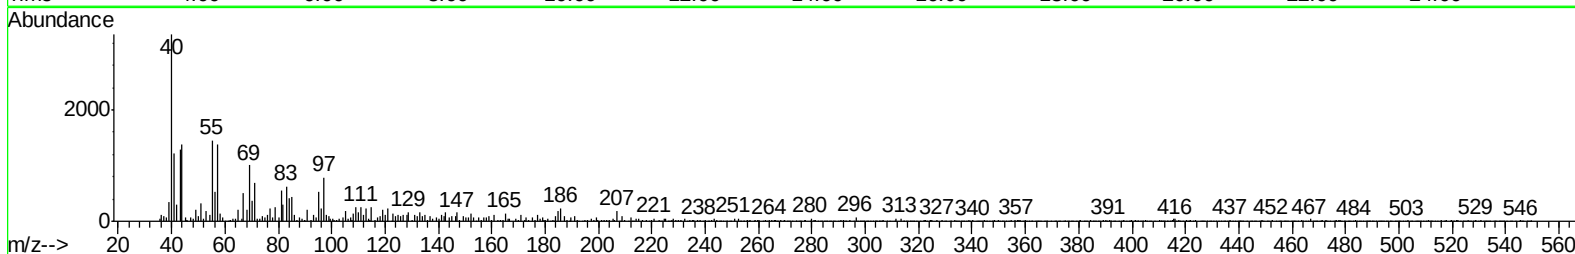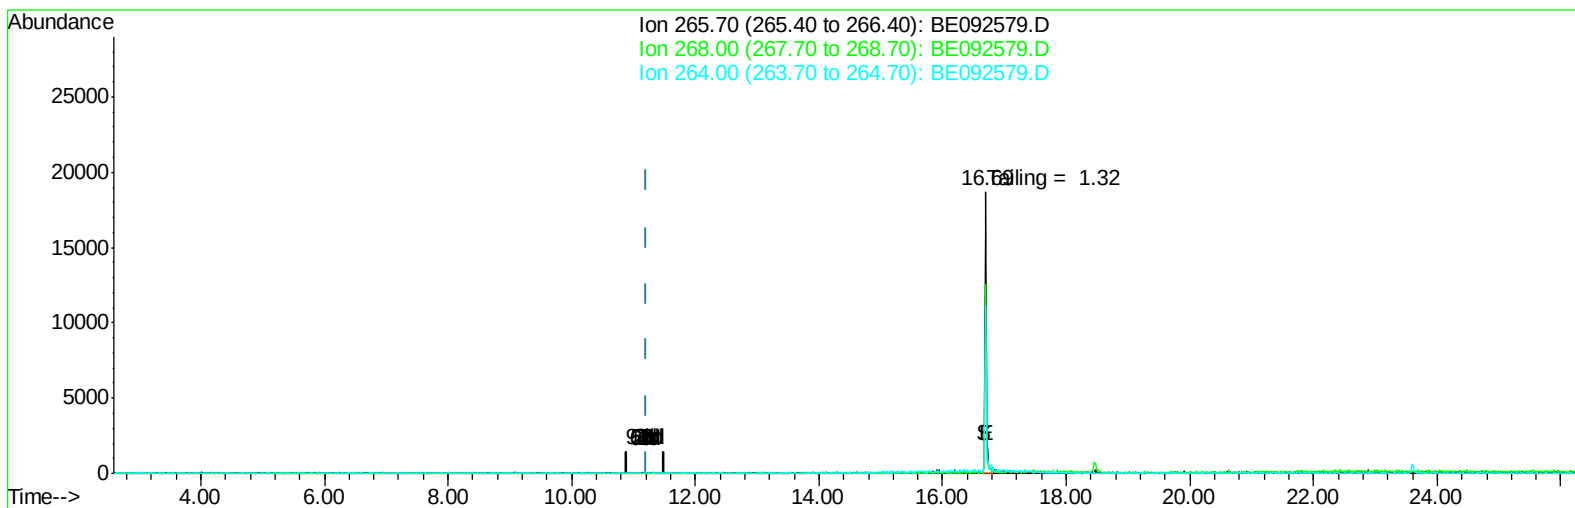

TIC: BE092579.D

(69) Pentachlorophenol (C)

11.171min (-0.036) 23.09ng

response 21

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	61.76
264.00	60.20	70.59
0.00	0.00	0.00