
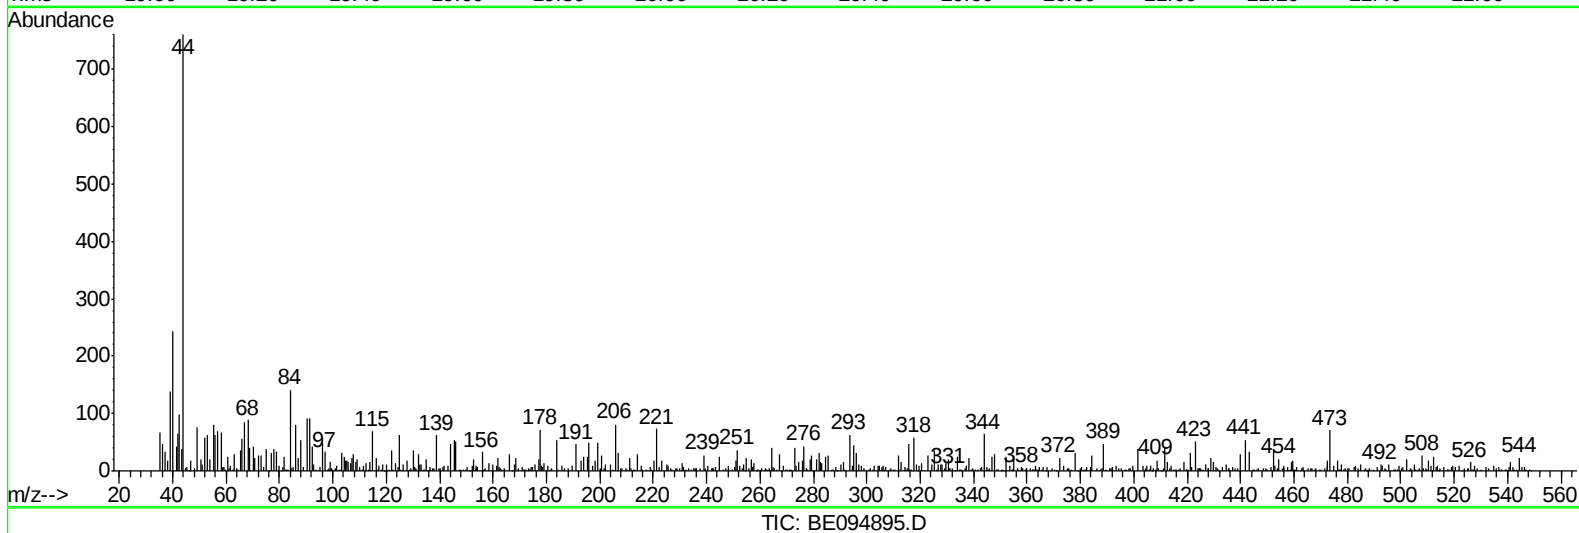


Data Path : Z:\HPCHEM1\BNA E\DATA\BE120117\
Data File : BE094895.D
Acq On : 1 Dec 2017 8:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 01:13:27 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 15:52:19 2017
Response via : Initial Calibration

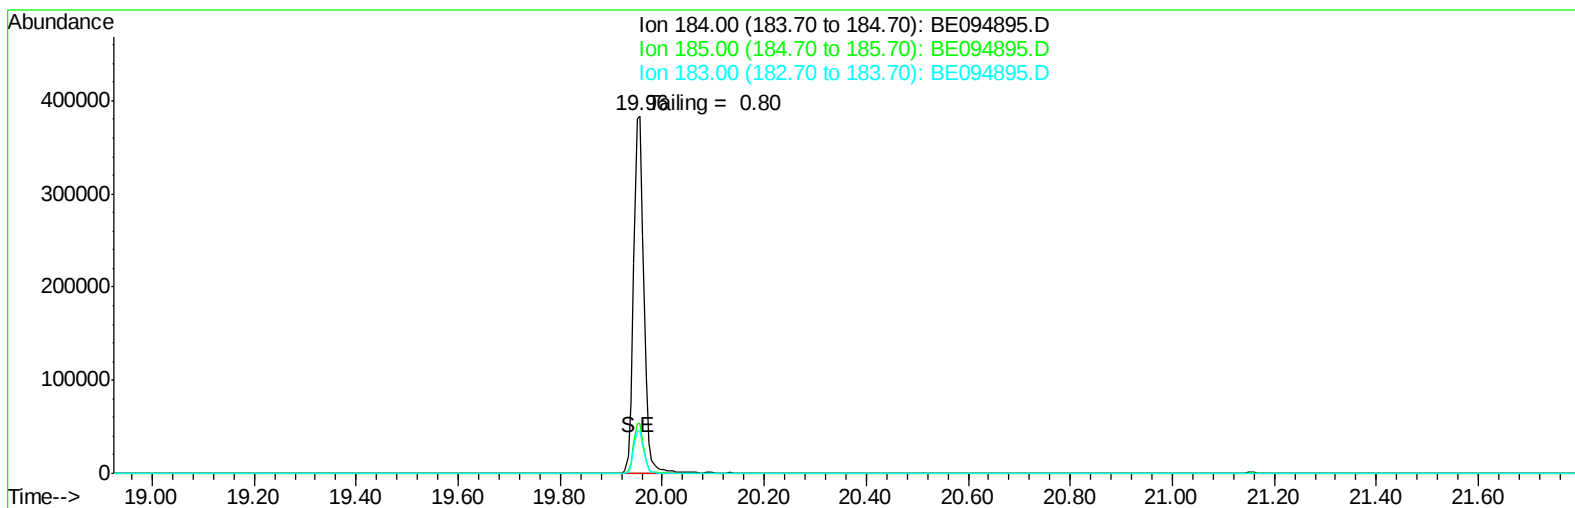

TIC: BE094895.D

(76) Benzidine



12.759min (+0.049) 45.80ng

response 70

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.86
183.00	11.60	96.43#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE120117\
Data File : BE094895.D
Acq On : 1 Dec 2017 8:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 01:13:27 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 15:52:19 2017
Response via : Initial Calibration

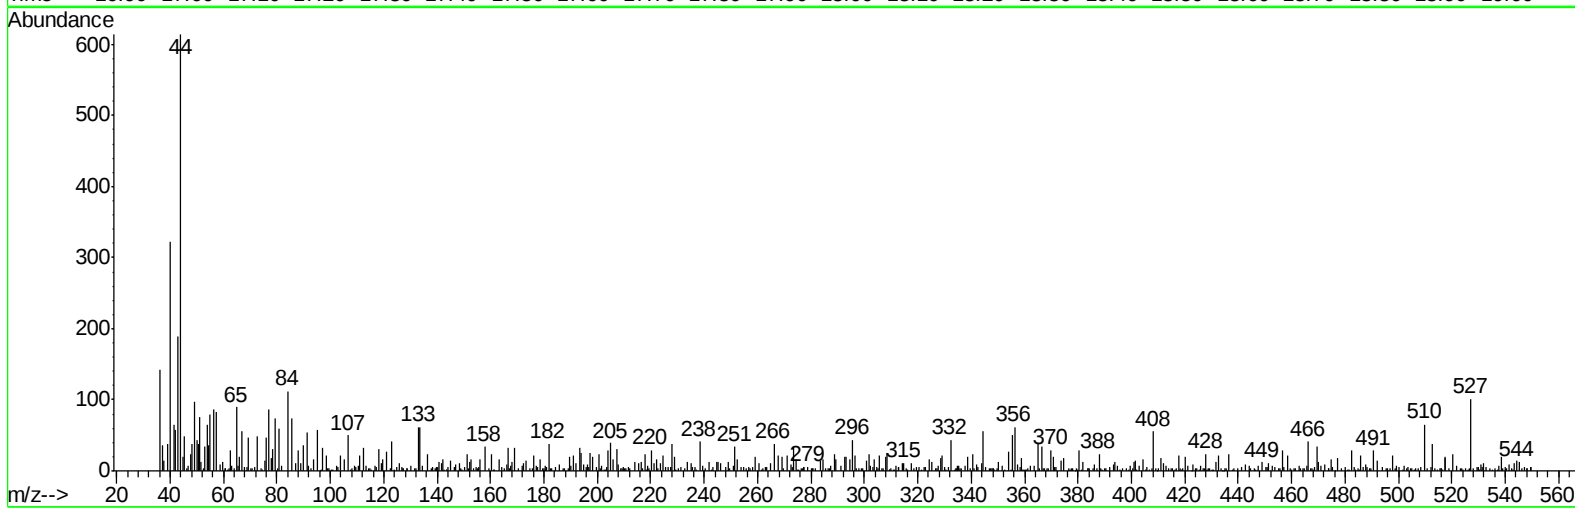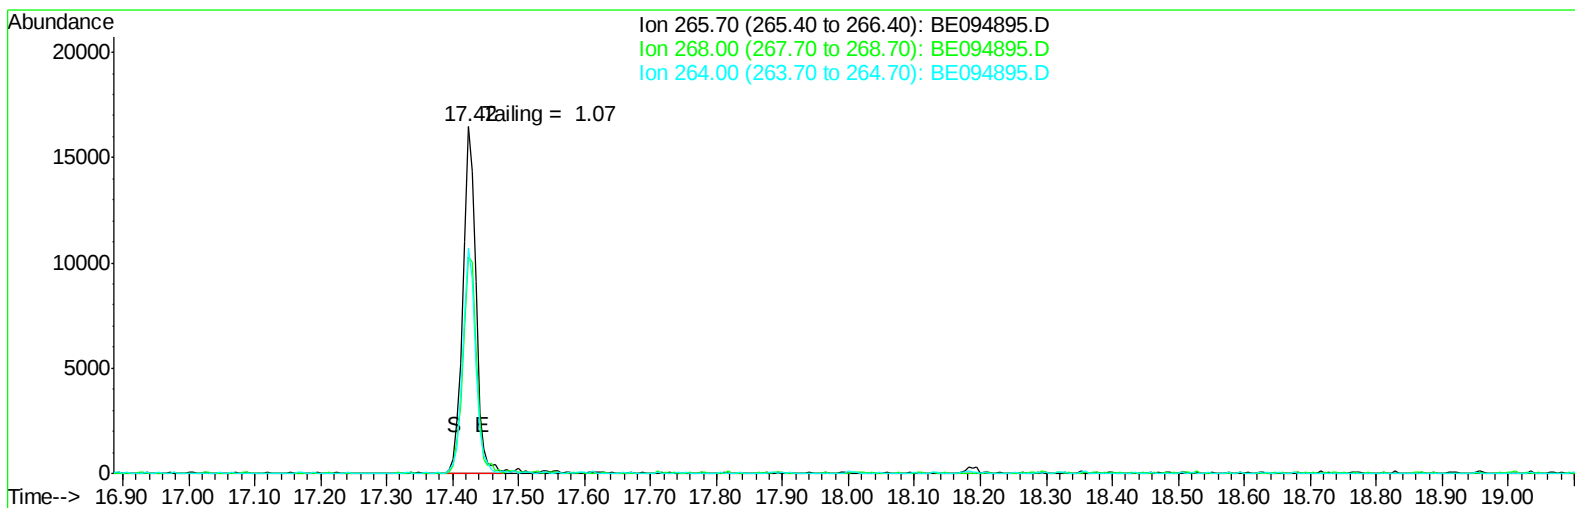

TIC: BE094895.D

(69) Pentachlorophenol (C)

11.167min (-0.014) 87.59ng

response 26

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.89
264.00	61.90	0.00#
0.00	0.00	0.00