
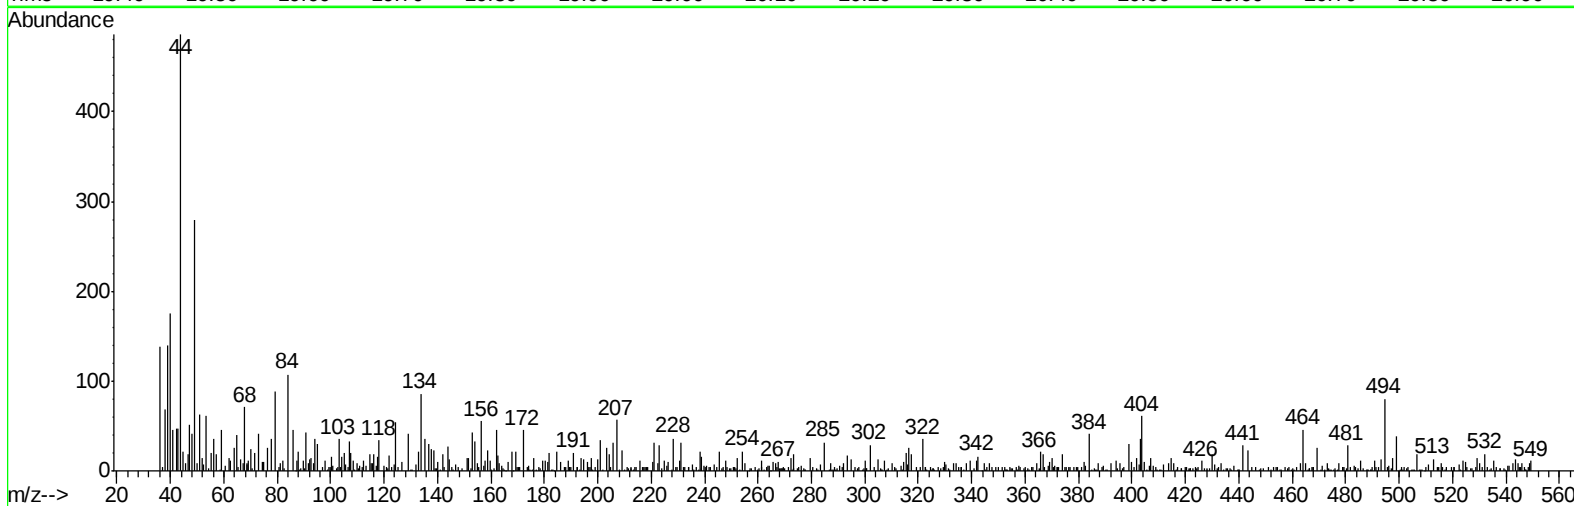


Data Path : Z:\HPCHEM1\BNA E\DATA\BE120117\
Data File : BE094905.D
Acq On : 1 Dec 2017 15:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 01:15:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 15:52:19 2017
Response via : Initial Calibration

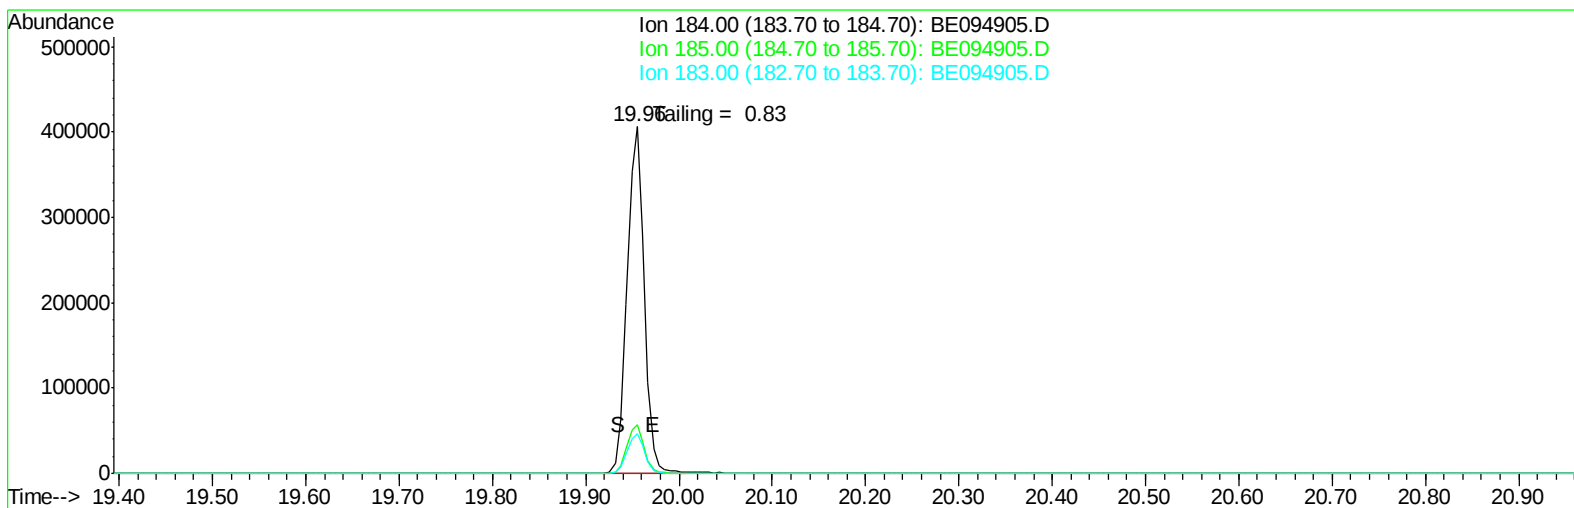

TIC: BE094905.D

(76) Benzidine



12.699min (-0.010) 103.79ng

response 27

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	13.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE120117\
Data File : BE094905.D
Acq On : 1 Dec 2017 15:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 01:15:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 15:52:19 2017
Response via : Initial Calibration

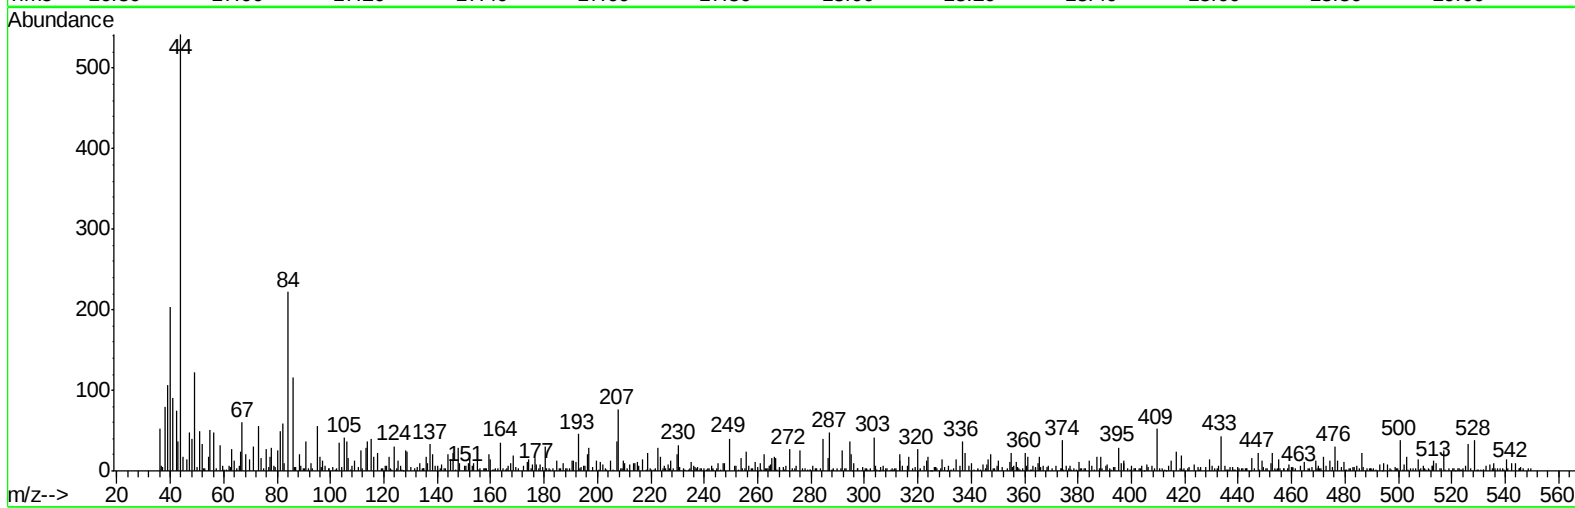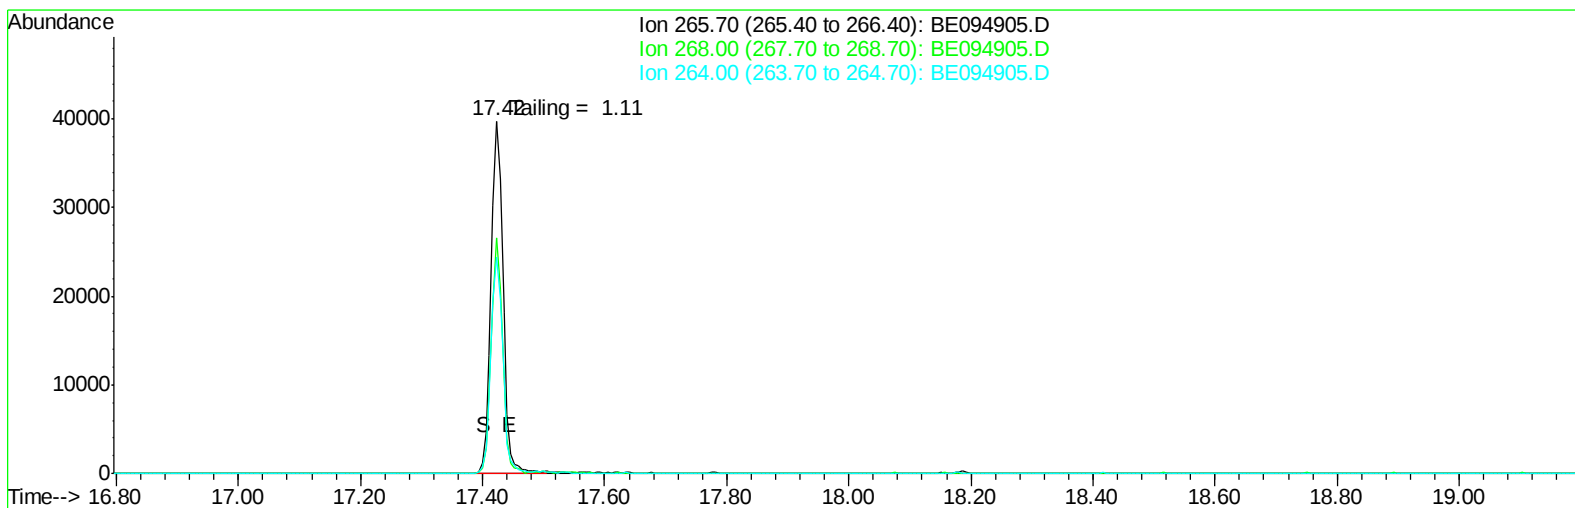

TIC: BE094905.D

(69) Pentachlorophenol (C)

11.160min (-0.020) 110.26ng

response 24

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	24.24#
264.00	61.90	30.30#
0.00	0.00	0.00