


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE120117\
 Data File : BE094895.D
 Acq On : 1 Dec 2017 8:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 01 13:33:28 2017

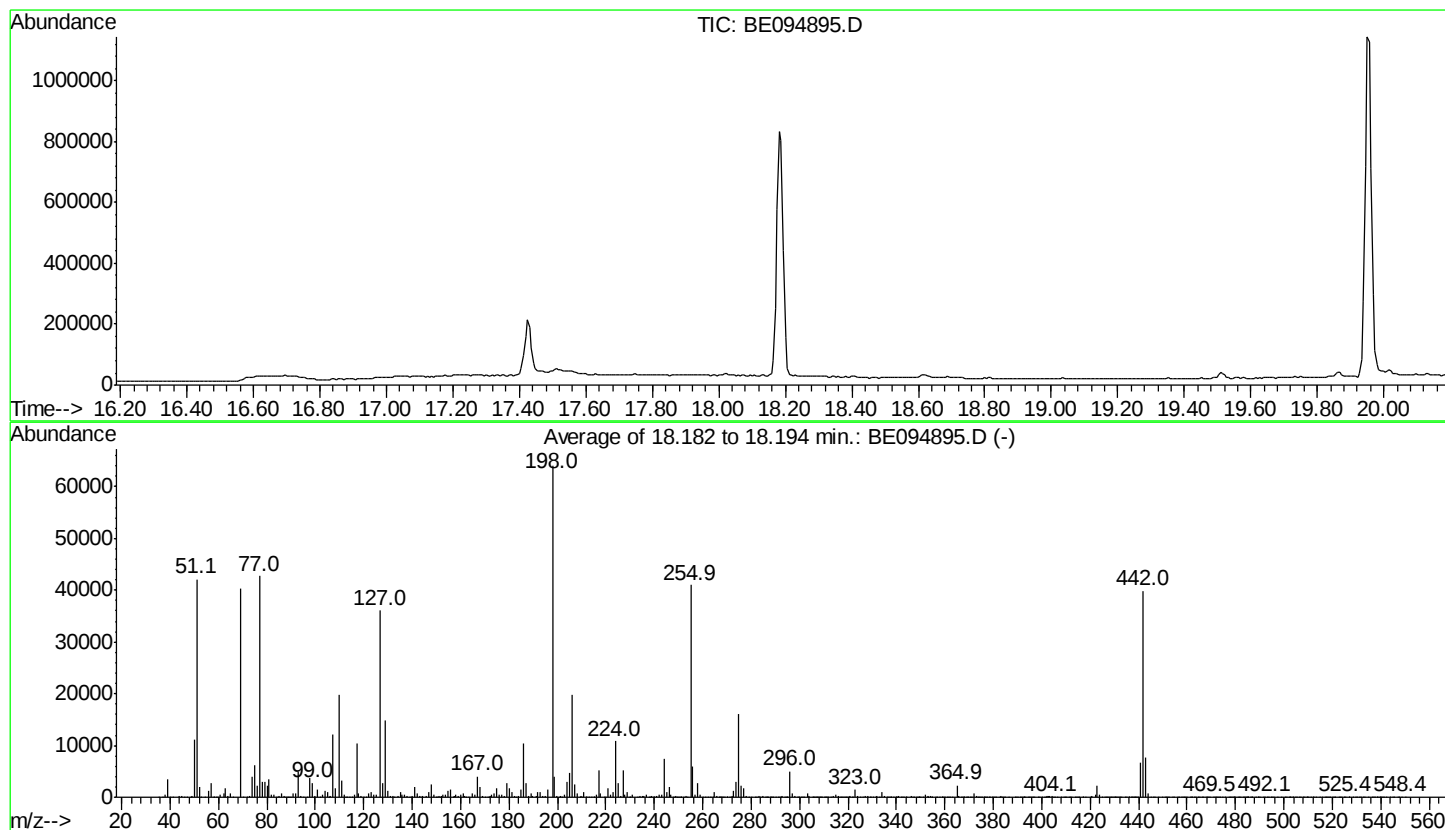

AutoFind: Scans 2654, 2655, 2656; Background Corrected with Scan 2642

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.7	42087	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	62.9	40327	PASS
70	69	0.00	2	0.1	49	PASS
127	198	10	80	56.3	36041	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64072	PASS
199	198	5	9	6.3	4011	PASS
275	198	10	60	25.2	16156	PASS
365	198	1	100	3.5	2237	PASS
441	442	0.01	24	16.7	6675	PASS
442	198	50	100	62.3	39893	PASS
443	442	15	24	19.0	7573	PASS