
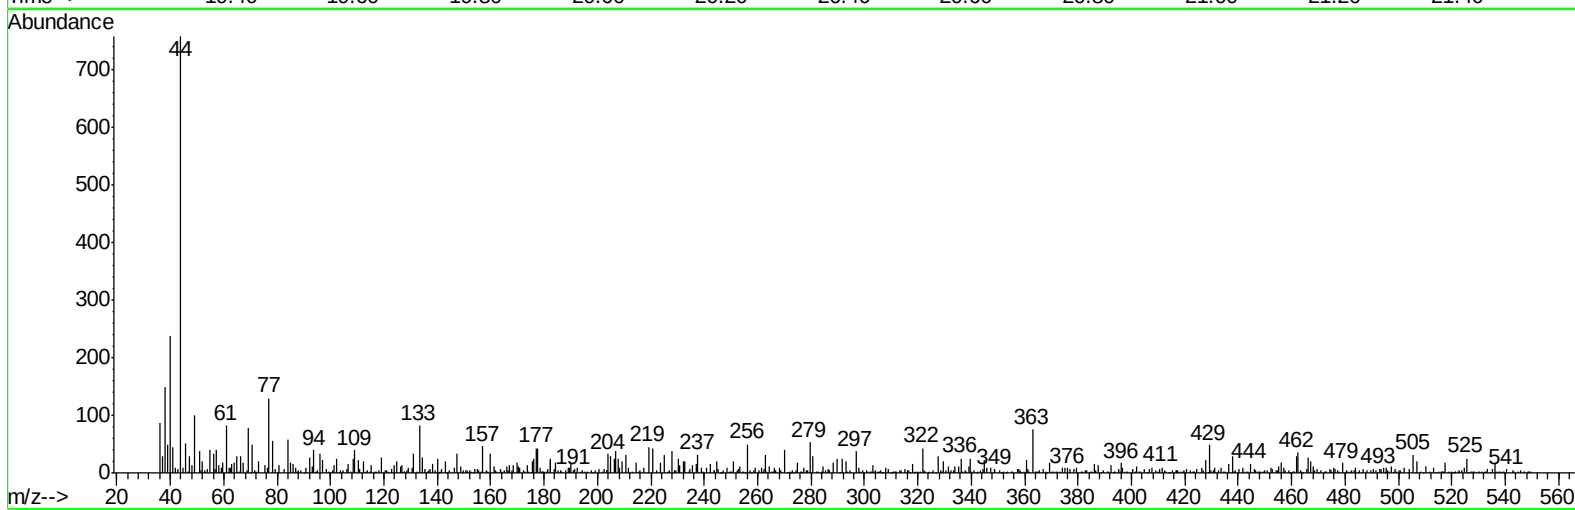


Data Path : Z:\HPCHEM1\BNA E\DATA\BE120517\
 Data File : BE094914.D
 Acq On : 5 Dec 2017 14:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 08:22:41 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 04 13:07:49 2017
 Response via : Initial Calibration

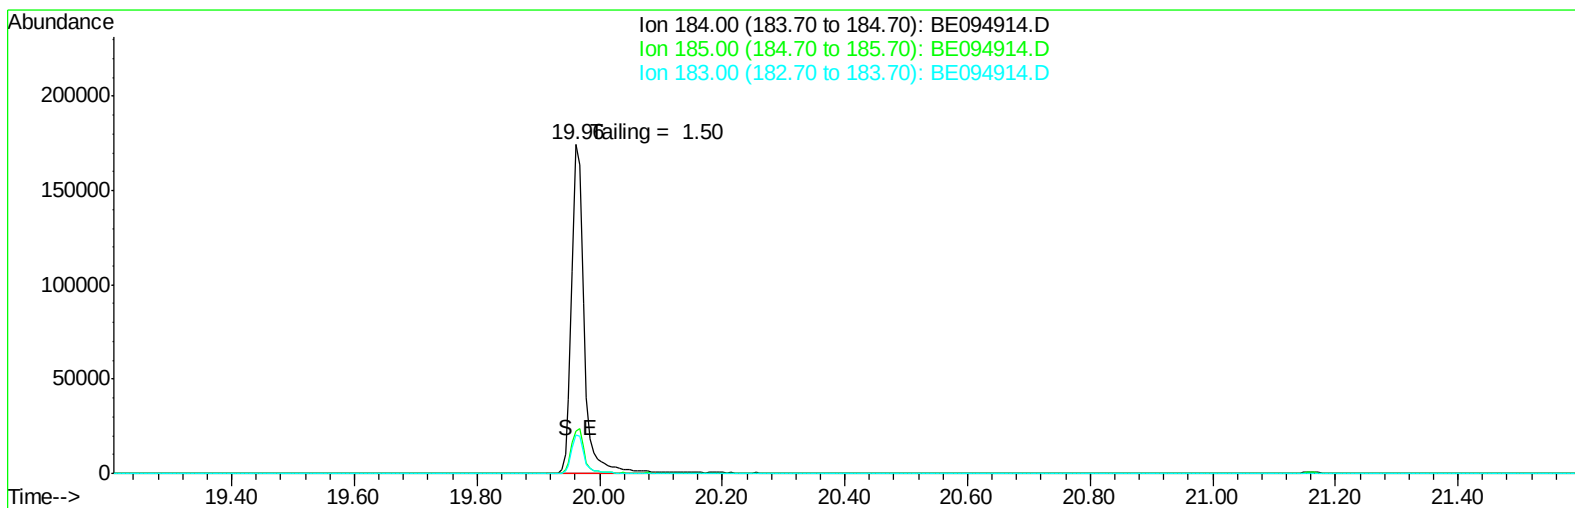

TIC: BE094914.D

(76) Benzidine



12.687min (-0.022) 32.95ng

response 15

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	23.53#
183.00	11.60	35.29#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE120517\
Data File : BE094914.D
Acq On : 5 Dec 2017 14:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 08:22:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

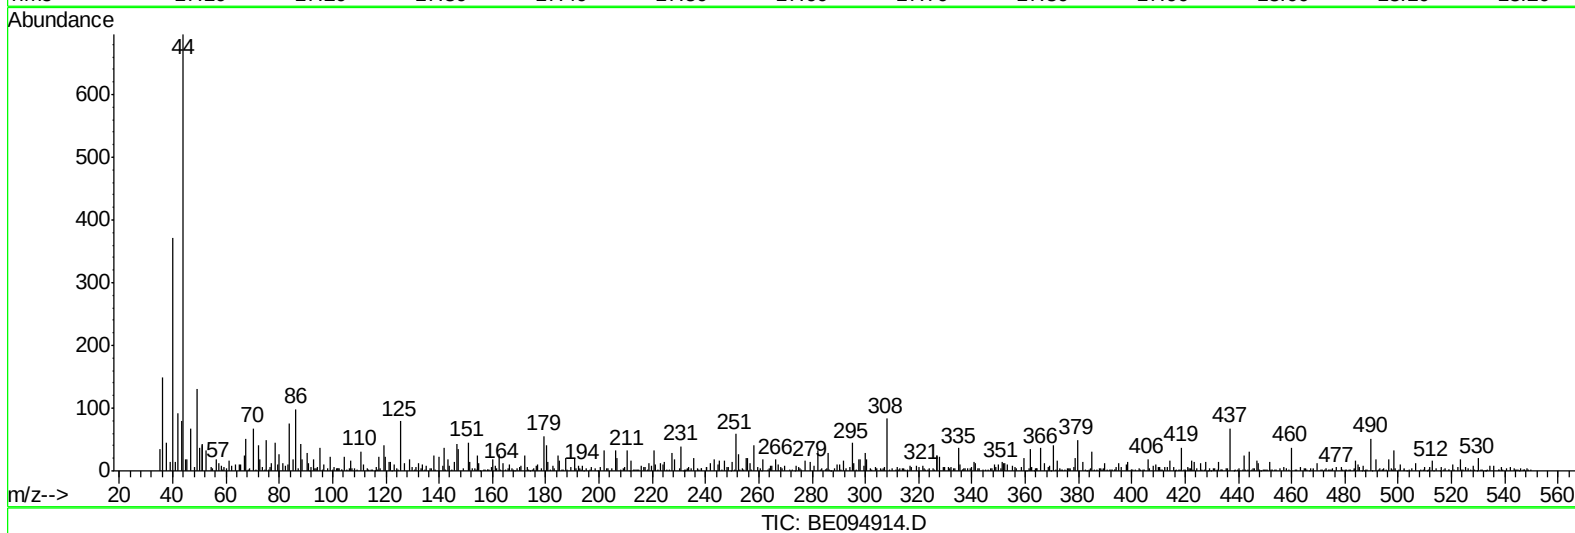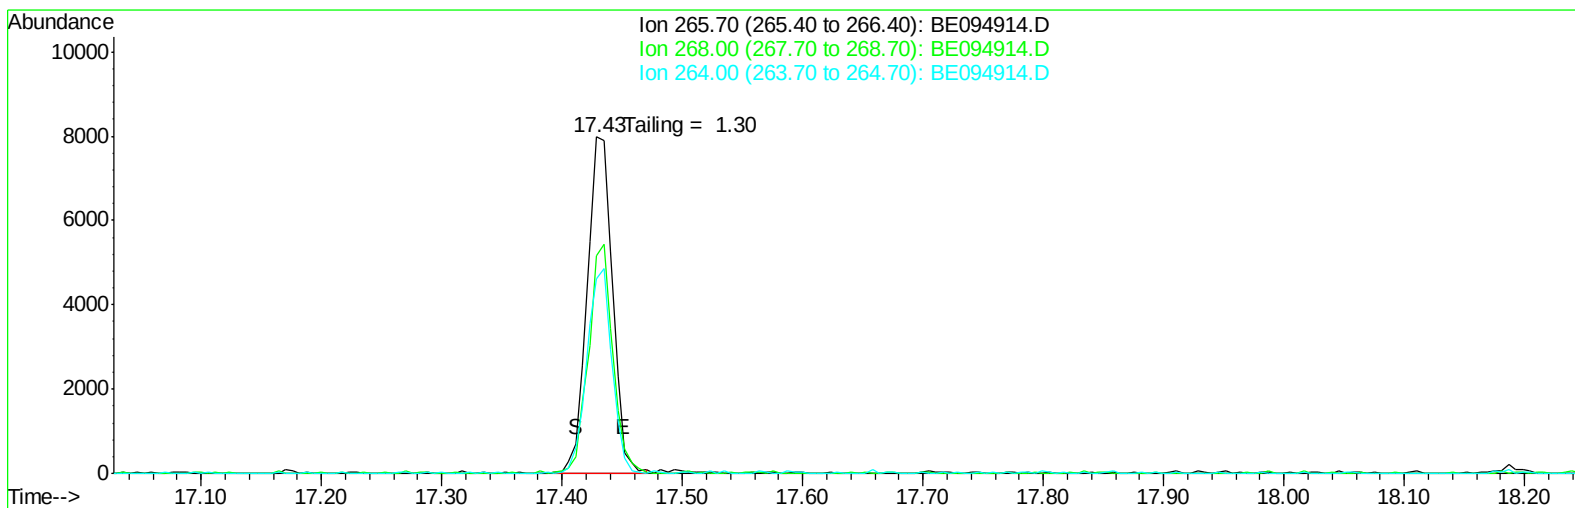

(69) Pentachlorophenol (C)

11.089min (-0.091) 75.80ng

response 11

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.11
264.00	61.90	72.22
0.00	0.00	0.00