
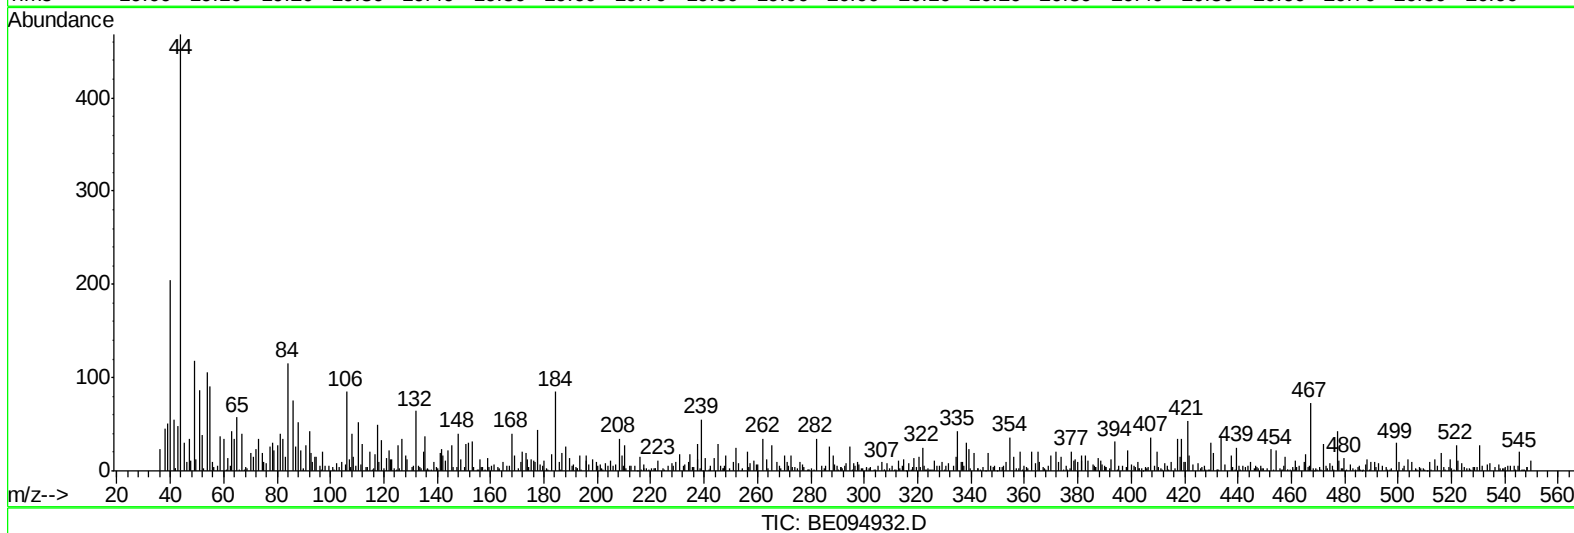


Data Path : Z:\HPCHEM1\BNA E\DATA\BE120517\  
Data File : BE094932.D  
Acq On : 6 Dec 2017 1:35  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 08:24:16 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 04 13:07:49 2017  
Response via : Initial Calibration

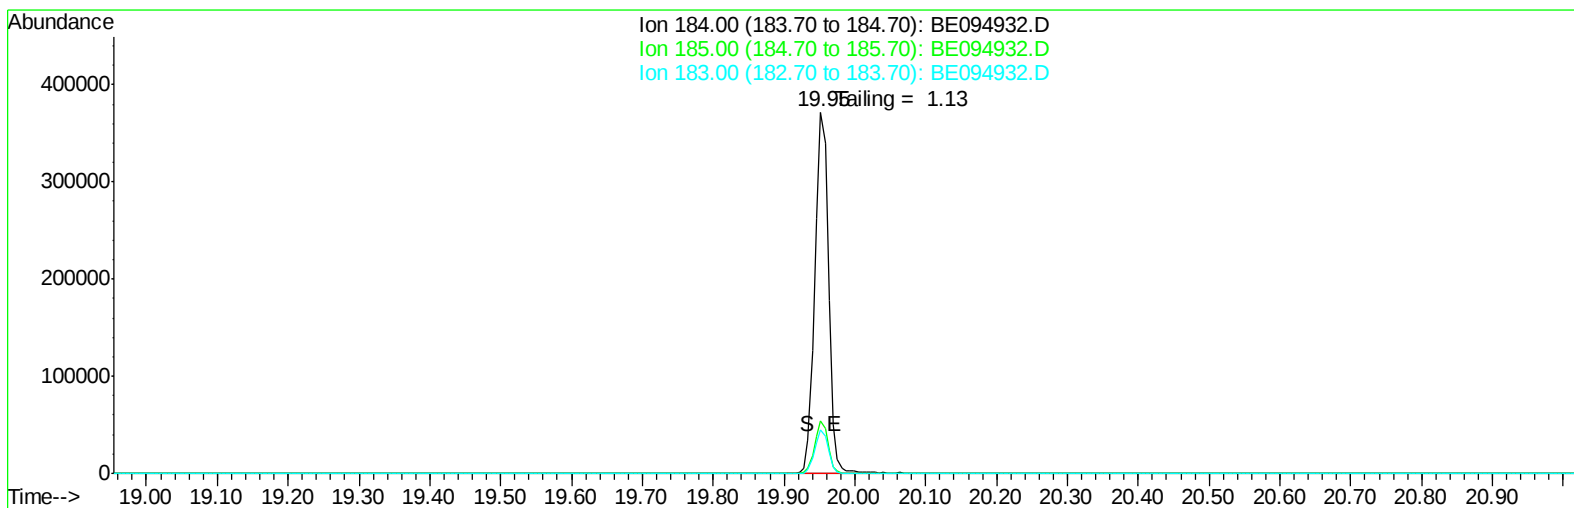

(76) Benzidine



12.713min (+0.004) 179.39ng

response 70

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 15.70 | 10.59# |
| 183.00 | 11.60 | 21.18# |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA E\DATA\BE120517\  
Data File : BE094932.D  
Acq On : 6 Dec 2017 1:35  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 08:24:16 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 04 13:07:49 2017  
Response via : Initial Calibration

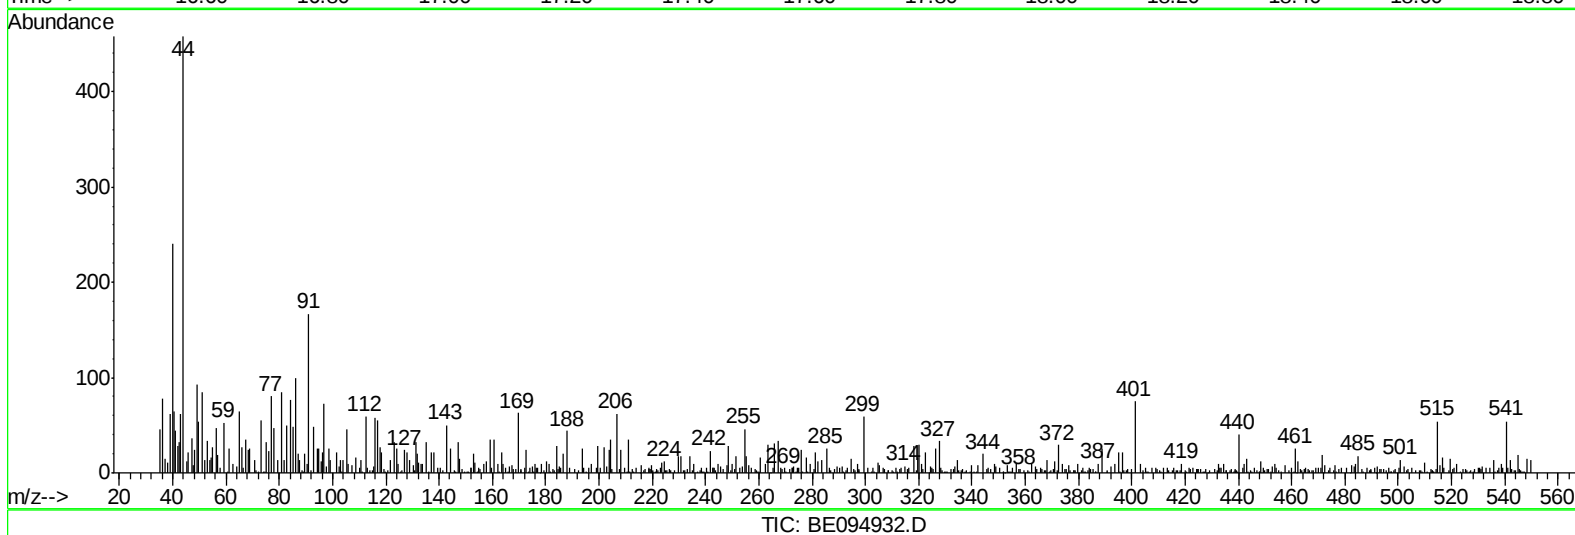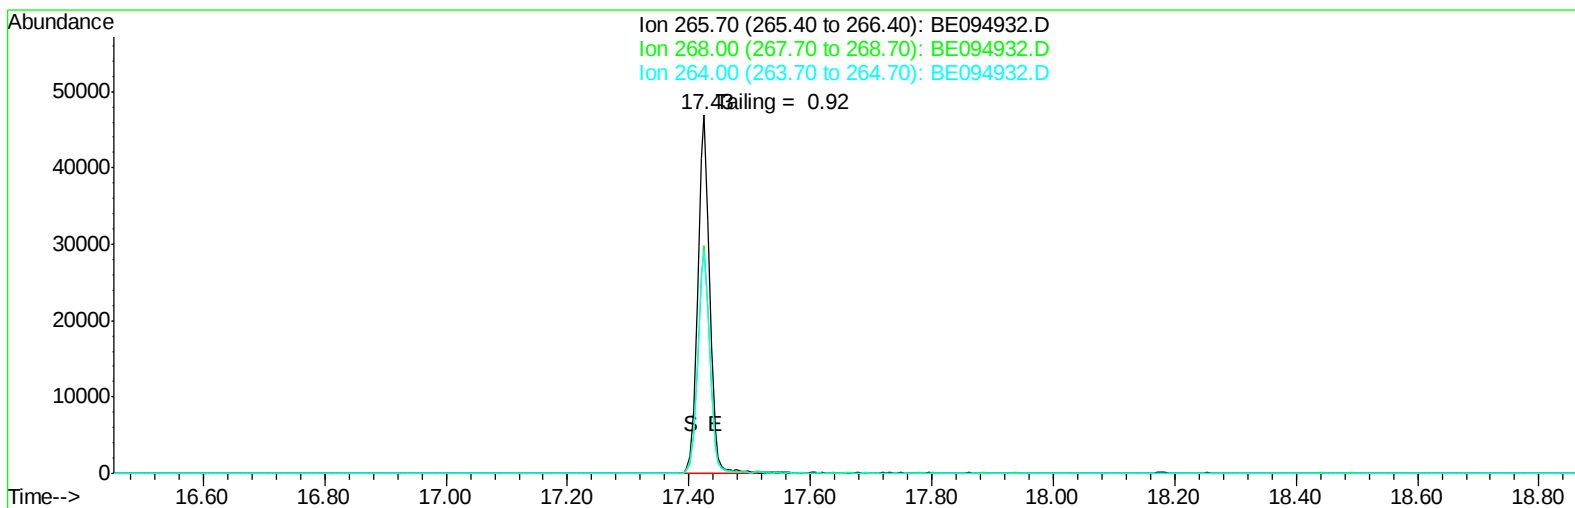

(69) Pentachlorophenol (C)

11.180min (-0.000) 327.14ng

response 41

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 265.70 | 100   | 100    |
| 268.00 | 63.90 | 29.03# |
| 264.00 | 61.90 | 0.00#  |
| 0.00   | 0.00  | 0.00   |