

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE120517\
 Data File : BE094936.D
 Acq On : 6 Dec 2017 3:58
 Operator : SJ/JU
 Sample : I6698-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 FT-DUP03-20171130

Manual Integrations
 APPROVED

Sohil
 12/6/2017 5:10:41 PM

Quant Time: Dec 06 07:04:39 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE113017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 13:33:28 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.48	152	8651	0.40	ng	0.00
7) Naphthalene-d8	11.33	136	18527	0.40	ng	0.00
13) Acenaphthene-d10	15.06	164	10808	0.40	ng	-0.02
19) Phenanthrene-d10	17.77	188	26499	0.40	ng	0.00
27) Chrysene-d12	21.87	240	28195	0.40	ng	-0.01
34) Perylene-d12	24.55	264	23331	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.95	112	2577	0.19	ng	0.00
5) Phenol-d6	7.60	99	2340	0.12	ng	0.01
8) Nitrobenzene-d5	9.67	82	5744	0.52	ng	0.00
11) 2-Methylnaphthalene-d10	12.87	152	11919	0.40	ng	0.00
14) 2,4,6-Tribromophenol	16.53	330	1315	0.55	ng	0.00
15) 2-Fluorobiphenyl	13.71	172	18644	0.40	ng	0.00
25) Fluoranthene-d10	19.75	212	142694	0.39	ng	0.00
29) Terphenyl-d14	20.31	244	28676	0.55	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.67	88	992	0.110	ng	Qvalue # 53
30) Benzo(a)anthracene	21.86	228	3194	0.037	ng	# 66
31) Chrysene	21.92	228	2974m	0.031	ng	
32) Bis(2-ethylhexyl)phthalate	21.75	149	23377	0.163	ng	100
33) Indeno(1,2,3-cd)pyrene	27.43	276	3038	0.039	ng	95
35) Benzo(b)fluoranthene	23.72	252	3259	0.038	ng	# 63
36) Benzo(k)fluoranthene	23.77	252	2735	0.031	ng	# 59
37) Benzo(a)pyrene	24.43	252	2757	0.037	ng	# 71
38) Dibenzo(a,h)anthracene	27.44	278	2527	0.037	ng	# 68
39) Benzo(a,h,i)perylene	28.30	276	2810	0.041	ng	# 61

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE120517\
Data File : BE094936.D
Acq On : 6 Dec 2017 3:58
Operator : SJ/JU
Sample : I6698-14
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
FT-DUP03-20171130

Manual Integrations
APPROVED

Sohil
12/6/2017 5:10:41 PM

Quant Time: Dec 06 07:04:39 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 13:33:28 2017
Response via : Initial Calibration

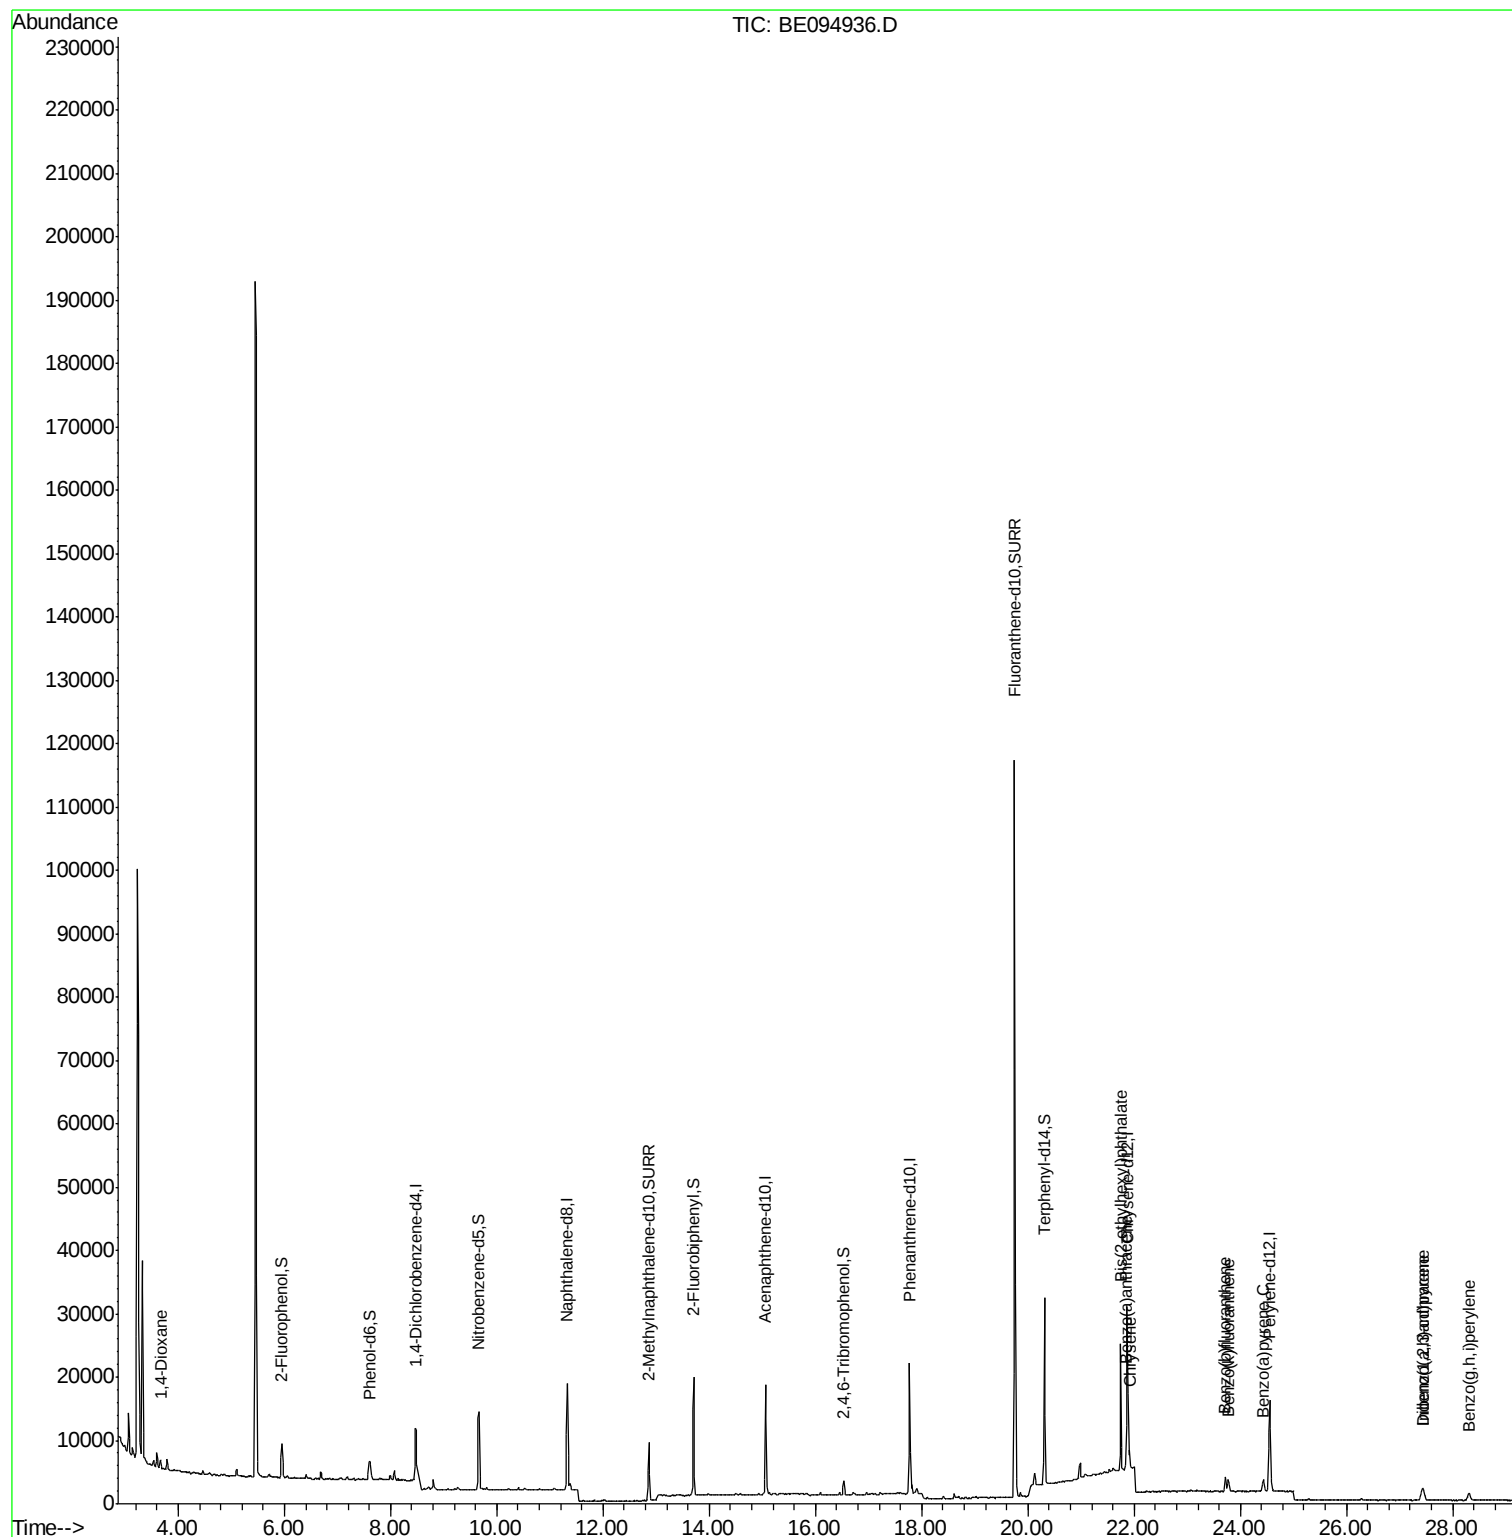

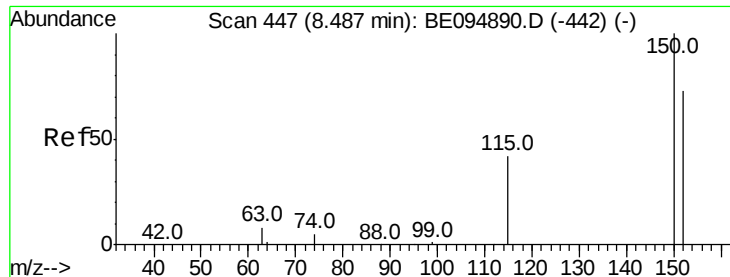

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 8.48 min Scan# 447

Delta R.T. -0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E


ClientSampleId :

FT-DUP03-20171130




Tot Ion:	152	Resp:	8651
Ion	Ratio	Lower	Upper
152	100		
150	139.0	117.2	175.8
115	61.4	57.0	85.6

Manual Integrations
APPROVED

Sohil
12/6/2017 5:10:41 PM

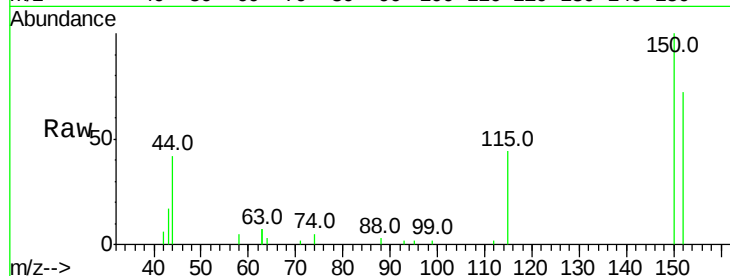

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

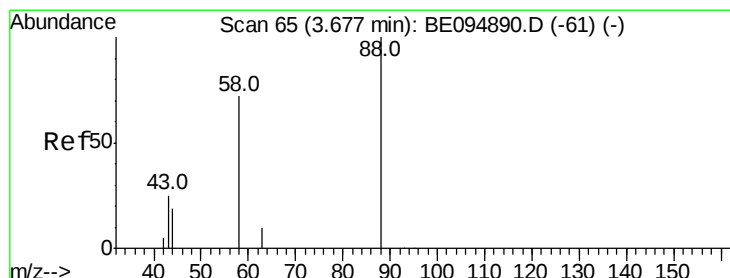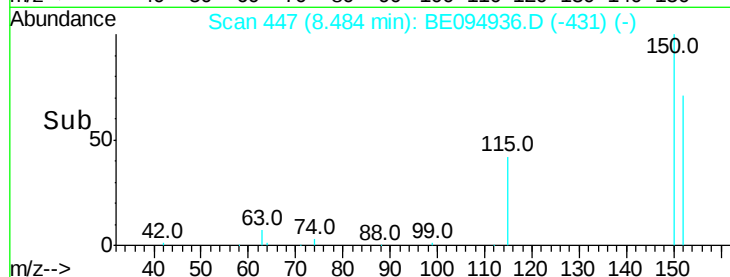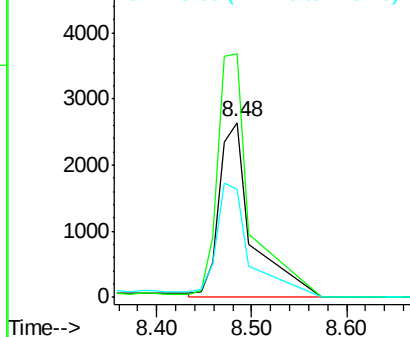

#2

1,4-Dioxane

Concen: 0.110 ng


RT: 3.67 min Scan# 65

Delta R.T. -0.00 min



Lab File: BE094936.D


Acq: 6 Dec 2017 3:58

Tgt Ion:	88	Resp:	992
Ion	Ratio	Lower	Upper
88	100		
58	115.6	63.2	94.8#
43	89.8	41.2	61.8#

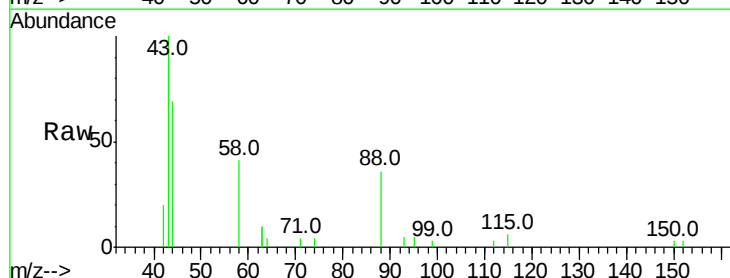

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

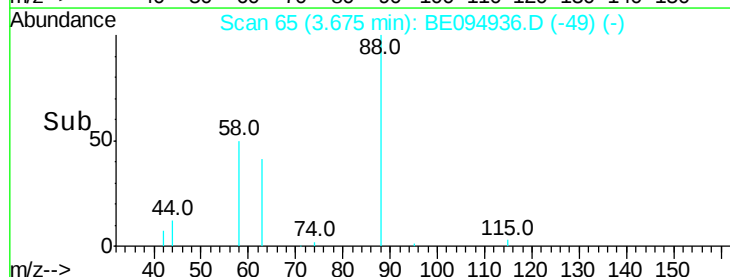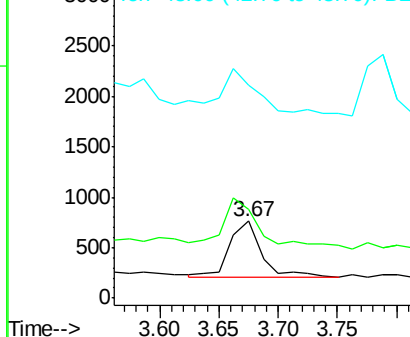

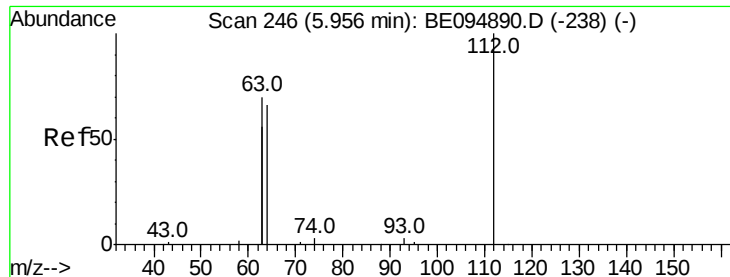

#4

2-Fluorophenol

Concen: 0.188 ng

RT: 5.95 min Scan# 246

Delta R.T. -0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E


ClientSampleId :

FT-DUP03-20171130

Tot Ion:	112	Resp:	2577
Ion Ratio	Lower	Upper	
112	100		
64	77.6	60.1	90.1
63	157.3	116.8	175.2

Manual Integrations
APPROVED




Sohil
12/6/2017 5:10:41 PM

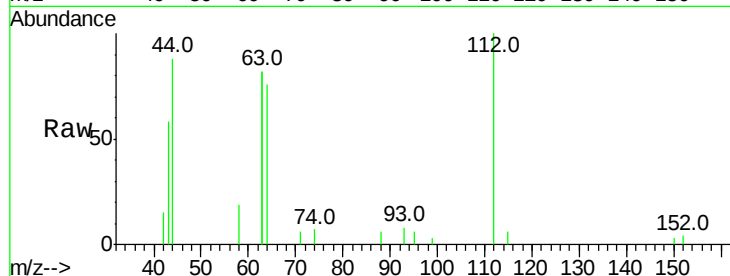

Abundance Ion 112.00 (111.70 to 112.70): BE094890.D (-238) (-)

Ion 64.00 (63.70 to 64.70): BE094890.D (-238) (-)

Ion 63.00 (62.70 to 63.70): BE094890.D (-238) (-)

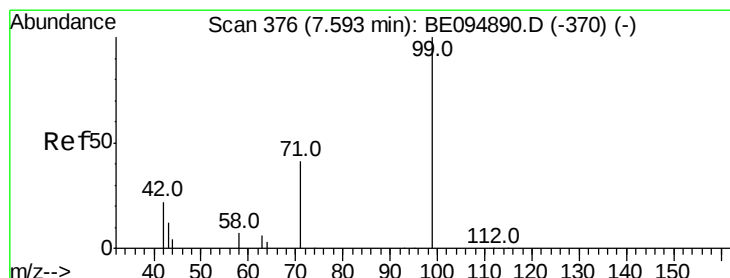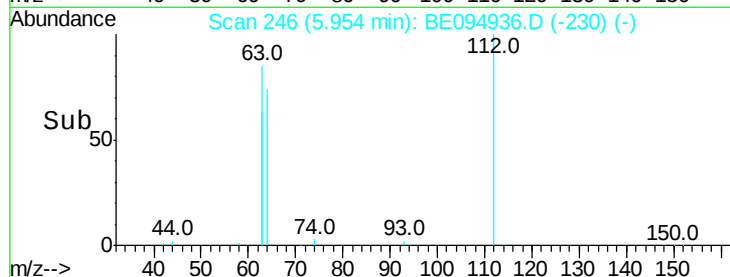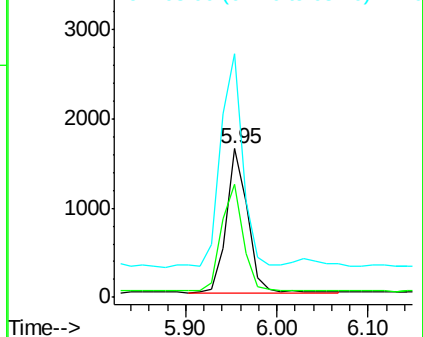

#5

Phenol-d6

Concen: 0.115 ng


RT: 7.60 min Scan# 377

Delta R.T. 0.01 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58



Tgt Ion:	99	Resp:	2340
Ion Ratio	Lower	Upper	
99	100		
42	32.6	20.2	30.2#
71	40.7	28.4	42.6

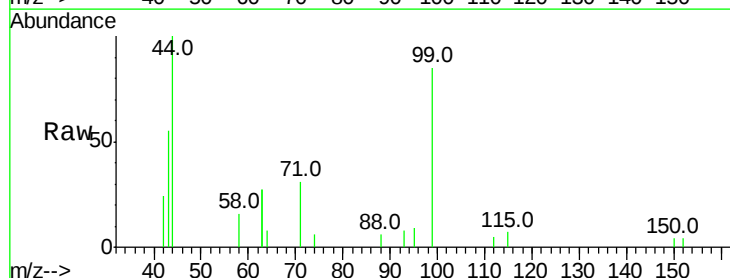


Abundance Ion 99.00 (98.70 to 99.70): BE094890.D (-370) (-)

Ion 42.00 (41.70 to 42.70): BE094890.D (-370) (-)

Ion 71.00 (70.70 to 71.70): BE094890.D (-370) (-)

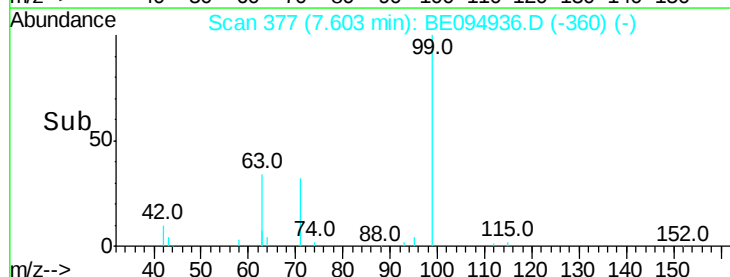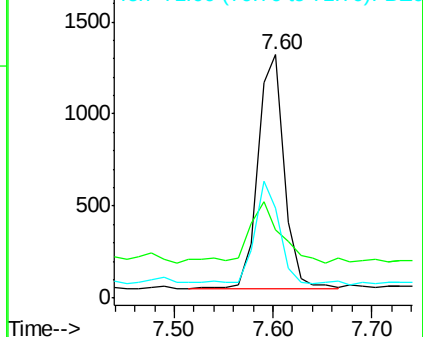



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.33 min Scan# 613

Delta R.T. 0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E


ClientSampleId :

FT-DUP03-20171130

Tot Ion	Ratio	Resp	Lower	Upper
136	100	18527		
137	11.0	9.5	14.3	
54	34.6	29.1	43.7	
68	7.0	6.2	9.2	

Manual Integrations
APPROVED

Sohil
12/6/2017 5:10:41 PM






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

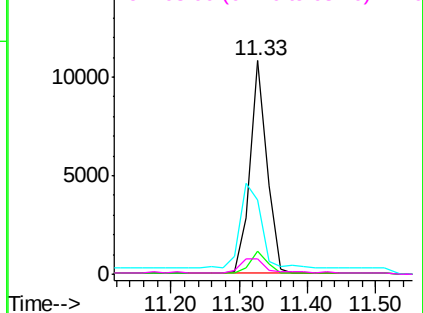

#8

Nitrobenzene-d5

Concen: 0.524 ng


RT: 9.67 min Scan# 514

Delta R.T. 0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58



Tgt Ion	Ratio	Resp	Lower	Upper
82	100	5744		
128	150.3	150.0	225.0	
54	186.2	154.2	231.4	




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

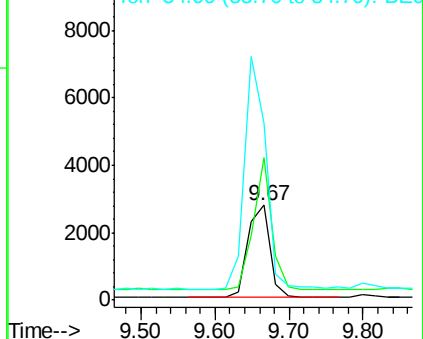

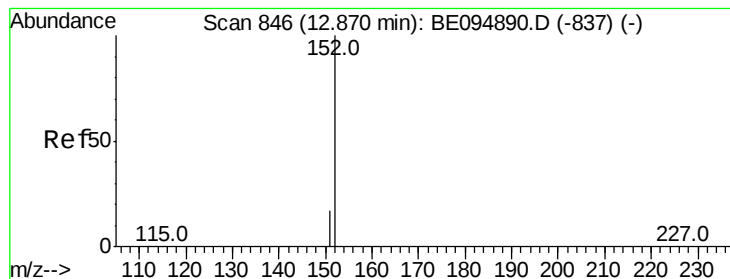

#11

2-Methylnaphthalene-d10

Concen: 0.403 ng

RT: 12.87 min Scan# 845

Delta R.T. -0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E

ClientSampleId :

FT-DUP03-20171130

Tot Ion:152 Resp: 11919

Ion Ratio Lower Upper


152 100

151 19.6 15.4 23.0

Manual Integrations
APPROVED




Sohil

12/6/2017 5:10:41 PM

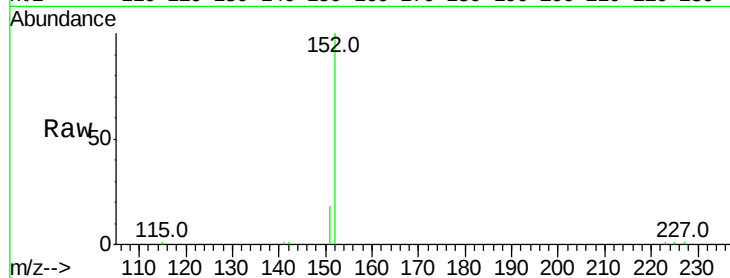

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

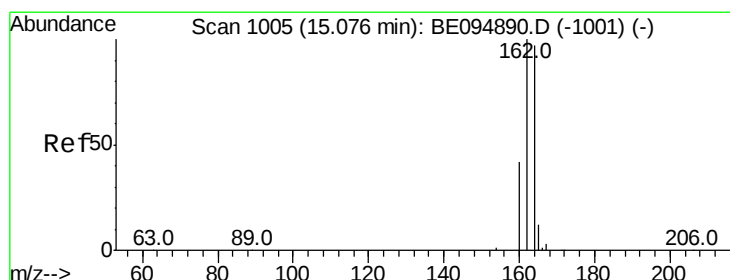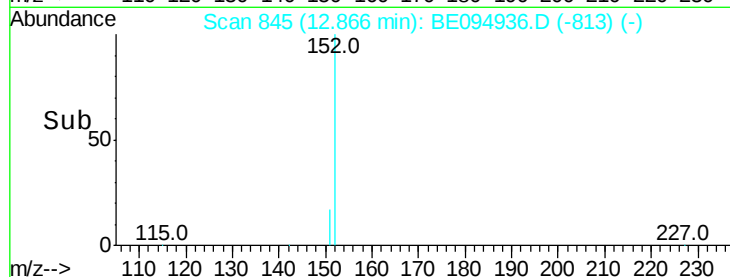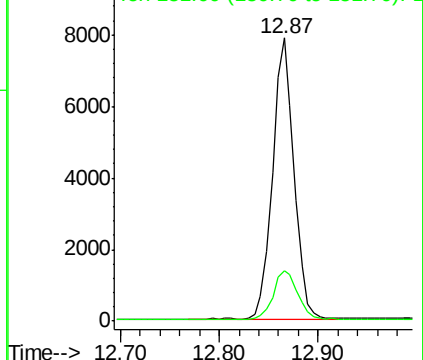

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 15.06 min Scan# 1004

Delta R.T. -0.02 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58


Tgt Ion:164 Resp: 10808

Ion Ratio Lower Upper

164 100

162 112.2 83.1 124.7



160 49.0 37.1 55.7

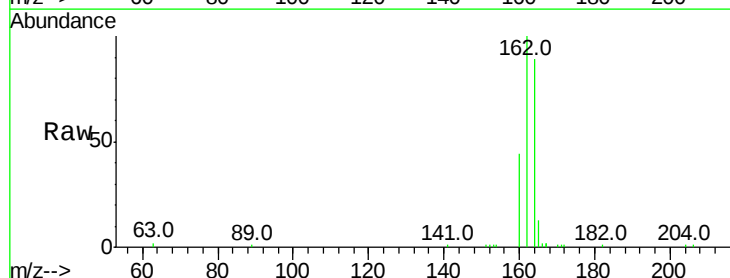


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

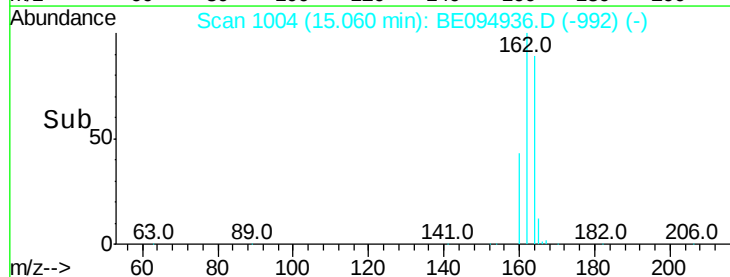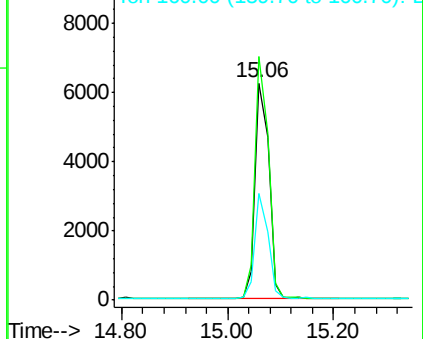



#14

2,4,6-Tribromophenol

Concen: 0.552 ng

RT: 16.53 min Scan# 1100

Delta R.T. 0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E





ClientSampleId :

FT-DUP03-20171130

Tot Ion	Ratio	Lower	Upper
330	100		
332	90.8	152.7	229.1#
141	53.5	33.7	50.5#

Manual Integrations
APPROVED

Sohil
12/6/2017 5:10:41 PM

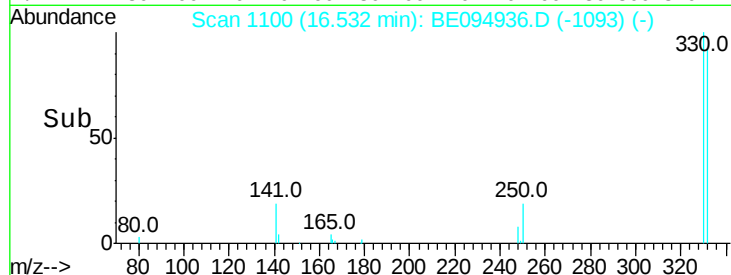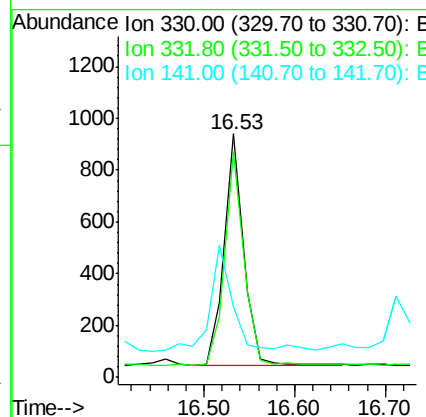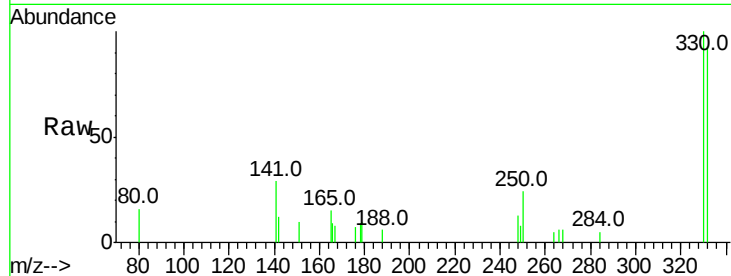

#15

2-Fluorobiphenyl

Concen: 0.403 ng




RT: 13.71 min Scan# 913


Delta R.T. -0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.6	29.9	44.9
170	20.1	21.8	32.8#

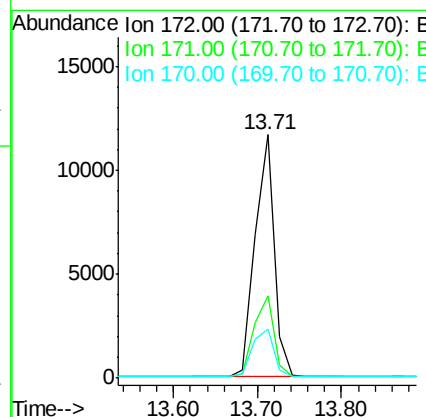



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.77 min Scan# 1183

Delta R.T. -0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E


ClientSampleId :

FT-DUP03-20171130

Tot Ion:	188	Resp:	26499
Ion Ratio	Lower	Upper	
188	100		
94	0.0	3.9	5.9#
80	11.4	3.6	5.4#

Manual Integrations
APPROVED




Sohil
12/6/2017 5:10:41 PM



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

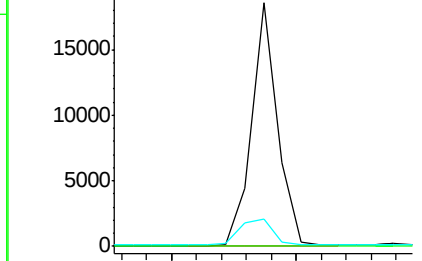

#25

Fluoranthene-d10

Concen: 0.394 ng


RT: 19.75 min Scan# 1431

Delta R.T. -0.01 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58



Tgt Ion:	212	Resp:	142694
Ion Ratio	Lower	Upper	
212	100		
106	3.4	2.8	4.2
104	2.0	1.6	2.4




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

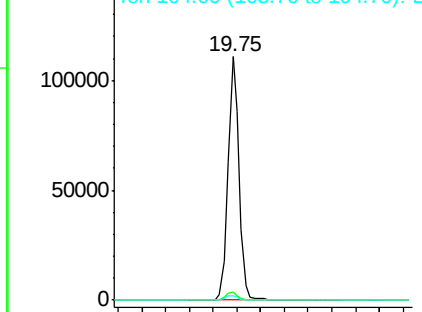







#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.87 min Scan# 1582
Delta R.T. -0.01 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Instrument :
BNA_E
ClientSampleId :
FT-DUP03-20171130

Tot Ion	Ratio	Lower	Upper
240	100		
120	13.2	5.5	8.3#
236	27.5	20.7	31.1




Manual Integrations
APPROVED


Sohil
12/6/2017 5:10:41 PM

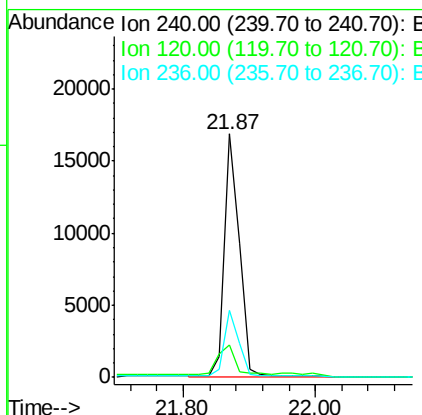

#29
Terphenyl-d14
Concen: 0.551 ng
RT: 20.31 min Scan# 1482
Delta R.T. -0.01 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Tgt Ion	Ratio	Lower	Upper
244	100		
212	10.4	25.4	38.0#
122	10.8	8.1	12.1

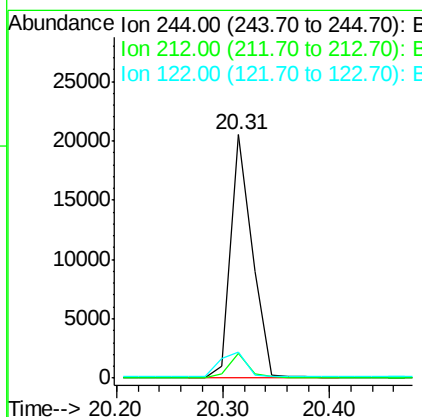



#30

Benzo(a)anthracene

Concen: 0.037 ng

RT: 21.86 min Scan# 1581

Delta R.T. -0.01 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E





ClientSampleId :

FT-DUP03-20171130

Tot Ion:	228	Resp:	3194
Ion Ratio	Lower	Upper	
228	100		
226	30.5	40.0	60.0#
229	22.6	40.0	60.0#

Manual Integrations
APPROVED

Sohil
12/6/2017 5:10:41 PM

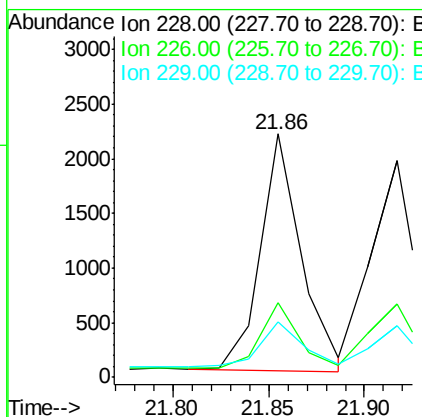

#31

Chrysene

Concen: 0.031 ng m




RT: 21.92 min Scan# 1585


Delta R.T. 0.00 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Tgt Ion:	228	Resp:	2974
Ion Ratio	Lower	Upper	
228	100		
226	33.8	40.0	60.0#
229	23.8	40.0	60.0#

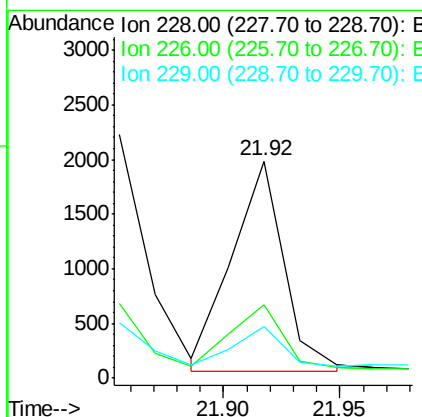



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.163 ng

RT: 21.75 min Scan# 1574

Delta R.T. -0.01 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Instrument :

BNA_E





ClientSampleId :

FT-DUP03-20171130

Tot Ion:	149	Resp:	23377
Ion Ratio	Lower	Upper	
149	100		
167	6.6	5.4	8.0
279	0.9	0.7	1.1

Manual Integrations
APPROVED

Sohil
12/6/2017 5:10:41 PM

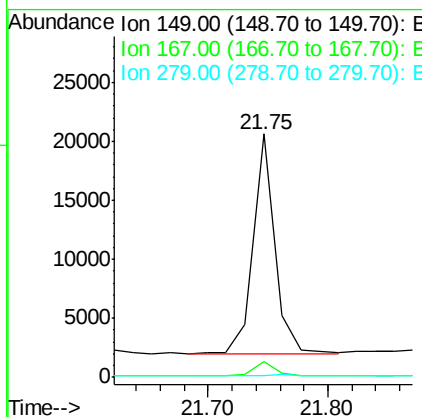

#33

Indeno(1,2,3-cd)pyrene

Concen: 0.039 ng




RT: 27.43 min Scan# 2772


Delta R.T. -0.01 min

Lab File: BE094936.D

Acq: 6 Dec 2017 3:58

Tgt Ion:	276	Resp:	3038
Ion Ratio	Lower	Upper	
276	100		
138	32.7	22.5	33.7
277	24.2	19.9	29.9

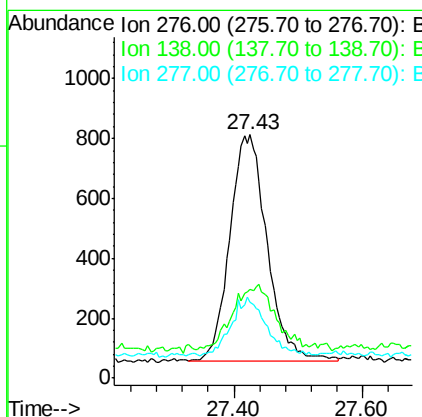

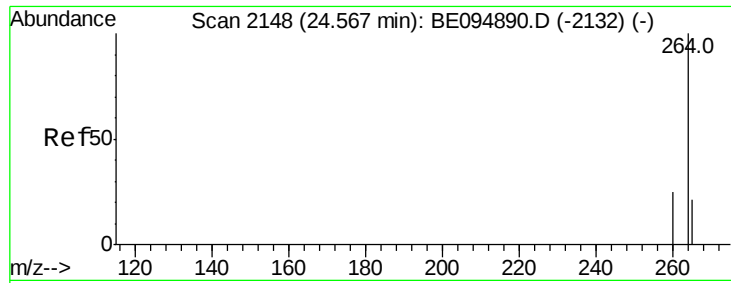




#34
Pervlene-d12
Concen: 0.400 ng
RT: 24.55 min Scan# 2145
Delta R.T. -0.01 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Instrument :
BNA_E
ClientSampleId :
FT-DUP03-20171130

Tot Ion	Ratio	Resp	Lower	Upper
264	100			
260	25.4	20.5	30.7	
265	31.2	22.8	34.2	





Manual Integrations
APPROVED


Sohil
12/6/2017 5:10:41 PM

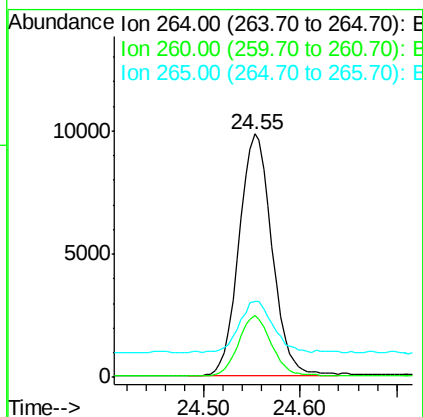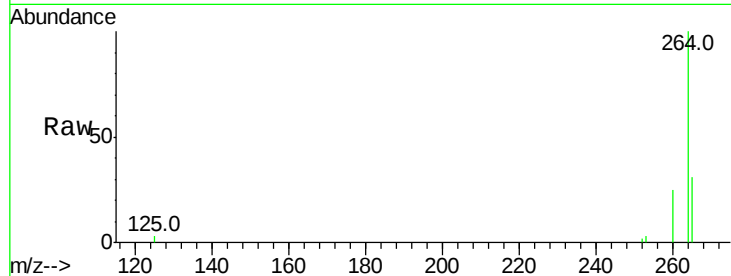

#35
Benzo(b)fluoranthene
Concen: 0.038 ng
RT: 23.72 min Scan# 1963
Delta R.T. -0.01 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Tgt Ion	Ratio	Resp	Lower	Upper
252	100			
253	37.3	48.0	72.0#	
125	35.0	56.0	84.0#	

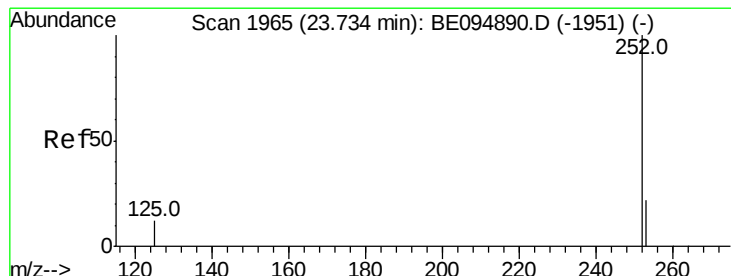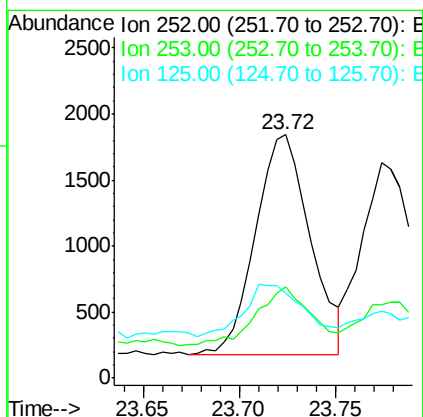

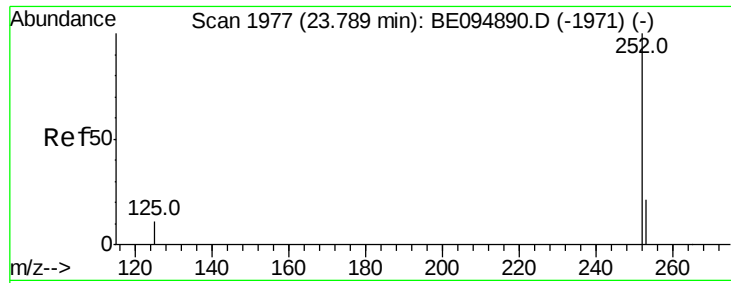





#36
Benzo(k)fluoranthene
Concen: 0.031 ng
RT: 23.77 min Scan# 1974
Delta R.T. -0.01 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Instrument :
BNA_E
ClientSampleId :
FT-DUP03-20171130

Tot Ion	Ratio	Lower	Upper
252	100		
253	33.9	48.0	72.0#
125	31.2	56.0	84.0#




Manual Integrations
APPROVED


Sohil
12/6/2017 5:10:41 PM

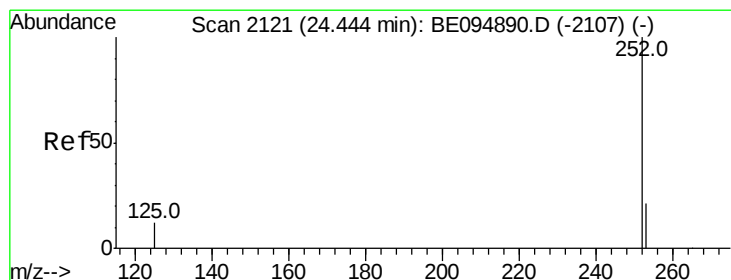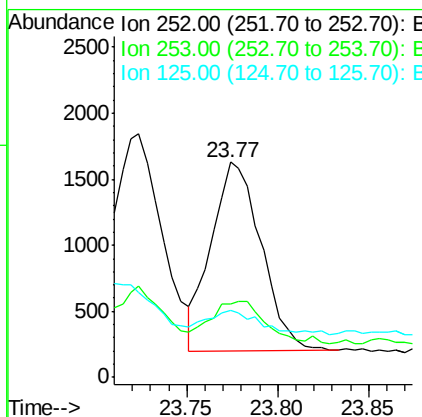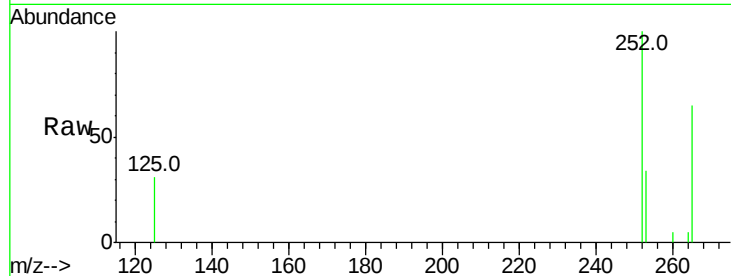

#37
Benzo(a)pyrene
Concen: 0.037 ng
RT: 24.43 min Scan# 2119
Delta R.T. -0.01 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Tgt Ion	Ratio	Lower	Upper
252	100		
253	40.4	52.0	78.0#
125	59.7	68.0	102.0#

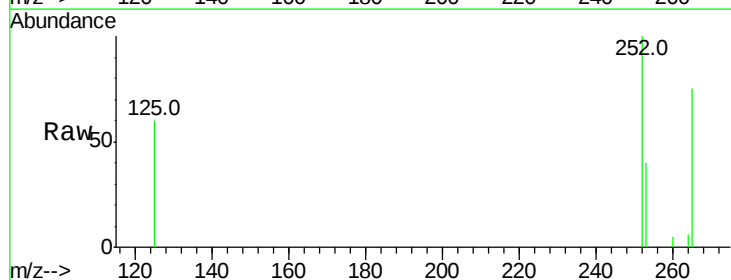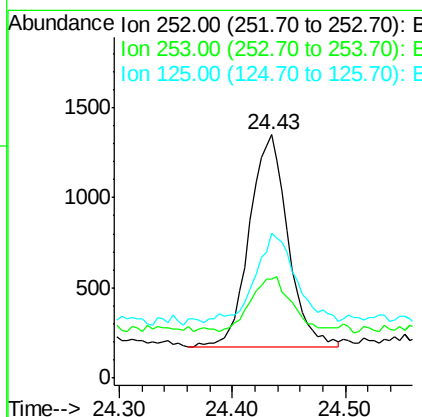







#38
Dibenzo(a,h)anthracene
Concen: 0.037 ng
RT: 27.44 min Scan# 2776
Delta R.T. -0.03 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Instrument :
BNA_E
ClientSampleId :
FT-DUP03-20171130

Tot Ion	Ratio	Lower	Upper
278	100		
139	43.9	56.0	84.0#
279	39.2	52.0	78.0#

Manual Integrations
APPROVED

Sohil
12/6/2017 5:10:41 PM

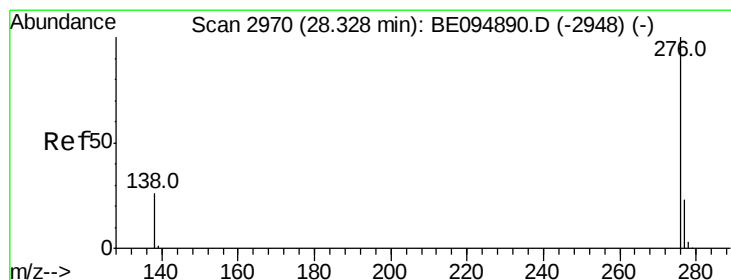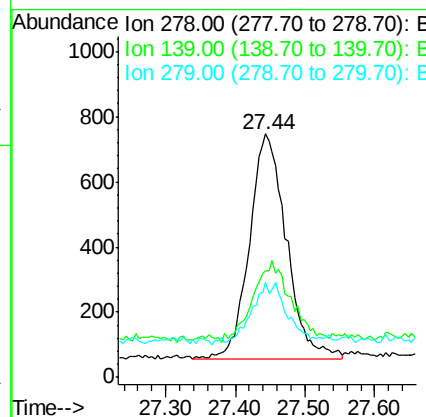

#39
Benzo(g,h,i)perylene
Concen: 0.041 ng
RT: 28.30 min Scan# 2965
Delta R.T. -0.02 min
Lab File: BE094936.D
Acq: 6 Dec 2017 3:58

Tgt Ion	Ratio	Lower	Upper
276	100		
277	30.0	52.0	78.0#
138	31.6	44.0	66.0#

