


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE120517\
 Data File : BE094932.D
 Acq On : 6 Dec 2017 1:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 01 13:33:28 2017

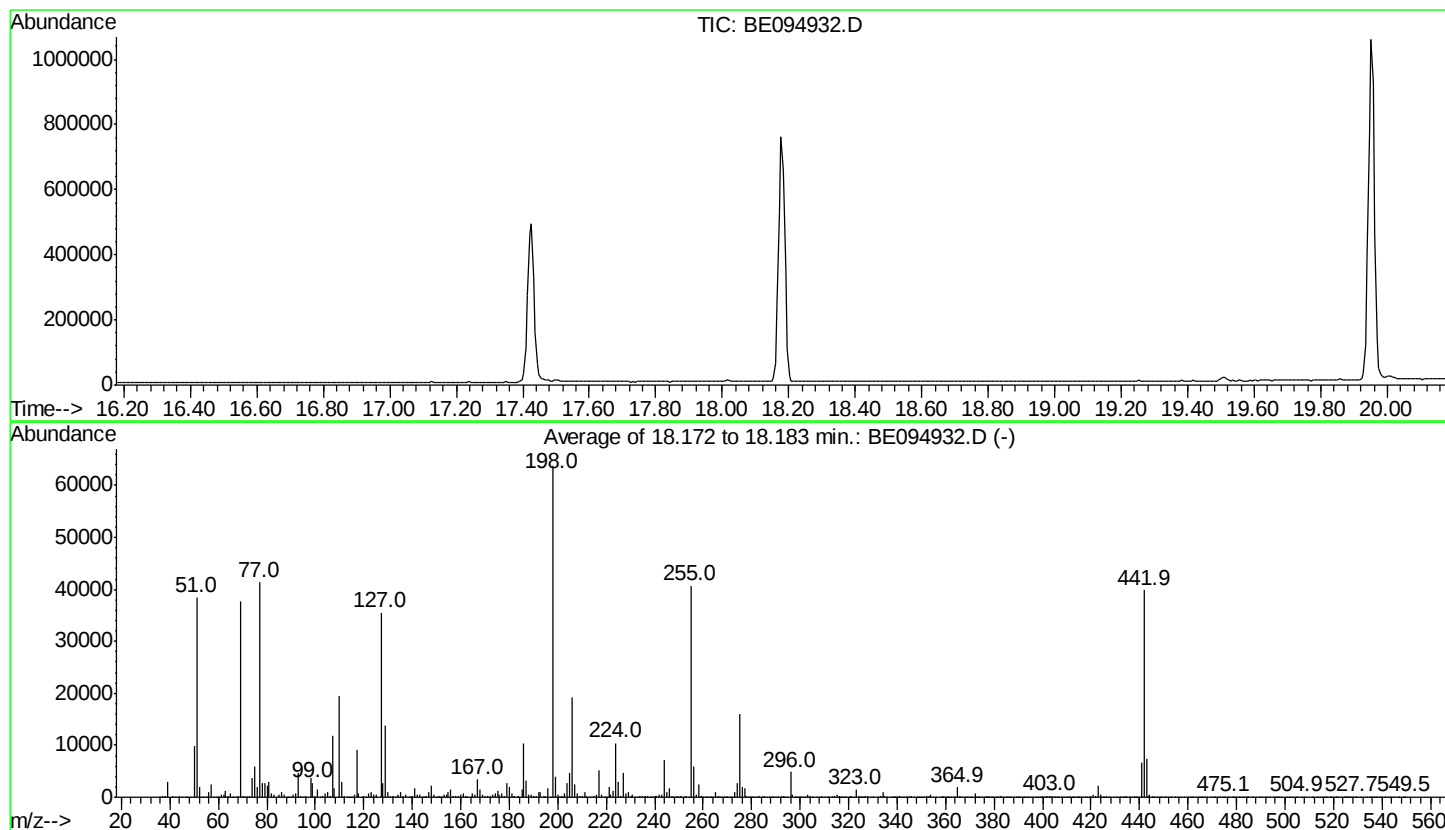

AutoFind: Scans 2652, 2653, 2654; Background Corrected with Scan 2643

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.1	38330	PASS
68	69	0.00	2	0.4	141	PASS
69	198	0.00	100	59.0	37628	PASS
70	69	0.00	2	0.8	285	PASS
127	198	10	80	55.7	35532	PASS
197	198	0.00	2	0.1	73	PASS
198	198	100	100	100.0	63816	PASS
199	198	5	9	6.4	4069	PASS
275	198	10	60	25.3	16120	PASS
365	198	1	100	3.0	1915	PASS
441	442	0.01	24	16.9	6711	PASS
442	198	50	100	62.4	39813	PASS
443	442	15	24	18.6	7421	PASS