


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE120619\
 Data File : BE100798.D
 Acq On : 6 Dec 2019 9:13
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 04 17:18:11 2019

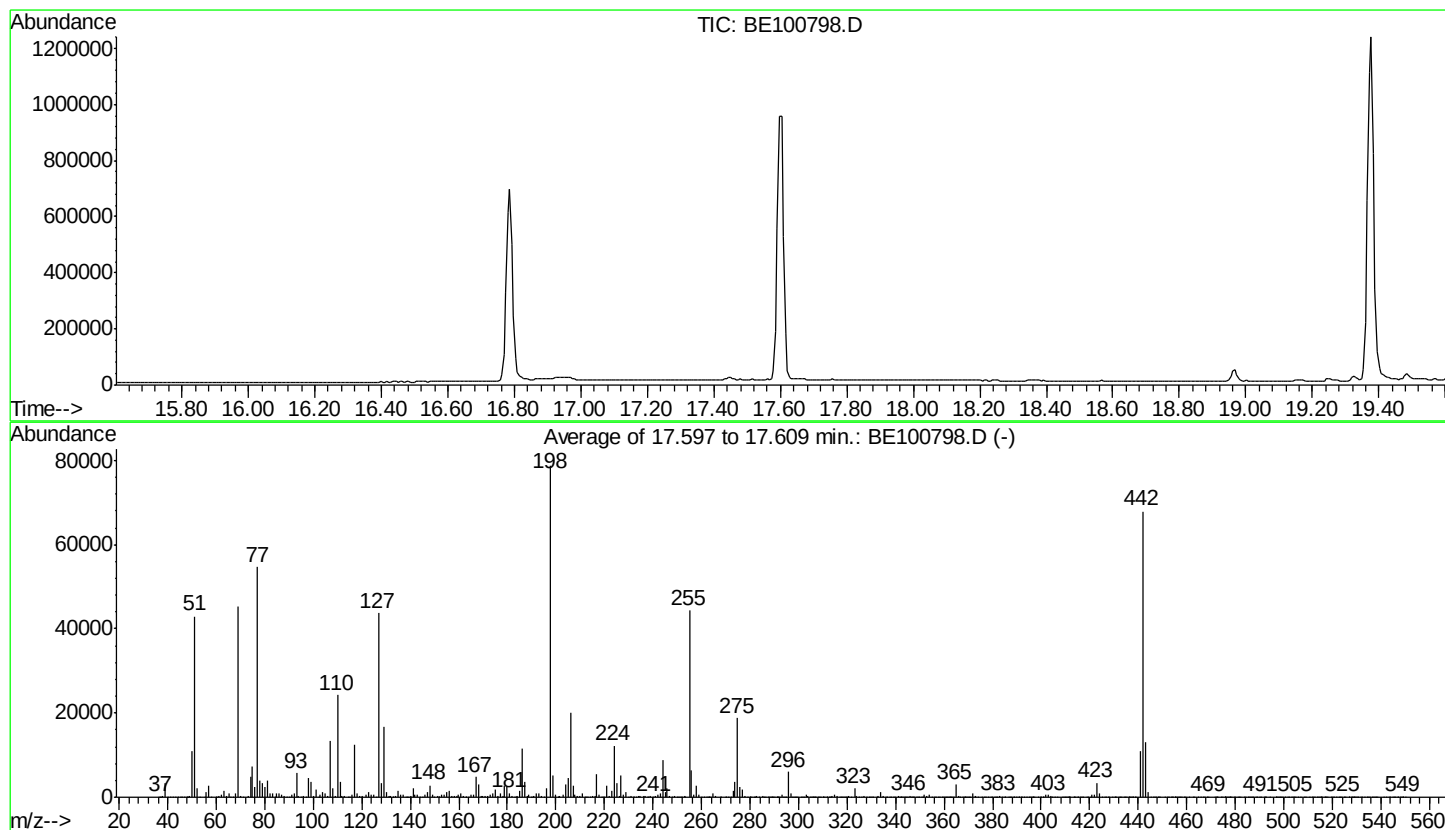

AutoFind: Scans 2554, 2555, 2556; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.6	43032	PASS
68	69	0.00	2	1.7	785	PASS
69	198	0.00	100	57.4	45193	PASS
70	69	0.00	2	0.5	243	PASS
127	198	10	80	55.5	43709	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78774	PASS
199	198	5	9	6.7	5270	PASS
275	198	10	60	23.9	18806	PASS
365	198	1	100	3.7	2950	PASS
441	198	0.01	100	14.0	11034	PASS
442	198	50	100	86.2	67870	PASS
443	442	15	24	19.5	13223	PASS