

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
 Data File : BE089180.D
 Acq On : 8 Dec 2014 23:27
 Operator : TP/JJ
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTDICC0.8

Quant Time: Dec 09 03:49:09 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-ACID-BE120814.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 09 03:43:23 2014
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	29077	5.00	ng	0.00
8) Naphthalene-d8	8.51	136	110751	5.00	ng	0.00
13) Acenaphthene-d10	10.66	164	54913	5.00	ng	0.00
19) Phenanthrene-d10	12.72	188	82253	5.00	ng	0.00
22) Chrysene-d12	18.08	240	60677	5.00	ng	0.00
23) Perylene-d12	21.12	264	54853	5.00	ng	0.00
System Monitoring Compounds						
2) 2-Fluorophenol	5.28	112	4825	0.64	ng	0.00
3) Phenol-d6	6.56	99	6760	0.70	ng	0.00
14) 2,4,6-Tribromophenol	11.67	330	1191	0.66	ng	0.00
Target Compounds						Qvalue
4) 2-Chlorophenol	6.69	128	5430	0.76	ng	89
5) Phenol	6.58	94	7936	0.76	ng	86
6) 2-Methylphenol	7.31	107	6479	0.33	ng	95
7) 3+4-Methylphenols	7.52	107	5308	0.22	ng	95
9) 2-Nitrophenol	8.06	139	2781	1.09	ng	95
10) 2,4-Dimethylphenol	8.15	122	4606	0.77	ng	97
11) 2,4-Dichlorophenol	8.38	162	4049	0.80	ng	94
12) 4-Chloro-3-methylphenol	9.25	107	4208	0.75	ng	94
15) 2,4,6-Trichlorophenol	9.75	196	2416	0.72	ng	# 82
16) 2,4,5-Trichlorophenol	9.75	196	2416	0.69	ng	99
17) 2,4-Dinitrophenol	10.80	184	476	1.36	ng	# 88
18) 4-Nitrophenol	10.91	139	5839	2.13	ng	92
20) 4,6-Dinitro-2-methylphenol	11.45	198	800	1.16	ng	88
21) Pentachlorophenol	12.44	266	634	0.66	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
Data File : BE089180.D
Acq On : 8 Dec 2014 23:27
Operator : TP/JJ
Sample : SSTDIC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
LabSampleId :
SSTDIC0.8

Quant Time: Dec 09 03:49:09 2014
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-ACID-BE120814.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 09 03:43:23 2014
Response via : Initial Calibration

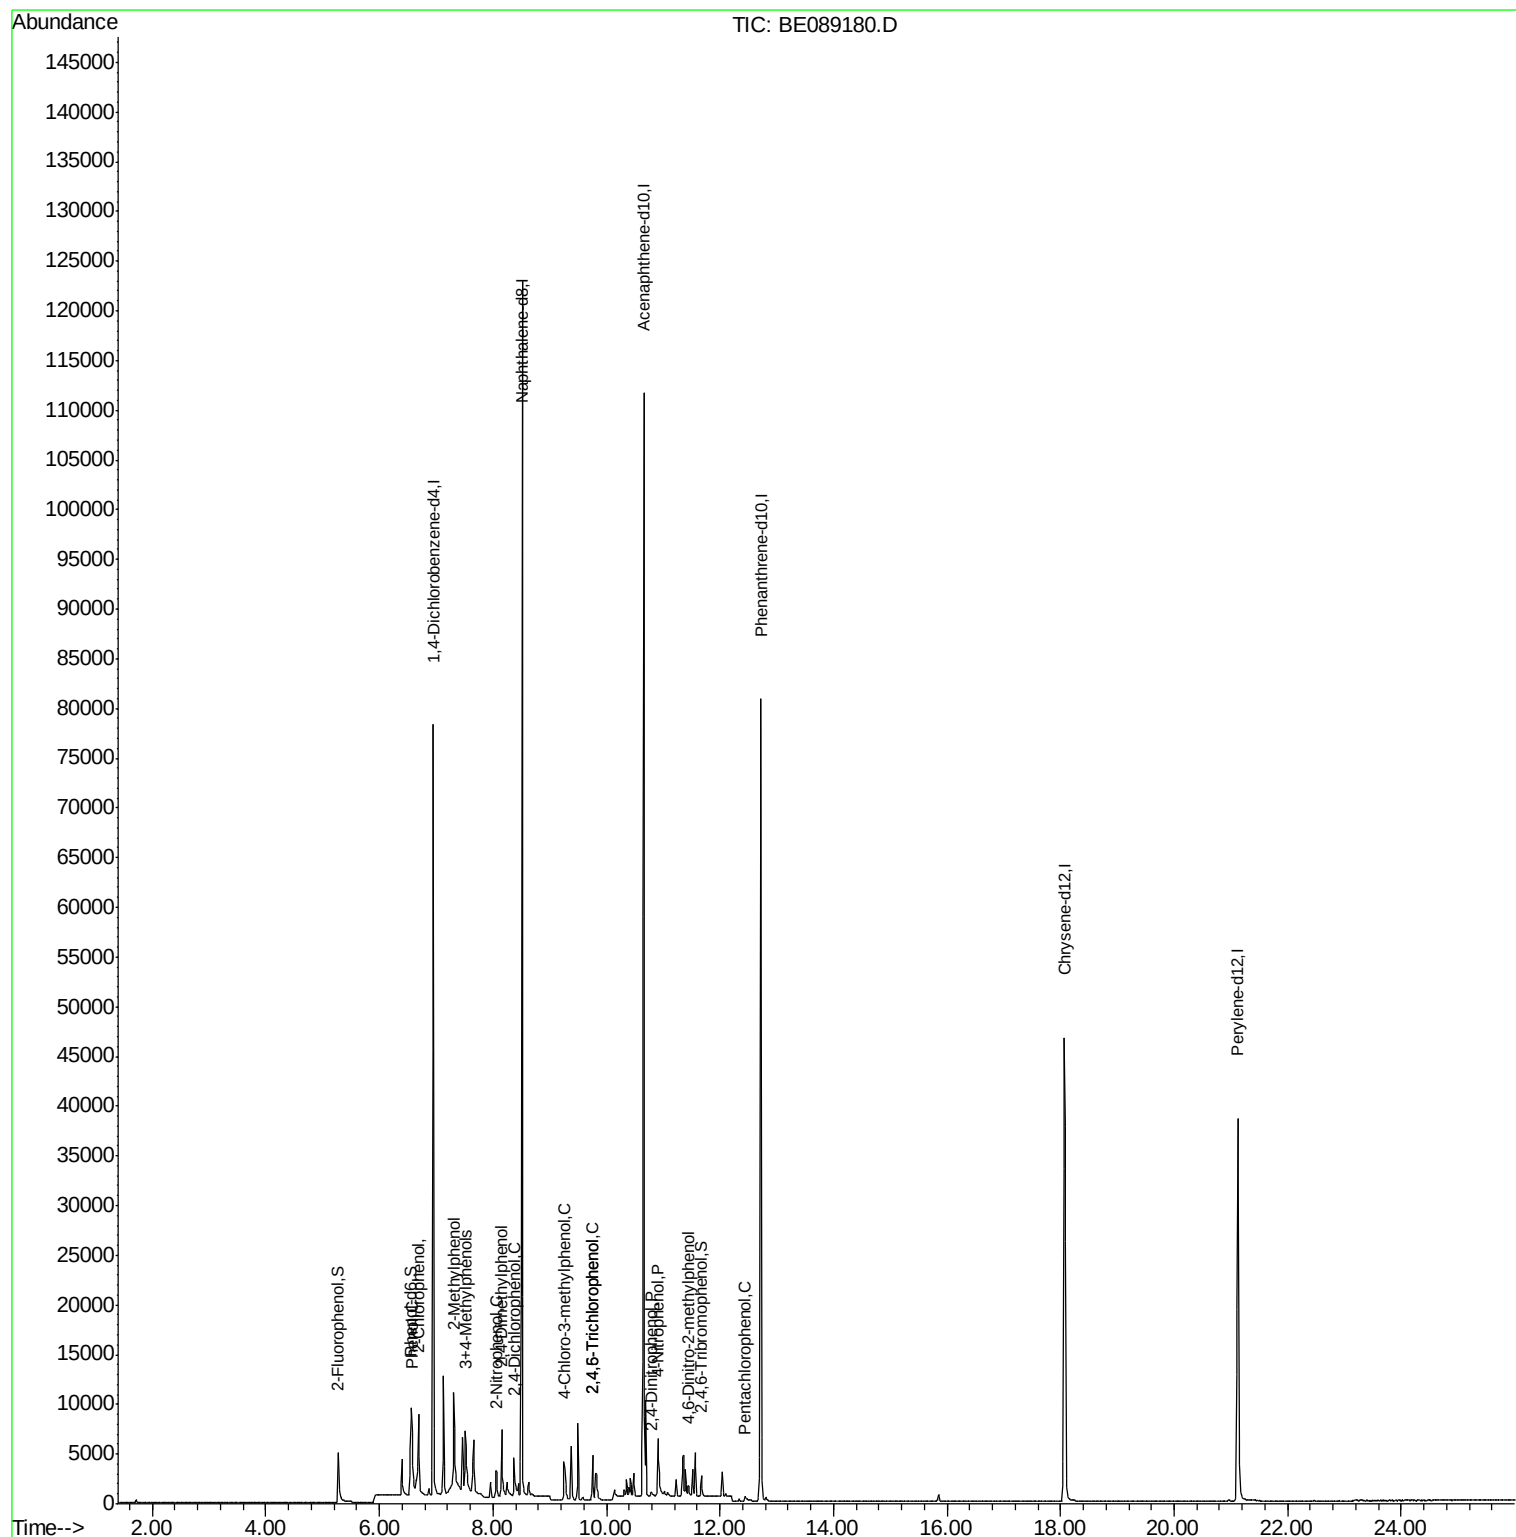



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 6.95 min Scan# 2025

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDIC0.8





Tgt Ion:152 Resp: 29077

Ion Ratio Lower Upper

152 100

150 148.1 115.4 173.2

115 45.2 33.3 49.9

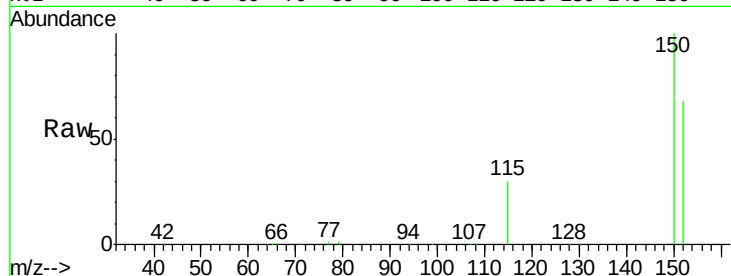

#2

2-Fluorophenol

Concen: 0.64 ng

RT: 5.28 min Scan# 1670

Delta R.T. 0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27




Tgt Ion:112 Resp: 4825


Ion Ratio Lower Upper

112 100

64 53.9 42.3 63.5

63 26.6 20.0 30.0



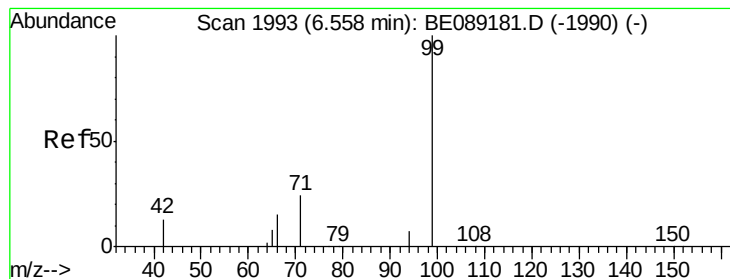

#3

Phenol-d6

Concen: 0.70 ng

RT: 6.56 min Scan# 1992

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDIC0.8


Tgt Ion: 99 Resp: 6760

Ion Ratio Lower Upper

99 100

42 19.6 11.2 16.8#




71 29.5 19.3 28.9#

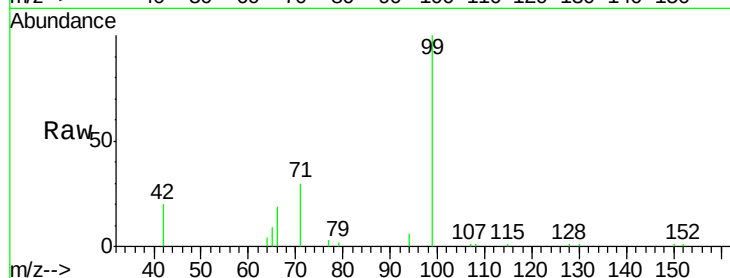

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

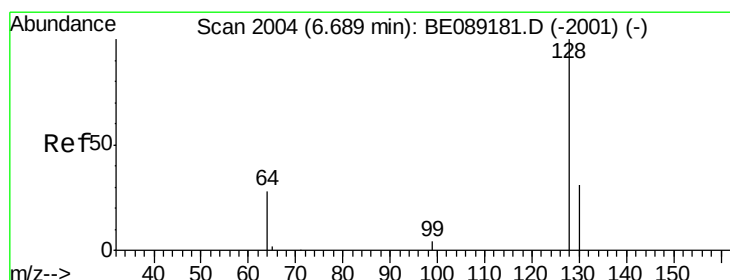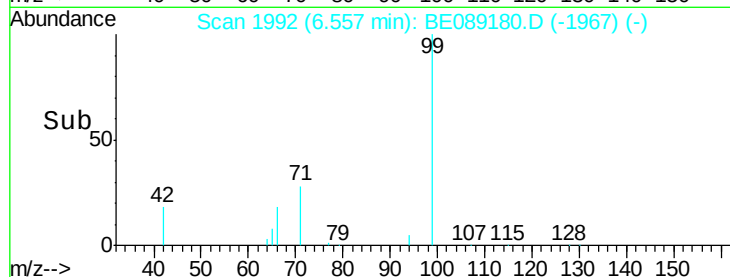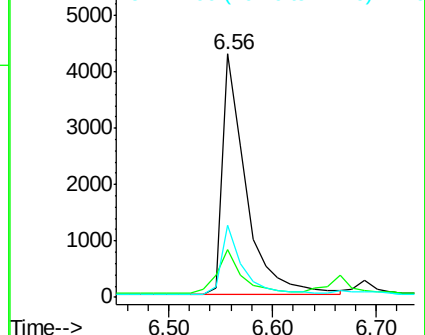

#4

2-Chlorophenol

Concen: 0.76 ng

RT: 6.69 min Scan# 2003

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27


Tgt Ion: 128 Resp: 5430

Ion Ratio Lower Upper

128 100

130 30.9 11.2 51.2



64 42.8 10.6 50.6

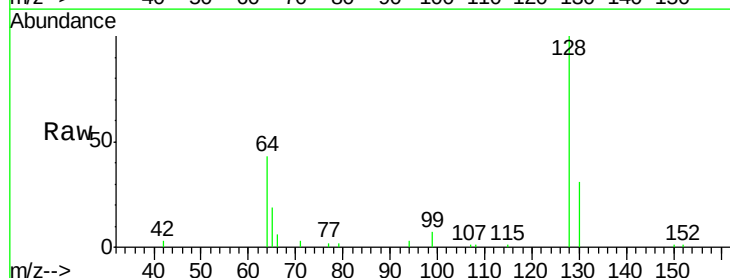


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 64.00 (63.70 to 64.70): BE0

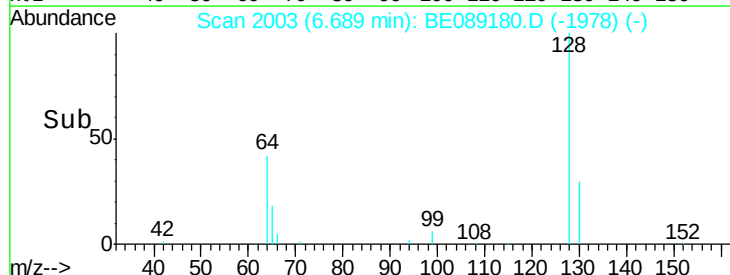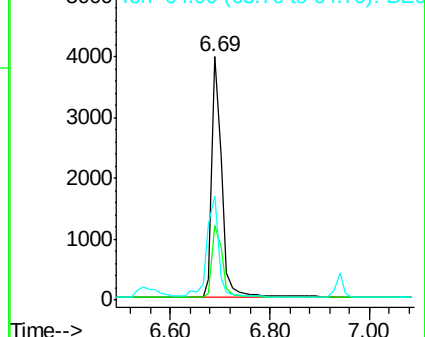

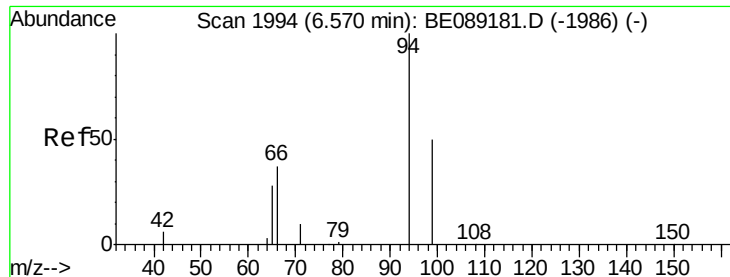

#5

Phenol

Concen: 0.76 ng

RT: 6.58 min Scan# 1994

Delta R.T. 0.01 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDIC0.8


Tgt Ion: 94 Resp: 7936

Ion Ratio Lower Upper

94 100

65 22.0 9.0 49.0




66 29.1 17.7 57.7

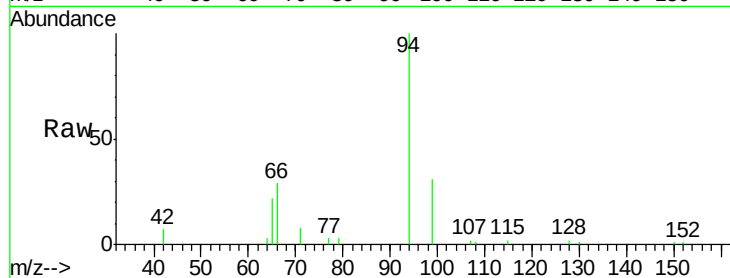

Abundance Ion 94.00 (93.70 to 94.70): BE0

Ion 65.00 (64.70 to 65.70): BE0

Ion 66.00 (65.70 to 66.70): BE0

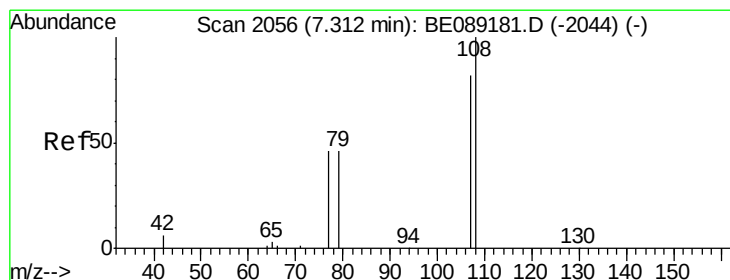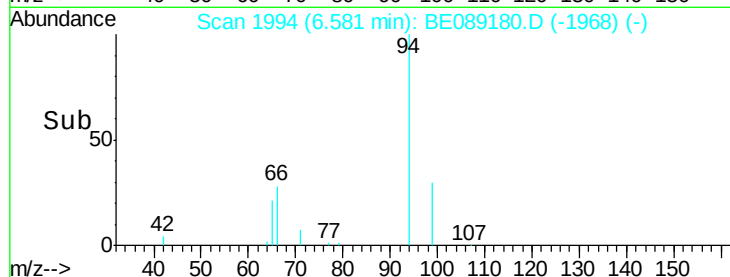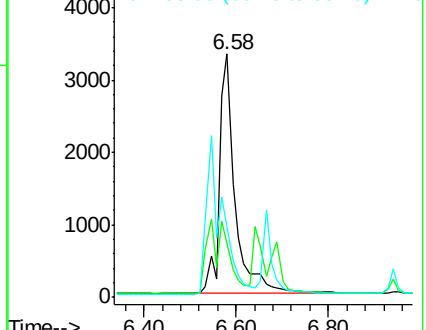

#6

2-Methylphenol

Concen: 0.33 ng

RT: 7.31 min Scan# 2055

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Tgt Ion: 107 Resp: 6479


Ion Ratio Lower Upper

107 100

108 120.6 97.6 146.4

77 63.4 45.8 68.6

79 63.9 46.1 69.1


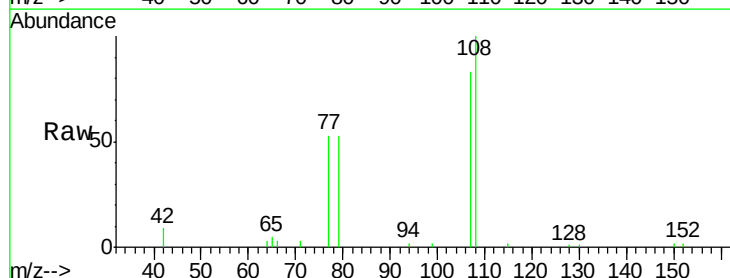



Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BE0

Ion 79.00 (78.70 to 79.70): BE0

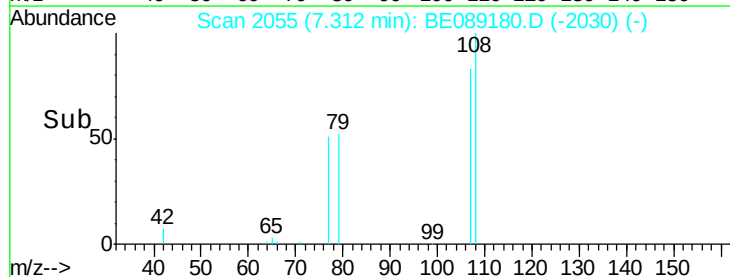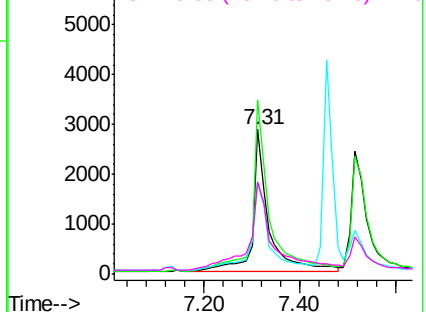

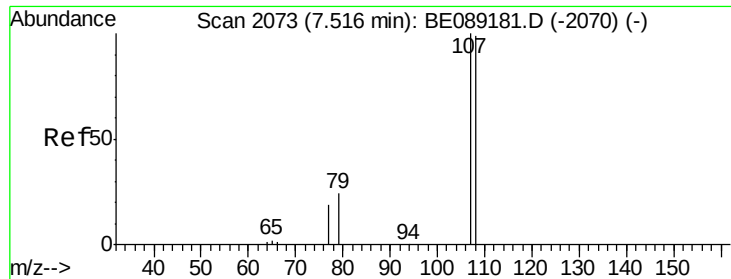

#7

3+4-Methylphenols

Concen: 0.22 ng

RT: 7.52 min Scan# 2072

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDICC0.8

Tgt Ion:107 Resp: 5308


Ion Ratio Lower Upper

107 100

108 95.4 80.4 120.4

77 35.6 12.4 52.4

79 30.2 8.3 48.3



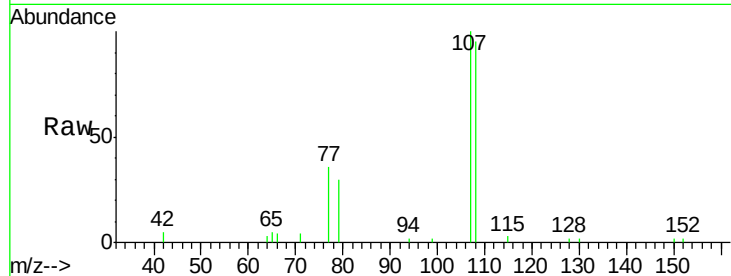


Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BE0

Ion 79.00 (78.70 to 79.70): BE0

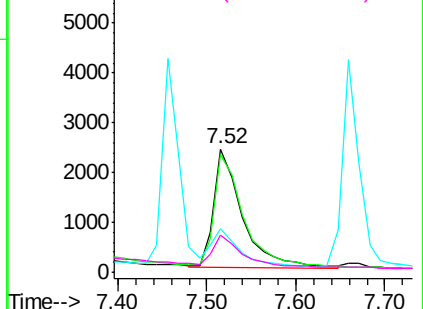

#8

Naphthalene-d8

Concen: 5.00 ng

RT: 8.51 min Scan# 2165

Delta R.T. 0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Tgt Ion:136 Resp: 110751


Ion Ratio Lower Upper

136 100

137 11.3 8.9 13.3

54 4.3 3.4 5.2

68 4.7 3.8 5.6






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

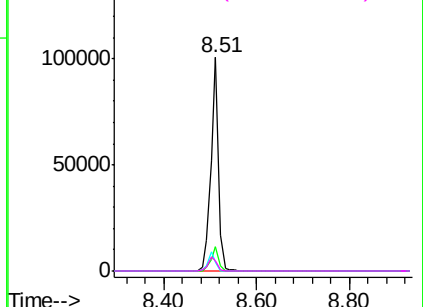

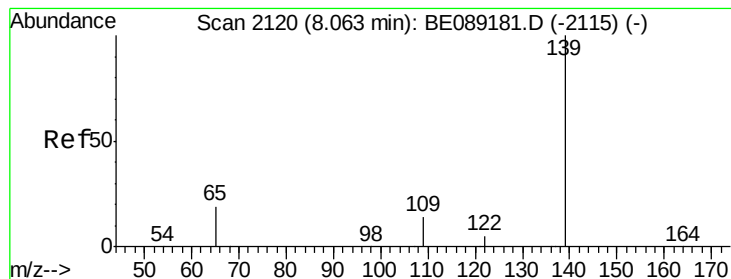

#9

2-Nitrophenol

Concen: 1.09 ng

RT: 8.06 min Scan# 2119

Delta R.T. 0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDIC0.8


Tgt Ion:139 Resp: 2781

Ion Ratio Lower Upper

139 100

109 18.5 13.0 19.4




65 23.0 16.4 24.6



Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): E

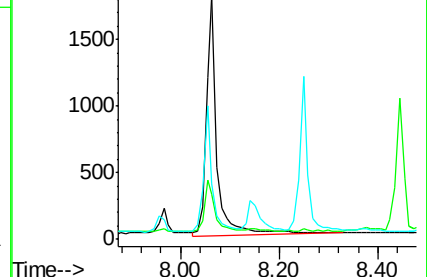

#10

2,4-Dimethylphenol

Concen: 0.77 ng

RT: 8.15 min Scan# 2128

Delta R.T. 0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27


Tgt Ion:122 Resp: 4606

Ion Ratio Lower Upper

122 100

107 96.5 74.3 111.5



121 52.4 41.5 62.3




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

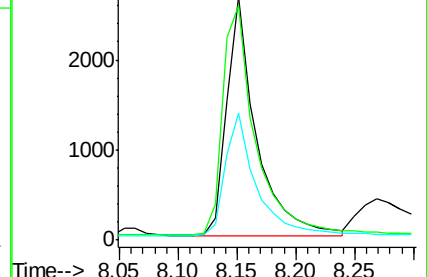


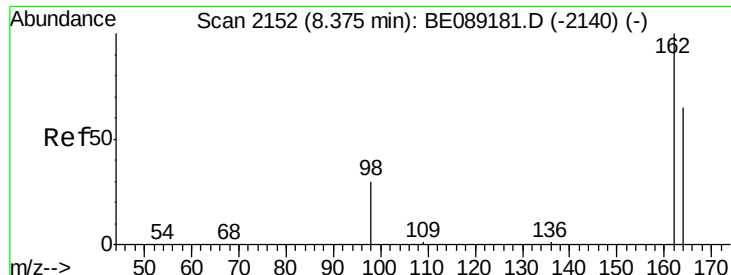




#11
 2,4-Dichlorophenol
 Concen: 0.80 ng
 RT: 8.38 min Scan# 2151
 Delta R.T. 0.00 min
 Lab File: BE089180.D
 Acq: 8 Dec 2014 23:27

Instrument :
 BNA_E
 LabSampleId :
 SSTDICC0.8

Tgt Ion	Ratio	Lower	Upper
162	100		
164	62.4	45.3	85.3
98	37.1	10.9	50.9

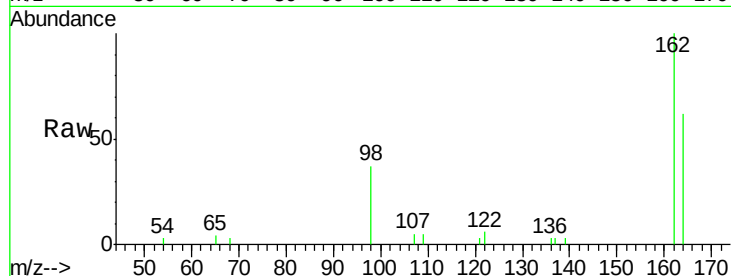


Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 98.00 (97.70 to 98.70): E

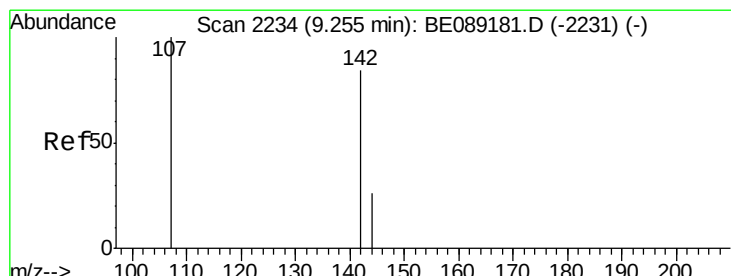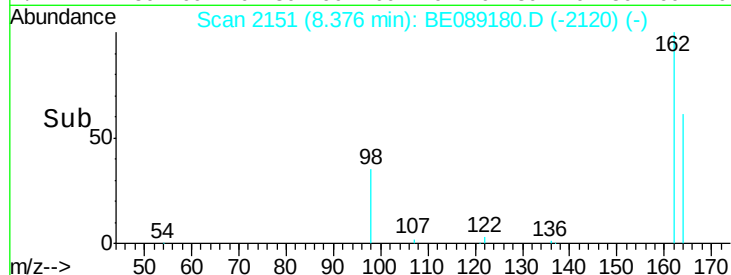
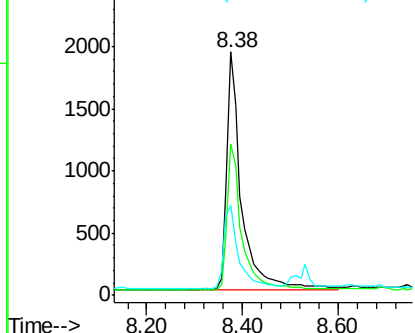



#12
 4-Chloro-3-methylphenol
 Concen: 0.75 ng
 RT: 9.25 min Scan# 2233
 Delta R.T. -0.00 min
 Lab File: BE089180.D
 Acq: 8 Dec 2014 23:27

Tgt Ion	Ratio	Lower	Upper
107	100		
144	23.7	21.3	31.9
142	77.9	66.7	100.1

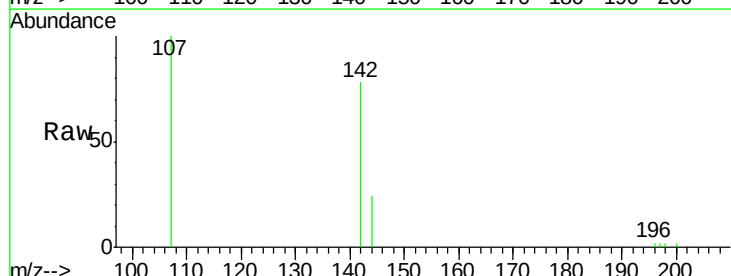

Abundance Ion 107.00 (106.70 to 107.70): E
 Ion 144.00 (143.70 to 144.70): E
 Ion 142.00 (141.70 to 142.70): E

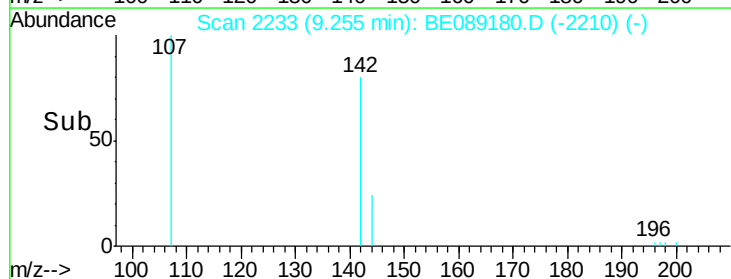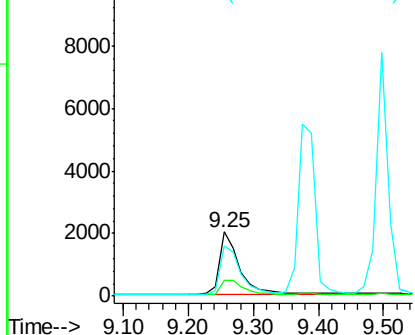



#13

Acenaphthene-d10

Concen: 5.00 ng

RT: 10.66 min Scan# 2342

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDIC0.8


Tgt Ion:164 Resp: 54913

Ion Ratio Lower Upper

164 100

162 87.2 68.0 102.0




160 37.3 28.2 42.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

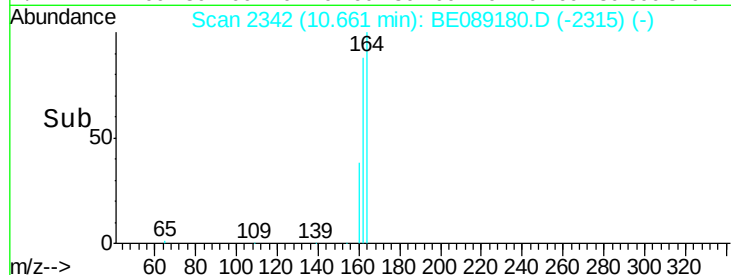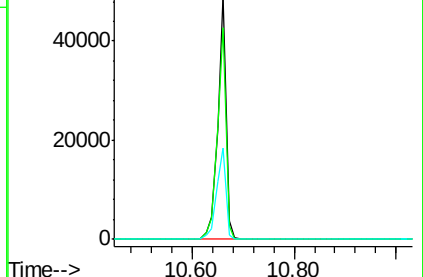

#14

2,4,6-Tribromophenol

Concen: 0.66 ng

RT: 11.67 min Scan# 2432

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27


Tgt Ion:330 Resp: 1191

Ion Ratio Lower Upper

330 100

332 97.2 76.8 115.2



141 35.1 28.4 42.6




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




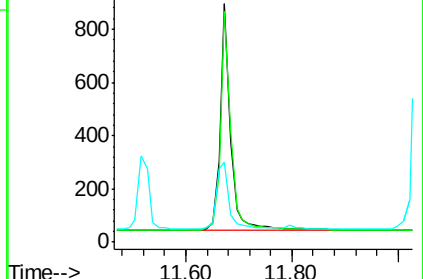


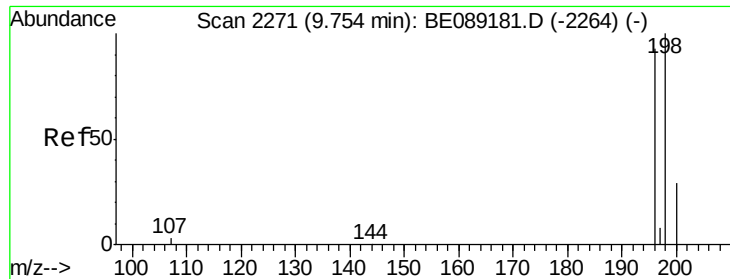

#15
2,4,6-Trichlorophenol
Concen: 0.72 ng
RT: 9.75 min Scan# 2270
Delta R.T. -0.00 min
Lab File: BE089180.D
Acq: 8 Dec 2014 23:27




Instrument :
BNA_E
LabSampleId :
SSTDIC0.8


Tgt Ion:196 Resp: 2416
Ion Ratio Lower Upper
196 100
198 87.4 85.6 128.4
200 23.8 25.4 38.2#

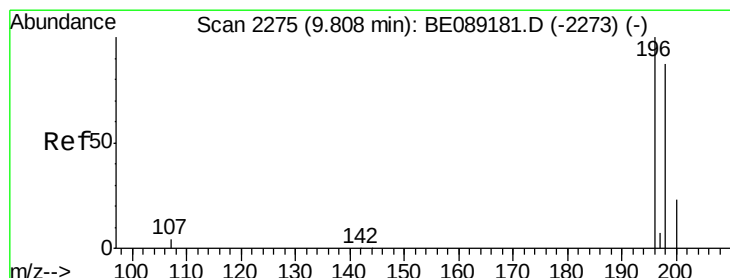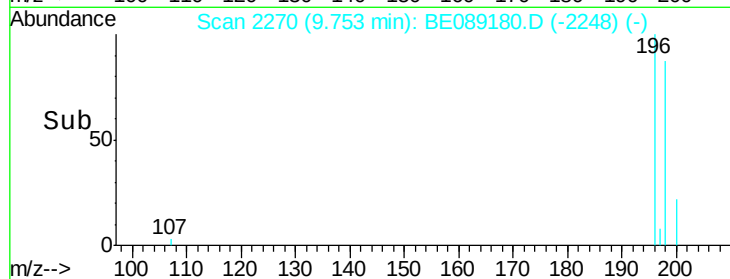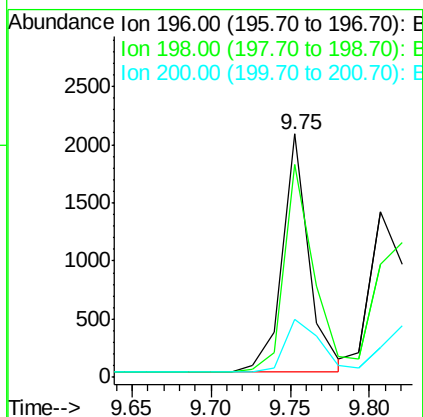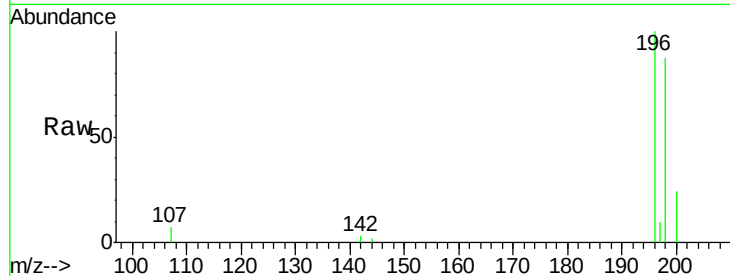

#16
2,4,5-Trichlorophenol
Concen: 0.69 ng
RT: 9.75 min Scan# 2270
Delta R.T. -0.05 min
Lab File: BE089180.D
Acq: 8 Dec 2014 23:27

Tgt Ion:196 Resp: 2416
Ion Ratio Lower Upper
196 100
198 87.4 70.8 106.2
97 0.0 0.0 0.0
132 0.0 0.0 0.0


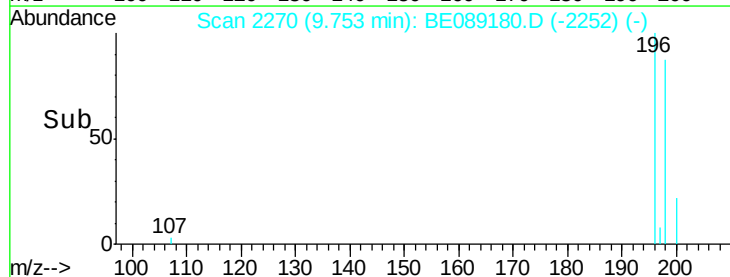
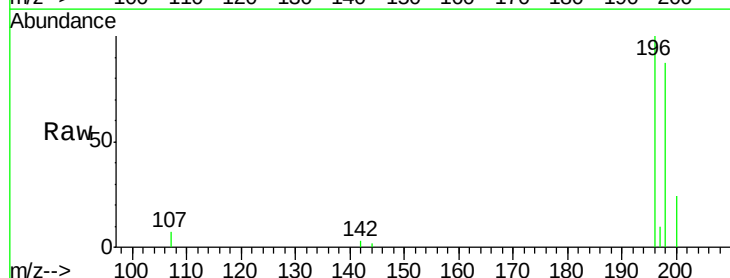
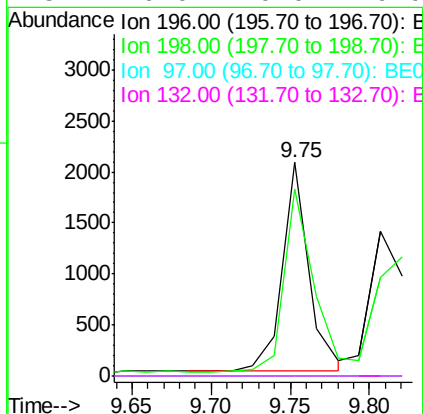


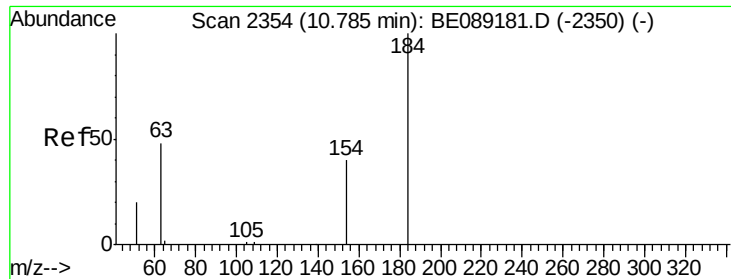

#17
2,4-Dinitrophenol
Concen: 1.36 ng
RT: 10.80 min Scan# 2354
Delta R.T. 0.01 min
Lab File: BE089180.D
Acq: 8 Dec 2014 23:27




Instrument :
BNA_E
LabSampleId :
SSTDIC0.8


Tgt Ion:184 Resp: 476
Ion Ratio Lower Upper
184 100
63 62.7 45.2 67.8
154 60.3 39.5 59.3#

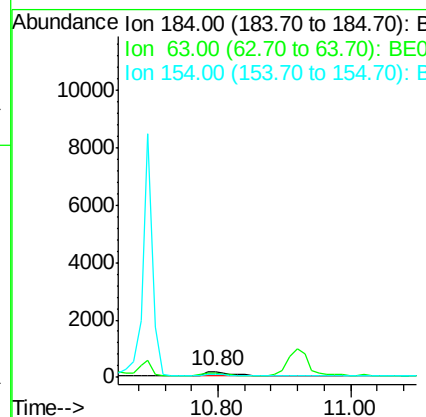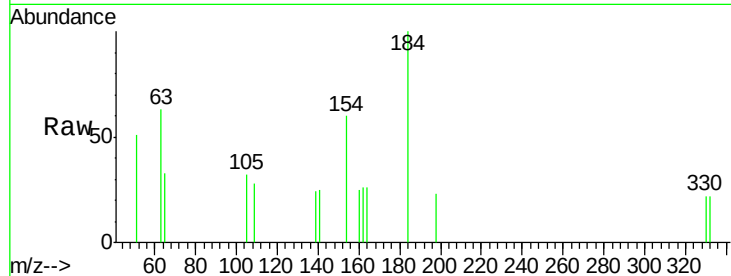

#18
4-Nitrophenol
Concen: 2.13 ng
RT: 10.91 min Scan# 2364
Delta R.T. -0.00 min
Lab File: BE089180.D
Acq: 8 Dec 2014 23:27

Tgt Ion:139 Resp: 5839
Ion Ratio Lower Upper
139 100
109 4.5 0.0 26.6
65 8.3 0.0 31.7

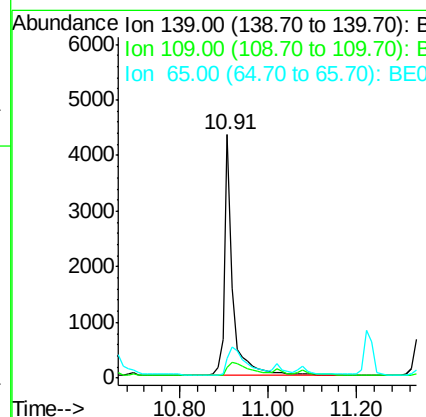

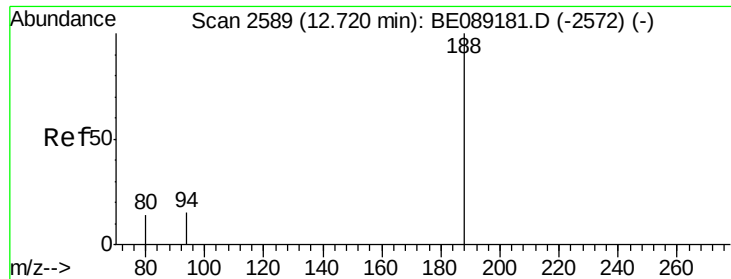

#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 12.72 min Scan# 2588

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDIC0.8


Tgt Ion:188 Resp: 82253

Ion Ratio Lower Upper

188 100

94 14.7 11.7 17.5




80 14.1 11.0 16.4



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

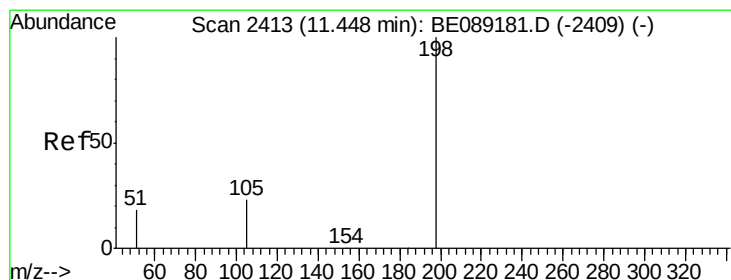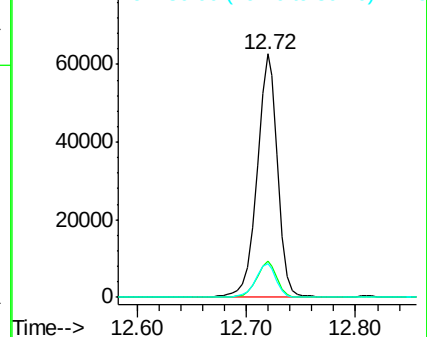

#20

4,6-Dinitro-2-methylphenol

Concen: 1.16 ng

RT: 11.45 min Scan# 2412

Delta R.T. -0.00 min

Lab File: BE089180.D

Acq: 8 Dec 2014 23:27


Tgt Ion:198 Resp: 800

Ion Ratio Lower Upper

198 100

51 37.3 10.8 50.8



105 37.3 10.4 50.4

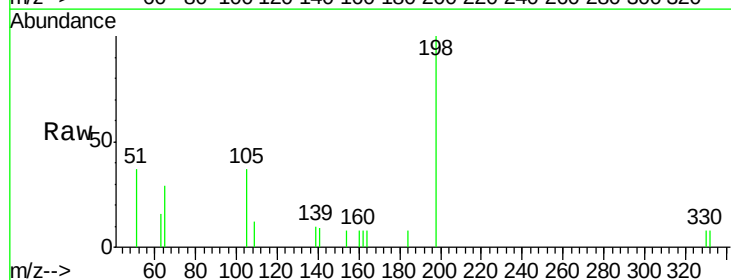


Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BE0

Ion 105.00 (104.70 to 105.70): E




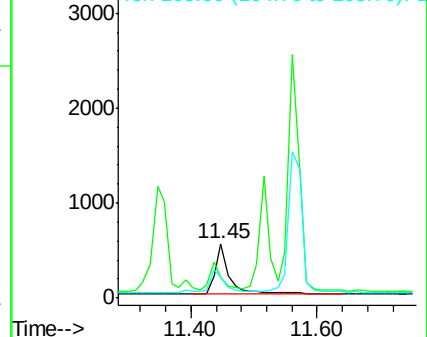


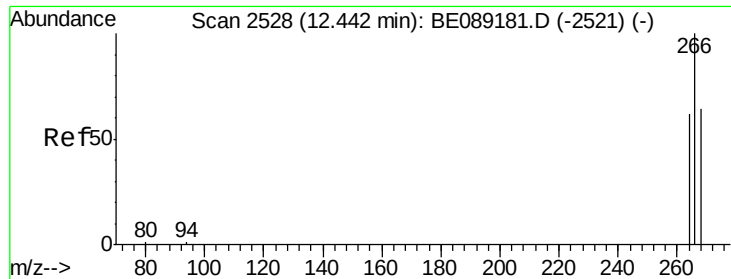

#21
 Pentachlorophenol
 Concen: 0.66 ng
 RT: 12.44 min Scan# 2527
 Delta R.T. -0.00 min
 Lab File: BE089180.D
 Acq: 8 Dec 2014 23:27




Instrument :
 BNA_E
 LabSampleId :
 SSTDICC0.8


Tgt Ion: 266 Resp: 634
 Ion Ratio Lower Upper
 266 100
 268 70.5 53.9 80.9
 264 70.1 52.6 78.8

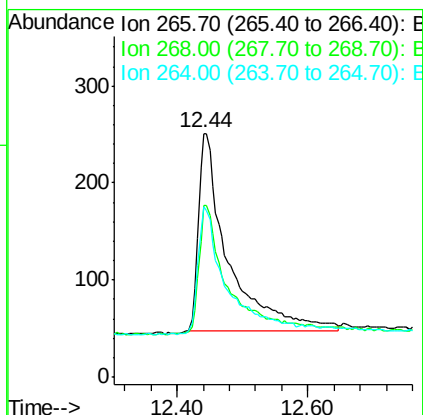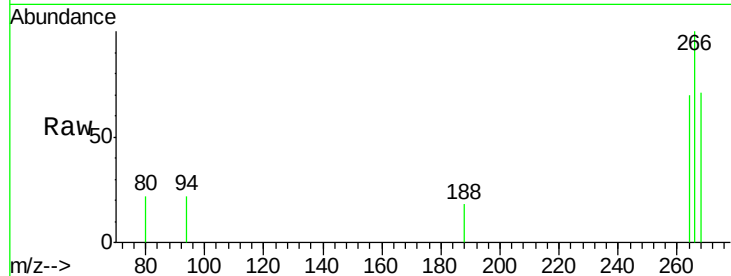

#22
 Chrysene-d12
 Concen: 5.00 ng
 RT: 18.08 min Scan# 3760
 Delta R.T. 0.00 min
 Lab File: BE089180.D
 Acq: 8 Dec 2014 23:27

Tgt Ion: 240 Resp: 60677
 Ion Ratio Lower Upper
 240 100
 120 19.9 15.8 23.8
 236 25.2 20.2 30.4

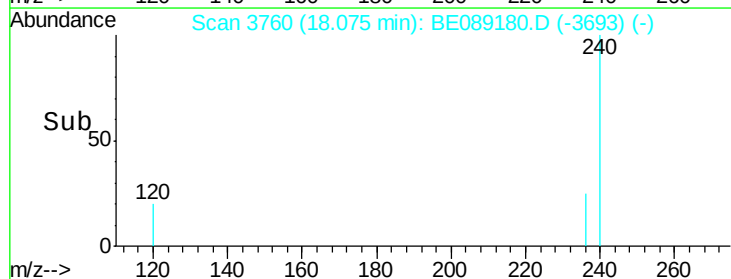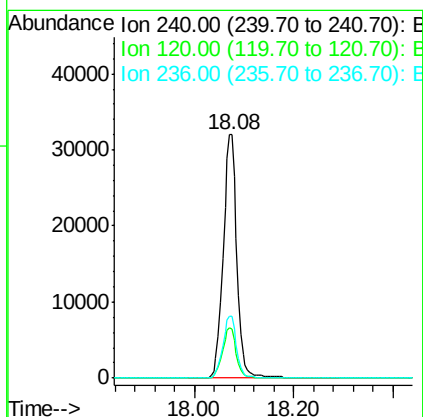

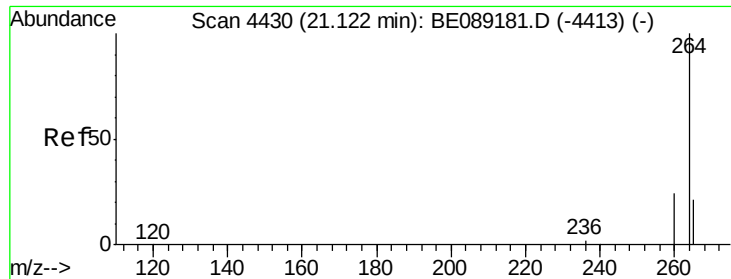

#23

Perylene-d12

Concen: 5.00 ng

RT: 21.12 min Scan# 4429

Delta R.T. -0.00 min

Lab File: BE089180.D


Acq: 8 Dec 2014 23:27

Instrument :

BNA_E

LabSampleId :

SSTDIC0.8



Tgt Ion: 264 Resp: 54853

Ion Ratio Lower Upper

264 100

260 23.9 19.0 28.4

265 21.6 17.2 25.8

