




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
Data File : BE089174.D
Acq On : 8 Dec 2014 14:37
Operator : TP/JJ
Sample : PB80725BL
Misc : SBLK64
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

mohammad
12/10/2014 4:24:05 PM

Quant Time: Dec 09 00:42:17 2014
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 09 00:37:23 2014
Response via : Initial Calibration

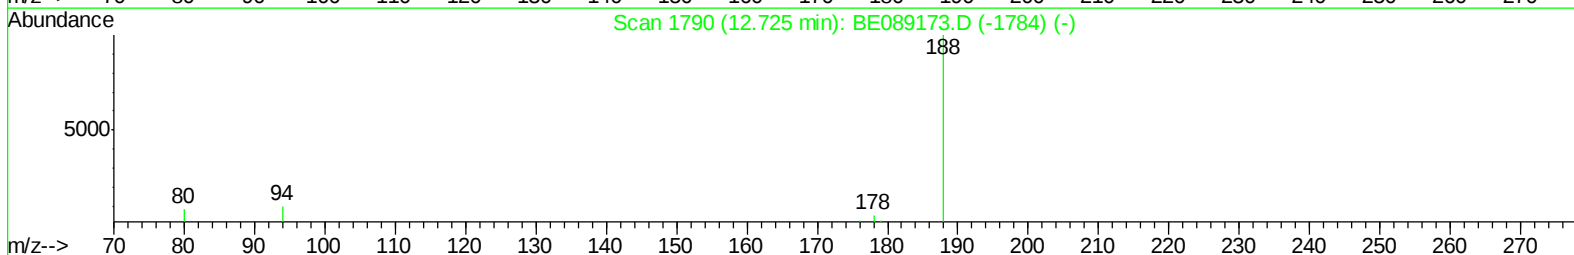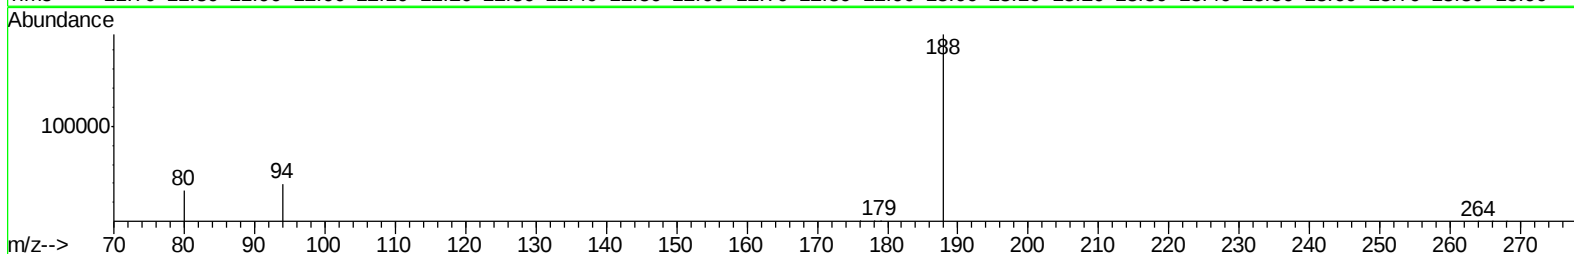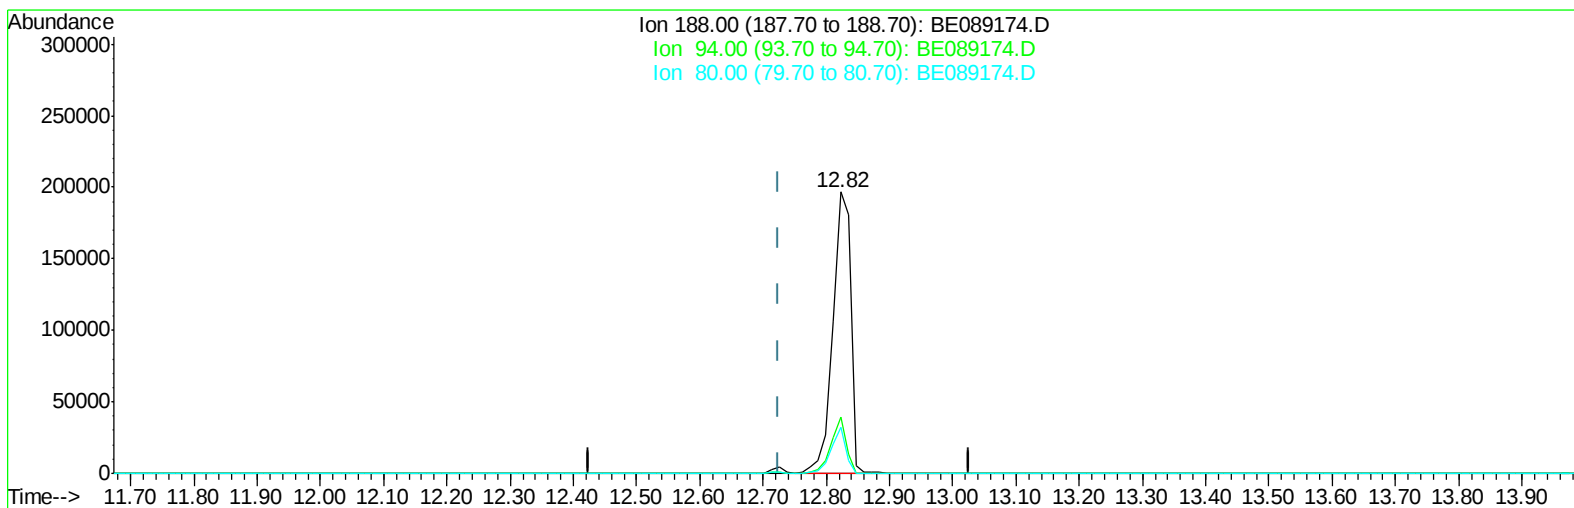

TIC: BE089174.D

(10) Phenanthrene-d10 (I)

12.823min (+0.097) 0.40ng/ul

response 388304

Ion	Exp%	Act%
188.00	100	100
94.00	10.20	20.19#
80.00	9.00	16.41#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
Data File : BE089174.D
Acq On : 8 Dec 2014 14:37
Operator : TP/JJ
Sample : PB80725BL
Misc : SBLK64
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

mohammad
12/10/2014 4:24:05 PM

Quant Time: Dec 09 00:42:17 2014
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 09 00:37:23 2014
Response via : Initial Calibration

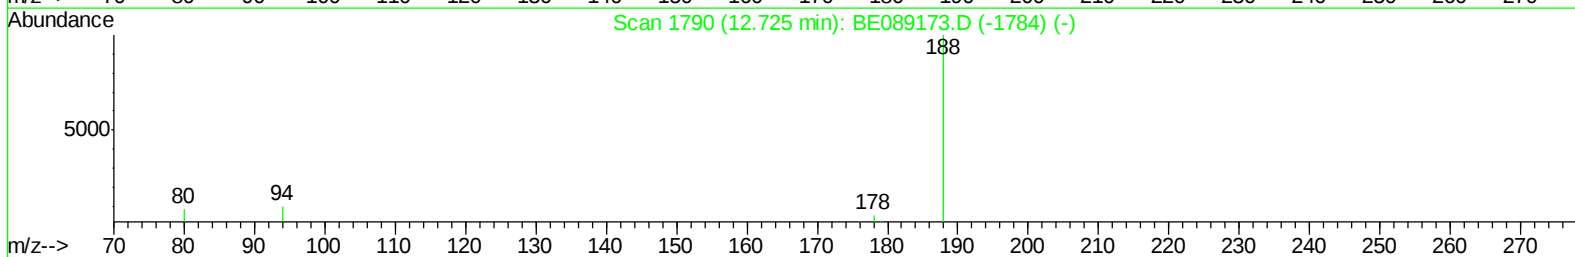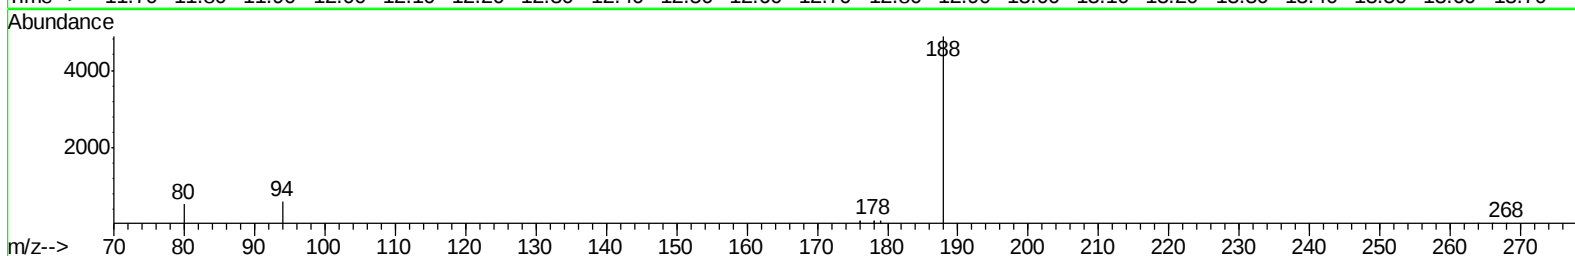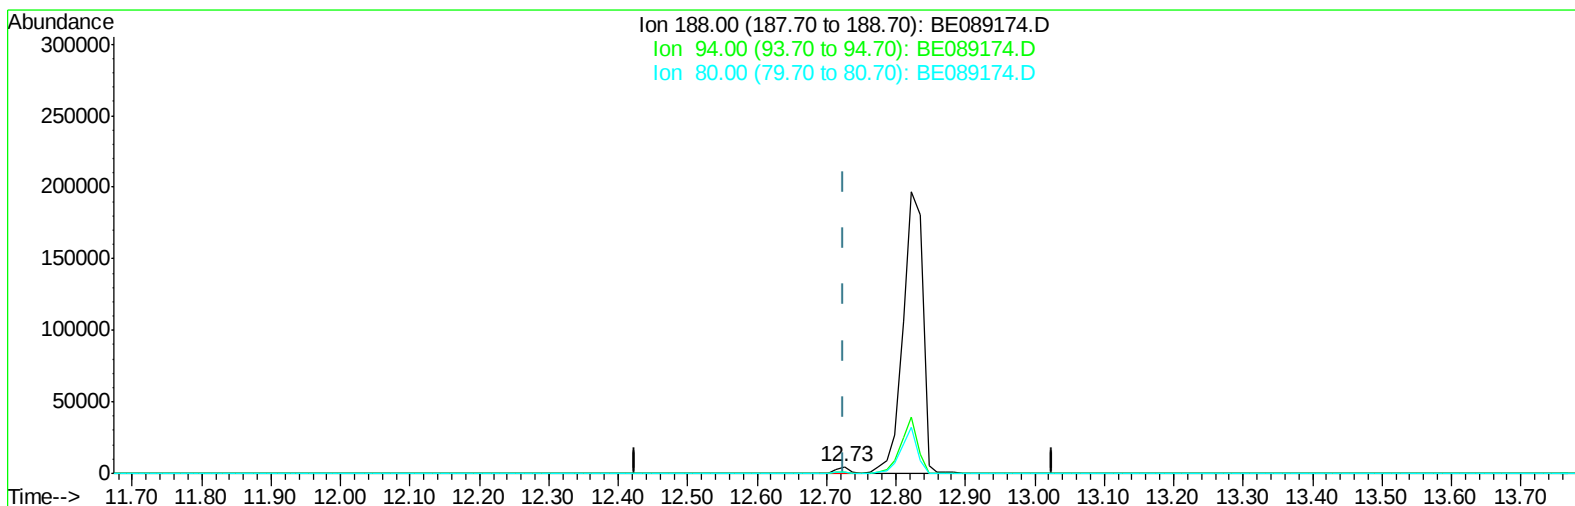

TIC: BE089174.D

(10) Phenanthrene-d10 (I)

12.726min (+0.000) 0.40ng/ul m

response 6638

Ion	Exp%	Act%
188.00	100	100
94.00	10.20	12.36#
80.00	9.00	10.92#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
 Data File : BE089174.D
 Acq On : 8 Dec 2014 14:37
 Operator : TP/JJ
 Sample : PB80725BL
 Misc : SBLK64
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK64

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:24:05 PM

Quant Time: Dec 09 00:42:17 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 09 00:37:23 2014
 Response via : Initial Calibration

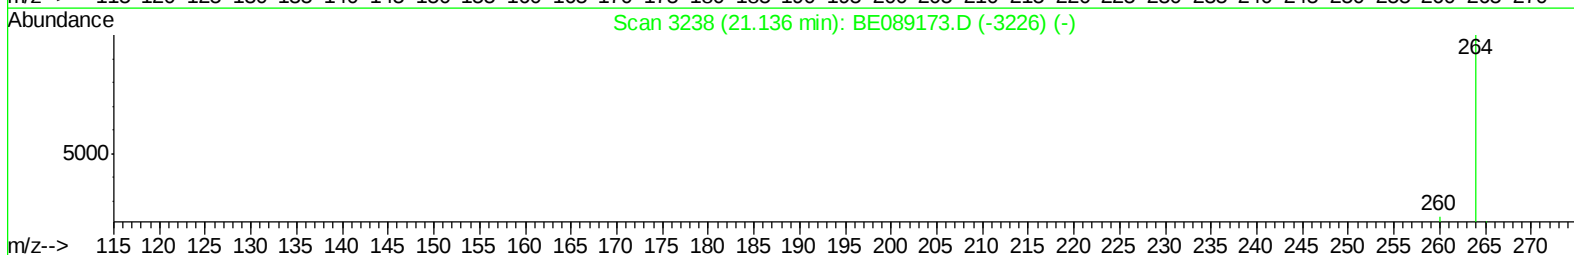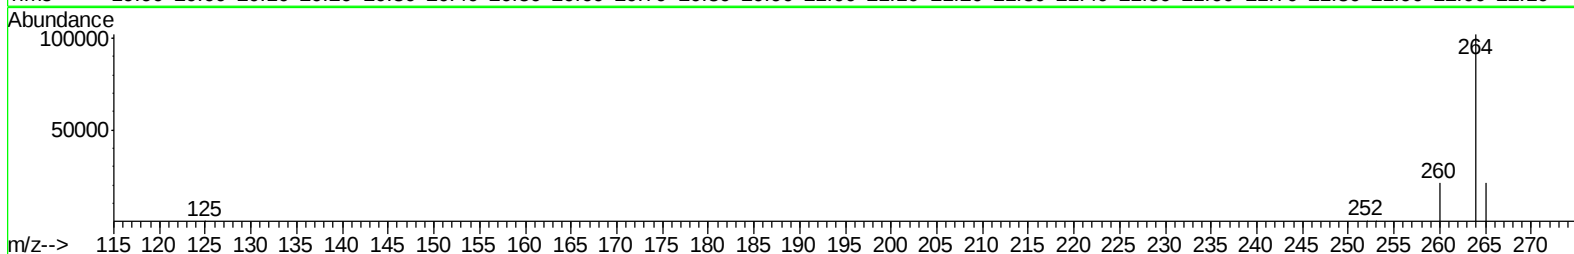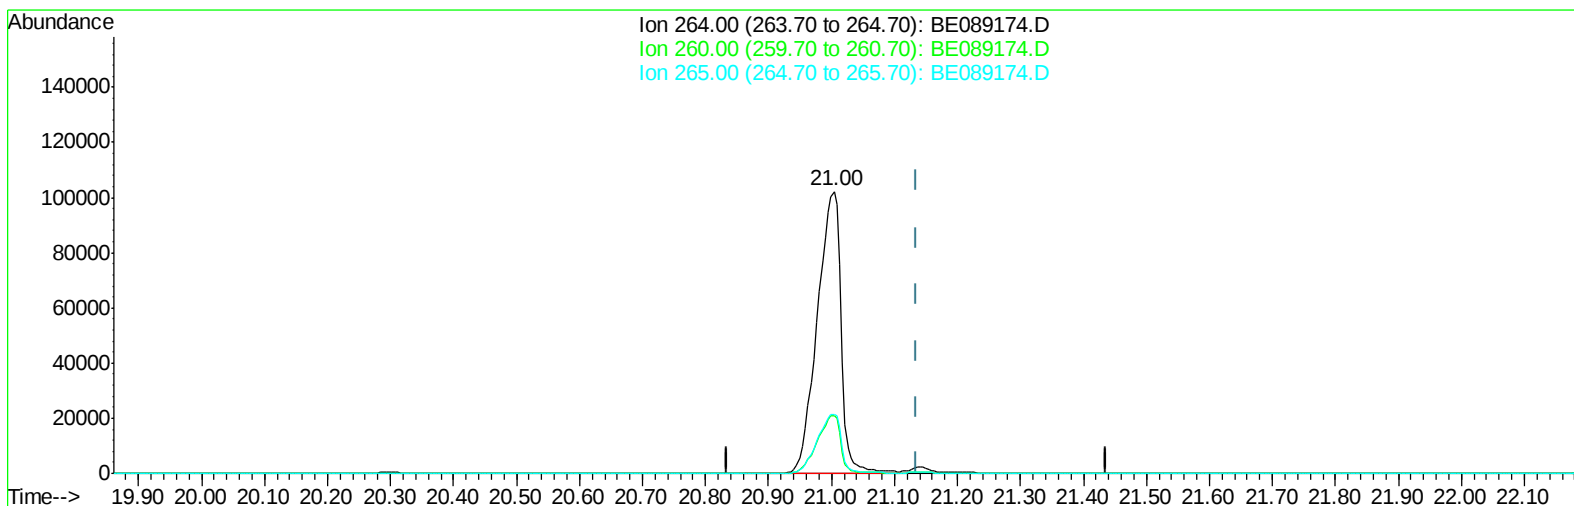

TIC: BE089174.D

(20) Perylene-d12 (I)

21.004min (-0.132) 0.40ng/ul

response 269086

Ion	Exp%	Act%
264.00	100	100
260.00	24.70	20.52
265.00	23.40	21.04
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
Data File : BE089174.D
Acq On : 8 Dec 2014 14:37
Operator : TP/JJ
Sample : PB80725BL
Misc : SBLK64
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

mohammad
12/10/2014 4:24:05 PM

Quant Time: Dec 09 00:42:17 2014
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 09 00:37:23 2014
Response via : Initial Calibration

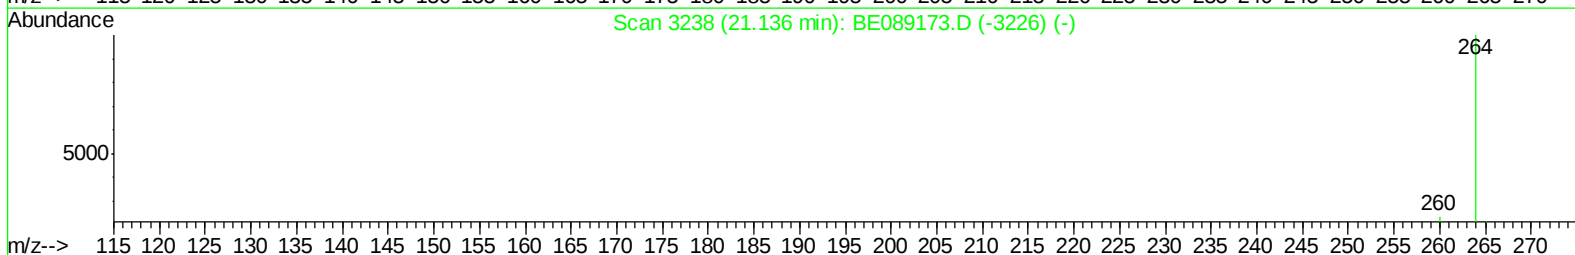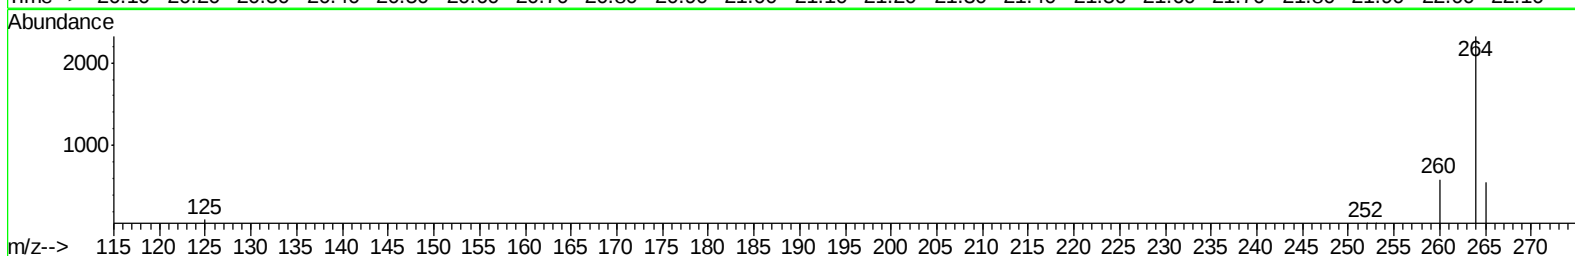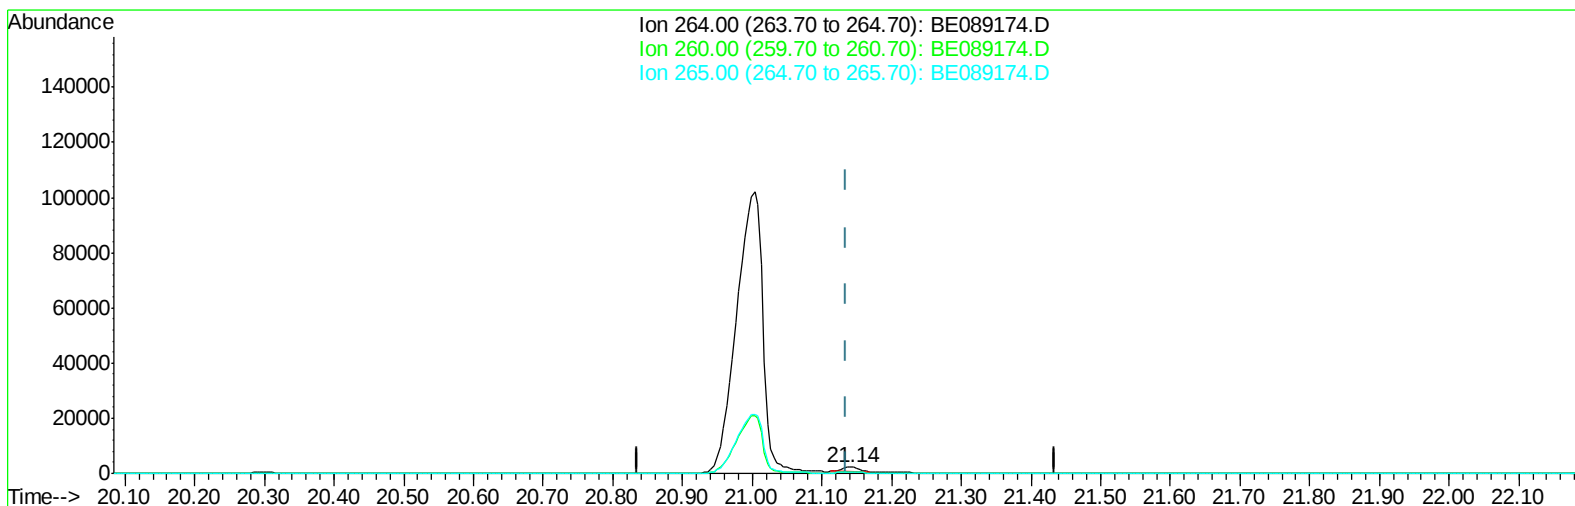

TIC: BE089174.D

(20) Perylene-d12 (I)

21.140min (+0.005) 0.40ng/ul m

response 2866

Ion	Exp%	Act%
264.00	100	100
260.00	24.70	25.32
265.00	23.40	24.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
 Data File : BE089174.D
 Acq On : 8 Dec 2014 14:37
 Operator : TP/JJ
 Sample : PB80725BL
 Misc : SBLK64
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK64

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:24:05 PM

Quant Time: Dec 09 00:44:34 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 09 00:37:23 2014
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	2190	0.40	ng/ul	0.00
2) Naphthalene-d8	8.51	136	8699	0.40	ng/ul	0.00
6) Acenaphthene-d10	10.67	164	4535	0.40	ng/ul	0.00
10) Phenanthrene-d10	12.73	188	6638m	0.40	ng/ul	0.00
16) Chrysene-d12	18.09	240	4562	0.40	ng/ul	0.00
20) Perylene-d12	21.14	264	2866m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	9.36	152	4681	0.46	ng/ul	0.00
14) Fluoranthene-d10	14.93	212	5300	0.45	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120814\
Data File : BE089174.D
Acq On : 8 Dec 2014 14:37
Operator : TP/JJ
Sample : PB80725BL
Misc : SBLK64
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

mohammad
12/10/2014 4:24:05 PM

Quant Time: Dec 09 00:44:34 2014
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 09 00:37:23 2014
Response via : Initial Calibration

