


Data Path : Z:\HPCHEM1\BNA_E\Data\BE120814\
 Data File : BE089176.D
 Acq On : 8 Dec 2014 21:12
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 05 23:47:26 2014

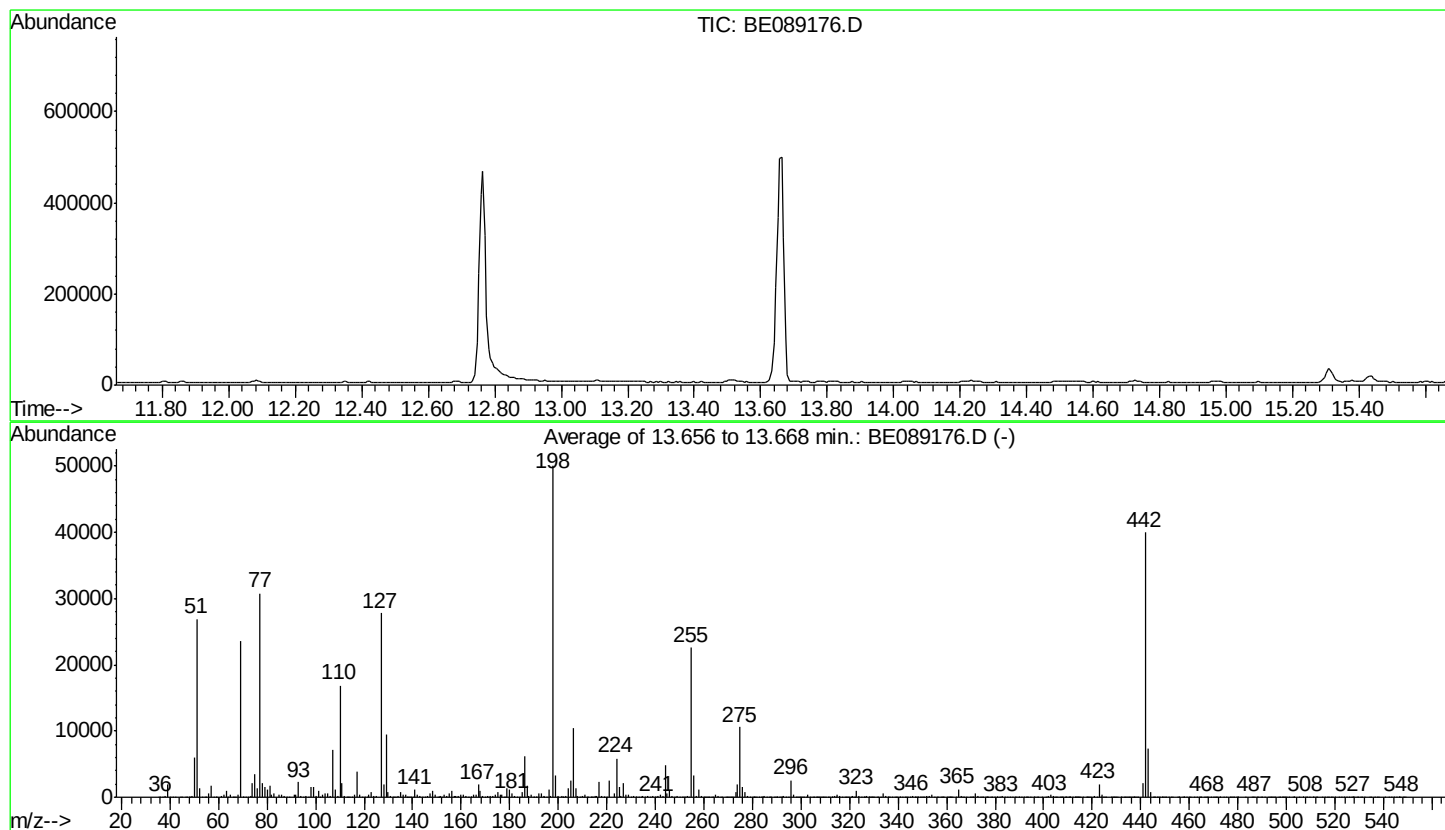

AutoFind: Scans 2088, 2089, 2090; Background Corrected with Scan 2073

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	26950	PASS
68	69	0.00	2	1.4	337	PASS
69	198	0.00	100	47.2	23631	PASS
70	69	0.00	2	0.3	64	PASS
127	198	10	80	55.5	27800	PASS
197	198	0.00	1	0.2	109	PASS
198	198	100	100	100.0	50058	PASS
199	198	5	9	6.5	3274	PASS
275	198	10	60	21.1	10571	PASS
365	198	1	100	2.5	1229	PASS
441	443	0.01	100	27.9	2064	PASS
442	198	50	100	79.8	39935	PASS
443	442	15	24	18.5	7407	PASS