
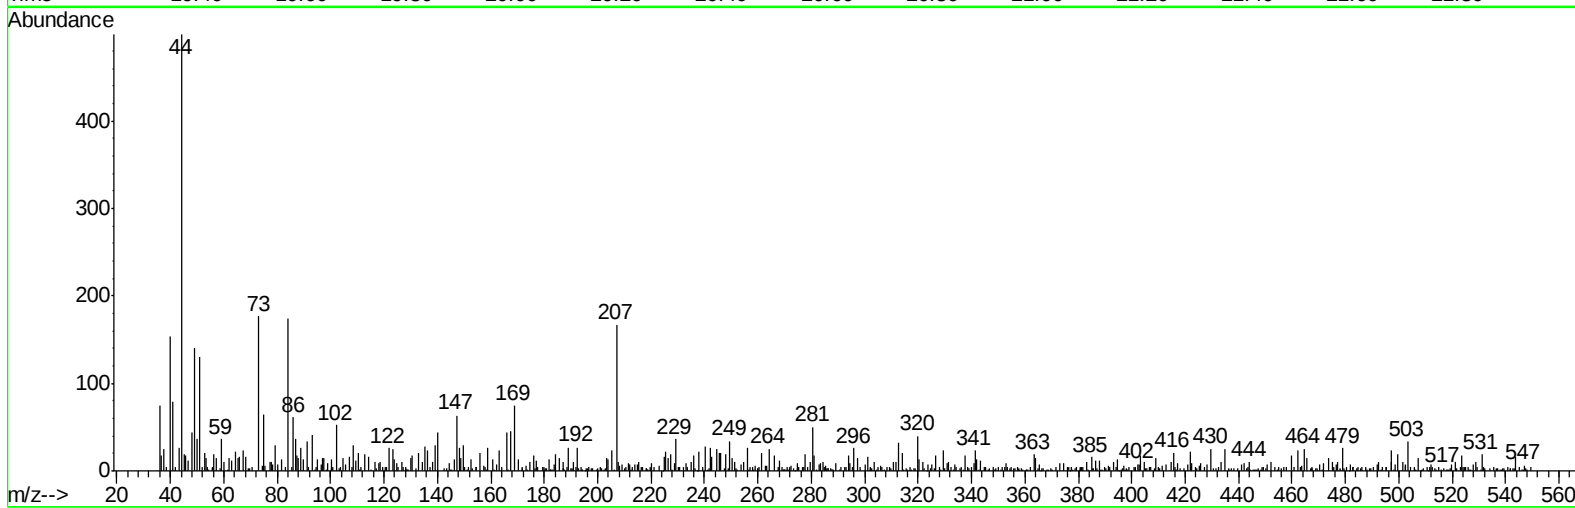


Data Path : Z:\HPCHEM1\BNA E\DATA\BE120817\
Data File : BE094963.D
Acq On : 8 Dec 2017 23:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 06:07:16 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 08 18:17:31 2017
Response via : Initial Calibration

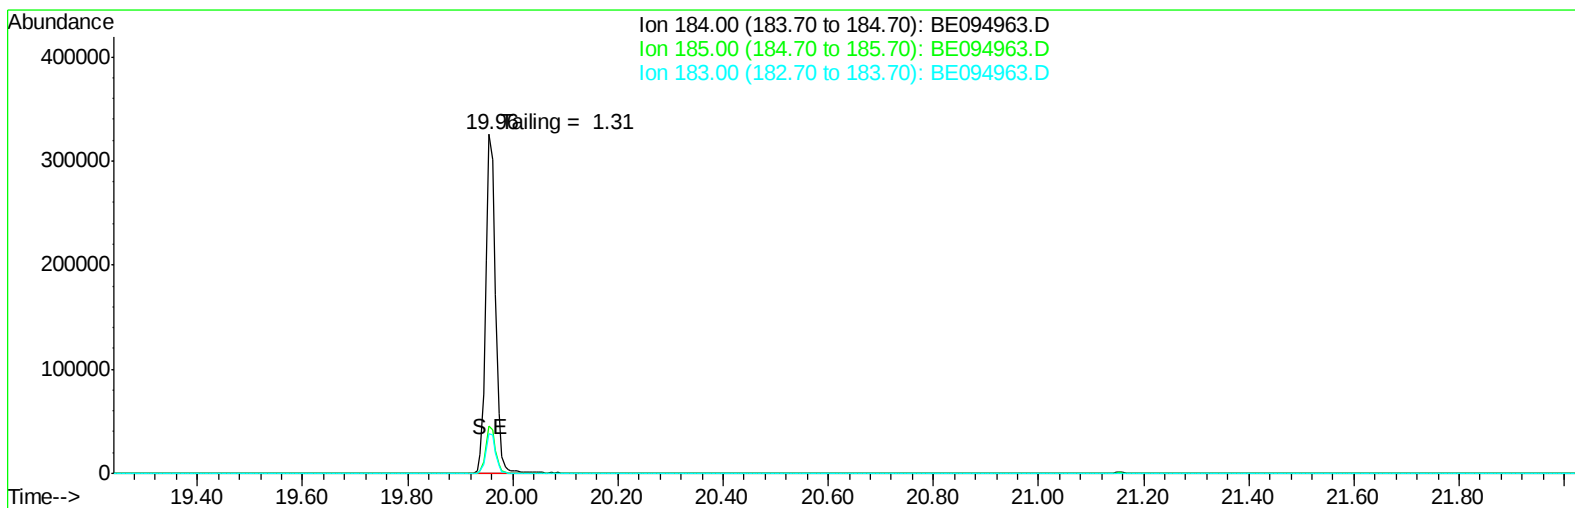

TIC: BE094963.D

(76) Benzidine



12.494min (-0.198) 21.04ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	57.69#
183.00	11.60	30.77#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE120817\
Data File : BE094963.D
Acq On : 8 Dec 2017 23:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 06:07:16 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 08 18:17:31 2017
Response via : Initial Calibration

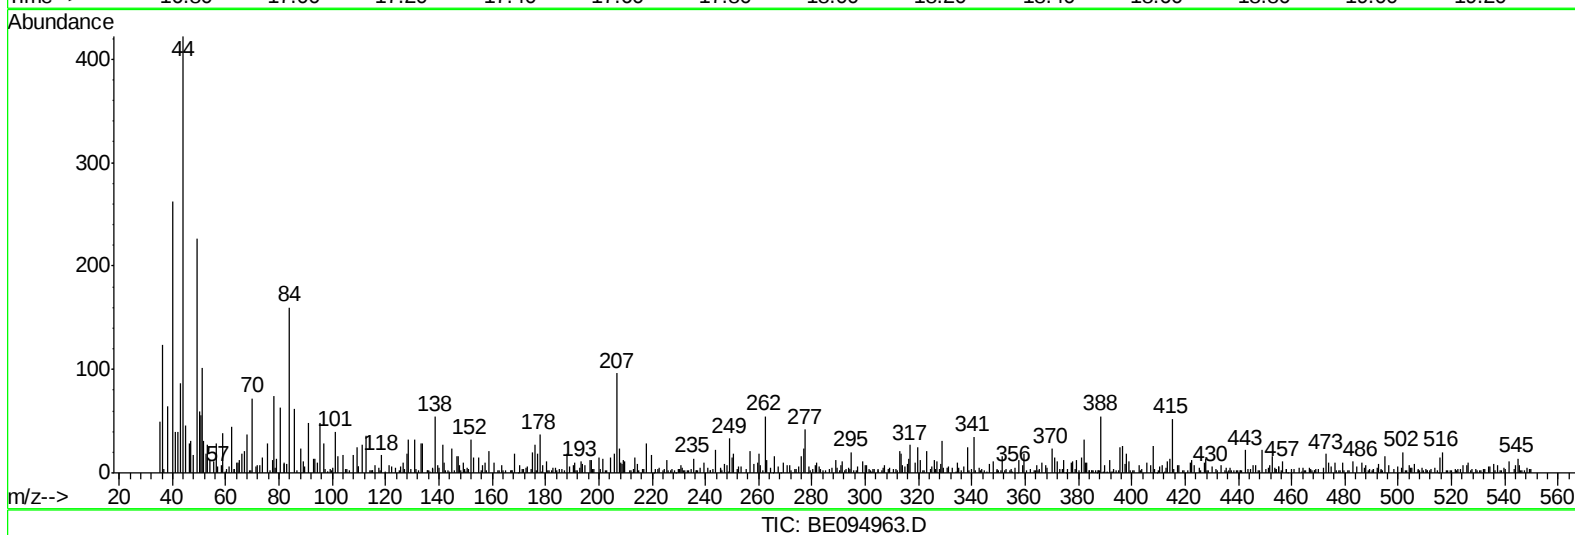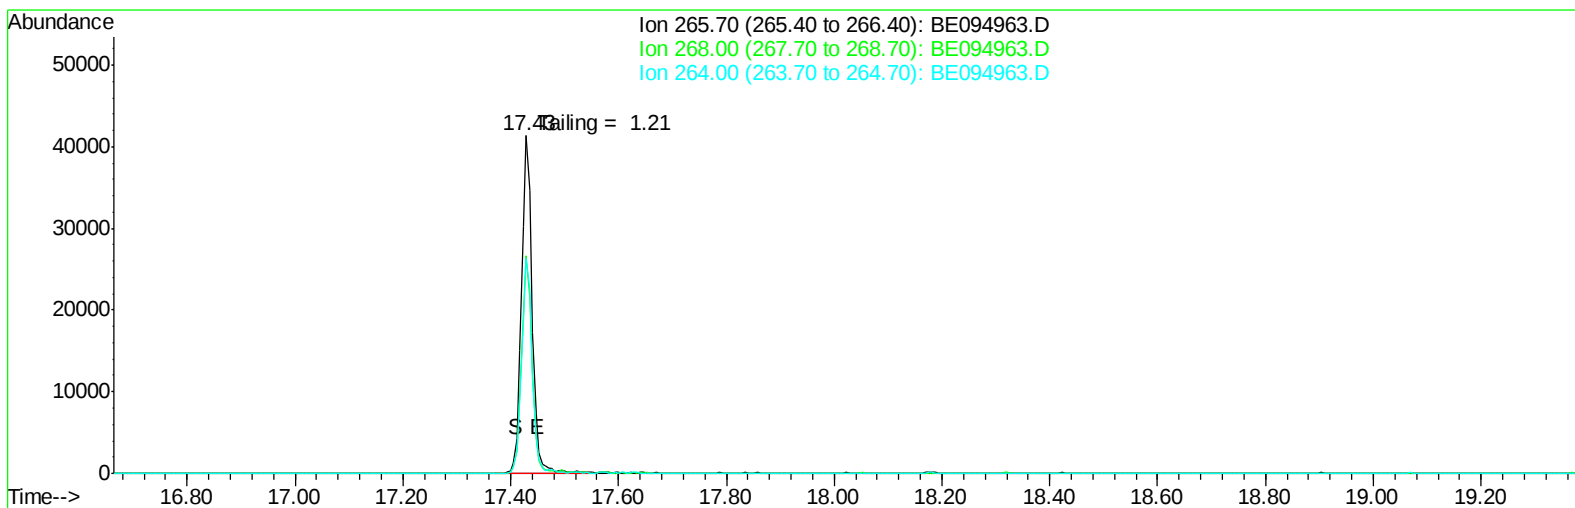

(69) Pentachlorophenol (C)
10.966min (-0.197) 303.21ng
response 14

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	0.00#
264.00	61.90	31.25#
0.00	0.00	0.00