


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE120817\
Data File : BE094949.D
Acq On : 8 Dec 2017 13:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE113017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 01 13:33:28 2017

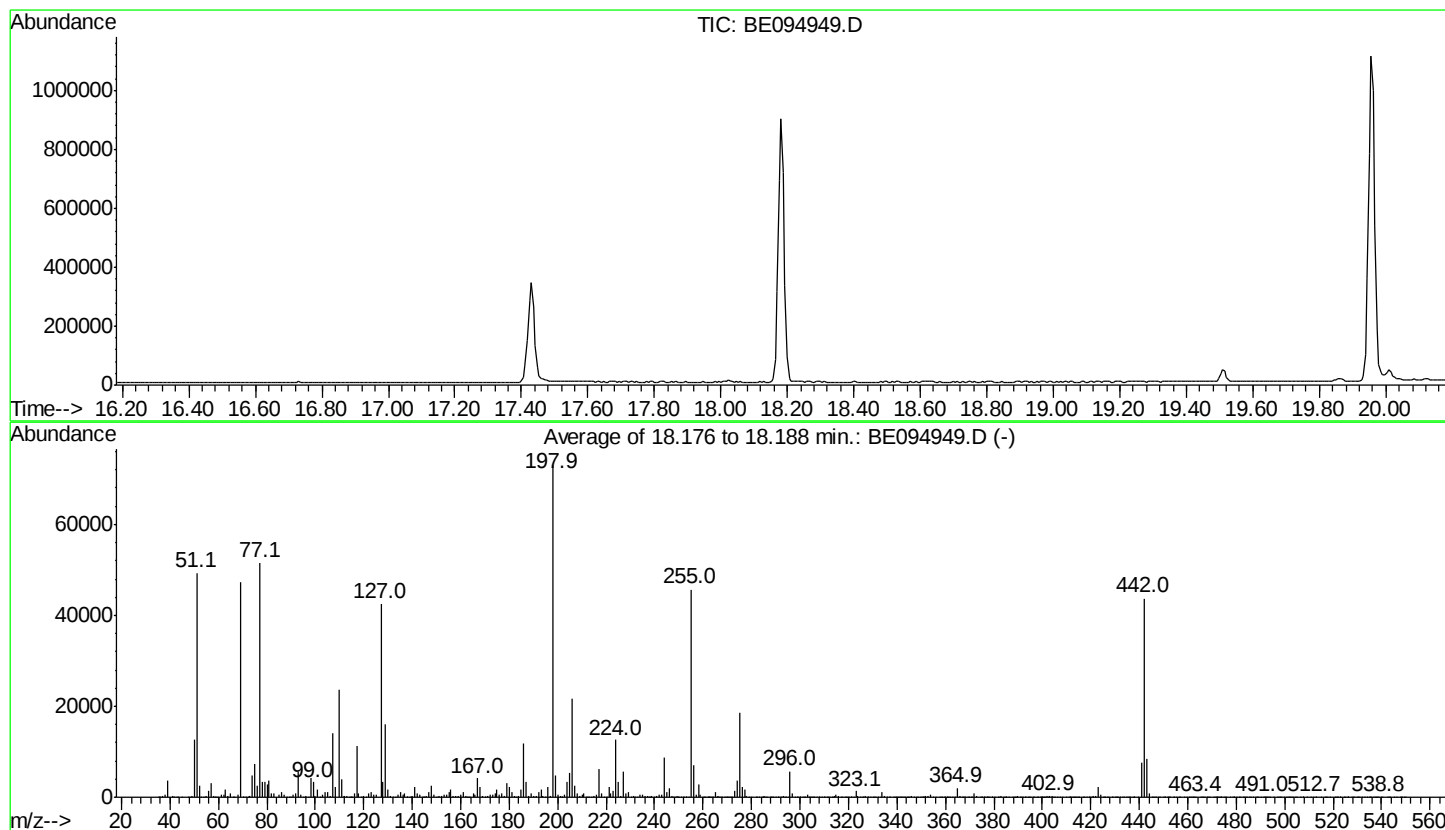

AutoFind: Scans 2653, 2654, 2655; Background Corrected with Scan 2643

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.7	49369	PASS
68	69	0.00	2	1.4	647	PASS
69	198	0.00	100	64.9	47296	PASS
70	69	0.00	2	0.3	141	PASS
127	198	10	80	58.4	42599	PASS
197	198	0.00	2	0.2	152	PASS
198	198	100	100	100.0	72924	PASS
199	198	5	9	6.7	4908	PASS
275	198	10	60	25.4	18543	PASS
365	198	1	100	2.9	2102	PASS
441	442	0.01	24	17.6	7677	PASS
442	198	50	100	59.9	43664	PASS
443	442	15	24	19.6	8575	PASS