


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE120817\
Data File : BE094963.D
Acq On : 8 Dec 2017 23:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE113017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 01 13:33:28 2017

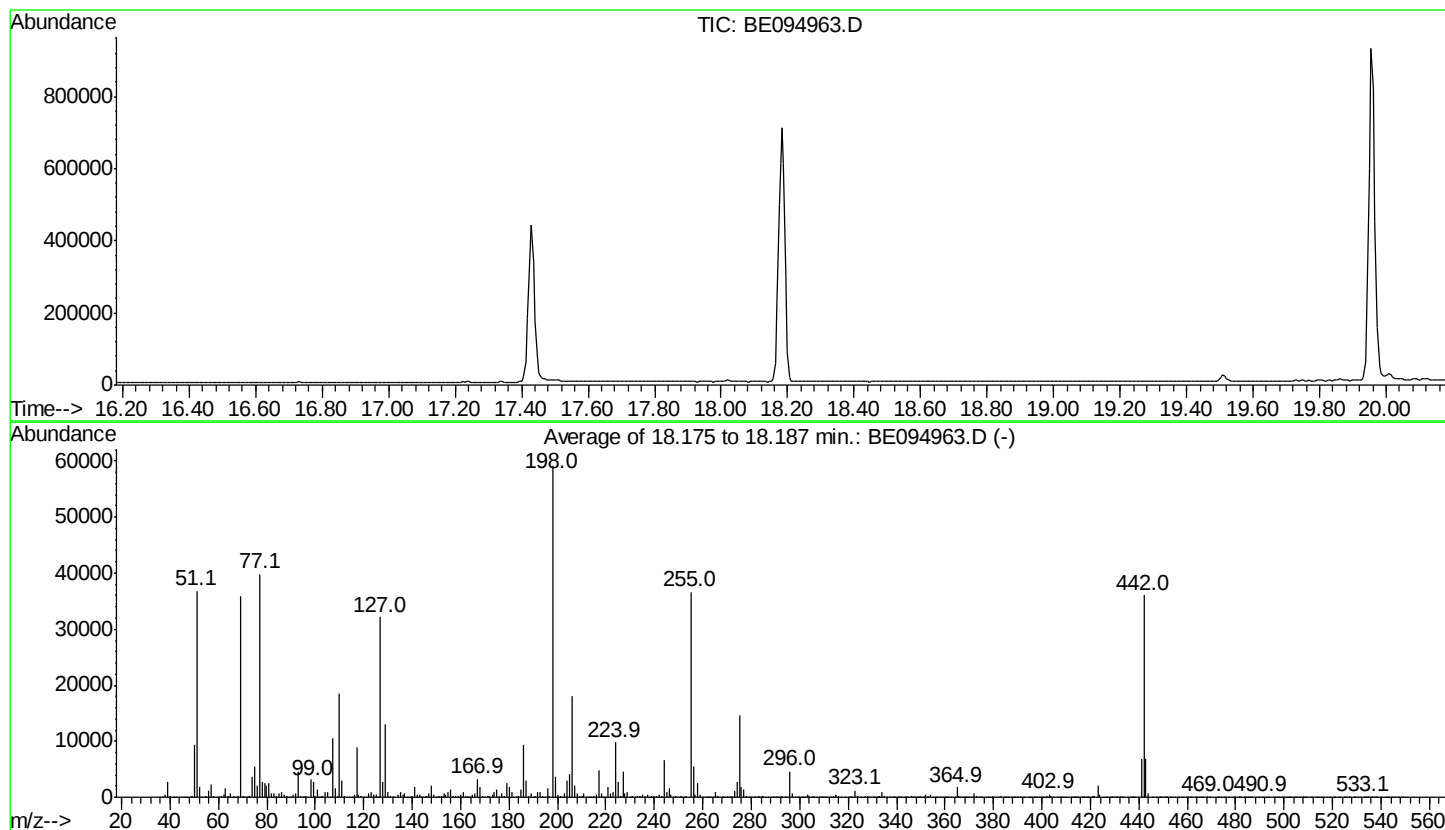

AutoFind: Scans 2653, 2654, 2655; Background Corrected with Scan 2644

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.2	36828	PASS
68	69	0.00	2	0.9	336	PASS
69	198	0.00	100	60.7	35909	PASS
70	69	0.00	2	0.5	164	PASS
127	198	10	80	54.4	32186	PASS
197	198	0.00	2	0.3	189	PASS
198	198	100	100	100.0	59197	PASS
199	198	5	9	6.4	3775	PASS
275	198	10	60	24.9	14713	PASS
365	198	1	100	3.0	1768	PASS
441	442	0.01	24	18.9	6809	PASS
442	198	50	100	61.0	36093	PASS
443	442	15	24	19.0	6865	PASS