

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089199.D
 Acq On : 9 Dec 2014 23:13
 Operator : TP/JJ
 Sample : PB80770BL
 Misc : SBLK68
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK68

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:44 PM

Quant Time: Dec 10 01:18:47 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

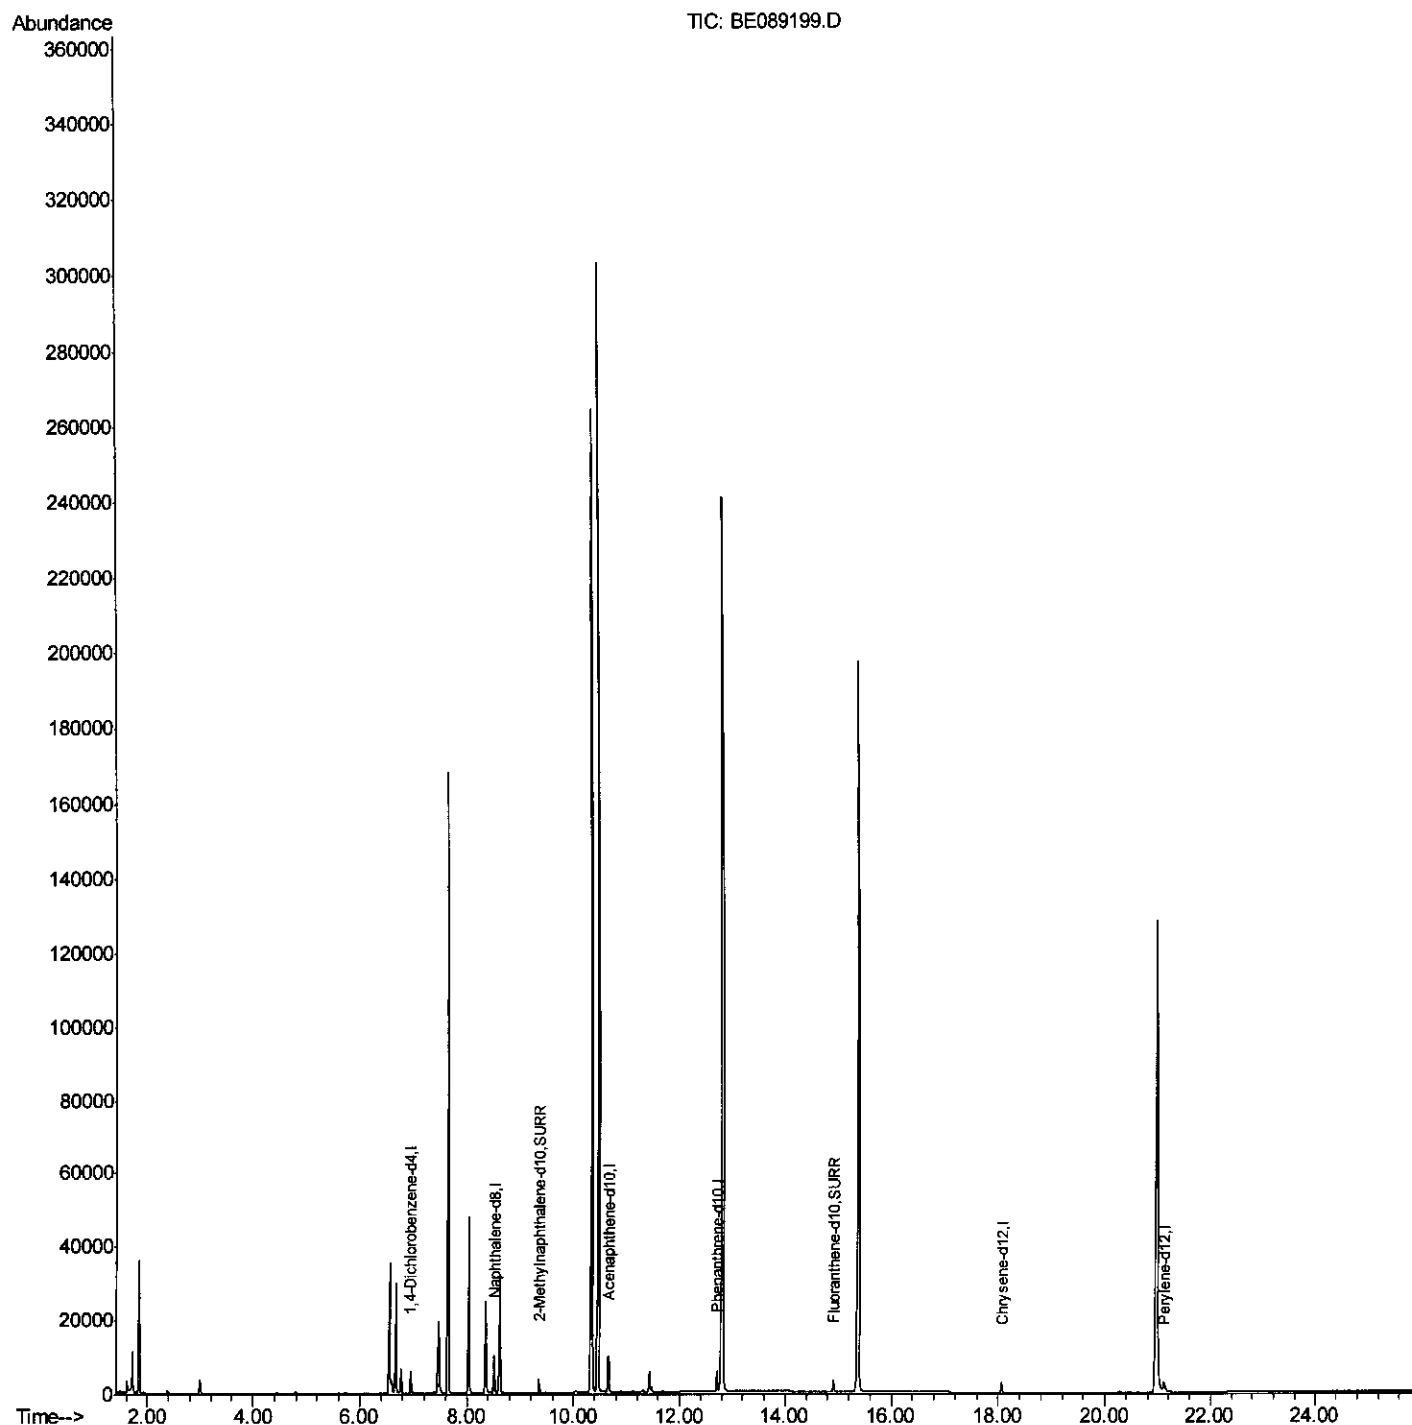

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089199.D
 Acq On : 9 Dec 2014 23:13
 Operator : TP/JJ
 Sample : PB80770BL
 Misc : SBLK68
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK68

Quant Time: Dec 10 01:07:48 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:44 PM

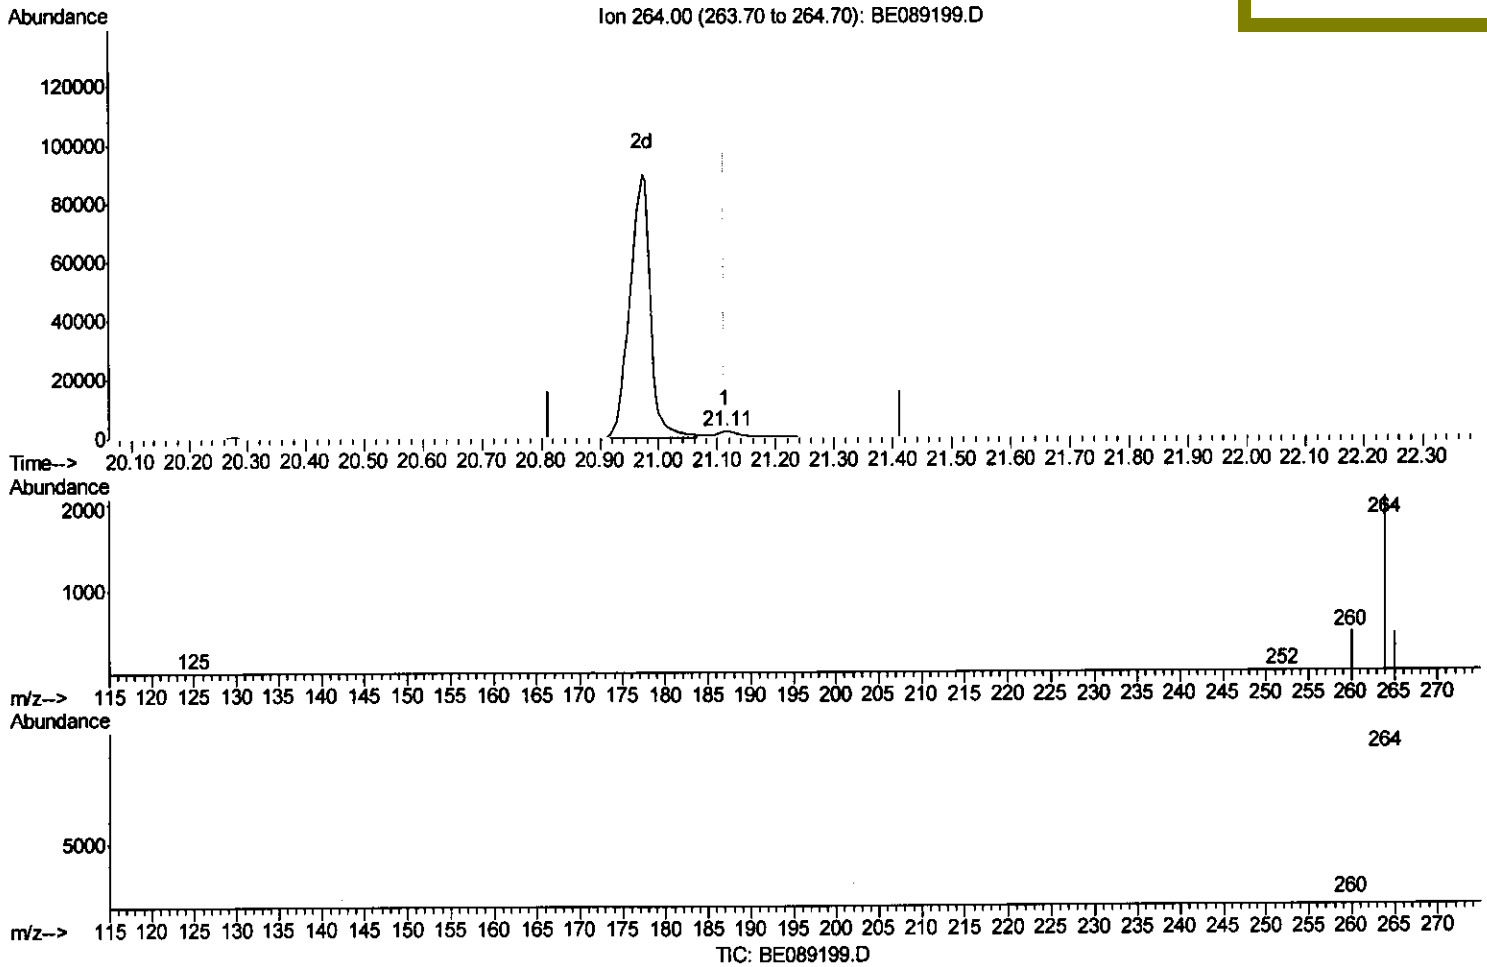

(20) Perylene-d12 (I)

21.113min (+0.001) 0.40ng/ul

response 6704

Ion	Exp%	Act%
264.00	100	100
260.00	24.70	24.40
265.00	23.40	23.72
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089199.D
 Acq On : 9 Dec 2014 23:13
 Operator : TP/JJ
 Sample : PB80770BL
 Misc : SBLK68
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK68

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:44 PM

Quant Time: Dec 10 01:07:48 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

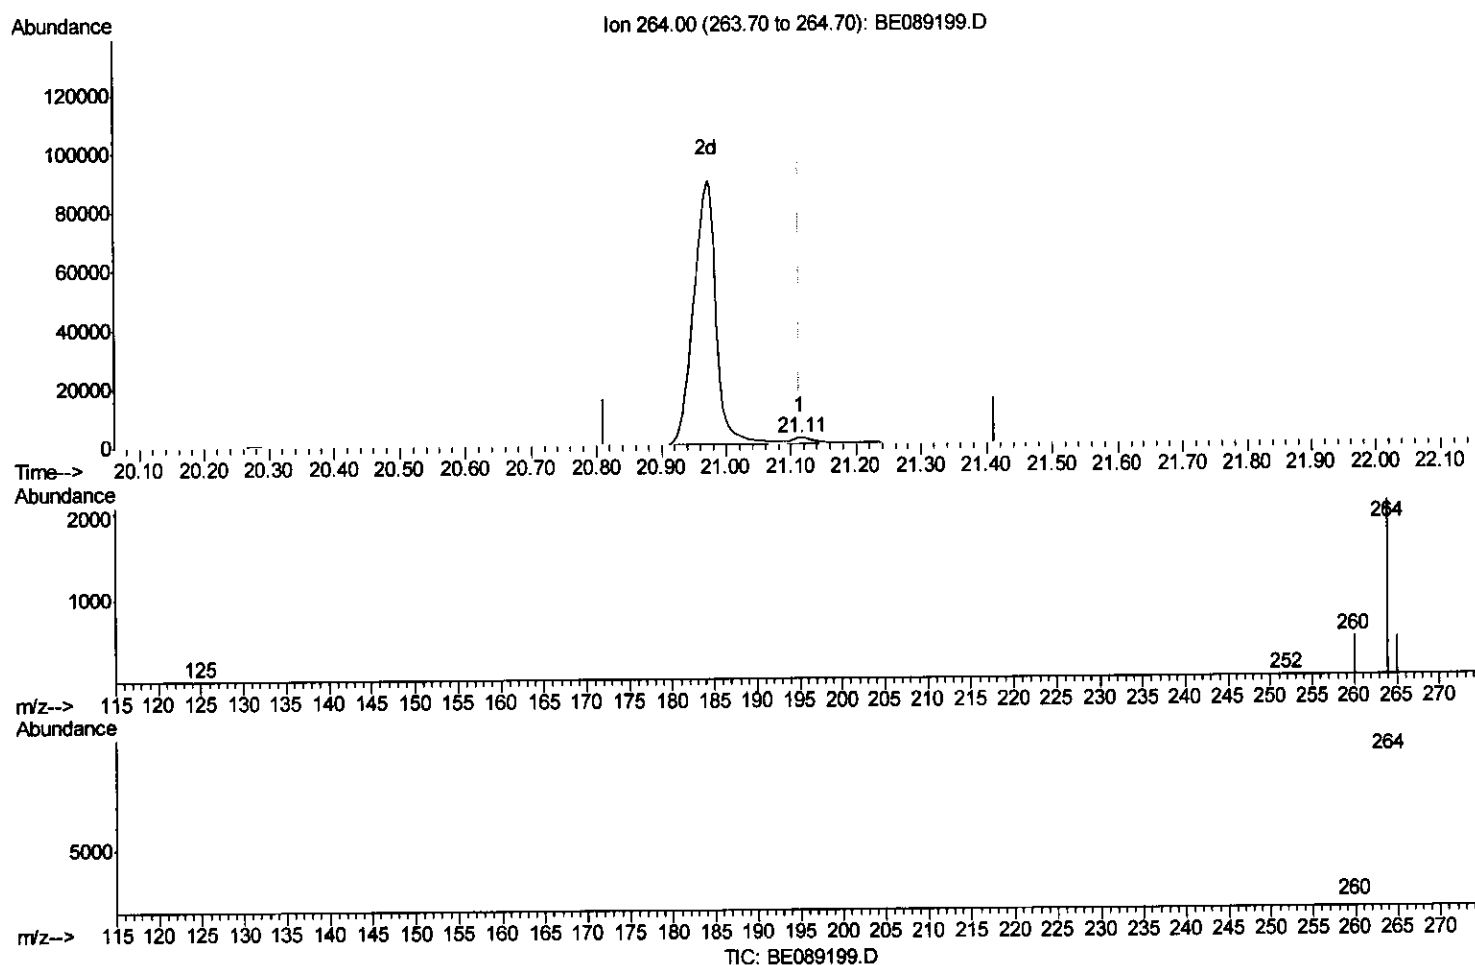

(20) Perylene-d12 (I)

21.113min (+0.001) 0.40ng/ul m

response 2675

Ion	Exp%	Act%
264.00	100	100
260.00	24.70	24.40
265.00	23.40	23.72
0.00	0.00	0.00

T.P
 12/23/14

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089199.D
 Acq On : 9 Dec 2014 23:13
 Operator : TP/JJ
 Sample : PB80770BL
 Misc : SBLK68
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
ClientSampleId :
 SBLK68

Quant Time: Dec 10 01:07:48 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
 12/10/2014 4:32:44 PM

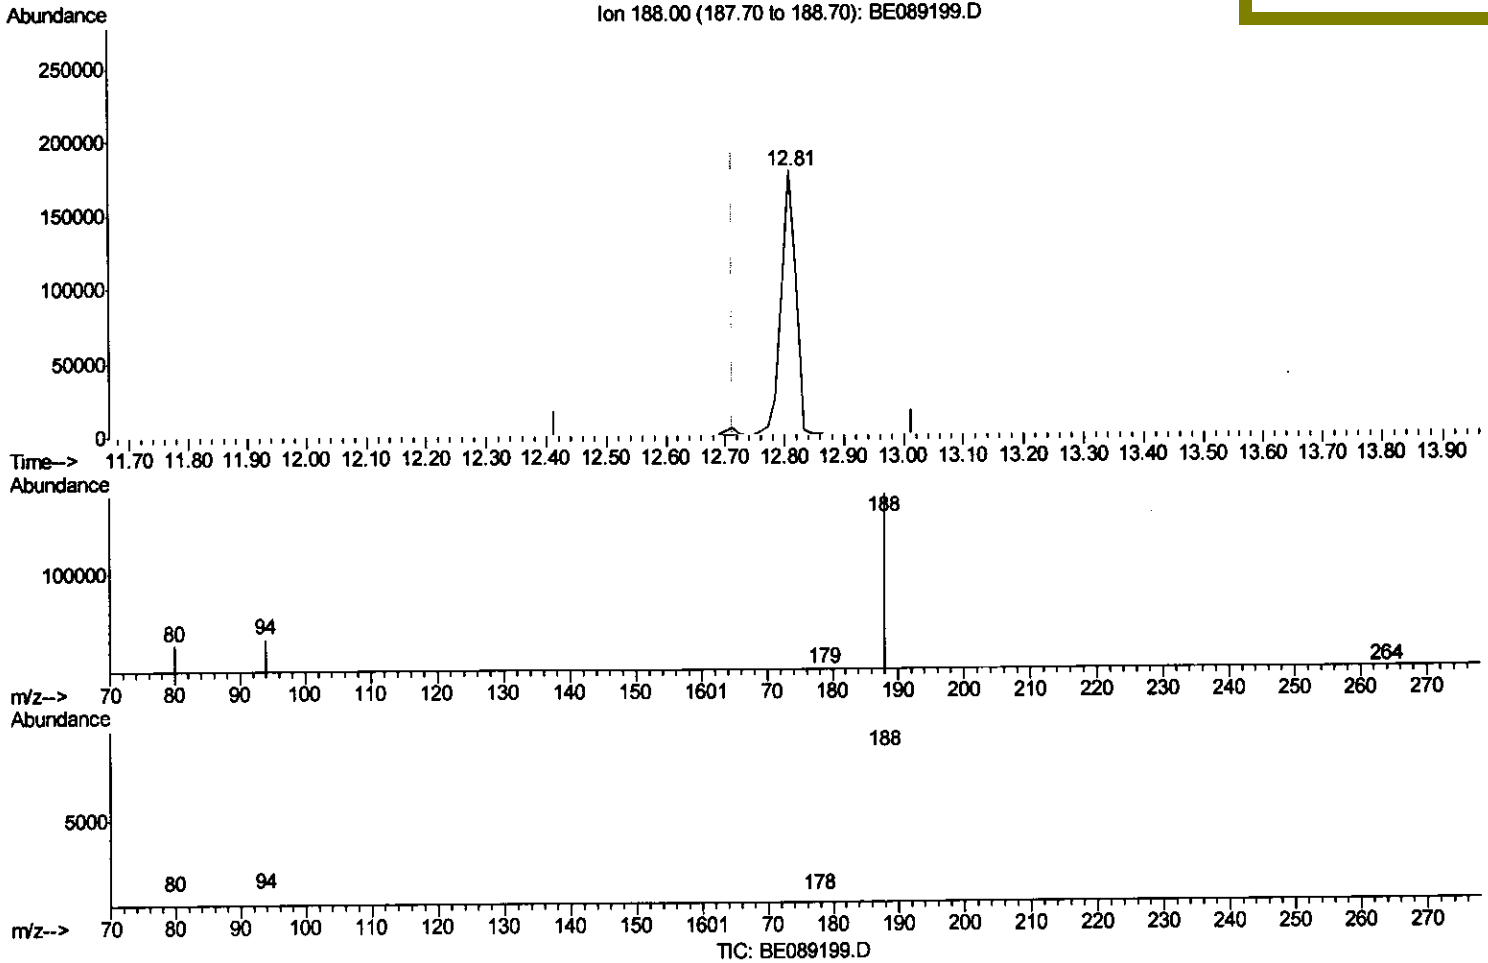

(10) Phenanthrene-d10 (I)

12.809min (+0.095) 0.40ng/ul

response 306204

Ion	Exp%	Act%
188.00	100	100
94.00	10.20	18.58#
80.00	9.00	14.78#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089199.D
 Acq On : 9 Dec 2014 23:13
 Operator : TP/JJ
 Sample : PB80770BL
 Misc : SBLK68
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK68

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:44 PM

Quant Time: Dec 10 01:07:48 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

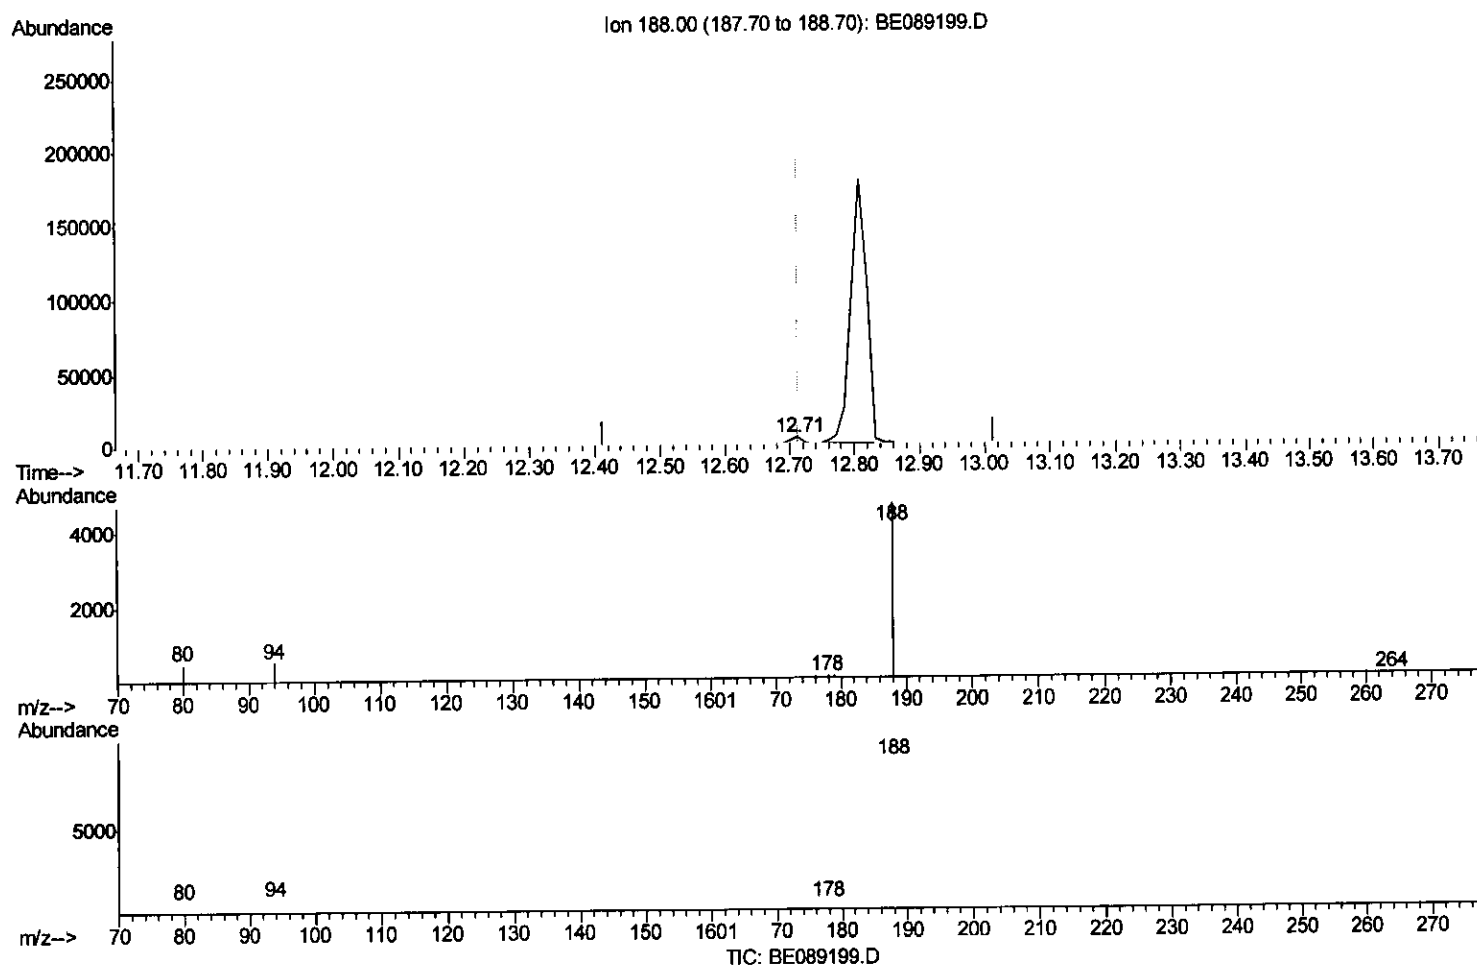

(10) Phenanthrene-d10 (I)

12.712min (-0.002) 0.40ng/ul m

response 6388

Ion Exp% Act%

188.00	100	100
94.00	10.20	11.64
80.00	9.00	10.52
0.00	0.00	0.00

TP
 12/23/14

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
Data File : BE089199.D
Acq On : 9 Dec 2014 23:13
Operator : TP/JJ
Sample : PB80770BL
Misc : SBLK68
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Quant Time: Dec 10 01:18:47 2014
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 10 01:02:19 2014
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
12/10/2014 4:32:44 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	2244	0.40	ng/ul	0.00
2) Naphthalene-d8	8.51	136	8877	0.40	ng/ul	0.00
6) Acenaphthene-d10	10.65	164	4559	0.40	ng/ul	0.00
10) Phenanthrene-d10	12.71	188	6388m	0.40	ng/ul	0.00
16) Chrysene-d12	18.06	240	4041	0.40	ng/ul	0.00
20) Perylene-d12	21.11	264	2675m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	9.35	152	3646	0.35	ng/ul	0.00
14) Fluoranthene-d10	14.91	212	3923	0.35	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

T.P
12/23/14