

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089201.D
 Acq On : 10 Dec 2014 00:18
 Operator : TP/JJ
 Sample : F4964-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BBTQ4

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:40 PM

Quant Time: Dec 10 01:34:29 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

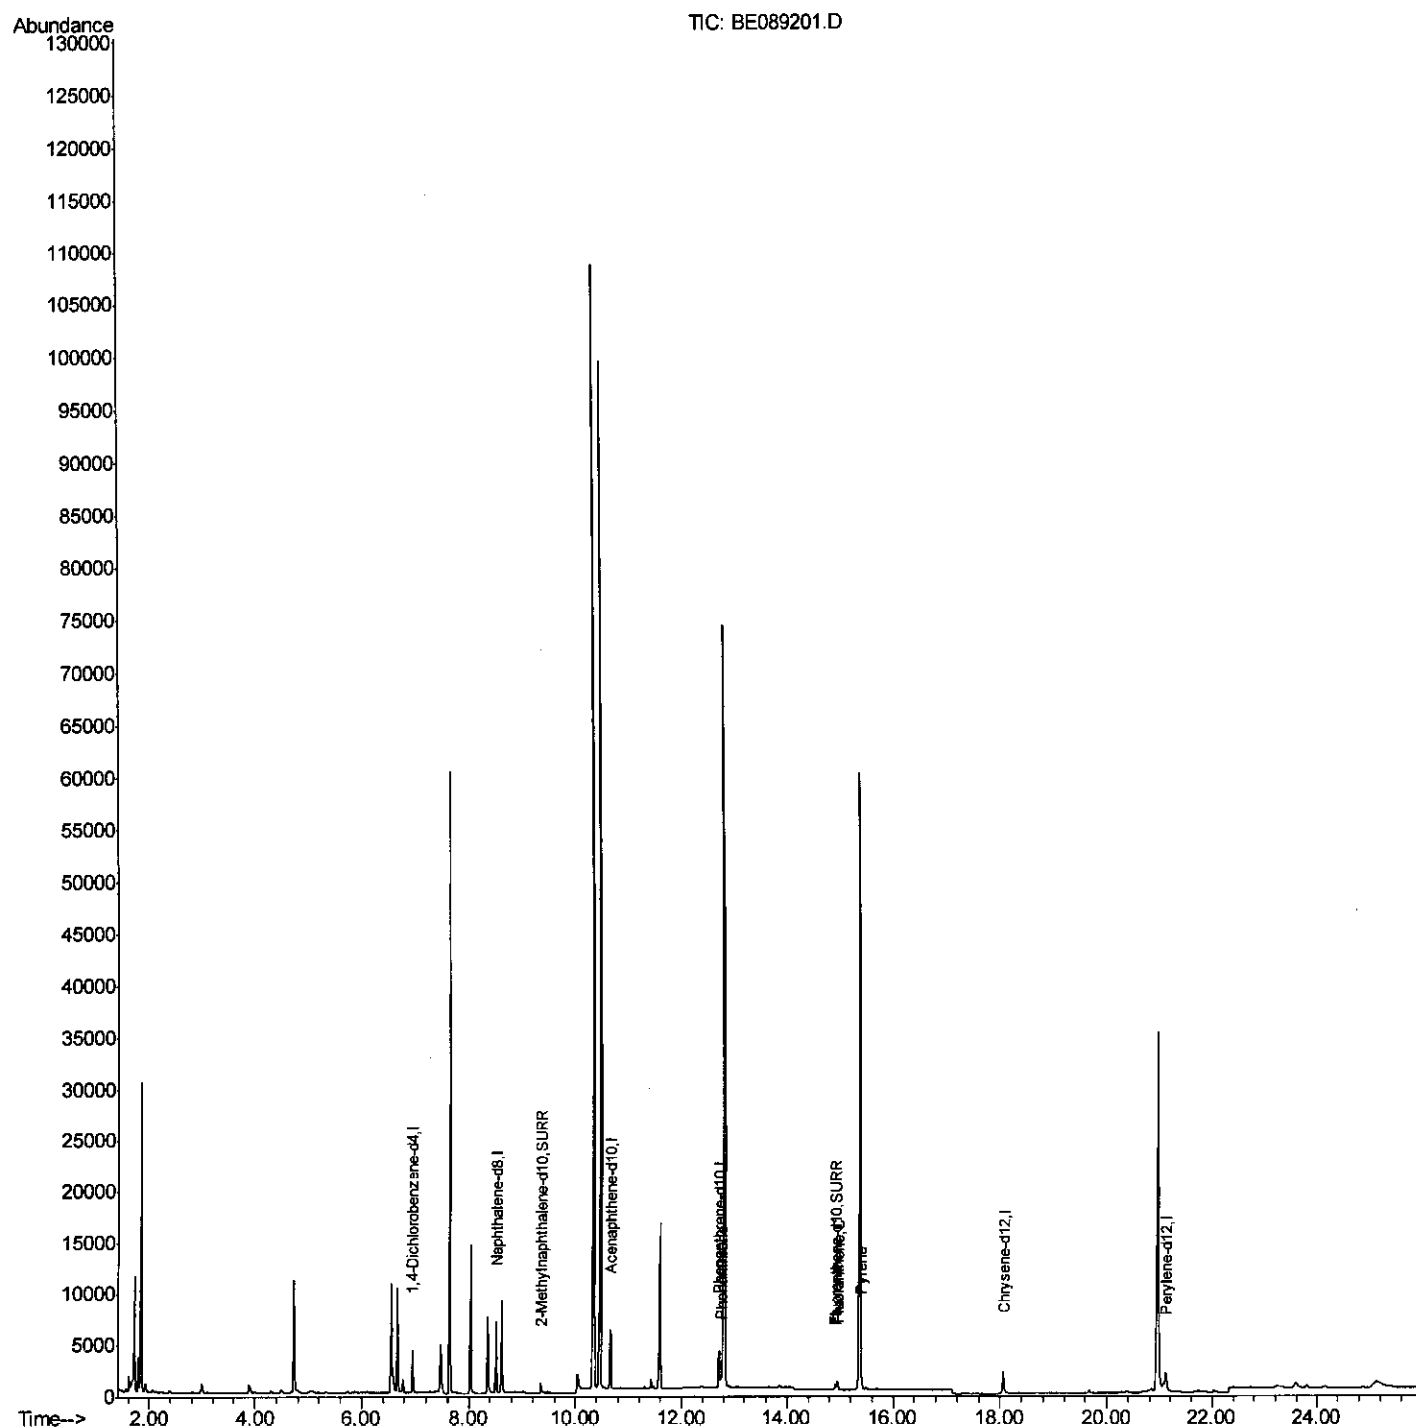

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089201.D
 Acq On : 10 Dec 2014 00:18
 Operator : TP/JJ
 Sample : F4964-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BBTQ4

Quant Time: Dec 10 01:08:08 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:40 PM

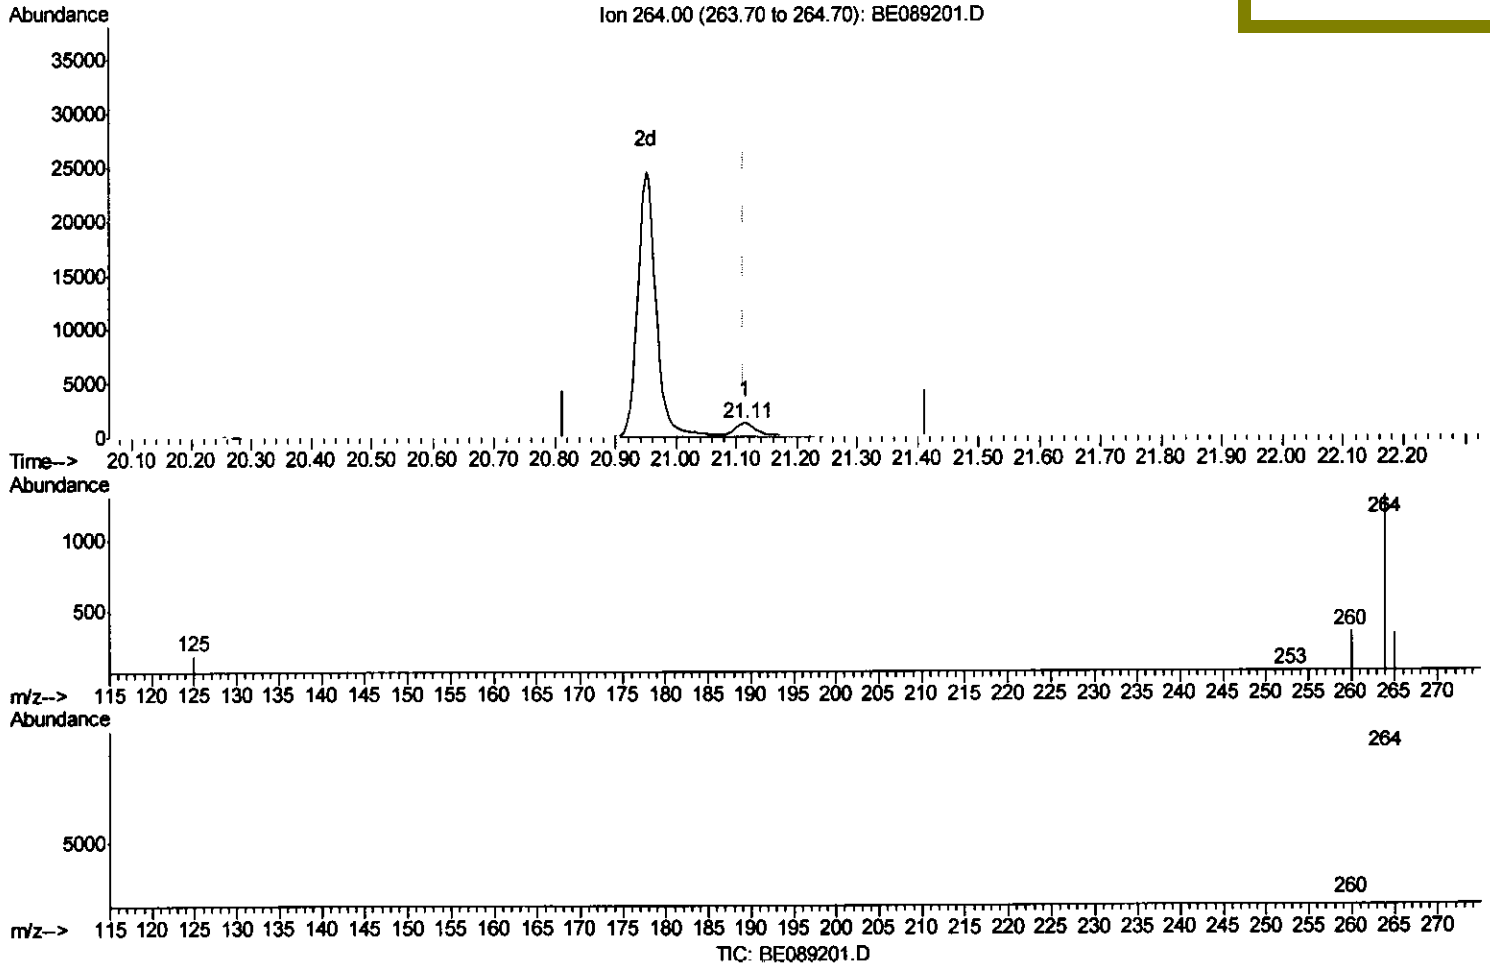

(20) Perylene-d12 (I)

21.114min (+0.001) 0.40ng/ul

response 3300

Ion	Exp%	Act%
264.00	100	100
260.00	24.70	26.14
265.00	23.40	24.85
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089201.D
 Acq On : 10 Dec 2014 00:18
 Operator : TP/JJ
 Sample : F4964-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BBTQ4

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:40 PM

Quant Time: Dec 10 01:08:08 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

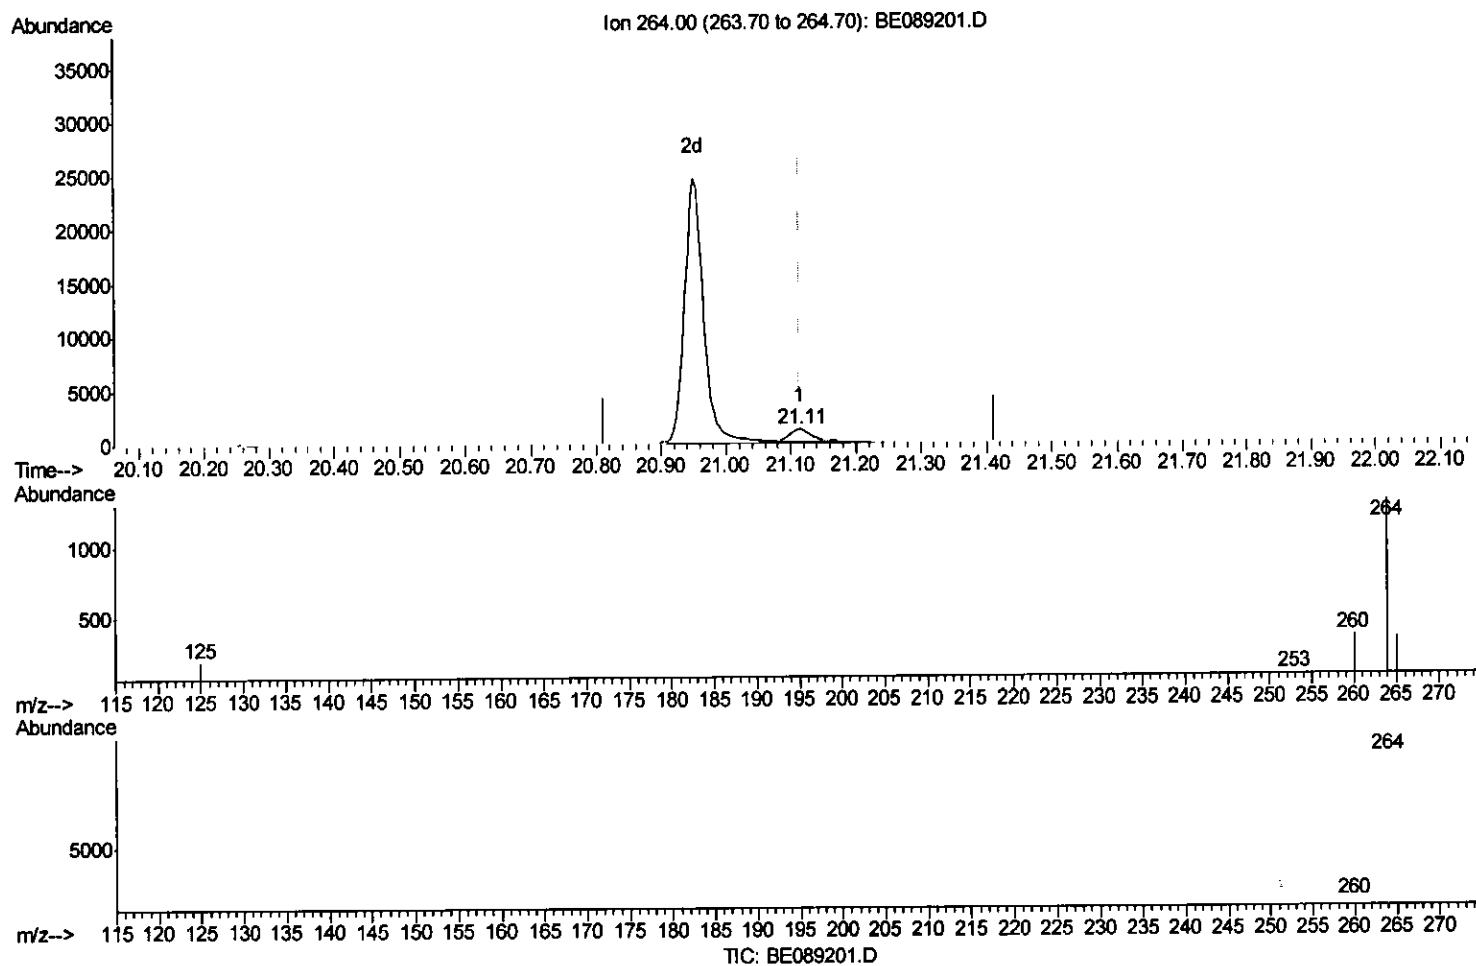

(20) Perylene-d12 (I)

21.114min (+0.001) 0.40ng/ul m

response 2219

Ion	Exp%	Act%
264.00	100	100
260.00	24.70	26.14
265.00	23.40	24.85
0.00	0.00	0.00

T.P
 12/23/14

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE120914\
 Data File : BE089201.D
 Acq On : 10 Dec 2014 00:18
 Operator : TP/JJ
 Sample : F4964-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BBTQ4

Quant Time: Dec 10 01:34:29 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE120514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 01:02:19 2014
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 12/10/2014 4:32:40 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1446	0.40	ng/ul	0.00
2) Naphthalene-d8	8.51	136	5735	0.40	ng/ul	0.00
6) Acenaphthene-d10	10.65	164	2802	0.40	ng/ul	0.00
10) Phenanthrene-d10	12.71	188	4118	0.40	ng/ul	0.00
16) Chrysene-d12	18.06	240	2834	0.40	ng/ul	0.00
20) Perylene-d12	21.11	264	2219m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	9.35	152	815	0.12	ng/ul	0.00
14) Fluoranthene-d10	14.92	212	811	0.11	ng/ul	0.00
Target Compounds						Qvalue
12) Phenanthrene	12.75	178	1138	0.03	ng/ul#	58
15) Fluoranthene	14.95	202	1108	0.03	ng/ul	66
17) Pyrene	15.40	202	956	0.02	ng/ul#	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed

TP
12/23/14