


Data Path : Z:\HPCHEM1\BNA_E\Data\BE120914\
 Data File : BE089186.D
 Acq On : 9 Dec 2014 10:20
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-ACID-BE120814.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 09 19:38:28 2014

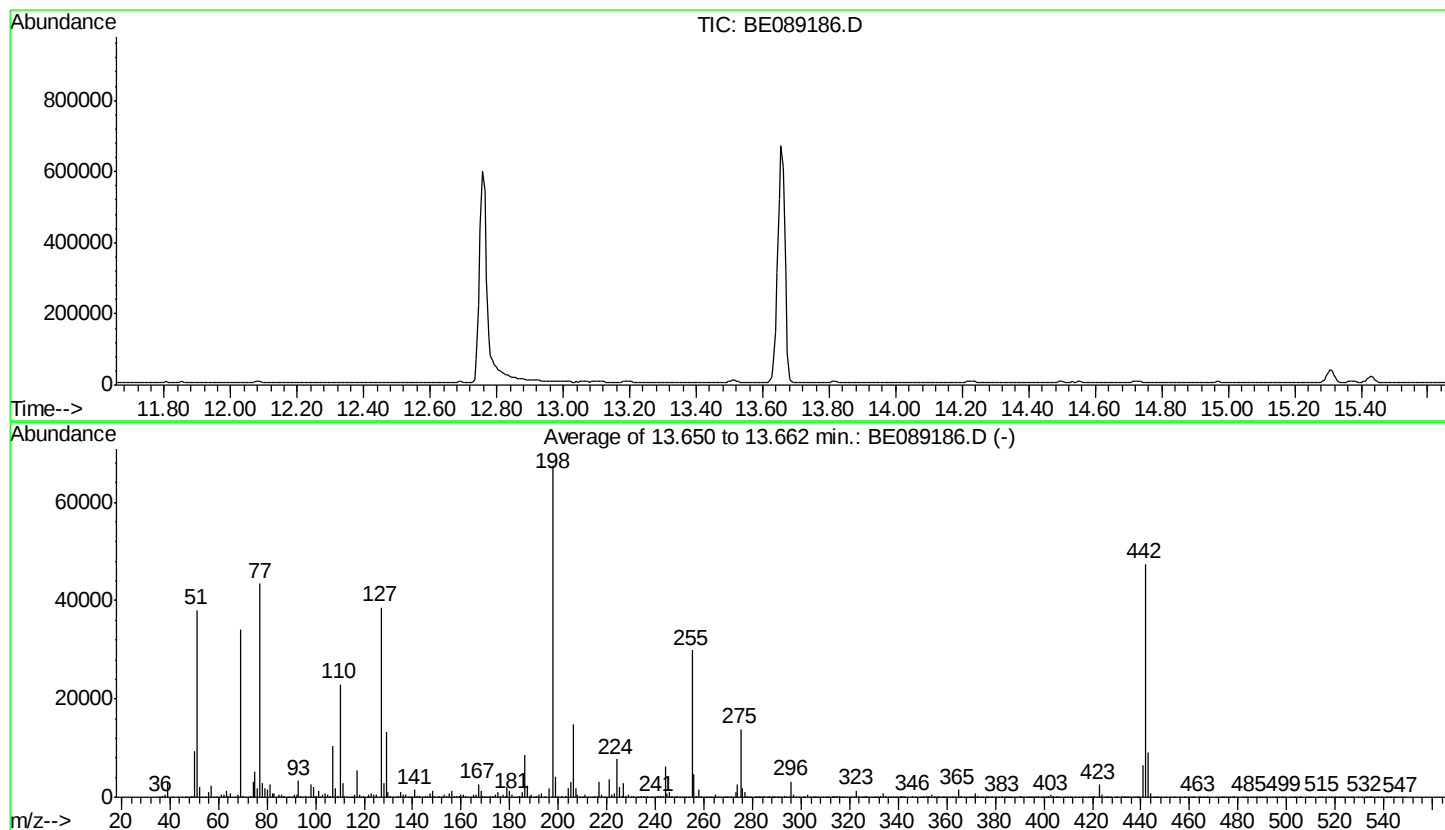

AutoFind: Scans 2087, 2088, 2089; Background Corrected with Scan 2077

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.5	38102	PASS
68	69	0.00	2	1.4	483	PASS
69	198	0.00	100	50.5	34087	PASS
70	69	0.00	2	0.5	162	PASS
127	198	10	80	57.2	38618	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67459	PASS
199	198	5	9	6.3	4232	PASS
275	198	10	60	20.5	13825	PASS
365	198	1	100	2.2	1469	PASS
441	442	0.01	24	14.0	6644	PASS
442	198	50	100	70.4	47473	PASS
443	442	15	24	19.3	9175	PASS