


Data Path : Z:\HPCHEM1\BNA E\DATA\BE120916\  
 Data File : BE092588.D  
 Acq On : 9 Dec 2016 9:38  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE111616.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Nov 16 15:43:18 2016

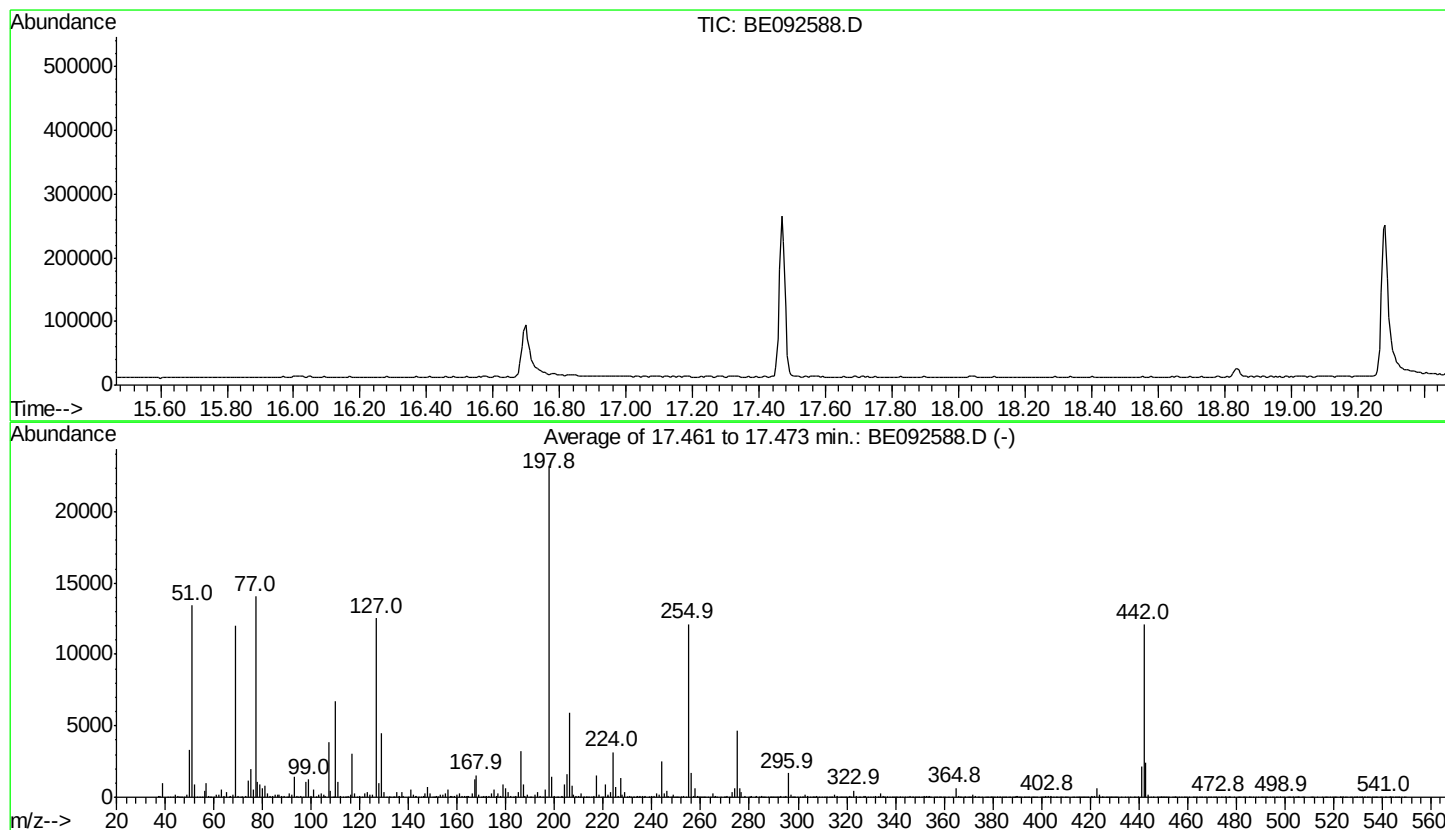

AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2516

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 57.9      | 13440   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 209     | PASS             |
| 69          | 198          | 0.00         | 100          | 51.8      | 12031   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 76      | PASS             |
| 127         | 198          | 10           | 80           | 54.0      | 12540   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.1       | 14      | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 23220   | PASS             |
| 199         | 198          | 5            | 9            | 6.2       | 1441    | PASS             |
| 275         | 198          | 10           | 60           | 20.2      | 4686    | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 666     | PASS             |
| 441         | 442          | 0.01         | 24           | 18.2      | 2198    | PASS             |
| 442         | 198          | 50           | 100          | 52.0      | 12070   | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 2385    | PASS             |