
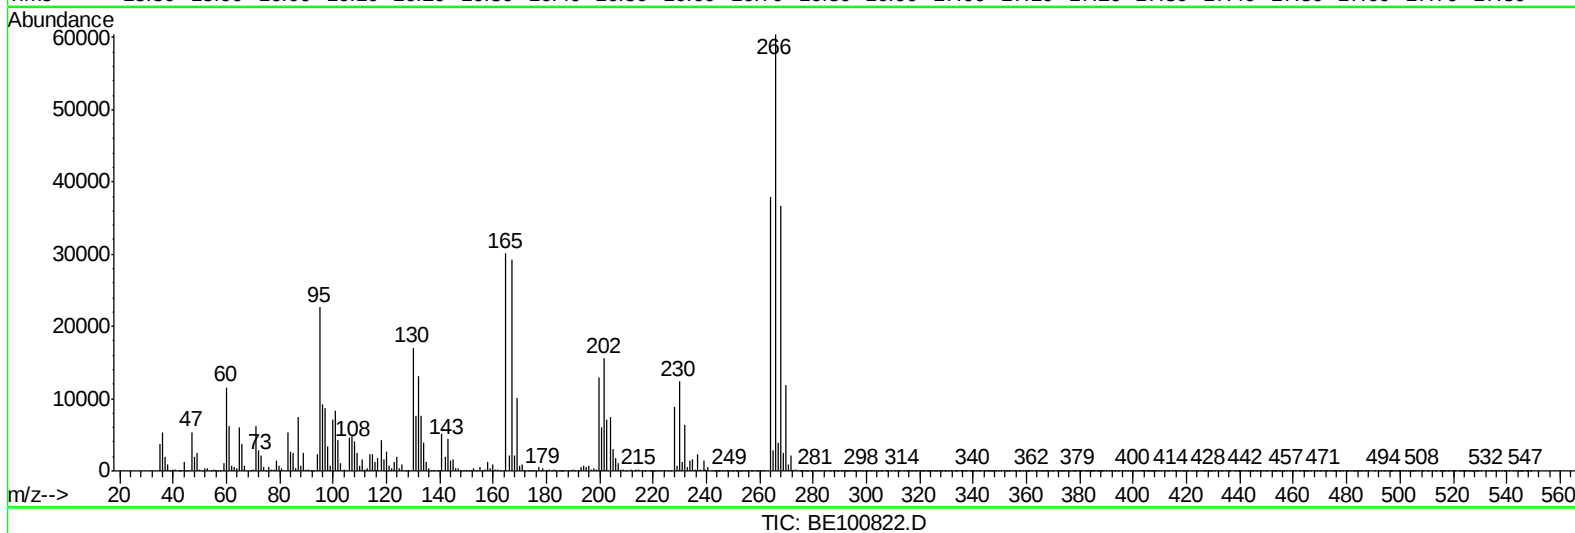


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121019\
Data File : BE100822.D
Acq On : 10 Dec 2019 22:38
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:56:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 04 17:18:11 2019
Response via : Initial Calibration

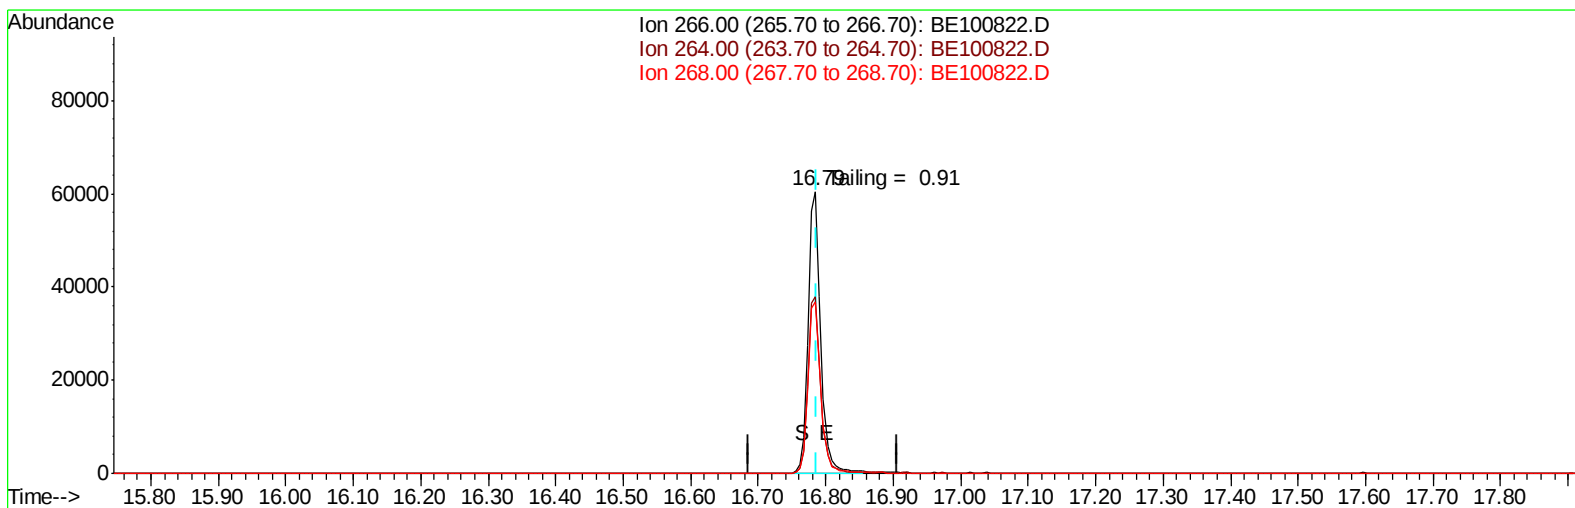

TIC: BE100822.D

(22) Pentachlorophenol

16.785min (-0.002) 432612.88ng

response 79746

Ion	Exp%	Act%
266.00	100	100
264.00	79.20	62.73#
268.00	82.30	64.80#
0.00	0.00	0.00