
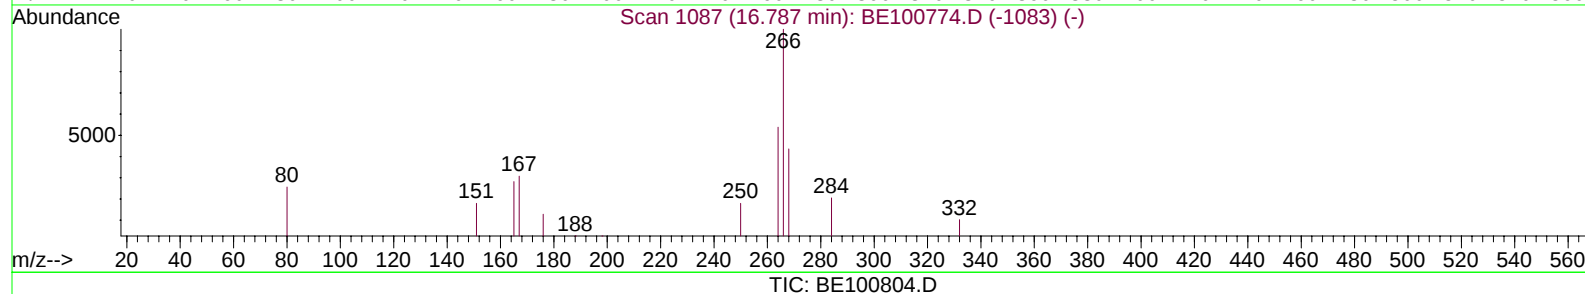
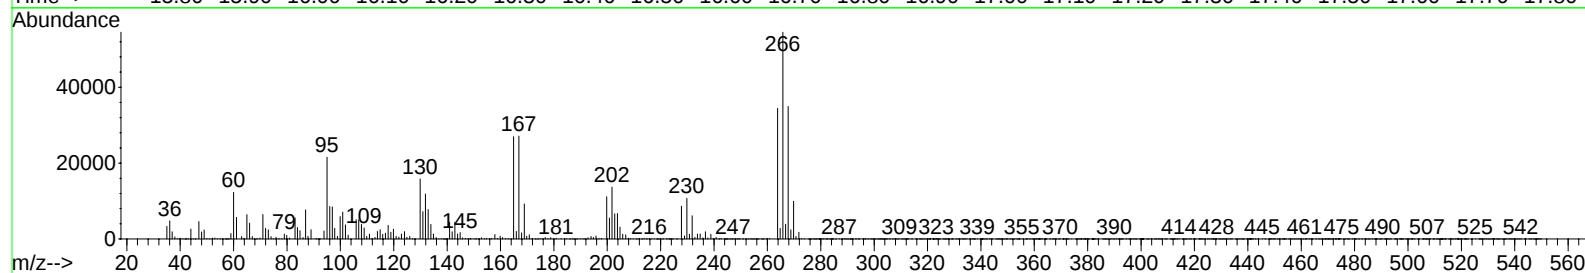


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121019\
Data File : BE100804.D
Acq On : 10 Dec 2019 10:20
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 17:22:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 04 17:18:11 2019
Response via : Initial Calibration

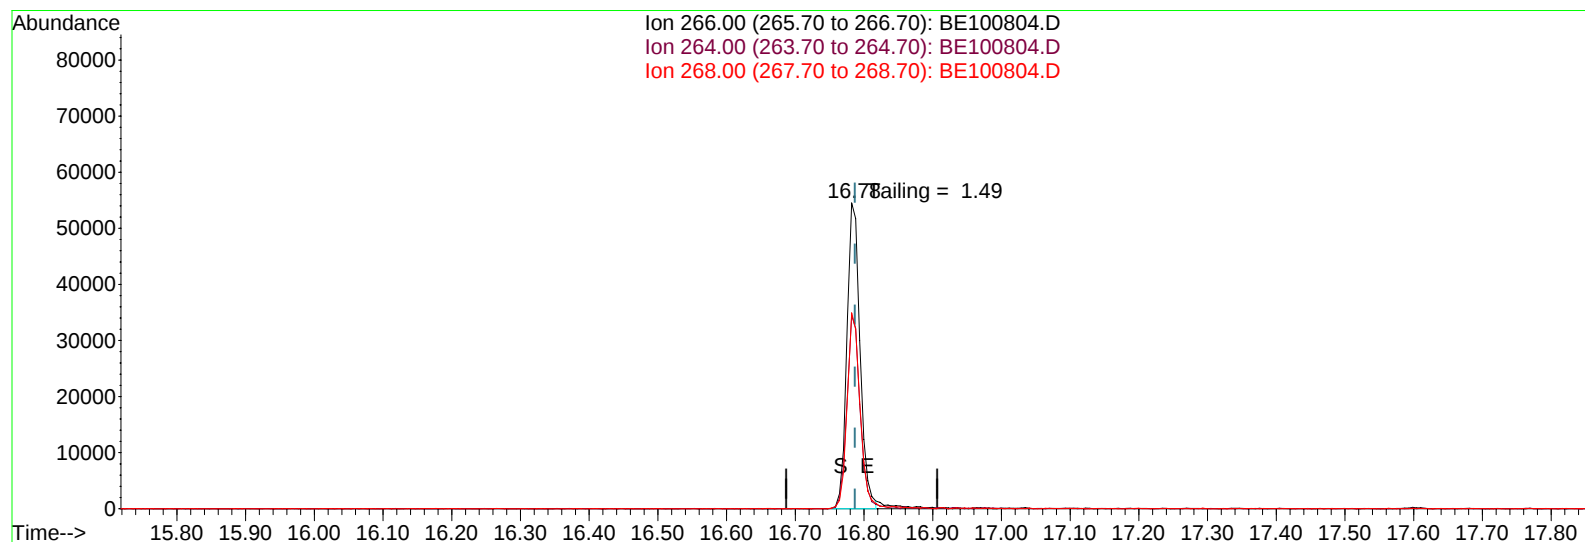

(22) Pentachlorophenol

16.782min (-0.005) 153691.16ng

response 73660

Ion	Exp%	Act%
266.00	100	100
264.00	79.20	63.18#
268.00	82.30	64.06#
0.00	0.00	0.00