

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121019\
 Data File : BE100811.D
 Acq On : 10 Dec 2019 15:13
 Operator : JU
 Sample : K6184-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE134D2-20191202

Quant Time: Dec 10 17:46:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 04 17:18:11 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	4978	0.40	ng	0.00
7) Naphthalene-d8	10.54	136	23072	0.40	ng	0.00
13) Acenaphthene-d10	14.40	164	13089	0.40	ng	0.00
19) Phenanthrene-d10	17.12	188	30767	0.40	ng	-0.01
27) Chrysene-d12	21.31	240	26335	0.40	ng	0.00
34) Perylene-d12	23.74	264	32592	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.38	112	2473	0.21	ng	0.00
5) Phenol-d6	6.93	99	2403	0.13	ng	0.00
8) Nitrobenzene-d5	8.90	82	6410	0.58	ng	0.00
11) 2-Methylnaphthalene-d10	12.14	152	14806	0.44	ng	0.00
14) 2,4,6-Tribromophenol	15.88	330	784	0.54	ng	0.00
15) 2-Fluorobiphenyl	13.03	172	20466	0.39	ng	0.00
25) Fluoranthene-d10	19.16	212	146043	0.40	ng	0.00
29) Terphenyl-d14	19.76	244	28434	0.45	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.34	88	63581	7.005	ng	89
32) Bis(2-ethylhexyl)phthalate	21.23	149	9786	0.145	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121019\
Data File : BE100811.D
Acq On : 10 Dec 2019 15:13
Operator : JU
Sample : K6184-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE134D2-20191202

Quant Time: Dec 10 17:46:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 04 17:18:11 2019
Response via : Initial Calibration

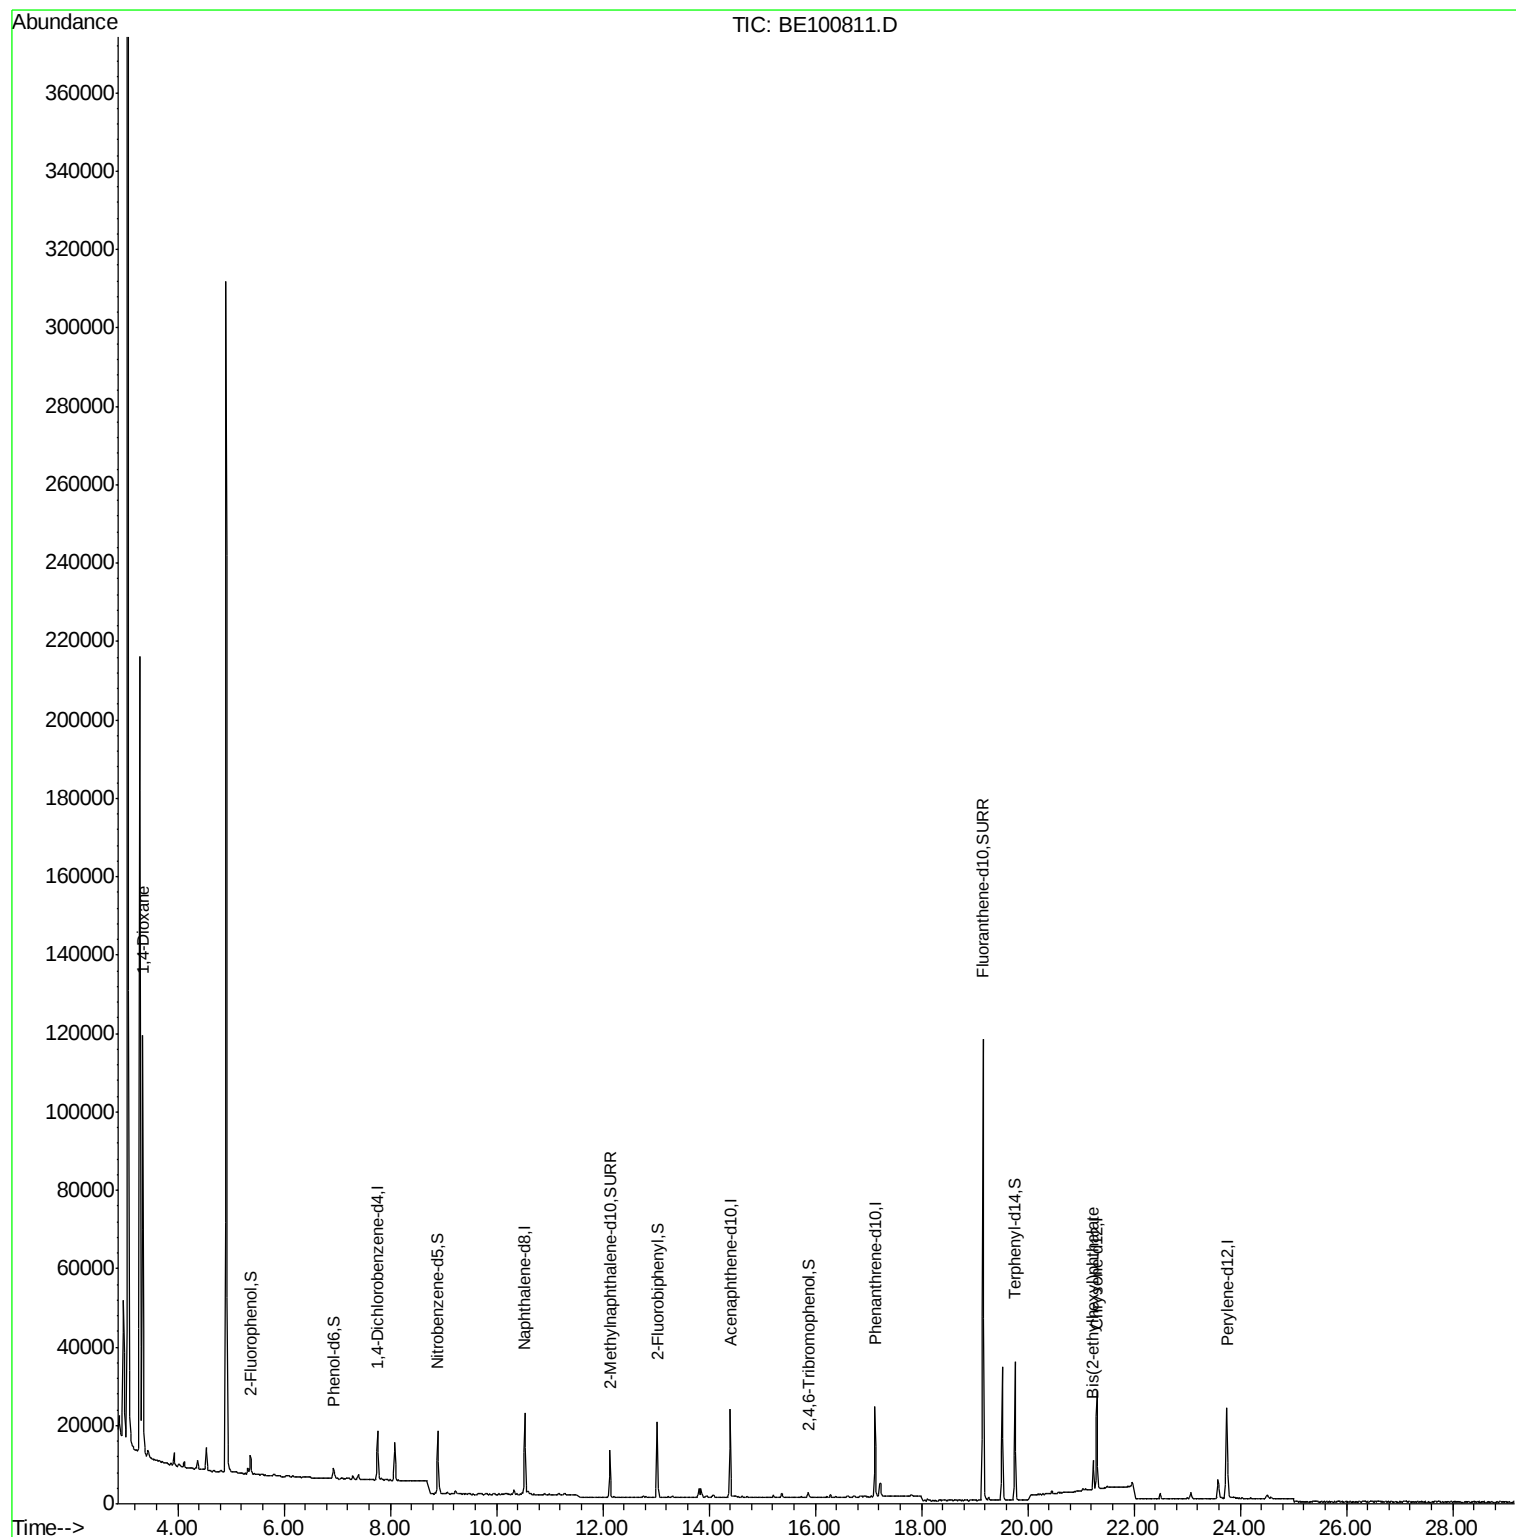




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.76 min Scan# 425
Delta R.T. -0.01 min
Lab File: BE100811.D
Acq: 10 Dec 2019 15:13

Instrument :
BNA_E
ClientSampleId :
RE134D2-20191202

Tot Ion:152 Resp: 4978
Ion Ratio Lower Upper
152 100
150 162.3 120.6 181.0
115 71.4 47.4 71.2#

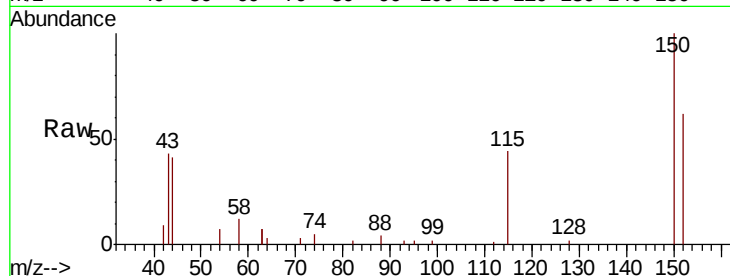


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

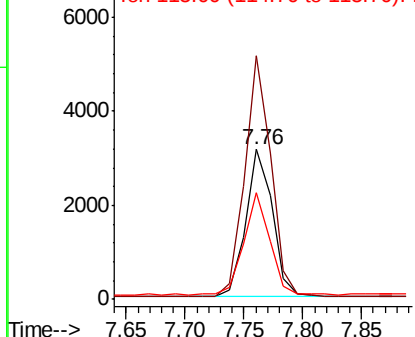



#2


1,4-Dioxane
Concen: 7.005 ng
RT: 3.34 min Scan# 41
Delta R.T. -0.01 min
Lab File: BE100811.D
Acq: 10 Dec 2019 15:13

Tgt Ion: 88 Resp: 63581
Ion Ratio Lower Upper
88 100
58 74.8 52.5 78.7
43 34.2 23.0 34.6



Abundance Ion 88.00 (87.70 to 88.70): BE1
Ion 58.00 (57.70 to 58.70): BE1
Ion 43.00 (42.70 to 43.70): BE1

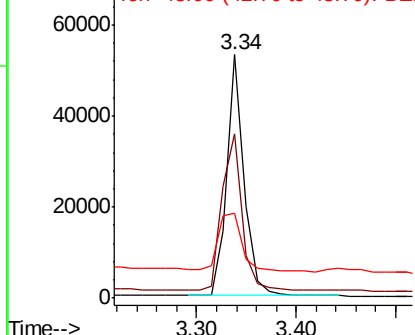



#4

2-Fluorophenol

Concen: 0.209 ng

RT: 5.38 min Scan# 218

Delta R.T. 0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13

Instrument :

BNA_E

ClientSampleId :

RE134D2-20191202


Tot Ion:112 Resp: 2473

Ion Ratio Lower Upper

112 100

64 67.4 54.1 81.1




63 147.8 113.2 169.8



Abundance Ion 112.00 (111.70 to 112.70): BE1

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

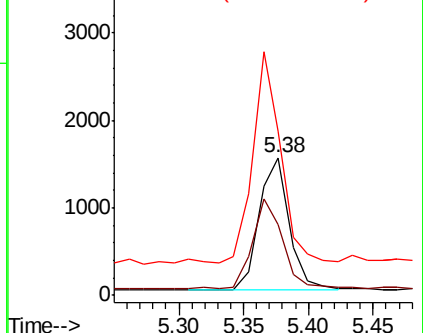

#5

Phenol-d6

Concen: 0.135 ng

RT: 6.93 min Scan# 353

Delta R.T. 0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13


Tgt Ion: 99 Resp: 2403

Ion Ratio Lower Upper

99 100

42 25.1 19.1 28.7



71 40.1 27.7 41.5




Abundance Ion 99.00 (98.70 to 99.70): BE1

Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

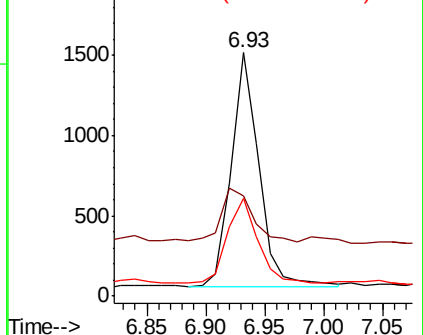



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.54 min Scan# 644

Delta R.T. -0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13

Instrument :

BNA_E

ClientSampleId :

RE134D2-20191202

Tot Ion:136 Resp: 23072


Ion Ratio Lower Upper

136 100

137 11.1 9.4 14.0

54 34.9 31.1 46.7

68 7.1 6.6 10.0



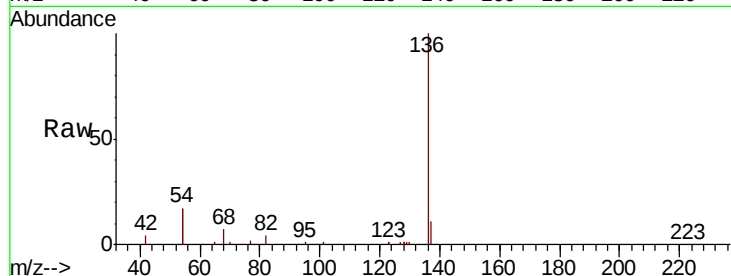


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

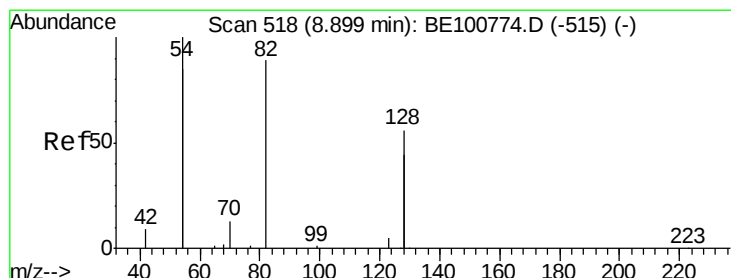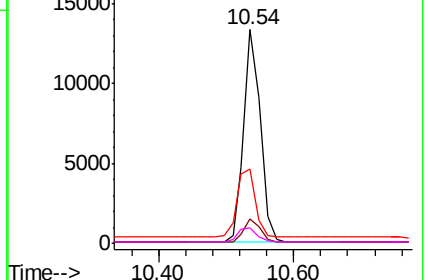

#8

Nitrobenzene-d5

Concen: 0.583 ng

RT: 8.90 min Scan# 518

Delta R.T. -0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13


Tgt Ion: 82 Resp: 6410

Ion Ratio Lower Upper

82 100

128 124.0 97.0 145.4



54 195.4 171.8 257.6

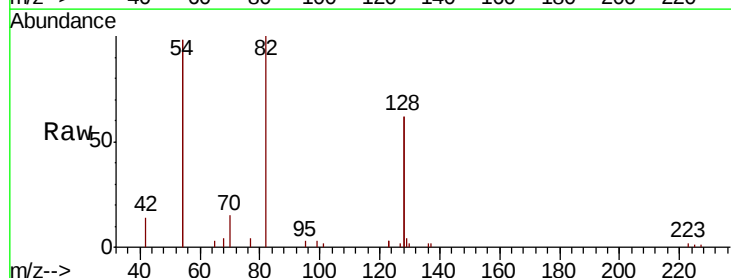


Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE1

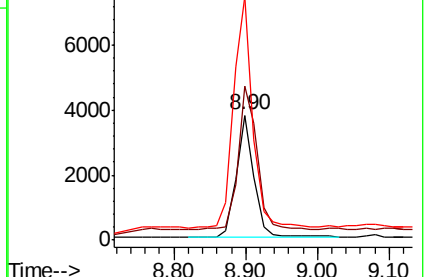

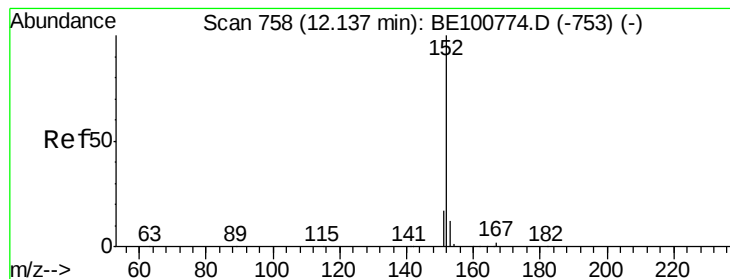

#11

2-Methylnaphthalene-d10

Concen: 0.443 ng

RT: 12.14 min Scan# 758

Delta R.T. -0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13

Instrument :

BNA_E

ClientSampleId :


RE134D2-20191202

Tot Ion:152 Resp: 14806

Ion Ratio Lower Upper




152 100

151 18.8 15.8 23.8



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

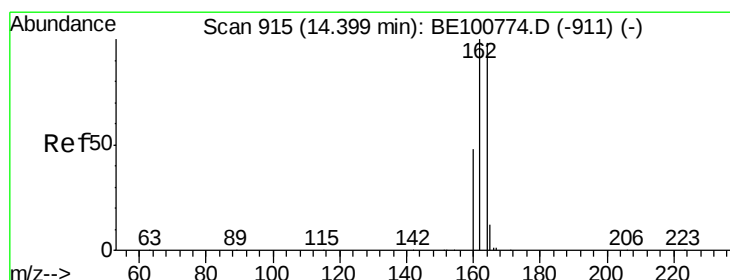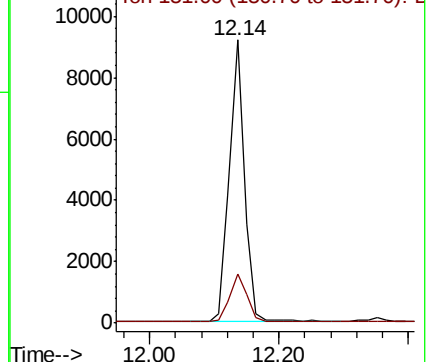

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.40 min Scan# 915

Delta R.T. -0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13


Tgt Ion:164 Resp: 13089

Ion Ratio Lower Upper

164 100

162 100.8 81.4 122.0



160 46.6 39.4 59.0




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

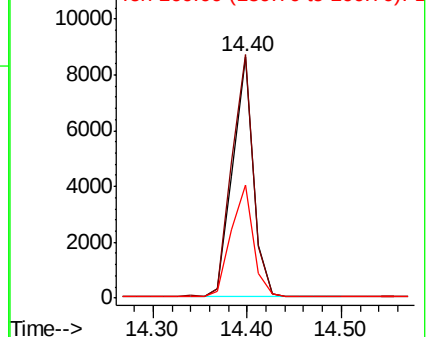



#14

2,4,6-Tribromophenol

Concen: 0.539 ng

RT: 15.88 min Scan# 1019

Delta R.T. -0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13

Instrument :

BNA_E

ClientSampleId :

RE134D2-20191202


Tot Ion:330 Resp: 784

Ion Ratio Lower Upper

330 100

332 94.4 69.4 104.2




141 55.7 51.1 76.7

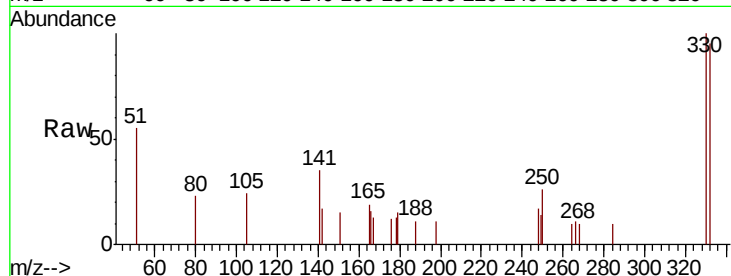

Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

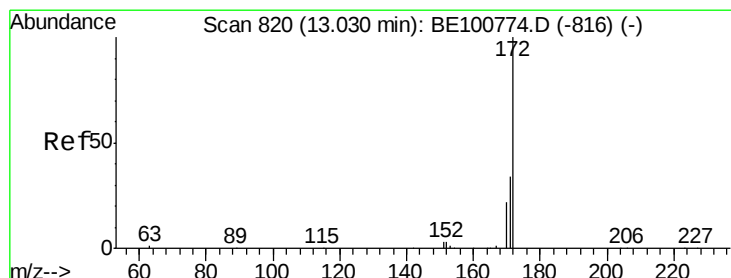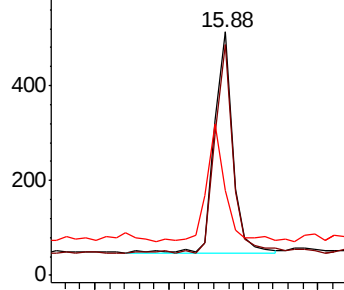

#15

2-Fluorobiphenyl

Concen: 0.394 ng

RT: 13.03 min Scan# 820

Delta R.T. -0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13


Tgt Ion:172 Resp: 20466

Ion Ratio Lower Upper

172 100

171 32.9 27.2 40.8



170 21.5 18.0 27.0

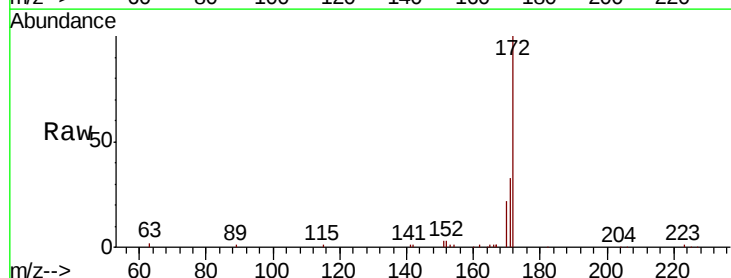


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

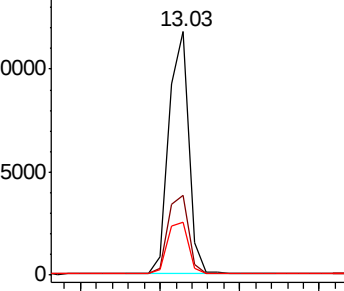

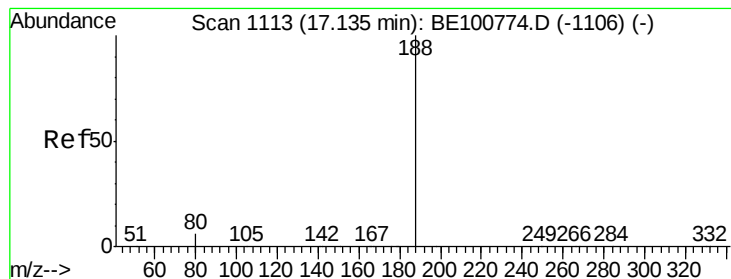

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.12 min Scan# 1112

Delta R.T. -0.01 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13

Instrument :

BNA_E

ClientSampleId :

RE134D2-20191202


Tot Ion:188 Resp: 30767

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 12.9 5.2 7.8#

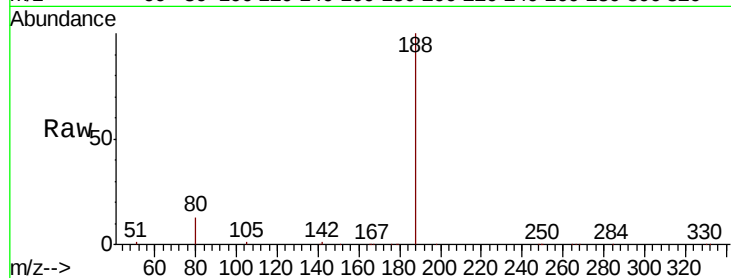

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE1

Ion 80.00 (79.70 to 80.70): BE1

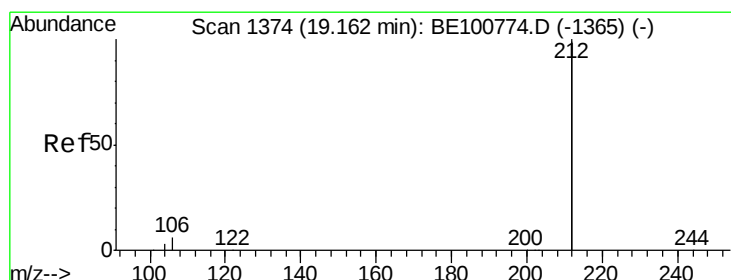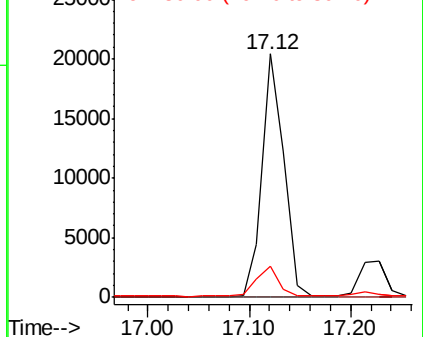

#25

Fluoranthene-d10

Concen: 0.402 ng

RT: 19.16 min Scan# 1373

Delta R.T. -0.01 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13


Tgt Ion:212 Resp: 146043

Ion Ratio Lower Upper

212 100

106 3.3 2.6 3.8



104 1.8 1.4 2.2

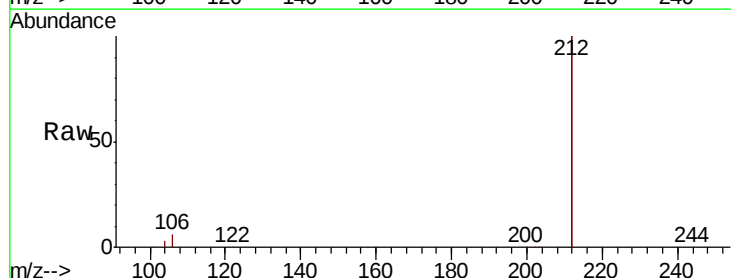


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

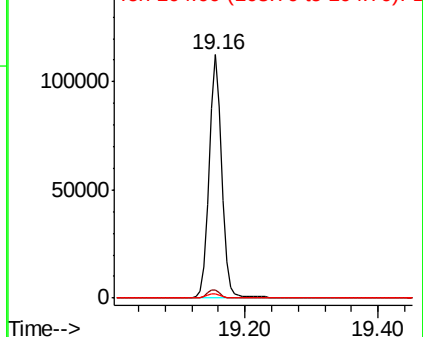



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.31 min Scan# 1625

Delta R.T. 0.00 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13

Instrument :

BNA_E

ClientSampleId :

RE134D2-20191202


Tot Ion:240 Resp: 26335

Ion Ratio Lower Upper

240 100

120 5.9 10.2 15.2#




236 26.1 22.3 33.5

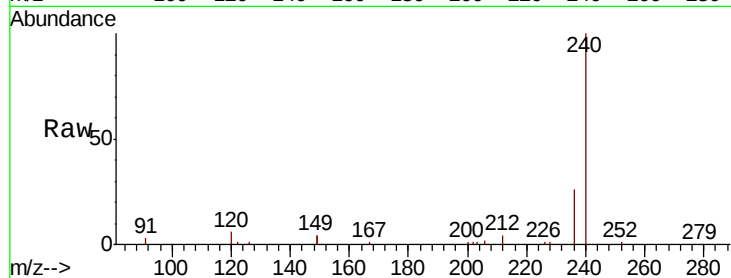

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

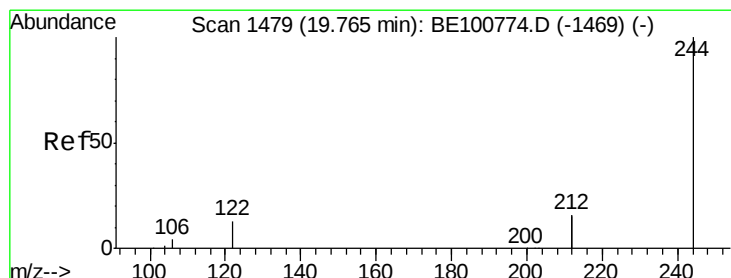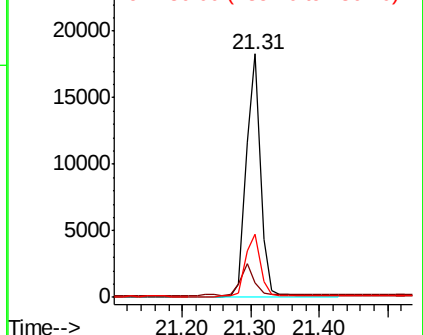

#29

Terphenyl-d14

Concen: 0.451 ng

RT: 19.76 min Scan# 1478

Delta R.T. -0.01 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13


Tgt Ion:244 Resp: 28434

Ion Ratio Lower Upper

244 100

212 31.7 26.2 39.4



122 12.2 10.2 15.4

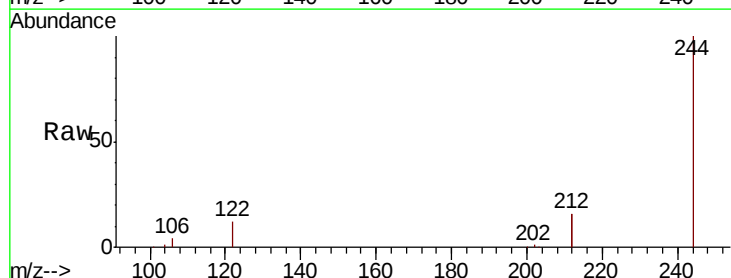


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

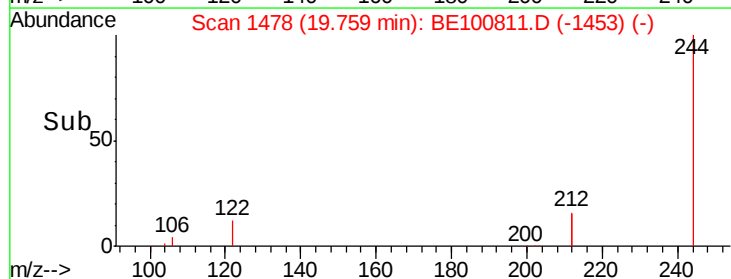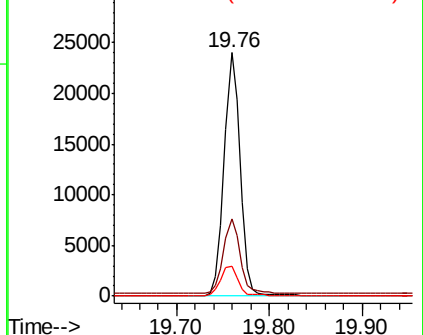



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.145 ng

RT: 21.23 min Scan# 1619

Delta R.T. -0.01 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13

Instrument :

BNA_E

ClientSampleId :

RE134D2-20191202


Tot Ion:149 Resp: 9786

Ion Ratio Lower Upper

149 100

167 6.5 5.0 7.6




279 0.9 0.7 1.1



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

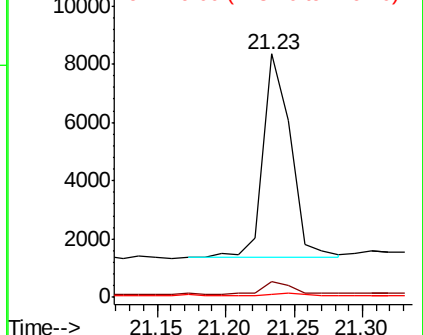

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.74 min Scan# 2165

Delta R.T. -0.02 min

Lab File: BE100811.D

Acq: 10 Dec 2019 15:13


Tgt Ion:264 Resp: 32592

Ion Ratio Lower Upper

264 100

260 23.7 19.4 29.2

265 25.2 21.8 32.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

