


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121019\
 Data File : BE100822.D
 Acq On : 10 Dec 2019 22:38
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 04 17:18:11 2019

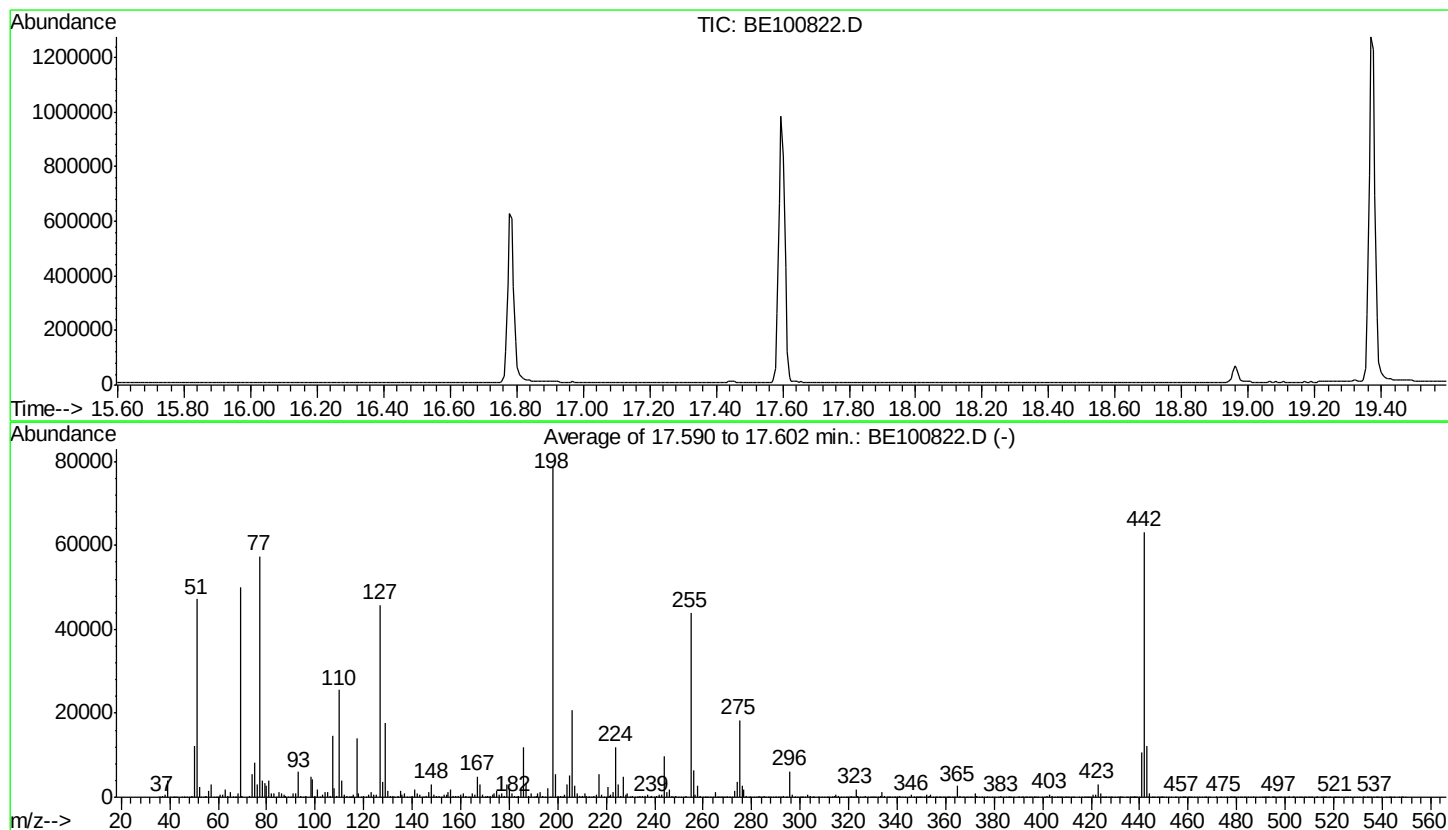

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.8	47255	PASS
68	69	0.00	2	1.8	920	PASS
69	198	0.00	100	63.4	50073	PASS
70	69	0.00	2	0.6	302	PASS
127	198	10	80	58.0	45875	PASS
197	198	0.00	2	0.2	162	PASS
198	198	100	100	100.0	79040	PASS
199	198	5	9	6.9	5445	PASS
275	198	10	60	23.2	18358	PASS
365	198	1	100	3.5	2741	PASS
441	198	0.01	100	13.4	10560	PASS
442	198	50	100	80.0	63210	PASS
443	442	15	24	19.2	12137	PASS