


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE121117\  
Data File : BE094970.D  
Acq On : 11 Dec 2017 11:57  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE113017.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Dec 01 13:33:28 2017

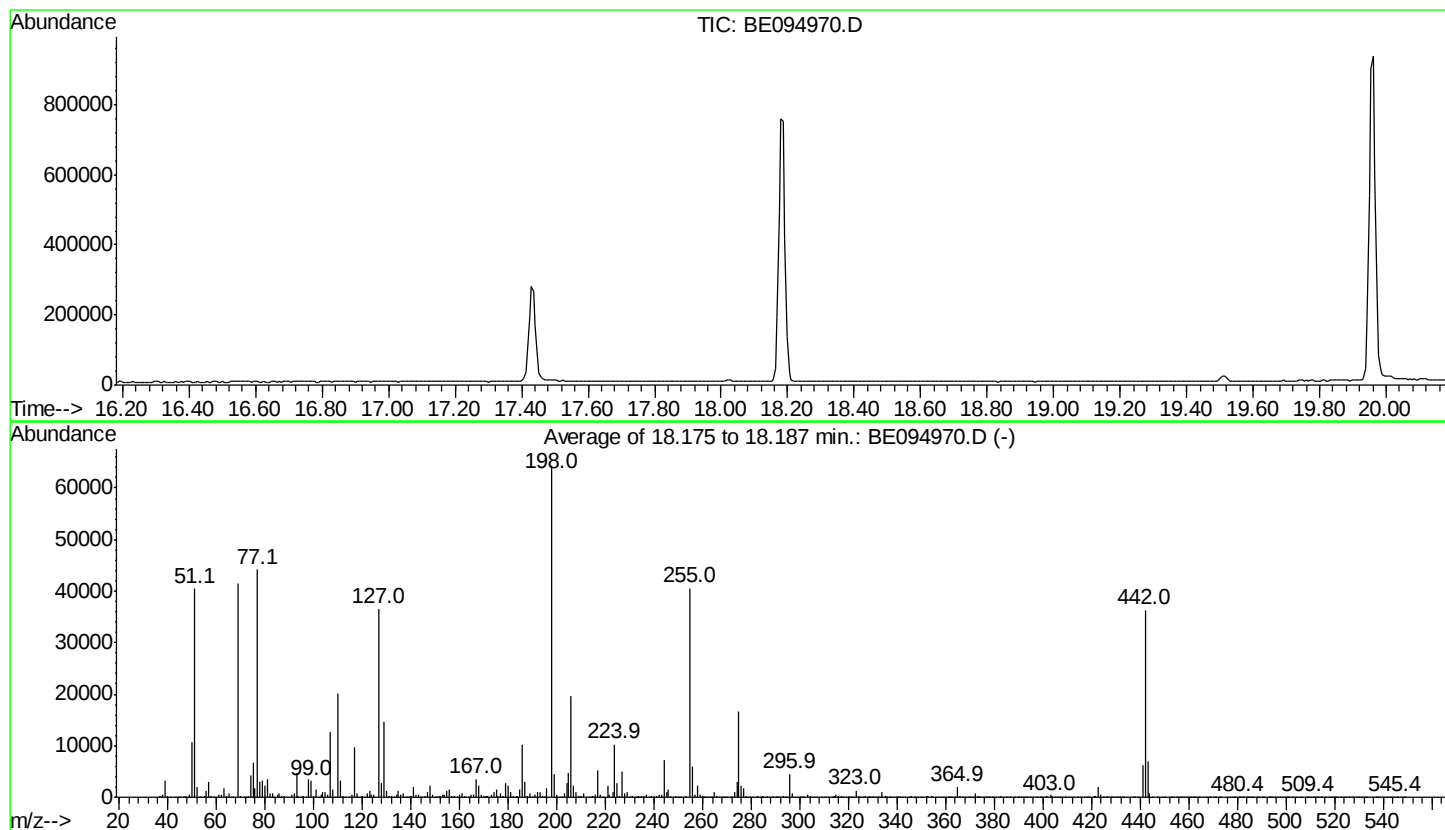

AutoFind: Scans 2653, 2654, 2655; Background Corrected with Scan 2647

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 62.9      | 40475   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 64.6      | 41554   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 234     | PASS             |
| 127         | 198          | 10           | 80           | 56.8      | 36565   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 64341   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 4382    | PASS             |
| 275         | 198          | 10           | 60           | 26.0      | 16735   | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 2033    | PASS             |
| 441         | 442          | 0.01         | 24           | 17.5      | 6336    | PASS             |
| 442         | 198          | 50           | 100          | 56.4      | 36277   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 6961    | PASS             |