

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121118\
 Data File : BE098349.D
 Acq On : 12 Dec 2018 1:07
 Operator : SJ/JU
 Sample : J6314-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Dec 12 17:26:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	1144	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	4961	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	3185	0.40	ng	0.00
19) Phenanthrene-d10	17.28	188	8466	0.40	ng	0.00
27) Chrysene-d12	21.46	240	10008	0.40	ng	0.00
34) Perylene-d12	24.01	264	9683	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	468	0.17	ng	0.00
5) Phenol-d6	7.04	99	394	0.10	ng	0.00
8) Nitrobenzene-d5	9.03	82	1962	0.43	ng	0.01
11) 2-Methylnaphthalene-d10	12.27	152	3289	0.41	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	577	0.49	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	8121	0.60	ng	0.00
25) Fluoranthene-d10	19.31	212	50307	0.46	ng	0.00
29) Terphenyl-d14	19.90	244	16980	0.70	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.37	88	175	0.088	ng	# 1
22) Pentachlorophenol	16.97	266	12	0.032	ng	# 72
32) Bis(2-ethylhexyl)phthalate	21.37	149	3985	0.069	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121118\
Data File : BE098349.D
Acq On : 12 Dec 2018 1:07
Operator : SJ/JU
Sample : J6314-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Dec 12 17:26:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

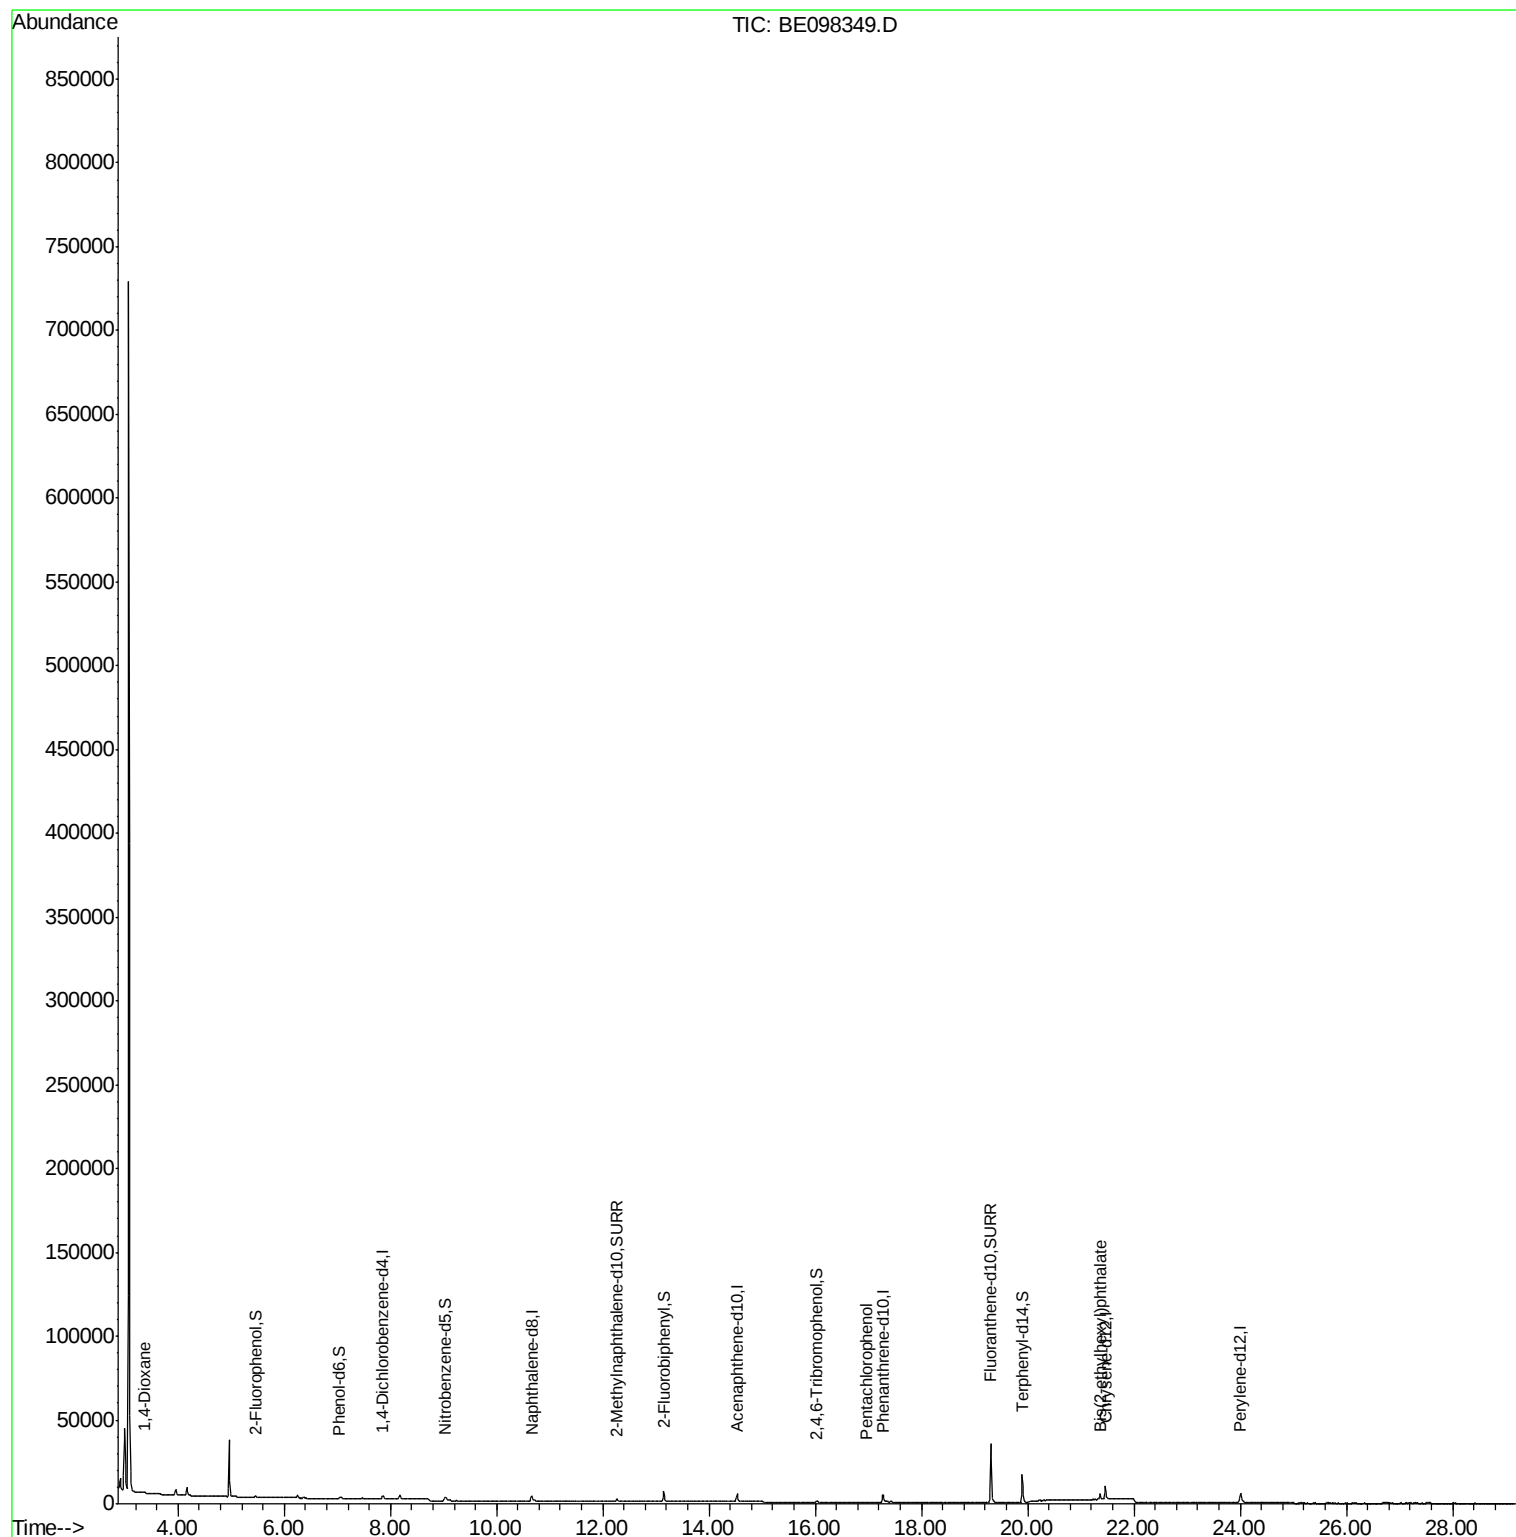




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 434
Delta R.T. -0.00 min
Lab File: BE098349.D
Acq: 12 Dec 2018 1:07

Instrument :
BNA_E
ClientSampleId :

Tot Ion:152 Resp: 1144
Ion Ratio Lower Upper
152 100
150 164.6 124.2 186.4
115 69.0 53.9 80.9

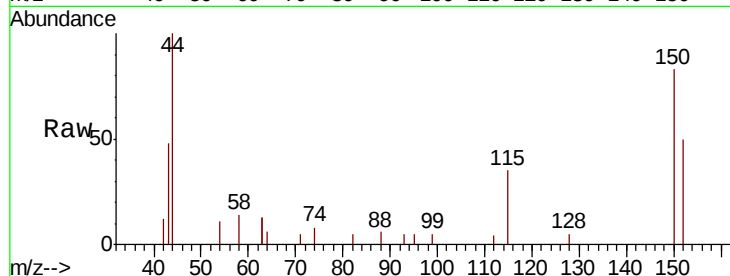


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

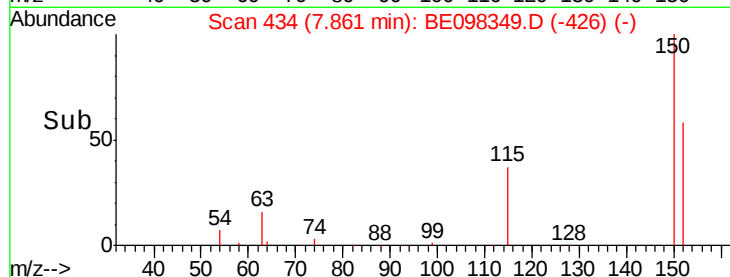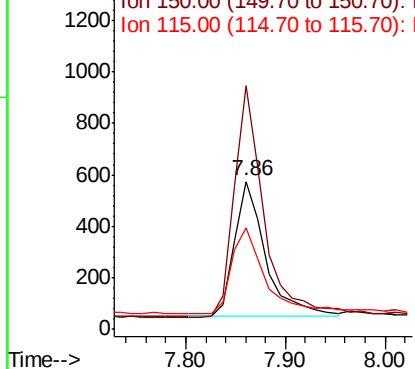



#2

1,4-Dioxane
Concen: 0.088 ng
RT: 3.37 min Scan# 44
Delta R.T. -0.00 min
Lab File: BE098349.D
Acq: 12 Dec 2018 1:07

Tgt Ion: 88 Resp: 175
Ion Ratio Lower Upper
88 100
58 70.3 75.0 112.6#
43 333.1 38.3 57.5#

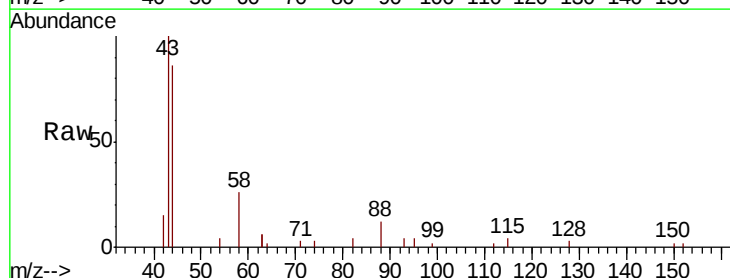

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

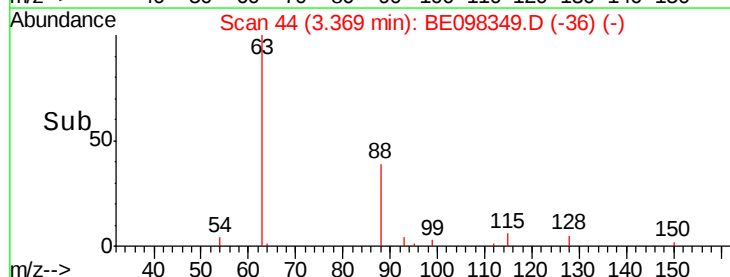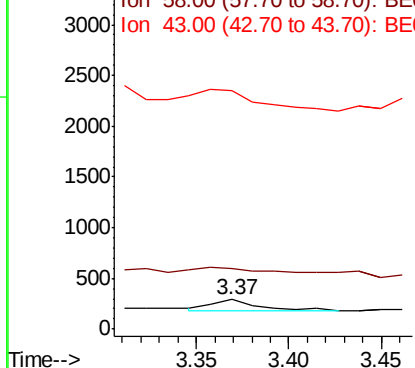



#4

2-Fluorophenol

Concen: 0.175 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 112 Resp: 468

Ion Ratio Lower Upper

112 100

64 78.4 59.8 89.8



63 195.5 133.7 200.5

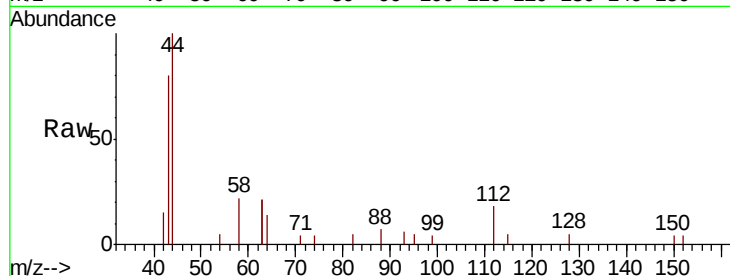

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

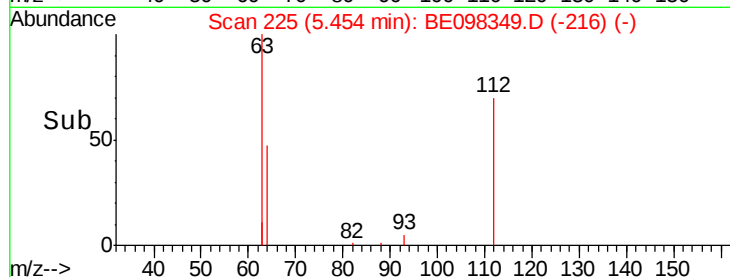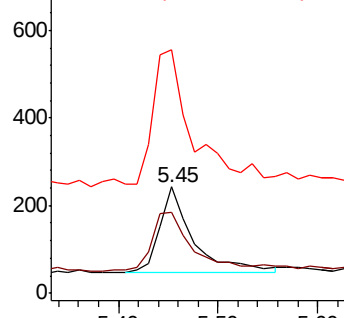

Time-->



#5

Phenol-d6

Concen: 0.104 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07


Tgt Ion: 99 Resp: 394

Ion Ratio Lower Upper

99 100

42 36.3 26.3 39.5



71 37.8 33.6 50.4

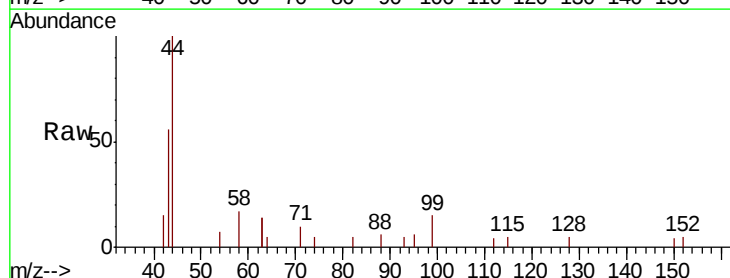

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

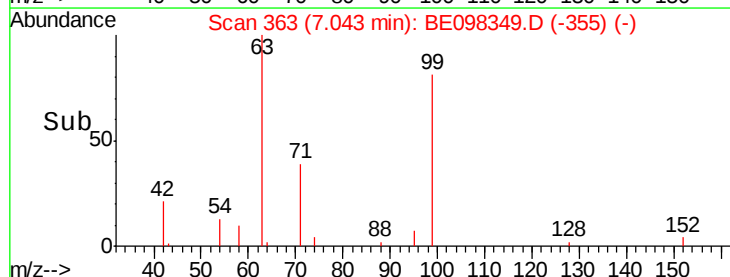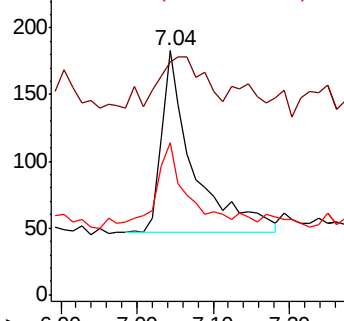

Time-->



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 655

Delta R.T. 0.00 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 4961


Ion Ratio Lower Upper

136 100

137 13.2 9.2 13.8

54 42.7 28.4 42.6#

68 8.0 5.4 8.0



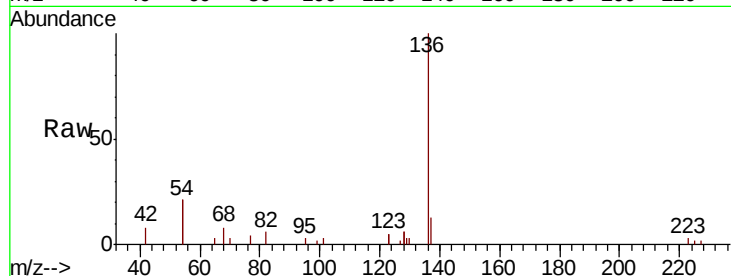


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

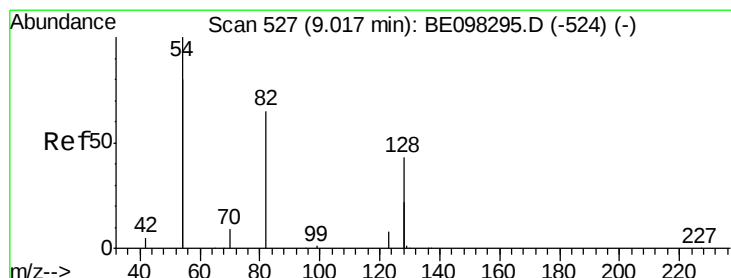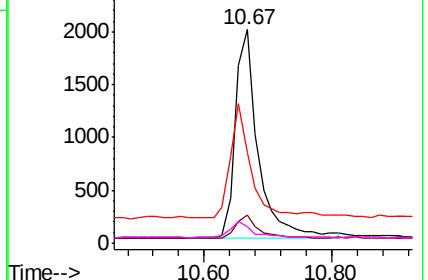

#8

Nitrobenzene-d5

Concen: 0.434 ng

RT: 9.03 min Scan# 529

Delta R.T. 0.01 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07


Tgt Ion: 82 Resp: 1962

Ion Ratio Lower Upper

82 100

128 167.1 102.4 153.6#



54 283.2 221.8 332.8

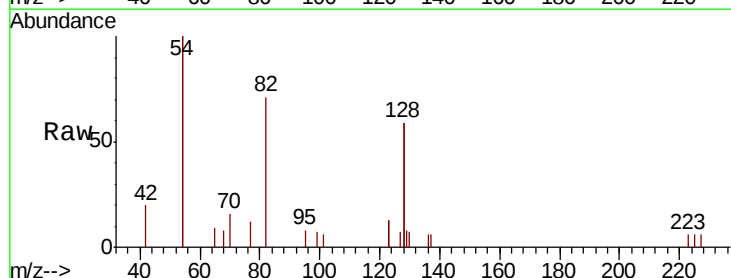


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



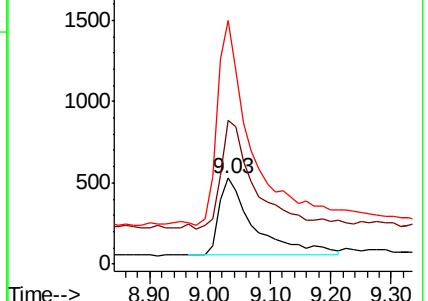



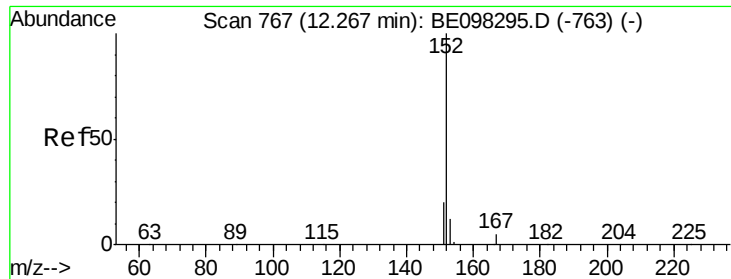

#11
 2-Methylnaphthalene-d10
 Concen: 0.408 ng
 RT: 12.27 min Scan# 768
 Delta R.T. -0.00 min
 Lab File: BE098349.D
 Acq: 12 Dec 2018 1:07




Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:152 Resp: 3289
 Ion Ratio Lower Upper
 152 100
 151 18.8 16.2 24.4

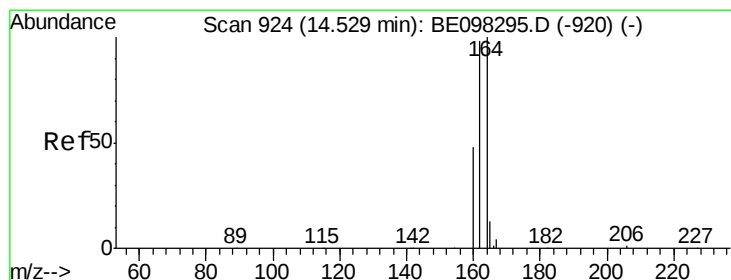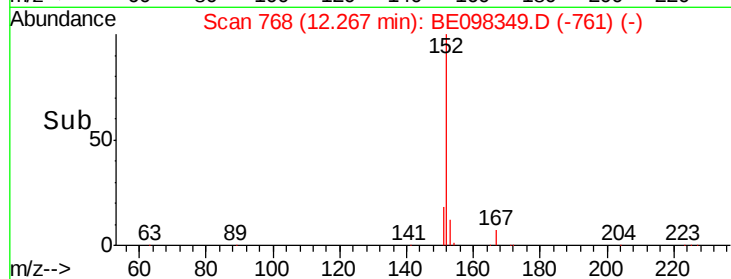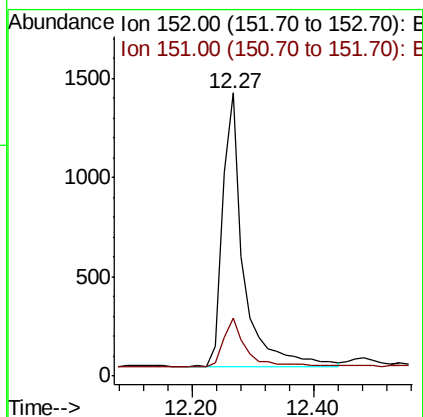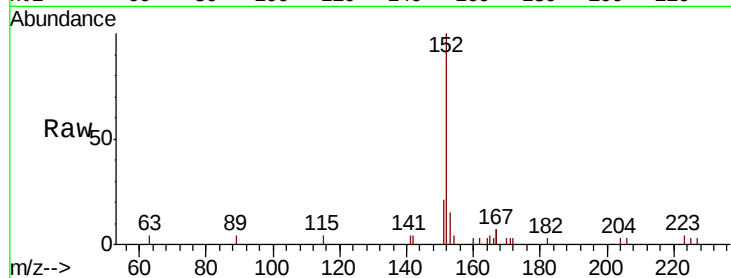

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.53 min Scan# 925
 Delta R.T. -0.00 min
 Lab File: BE098349.D
 Acq: 12 Dec 2018 1:07

Tgt Ion:164 Resp: 3185
 Ion Ratio Lower Upper
 164 100
 162 96.9 77.6 116.4
 160 47.9 36.0 54.0

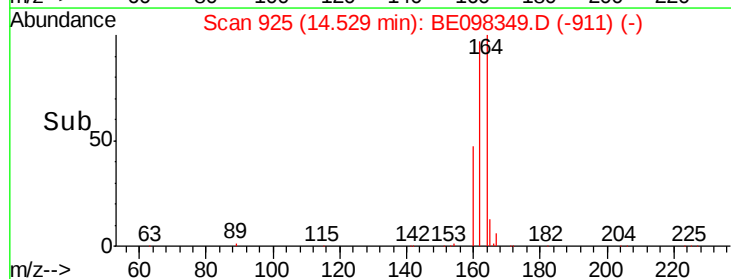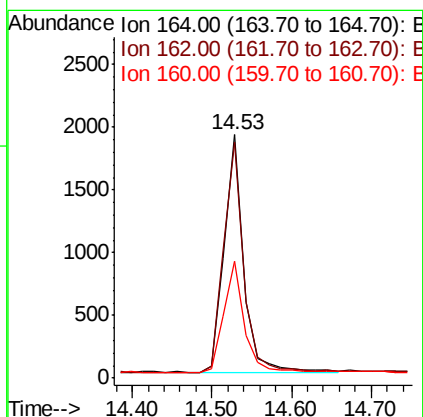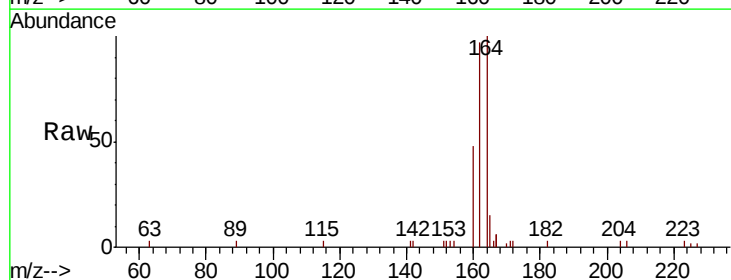






#14
 2,4,6-Tribromophenol
 Concen: 0.493 ng
 RT: 16.02 min Scan# 1042
 Delta R.T. -0.00 min
 Lab File: BE098349.D
 Acq: 12 Dec 2018 1:07

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:330 Resp: 577
 Ion Ratio Lower Upper
 330 100
 332 94.5 76.2 114.4
 141 43.8 39.0 58.4

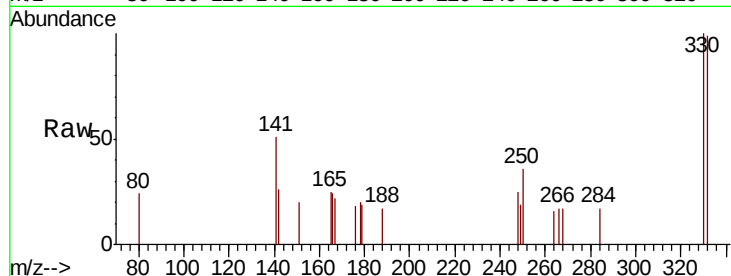


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


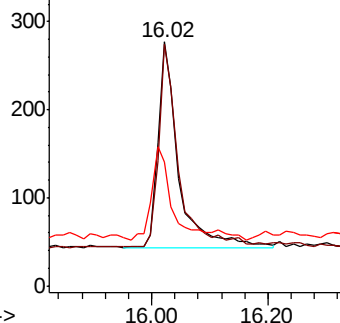


#15
 2-Fluorobiphenyl
 Concen: 0.605 ng
 RT: 13.15 min Scan# 829
 Delta R.T. -0.00 min
 Lab File: BE098349.D
 Acq: 12 Dec 2018 1:07

Tgt Ion:172 Resp: 8121
 Ion Ratio Lower Upper
 172 100
 171 33.7 27.5 41.3
 170 24.3 19.6 29.4

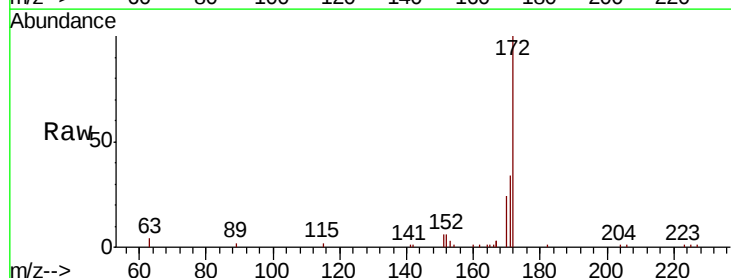

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

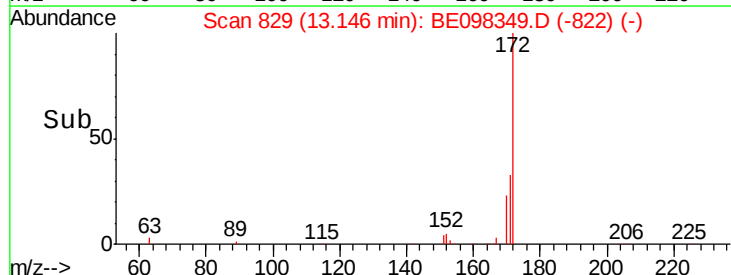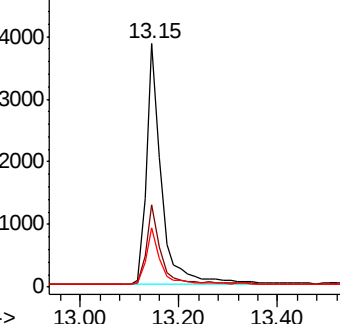



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.28 min Scan# 1150

Delta R.T. -0.00 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 8466

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 8.7 7.2 10.8

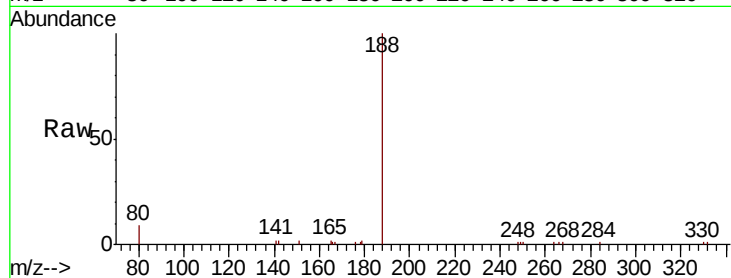

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

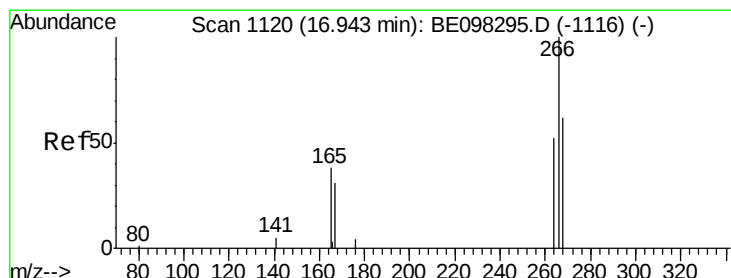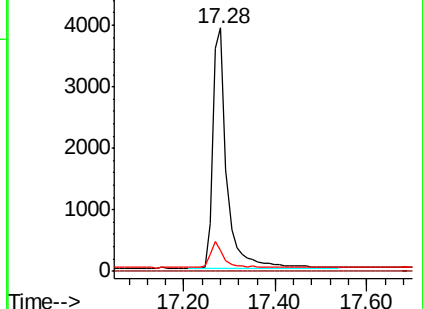

#22

Pentachlorophenol

Concen: 0.032 ng

RT: 16.97 min Scan# 1123

Delta R.T. 0.02 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07


Tgt Ion:266 Resp: 12

Ion Ratio Lower Upper

266 100

264 92.0 59.0 88.4#



268 98.0 55.1 82.7#

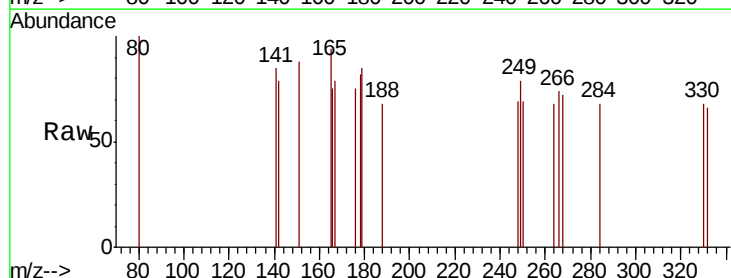


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E



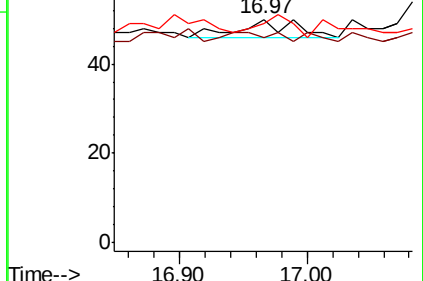



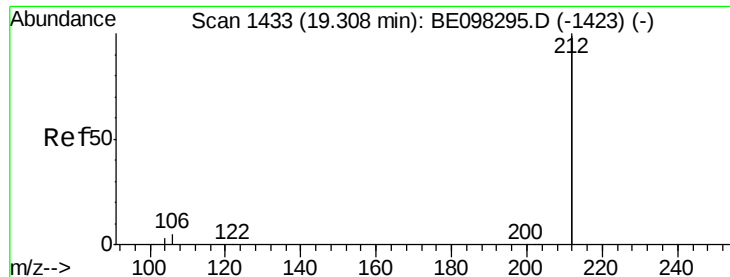

#25
 Fluoranthene-d10
 Concen: 0.463 ng
 RT: 19.31 min Scan# 1434
 Delta R.T. -0.00 min
 Lab File: BE098349.D
 Acq: 12 Dec 2018 1:07




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:212 Resp: 50307
 Ion Ratio Lower Upper
 212 100
 106 2.7 2.2 3.2
 104 1.6 1.3 1.9

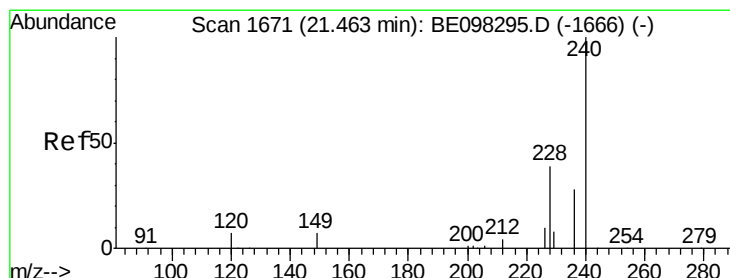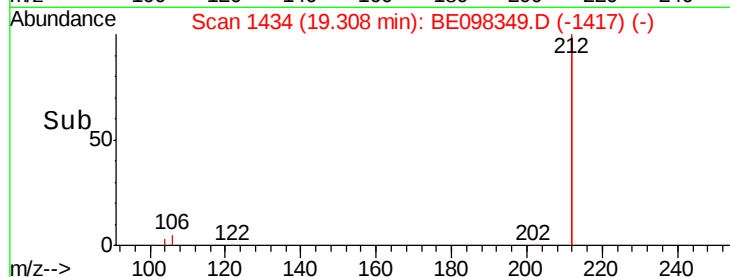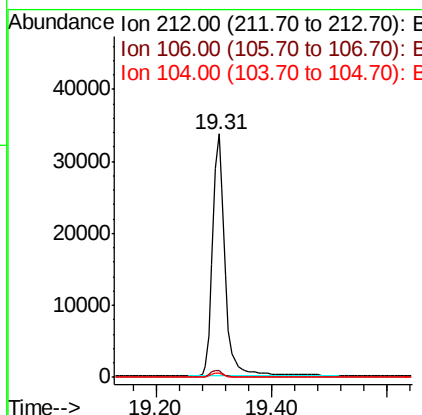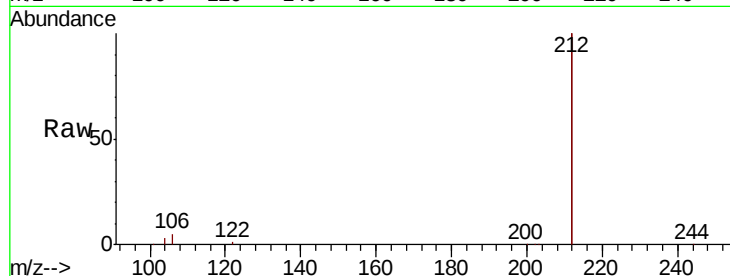

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.46 min Scan# 1672
 Delta R.T. -0.00 min
 Lab File: BE098349.D
 Acq: 12 Dec 2018 1:07

Tgt Ion:240 Resp: 10008
 Ion Ratio Lower Upper
 240 100
 120 8.5 9.5 14.3#
 236 27.2 22.7 34.1

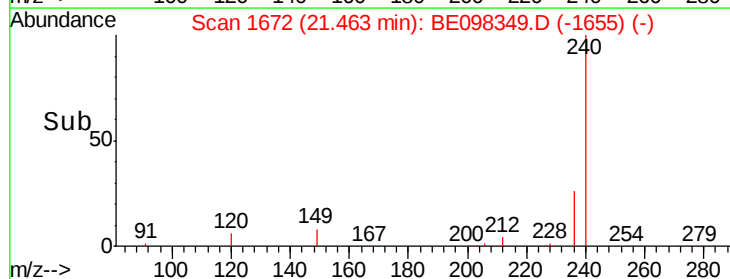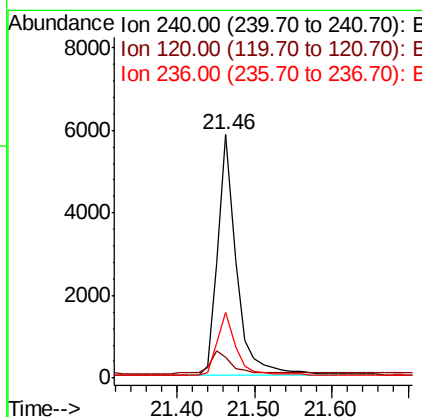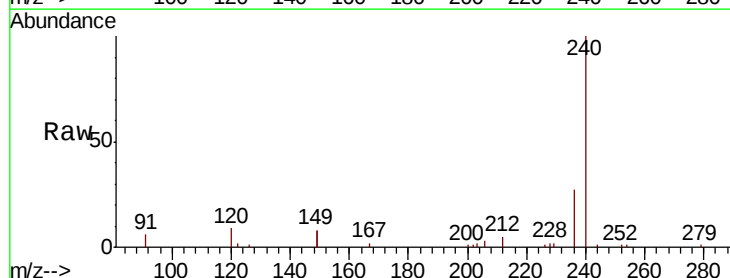



#29

Terphenyl-d14

Concen: 0.698 ng

RT: 19.90 min Scan# 1537

Delta R.T. -0.01 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07

Instrument :

BNA_E

ClientSampleId :


Tot Ion:244 Resp: 16980

Ion Ratio Lower Upper

244 100

212 33.9 27.4 41.0

122 10.9 8.3 12.5



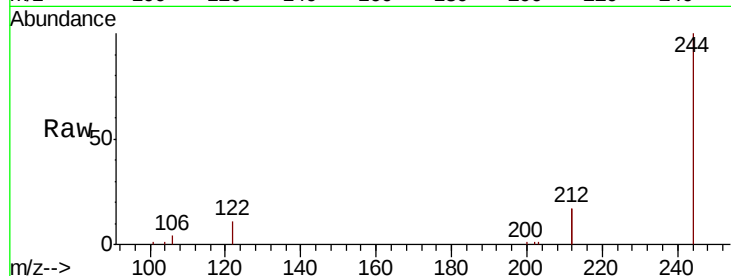


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

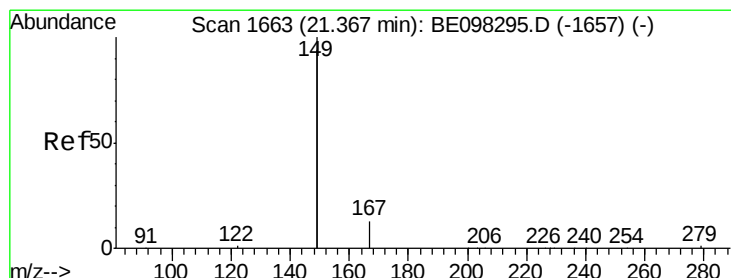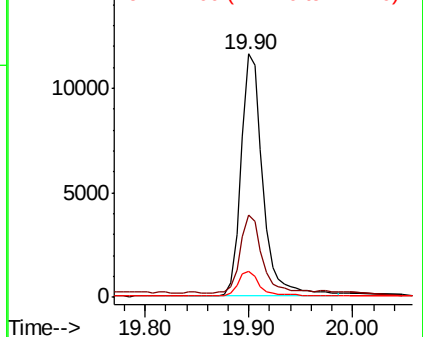

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.069 ng

RT: 21.37 min Scan# 1664

Delta R.T. -0.00 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07


Tgt Ion:149 Resp: 3985

Ion Ratio Lower Upper

149 100

167 7.5 5.7 8.5

279 1.2 1.0 1.4


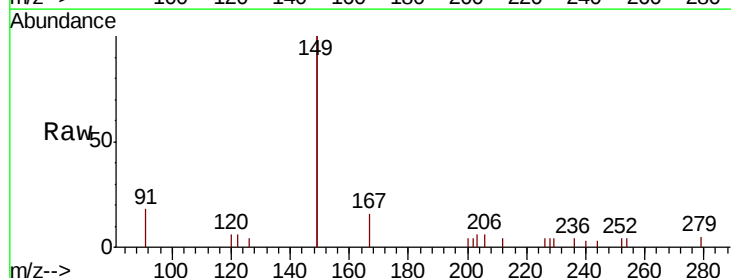





Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

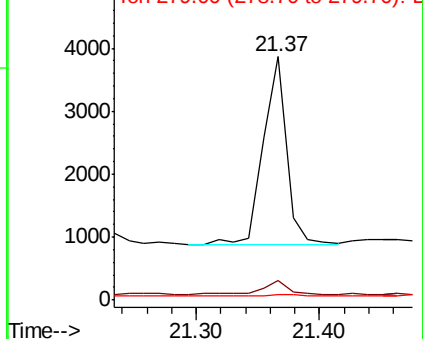

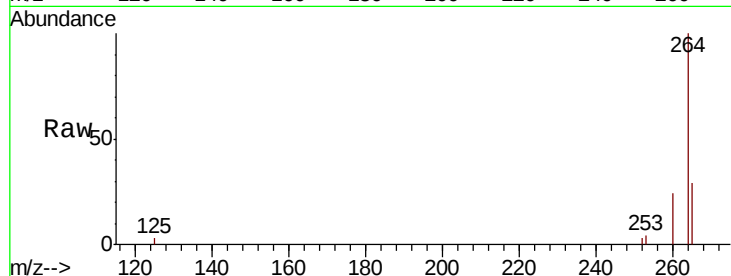

#34

Pervlene-d12

Concen: 0.400 ng

RT: 24.01 min Scan# 2273

Delta R.T. -0.00 min

Lab File: BE098349.D

Acq: 12 Dec 2018 1:07

Instrument :

BNA_E

ClientSampleId :

Tot Ion:264 Resp: 9683

Ion Ratio Lower Upper

264 100

260 24.1 20.2 30.2

265 28.8 25.2 37.8

