

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121118\
 Data File : BE098341.D
 Acq On : 11 Dec 2018 20:12
 Operator : SJ/JU
 Sample : J6288-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW301D-20181206

Quant Time: Dec 12 02:01:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	1090	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	4738	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	3104	0.40	ng	0.00
19) Phenanthrene-d10	17.28	188	7732	0.40	ng	0.00
27) Chrysene-d12	21.46	240	9841	0.40	ng	0.00
34) Perylene-d12	24.01	264	9344	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	448	0.18	ng	0.00
5) Phenol-d6	7.04	99	335	0.09	ng	0.00
8) Nitrobenzene-d5	9.03	82	1795	0.42	ng	0.01
11) 2-Methylnaphthalene-d10	12.27	152	3233	0.42	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	488	0.43	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	6040	0.46	ng	0.00
25) Fluoranthene-d10	19.31	212	48703	0.49	ng	0.00
29) Terphenyl-d14	19.90	244	13953	0.58	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.37	88	419	0.222	ng	# 6
32) Bis(2-ethylhexyl)phthalate	21.37	149	7977	0.140	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121118\
Data File : BE098341.D
Acq On : 11 Dec 2018 20:12
Operator : SJ/JU
Sample : J6288-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW301D-20181206

Quant Time: Dec 12 02:01:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

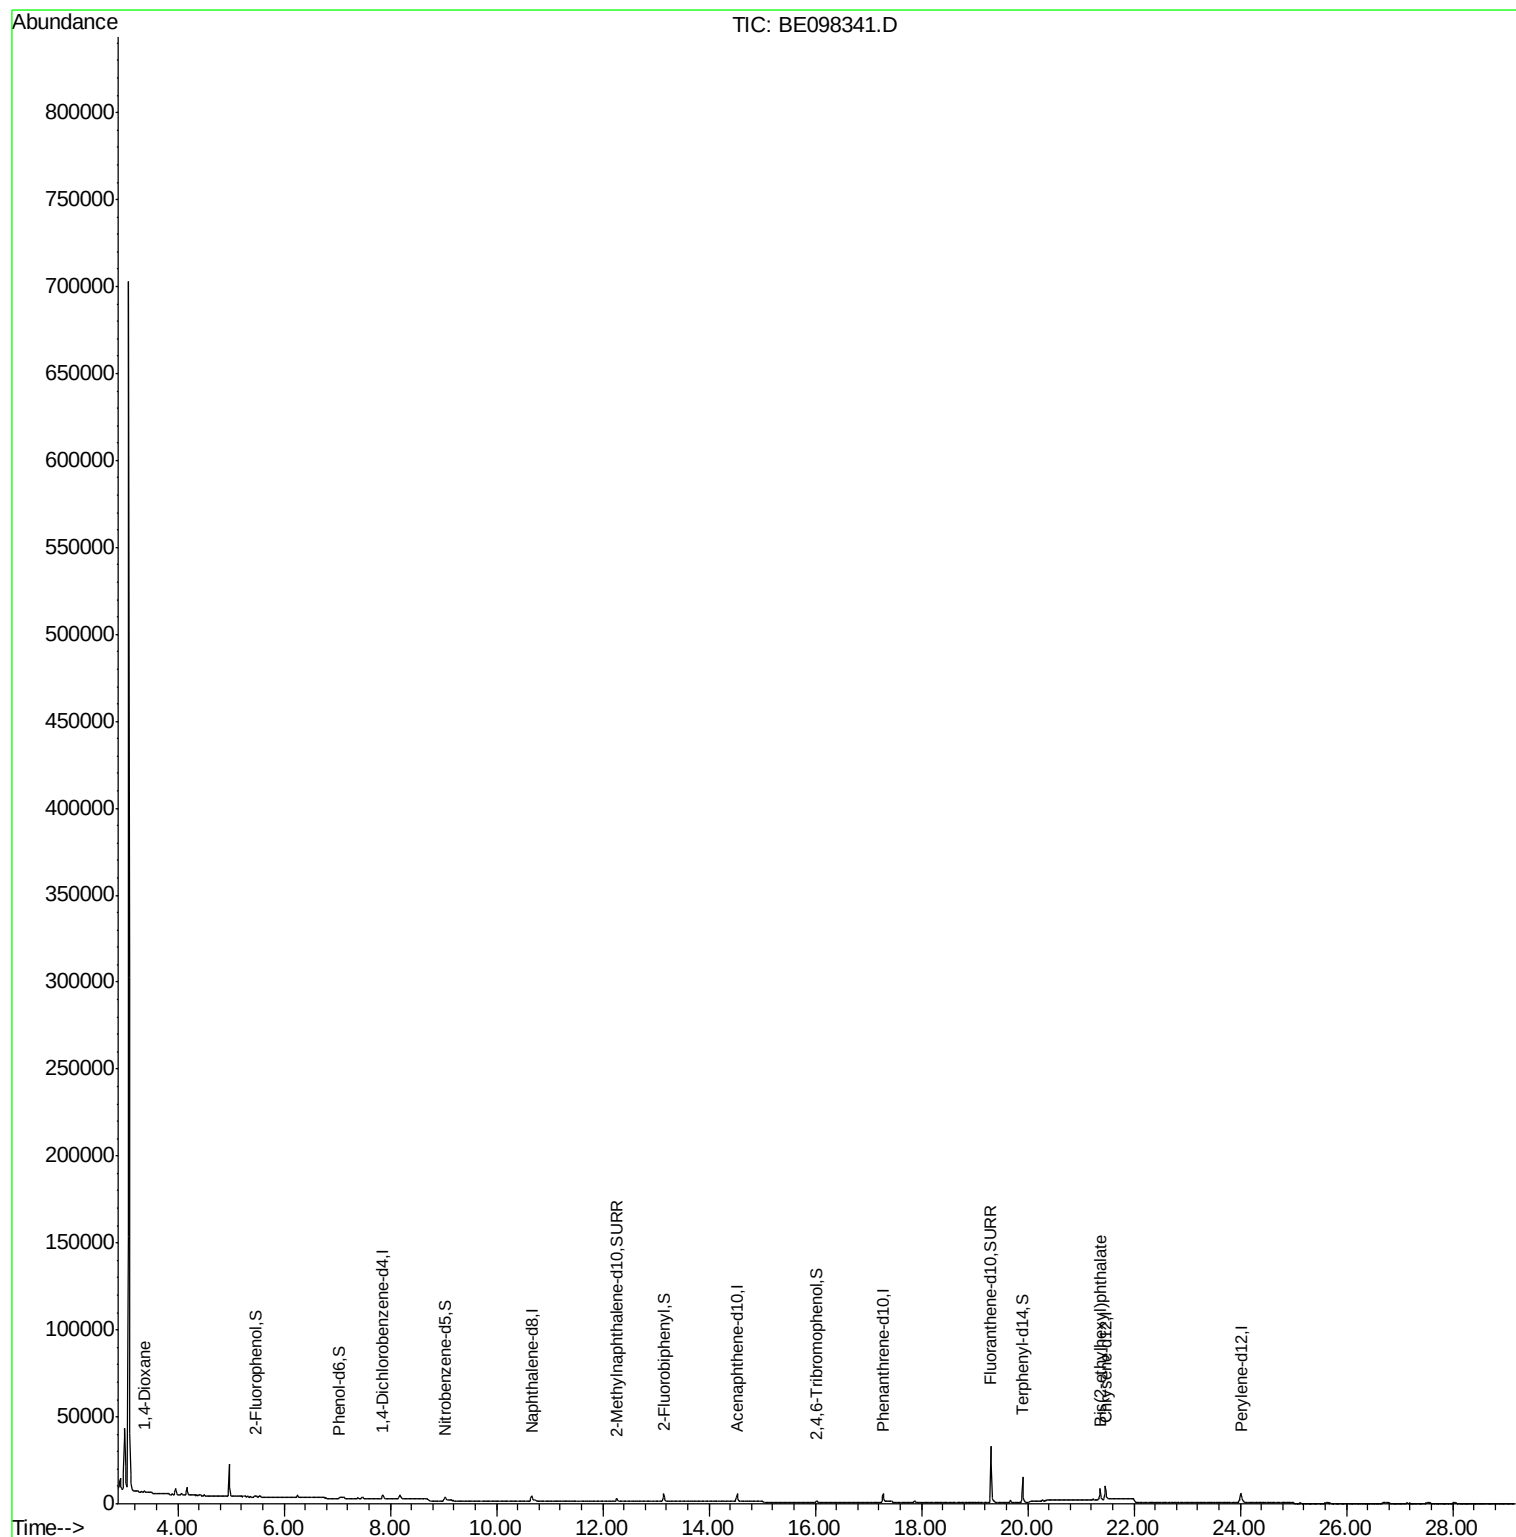

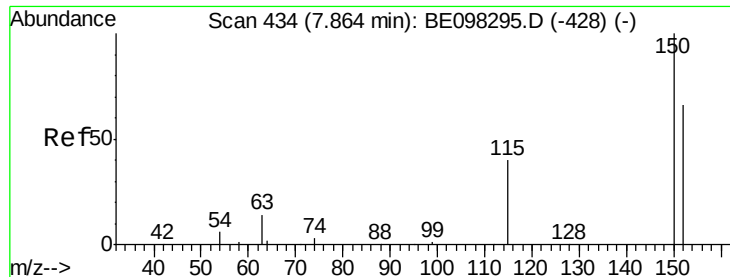


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 434
Delta R.T. -0.00 min
Lab File: BE098341.D
Acq: 11 Dec 2018 20:12

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW301D-20181206

Tot Ion:152 Resp: 1090
Ion Ratio Lower Upper
152 100
150 152.9 124.2 186.4
115 71.5 53.9 80.9

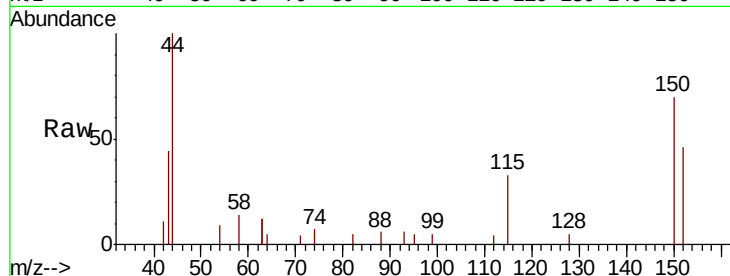


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

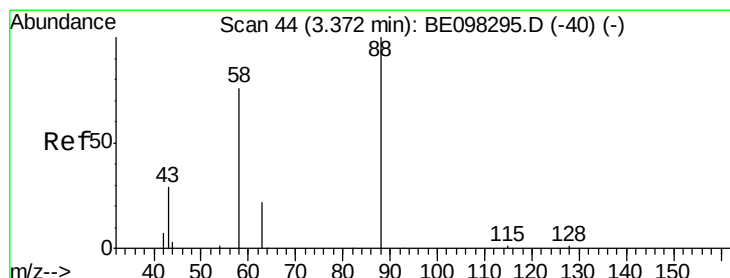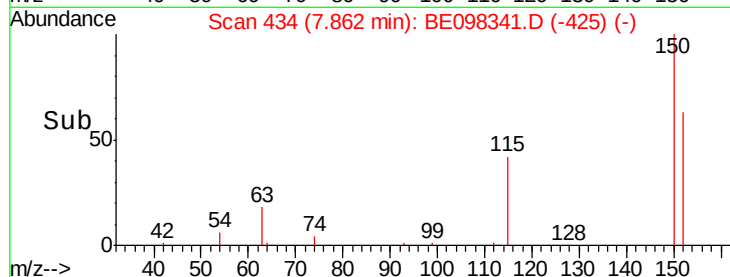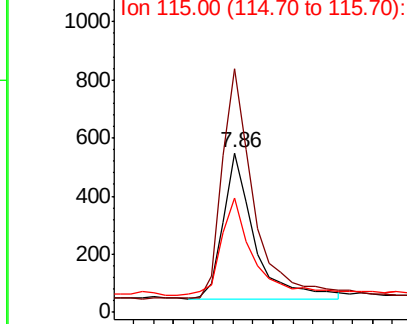



#2


1,4-Dioxane
Concen: 0.222 ng
RT: 3.37 min Scan# 44
Delta R.T. -0.00 min
Lab File: BE098341.D
Acq: 11 Dec 2018 20:12

Tgt Ion: 88 Resp: 419
Ion Ratio Lower Upper
88 100
58 116.2 75.0 112.6#
43 203.8 38.3 57.5#

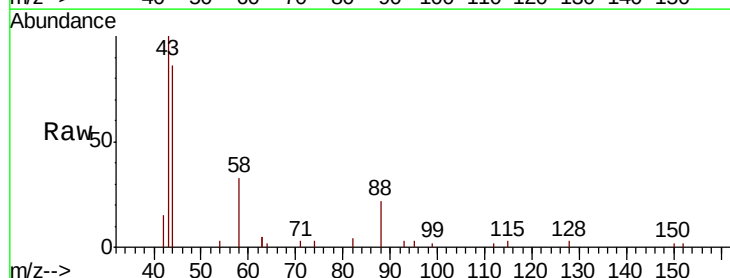

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

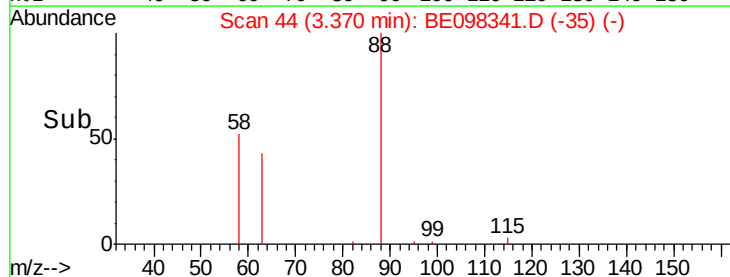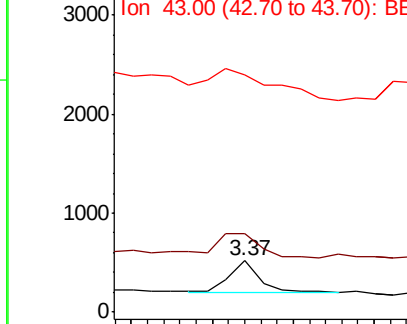

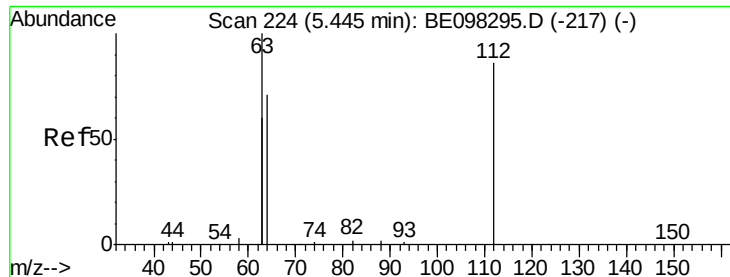

#4

2-Fluorophenol

Concen: 0.176 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW301D-20181206


Tot Ion:112 Resp: 448

Ion Ratio Lower Upper

112 100

64 62.1 59.8 89.8

63 204.2 133.7 200.5#

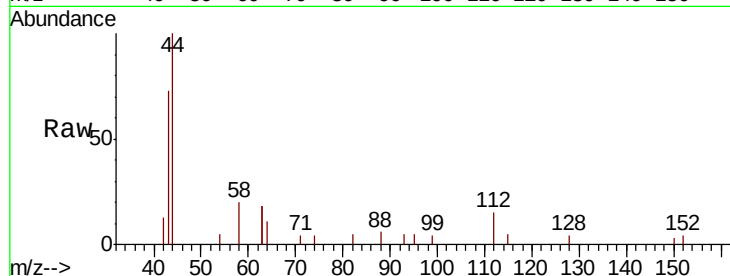


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0


Ion 63.00 (62.70 to 63.70): BE0

5.45

Time-->

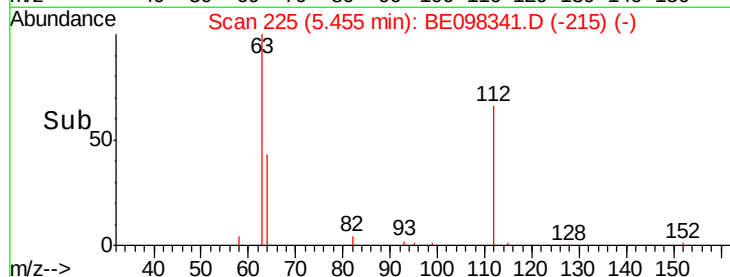

Time-->

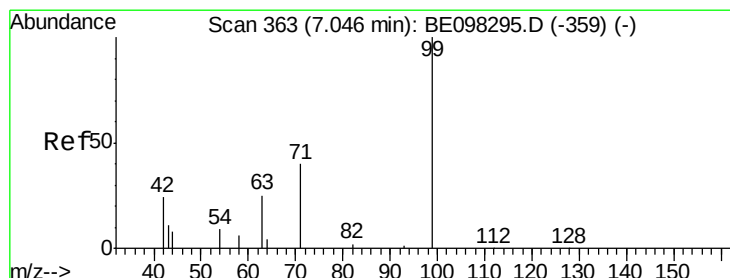

#5

Phenol-d6

Concen: 0.093 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12


Tgt Ion: 99 Resp: 335

Ion Ratio Lower Upper

99 100

42 31.0 26.3 39.5

71 63.9 33.6 50.4#

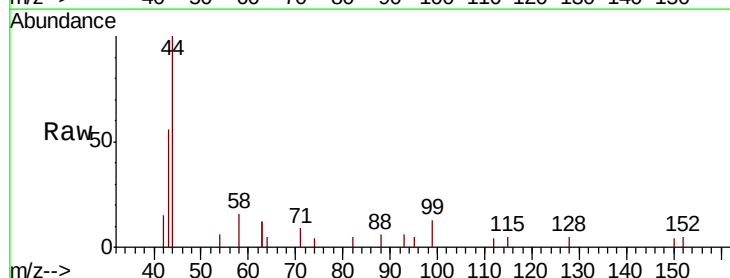


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0


Ion 71.00 (70.70 to 71.70): BE0

7.04

Time-->

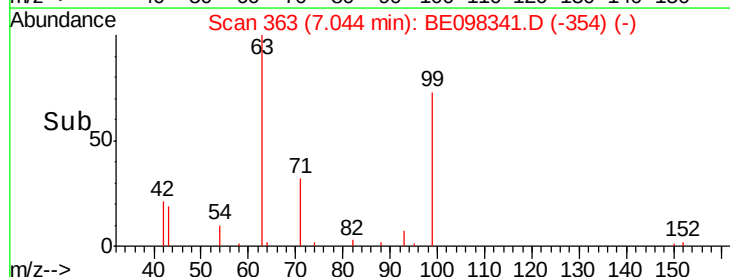

Time-->



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. 0.00 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW301D-20181206

Tot Ion:136 Resp: 4738


Ion Ratio Lower Upper

136 100

137 13.0 9.2 13.8

54 43.9 28.4 42.6#

68 8.0 5.4 8.0






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

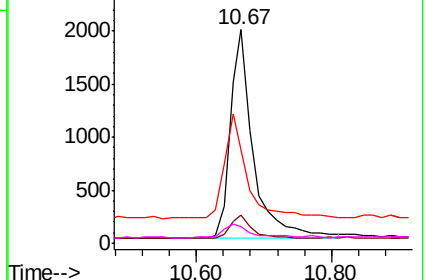

#8

Nitrobenzene-d5

Concen: 0.416 ng

RT: 9.03 min Scan# 528

Delta R.T. 0.01 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12


Tgt Ion: 82 Resp: 1795

Ion Ratio Lower Upper

82 100

128 162.1 102.4 153.6#



54 284.1 221.8 332.8




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

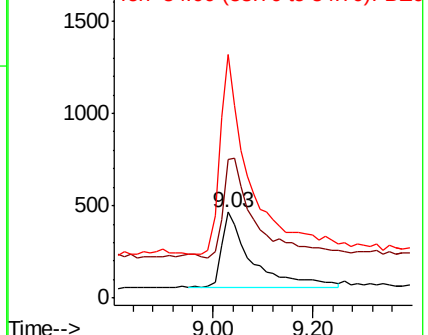

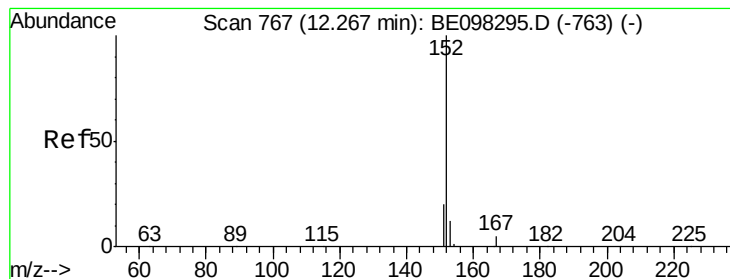

#11

2-Methylnaphthalene-d10

Concen: 0.420 ng

RT: 12.27 min Scan# 767

Delta R.T. 0.00 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12

Instrument :

BNA_E

ClientSampleId :


BPS1-TT-MW301D-20181206

Tot Ion:152 Resp: 3233

Ion Ratio Lower Upper




152 100

151 18.5 16.2 24.4

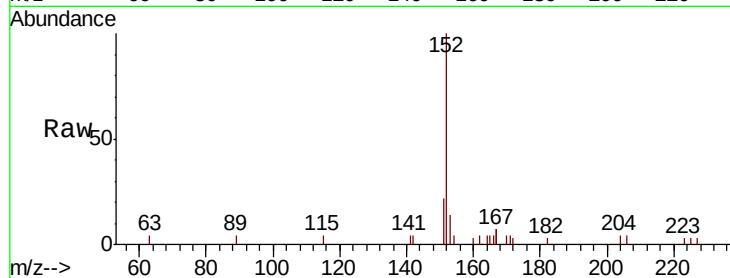

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

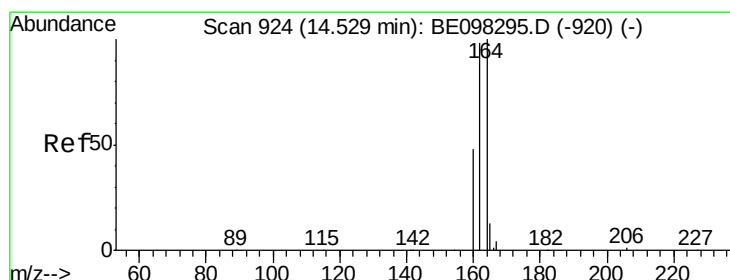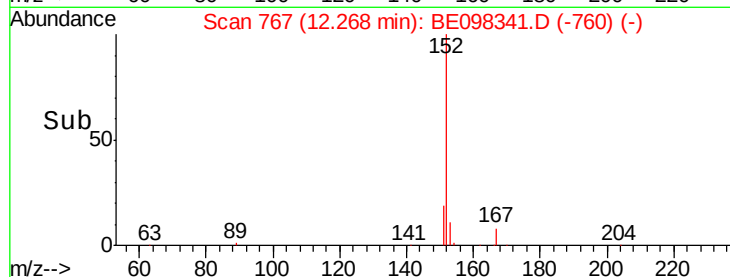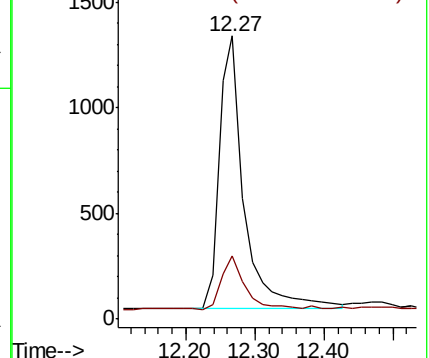

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.53 min Scan# 924

Delta R.T. 0.00 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12


Tgt Ion:164 Resp: 3104

Ion Ratio Lower Upper

164 100

162 97.0 77.6 116.4



160 49.2 36.0 54.0

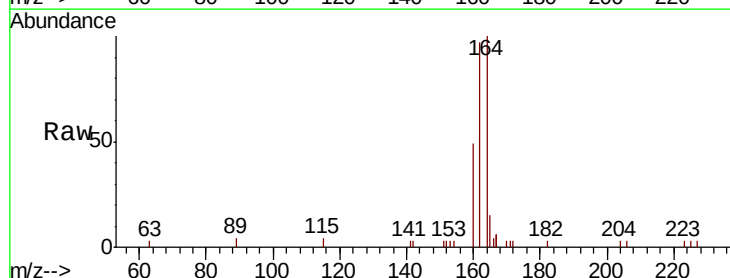


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

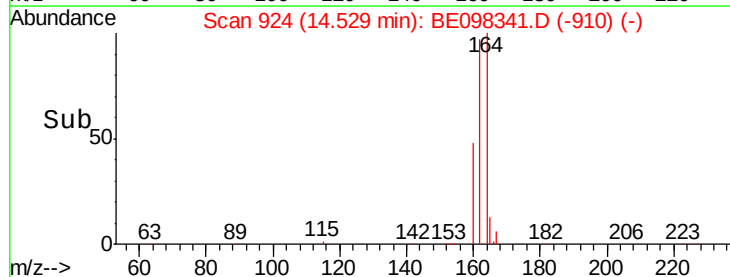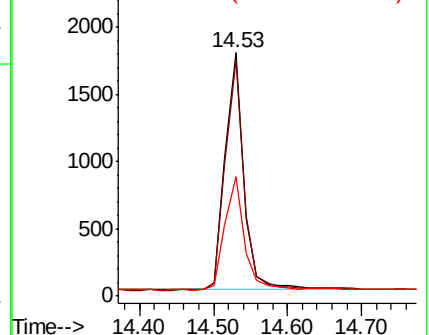







#14
 2,4,6-Tribromophenol
 Concen: 0.428 ng
 RT: 16.02 min Scan# 1041
 Delta R.T. -0.00 min
 Lab File: BE098341.D
 Acq: 11 Dec 2018 20:12

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW301D-20181206

Tot Ion:330 Resp: 488
 Ion Ratio Lower Upper
 330 100
 332 99.4 76.2 114.4
 141 43.2 39.0 58.4

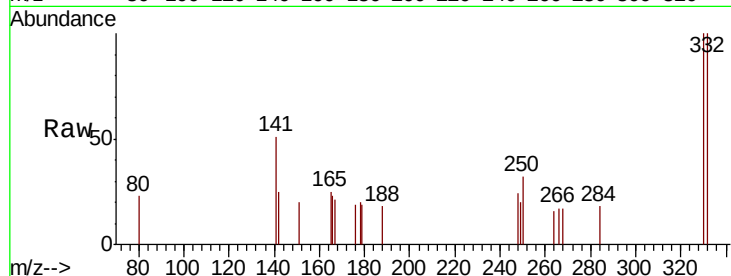


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


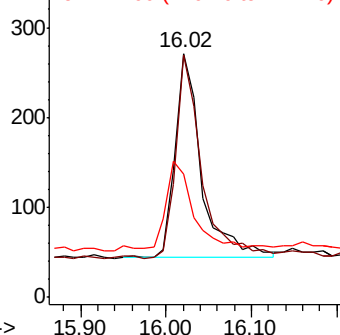



#15
 2-Fluorobiphenyl
 Concen: 0.461 ng
 RT: 13.15 min Scan# 828
 Delta R.T. 0.00 min
 Lab File: BE098341.D
 Acq: 11 Dec 2018 20:12

Tgt Ion:172 Resp: 6040
 Ion Ratio Lower Upper
 172 100
 171 32.3 27.5 41.3
 170 24.4 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

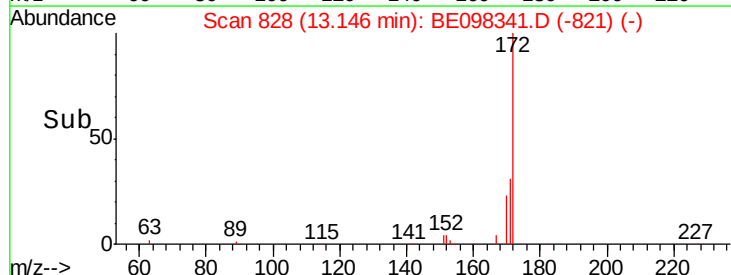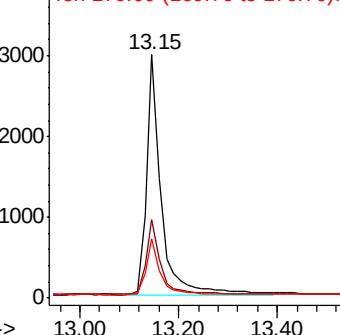



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.28 min Scan# 1149

Delta R.T. -0.00 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW301D-20181206


Tot Ion:188 Resp: 7732

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 8.3 7.2 10.8

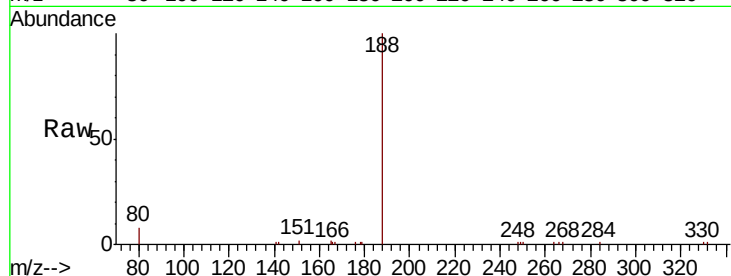

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

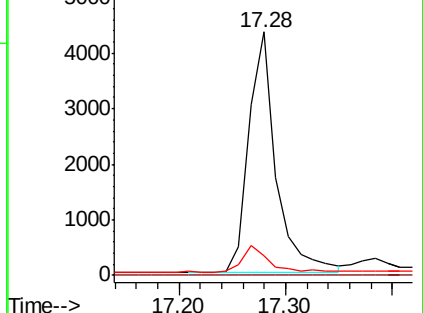

#25

Fluoranthene-d10

Concen: 0.491 ng

RT: 19.31 min Scan# 1433

Delta R.T. 0.00 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12


Tgt Ion:212 Resp: 48703

Ion Ratio Lower Upper

212 100

106 2.7 2.2 3.2



104 1.5 1.3 1.9




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

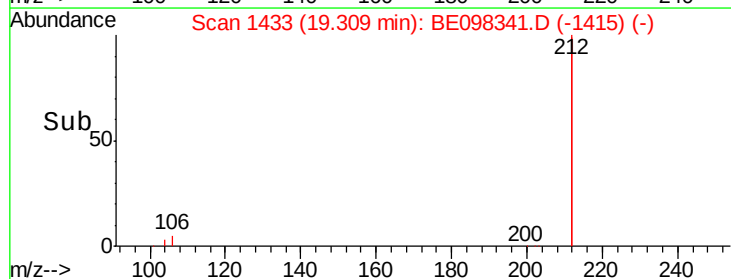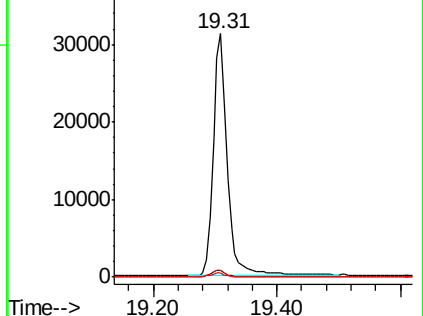



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.46 min Scan# 1671

Delta R.T. -0.00 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW301D-20181206


Tot Ion:240 Resp: 9841

Ion Ratio Lower Upper

240 100

120 8.9 9.5 14.3#




236 27.4 22.7 34.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

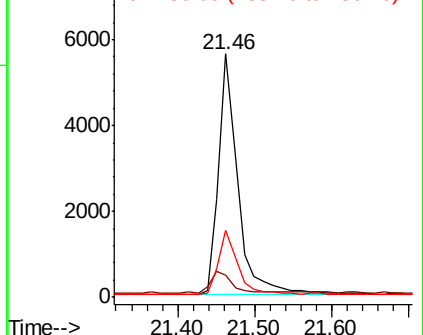

#29

Terphenyl-d14

Concen: 0.583 ng

RT: 19.90 min Scan# 1536

Delta R.T. -0.01 min

Lab File: BE098341.D

Acq: 11 Dec 2018 20:12


Tgt Ion:244 Resp: 13953

Ion Ratio Lower Upper

244 100

212 35.1 27.4 41.0



122 11.1 8.3 12.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



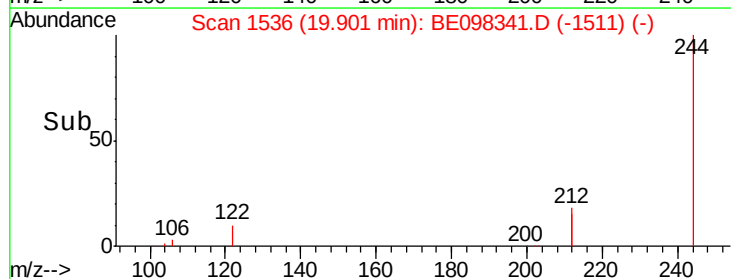
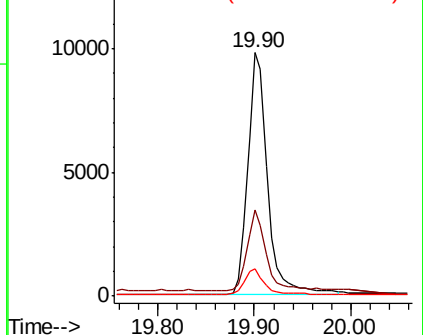




#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.140 ng
 RT: 21.37 min Scan# 1663
 Delta R.T. -0.00 min
 Lab File: BE098341.D
 Acq: 11 Dec 2018 20:12

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW301D-20181206

Tot Ion:149 Resp: 7977
 Ion Ratio Lower Upper
 149 100
 167 6.5 5.7 8.5
 279 1.4 1.0 1.4#

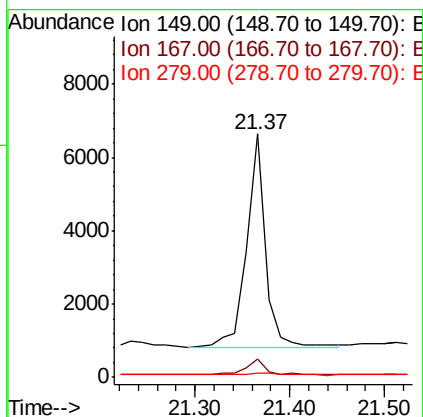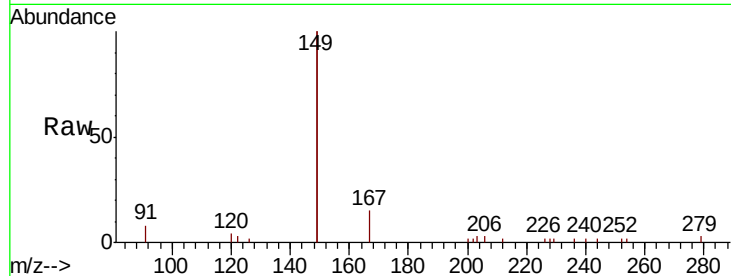

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.01 min Scan# 2273
 Delta R.T. 0.00 min
 Lab File: BE098341.D
 Acq: 11 Dec 2018 20:12

Tgt Ion:264 Resp: 9344
 Ion Ratio Lower Upper
 264 100
 260 25.9 20.2 30.2
 265 30.2 25.2 37.8

