


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121118\
 Data File : BE098333.D
 Acq On : 11 Dec 2018 15:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

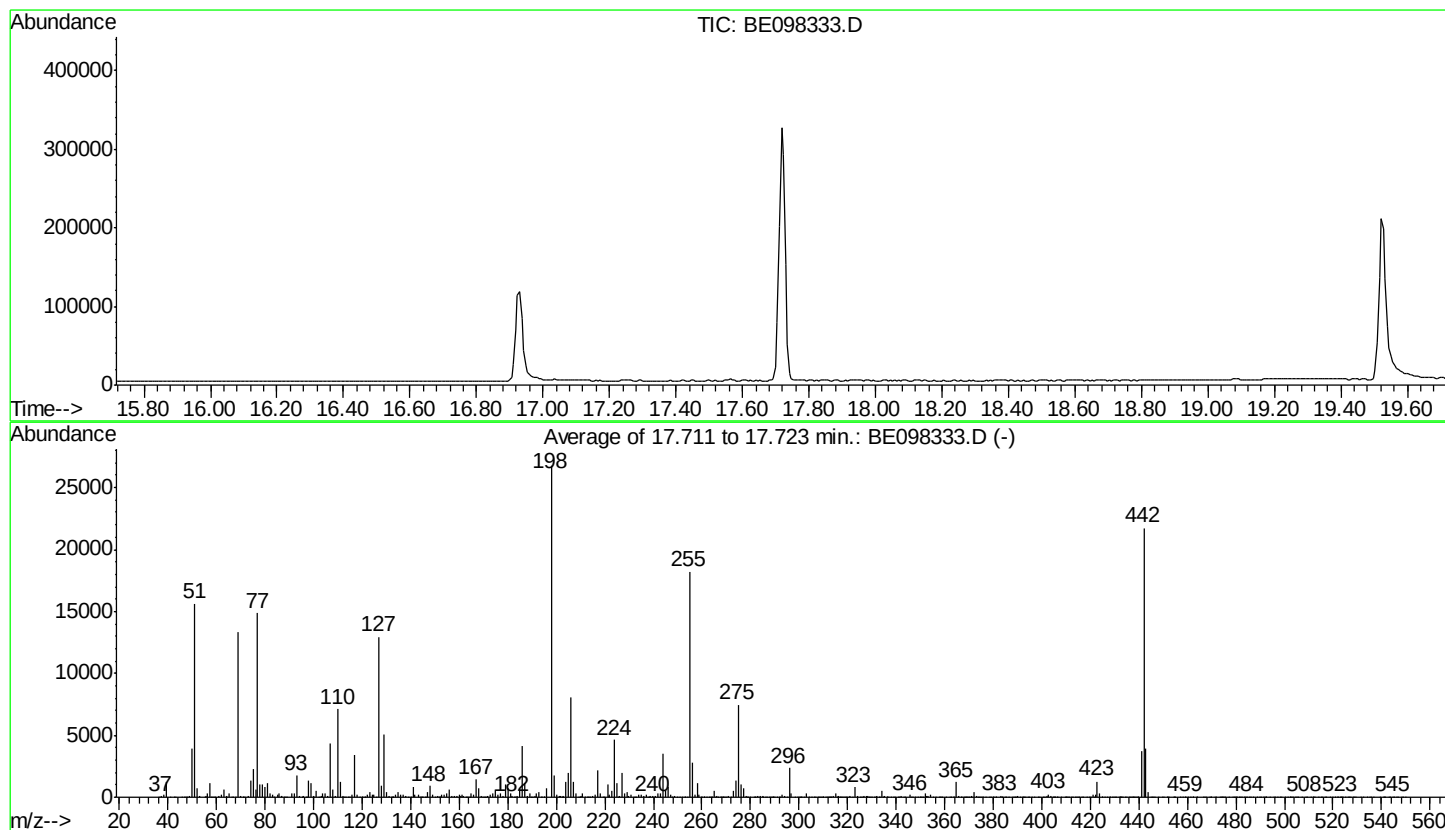

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.3	15607	PASS
68	69	0.00	2	0.4	48	PASS
69	198	0.00	100	49.9	13351	PASS
70	69	0.00	2	0.6	81	PASS
127	198	10	80	48.4	12966	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26771	PASS
199	198	5	9	6.7	1788	PASS
275	198	10	60	27.8	7447	PASS
365	198	1	100	4.5	1217	PASS
441	198	0.01	100	14.0	3759	PASS
442	198	50	100	81.1	21714	PASS
443	442	15	24	18.2	3949	PASS