


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121118\
 Data File : BE098351.D
 Acq On : 12 Dec 2018 2:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

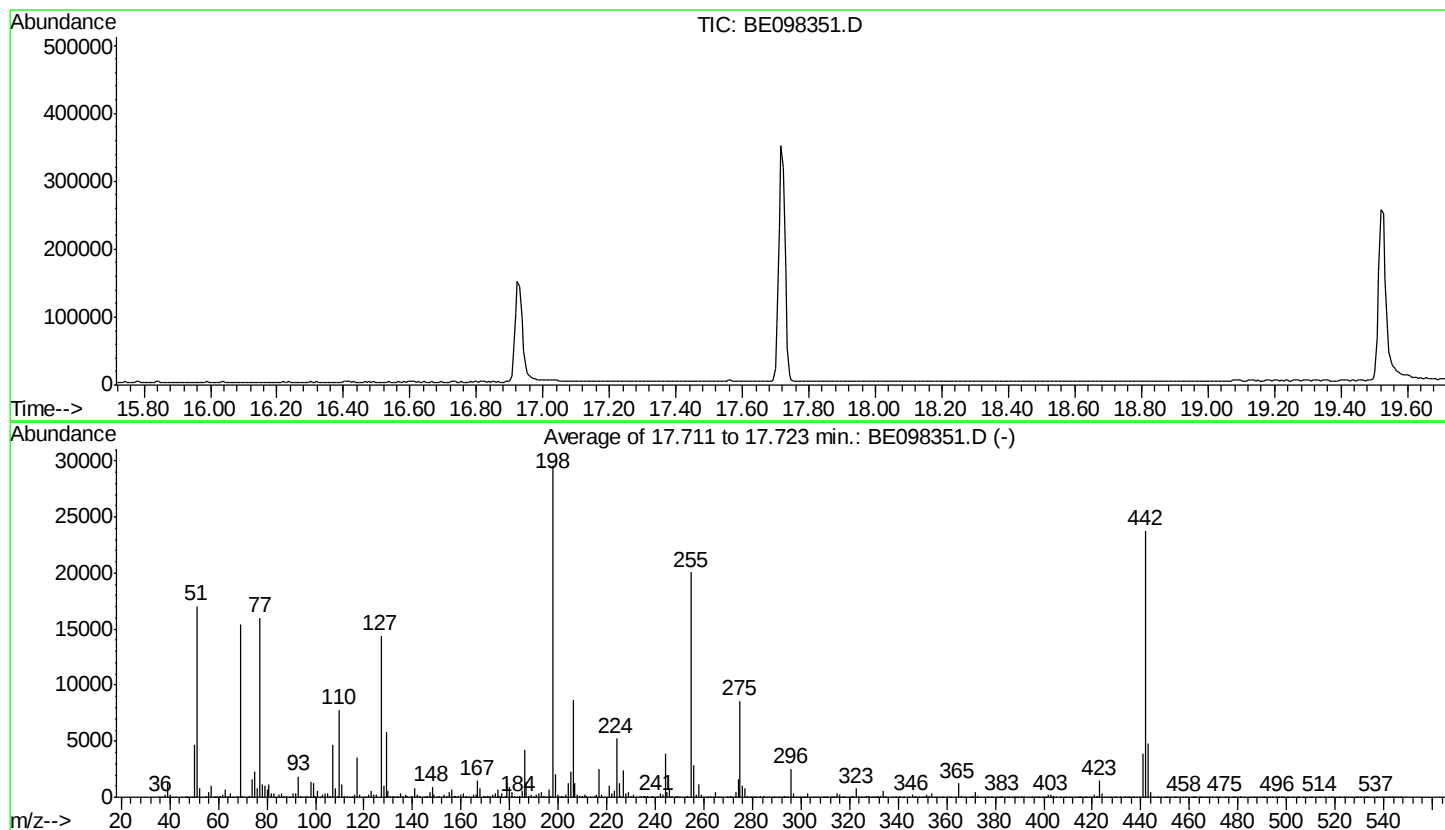

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.7	17079	PASS
68	69	0.00	2	1.1	167	PASS
69	198	0.00	100	52.3	15479	PASS
70	69	0.00	2	0.5	77	PASS
127	198	10	80	48.7	14412	PASS
197	198	0.00	2	0.3	81	PASS
198	198	100	100	100.0	29590	PASS
199	198	5	9	6.9	2042	PASS
275	198	10	60	29.0	8582	PASS
365	198	1	100	4.1	1213	PASS
441	198	0.01	100	13.1	3864	PASS
442	198	50	100	80.4	23791	PASS
443	442	15	24	20.2	4797	PASS