

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121119\
 Data File : BE100844.D
 Acq On : 11 Dec 2019 13:08
 Operator : JU
 Sample : K6185-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE131D2-20191205

Quant Time: Dec 11 14:24:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 04 17:18:11 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	4896	0.40	ng	-0.01
7) Naphthalene-d8	10.54	136	22255	0.40	ng	0.00
13) Acenaphthene-d10	14.40	164	12822	0.40	ng	0.00
19) Phenanthrene-d10	17.12	188	33280	0.40	ng	-0.01
27) Chrysene-d12	21.30	240	28125	0.40	ng	0.00
34) Perylene-d12	23.74	264	36747	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.37	112	3023	0.26	ng	0.00
5) Phenol-d6	6.93	99	2483	0.14	ng	0.00
8) Nitrobenzene-d5	8.90	82	5626	0.53	ng	0.00
11) 2-Methylnaphthalene-d10	12.14	152	14262	0.44	ng	0.00
14) 2,4,6-Tribromophenol	15.88	330	1205	0.84	ng	0.00
15) 2-Fluorobiphenyl	13.02	172	21372	0.42	ng	-0.01
25) Fluoranthene-d10	19.16	212	158400	0.40	ng	0.00
29) Terphenyl-d14	19.76	244	30241	0.45	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.34	88	71254	7.982	ng	Qvalue 90
22) Pentachlorophenol	16.79	266	27	0.022	ng	# 84
32) Bis(2-ethylhexyl)phthalate	21.23	149	9236	0.119	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121119\
Data File : BE100844.D
Acq On : 11 Dec 2019 13:08
Operator : JU
Sample : K6185-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE131D2-20191205

Quant Time: Dec 11 14:24:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 04 17:18:11 2019
Response via : Initial Calibration

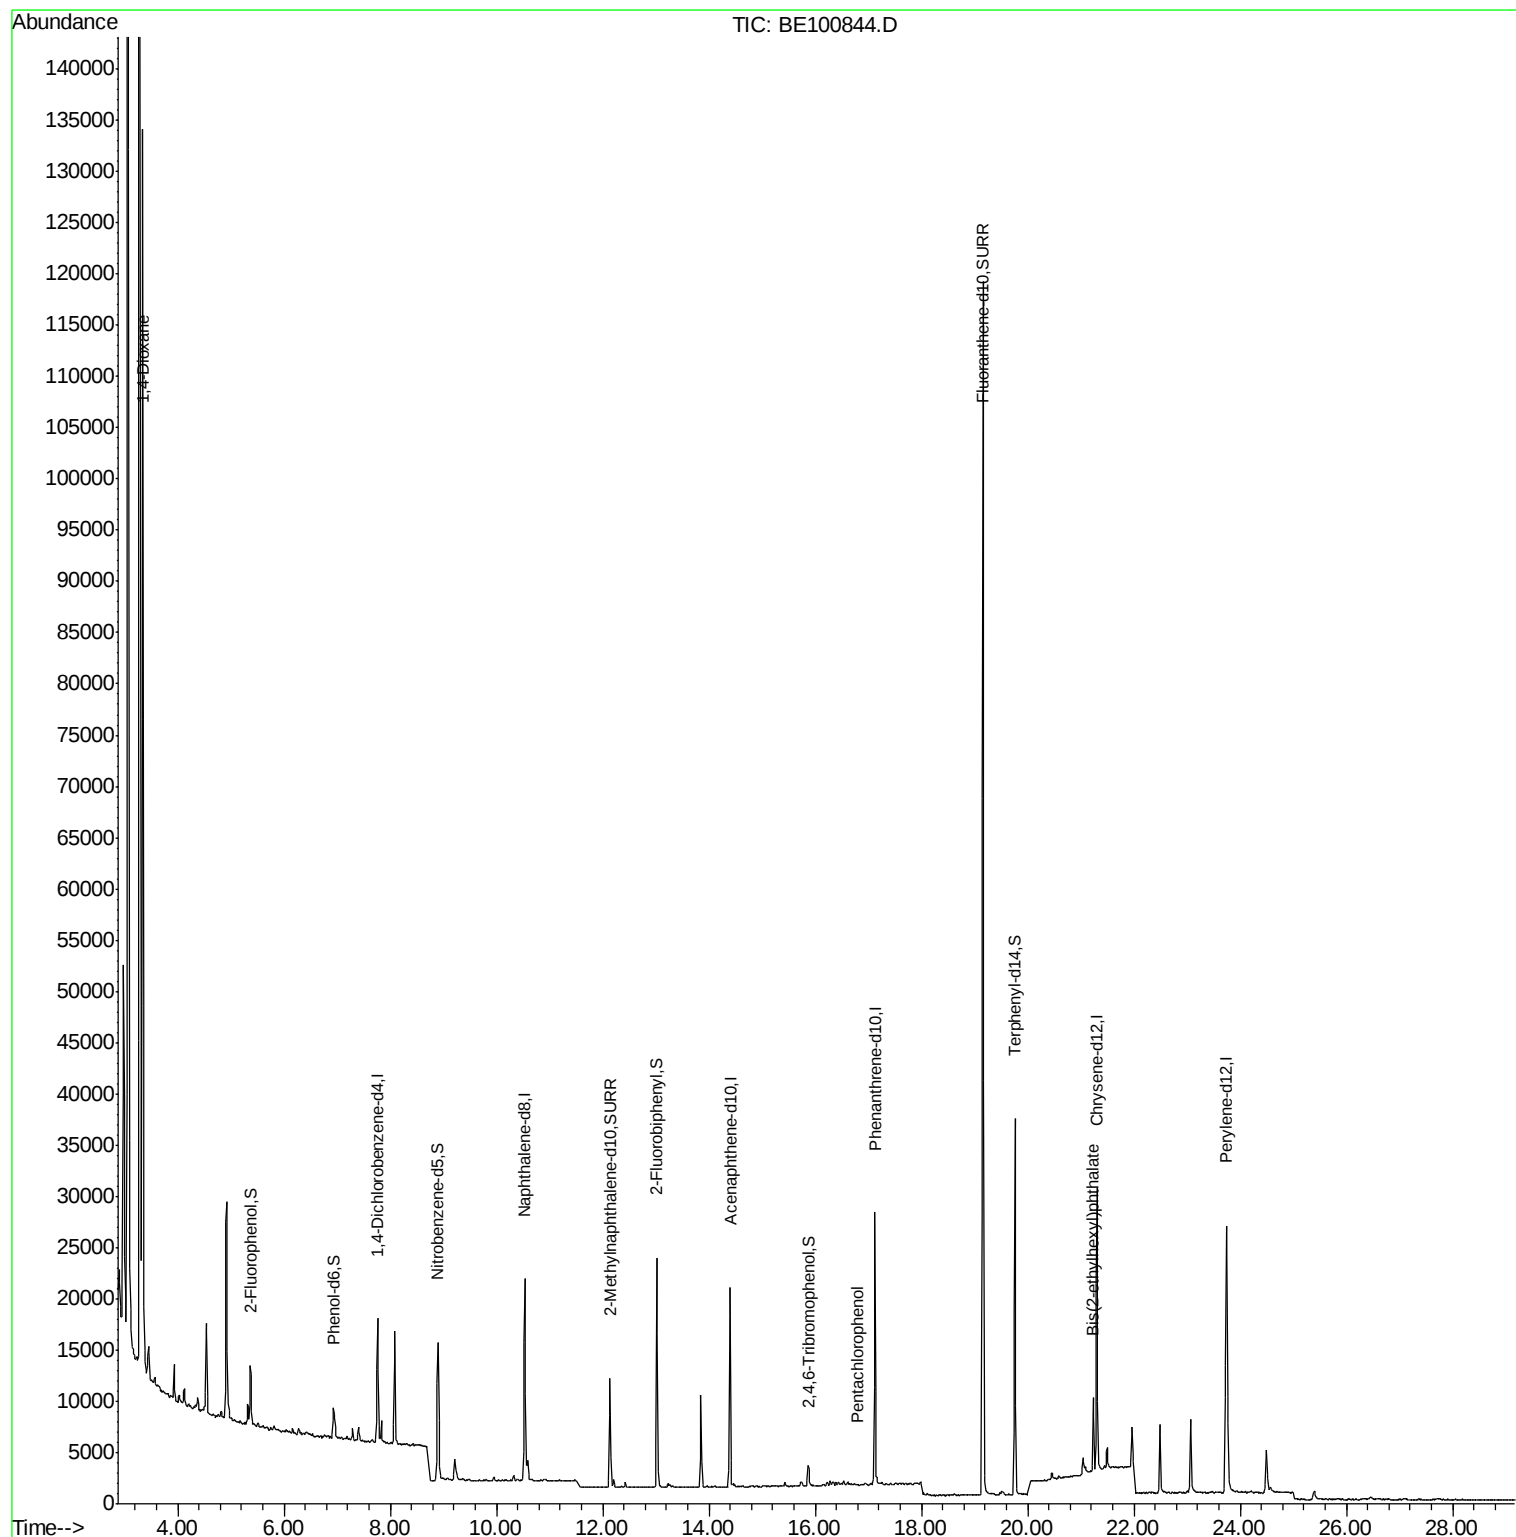




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.76 min Scan# 425
Delta R.T. -0.01 min
Lab File: BE100844.D
Acq: 11 Dec 2019 13:08

Instrument :
BNA_E
ClientSampleId :
RE131D2-20191205

Tot Ion:152 Resp: 4896
Ion Ratio Lower Upper
152 100
150 157.7 120.6 181.0
115 68.9 47.4 71.2

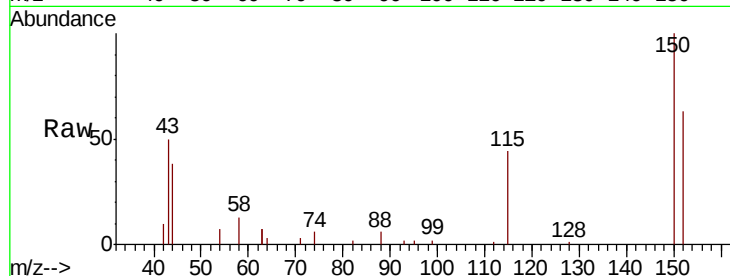


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

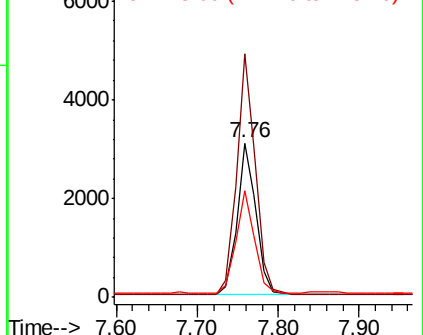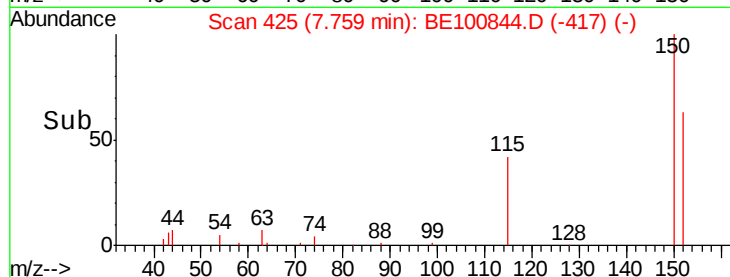



#2

1,4-Dioxane
Concen: 7.982 ng
RT: 3.34 min Scan# 41
Delta R.T. -0.01 min
Lab File: BE100844.D
Acq: 11 Dec 2019 13:08

Tgt Ion: 88 Resp: 71254
Ion Ratio Lower Upper
88 100
58 74.9 52.5 78.7
43 32.8 23.0 34.6

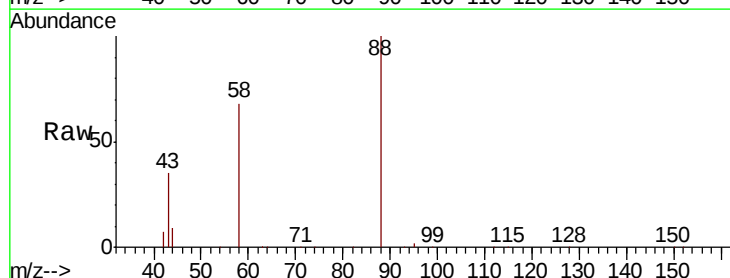

Abundance Ion 88.00 (87.70 to 88.70): BE1
Ion 58.00 (57.70 to 58.70): BE1
Ion 43.00 (42.70 to 43.70): BE1

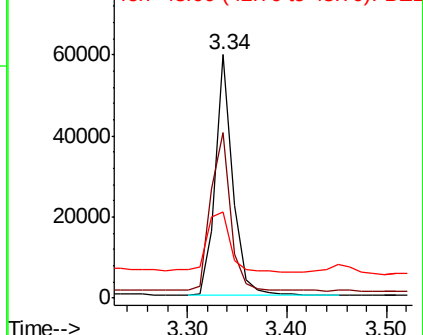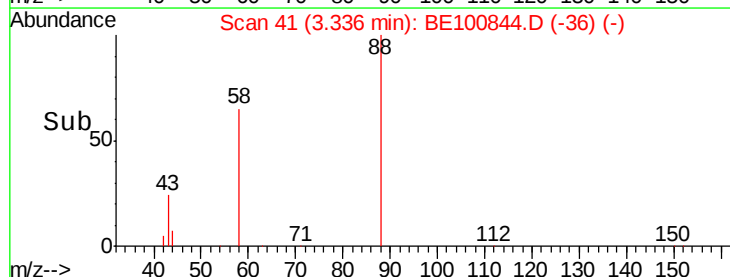



#4

2-Fluorophenol

Concen: 0.260 ng

RT: 5.37 min Scan# 218

Delta R.T. -0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08

Instrument :

BNA_E

ClientSampleId :

RE131D2-20191205


Tot Ion:112 Resp: 3023

Ion Ratio Lower Upper

112 100

64 70.1 54.1 81.1



63 136.6 113.2 169.8

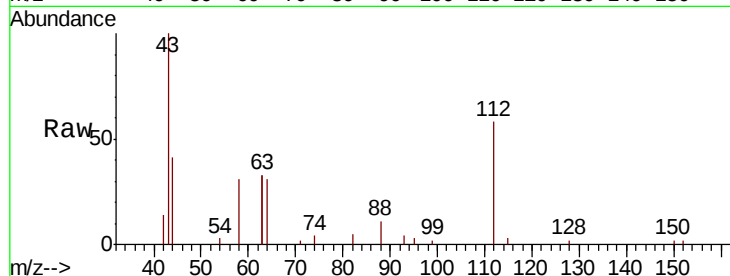

Abundance Ion 112.00 (111.70 to 112.70): BE1

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

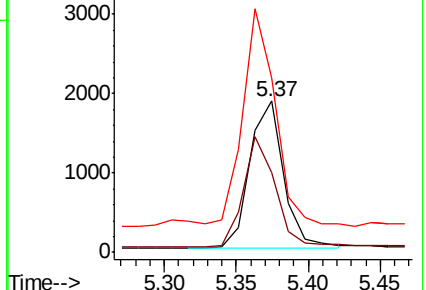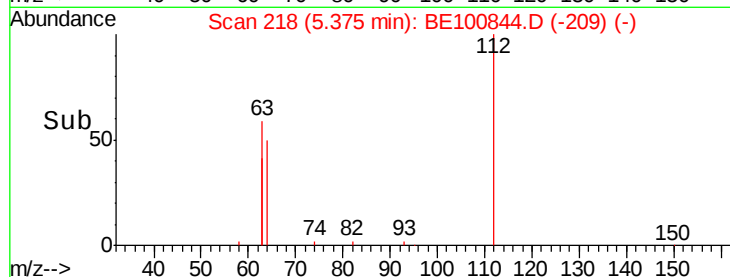

#5

Phenol-d6

Concen: 0.142 ng

RT: 6.93 min Scan# 353

Delta R.T. -0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08


Tgt Ion: 99 Resp: 2483

Ion Ratio Lower Upper

99 100

42 30.4 19.1 28.7#



71 37.2 27.7 41.5

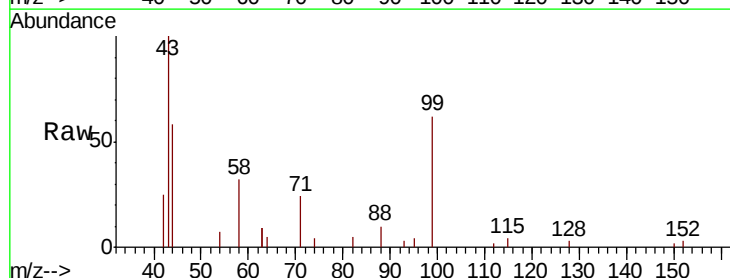


Abundance Ion 99.00 (98.70 to 99.70): BE1

Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

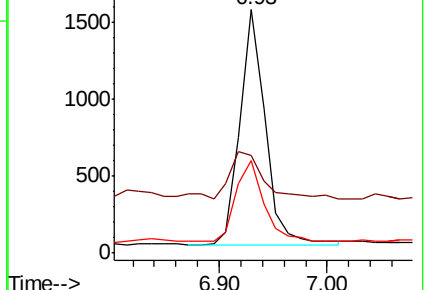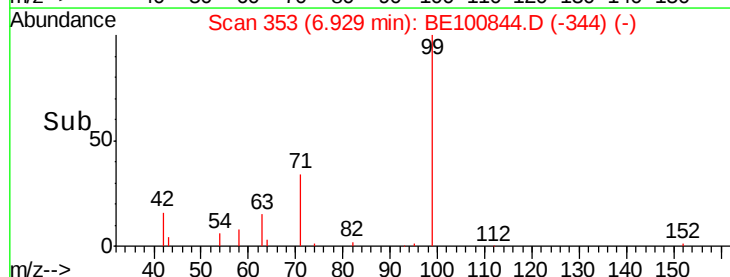

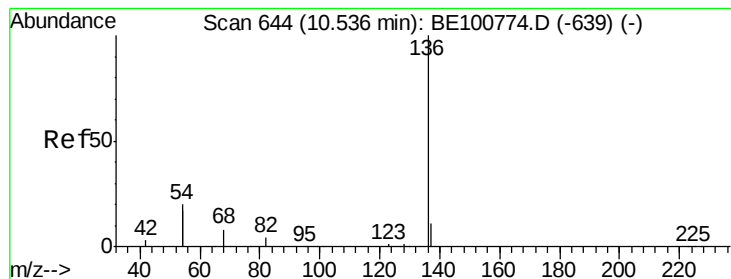

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.54 min Scan# 644

Delta R.T. 0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08

Instrument :

BNA_E

ClientSampleId :

RE131D2-20191205

Tot Ion:136 Resp: 22255


Ion Ratio Lower Upper

136 100

137 11.3 9.4 14.0

54 27.7 31.1 46.7#

68 6.3 6.6 10.0#

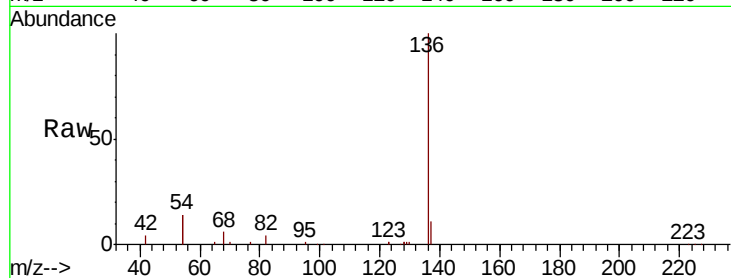




Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

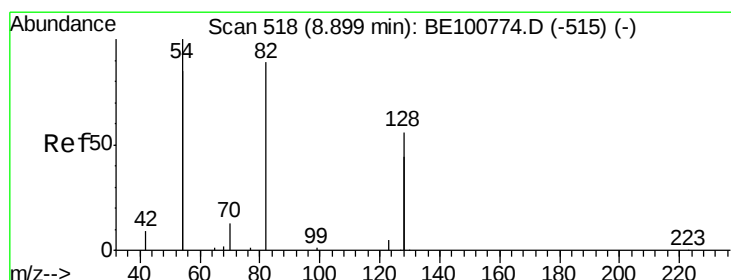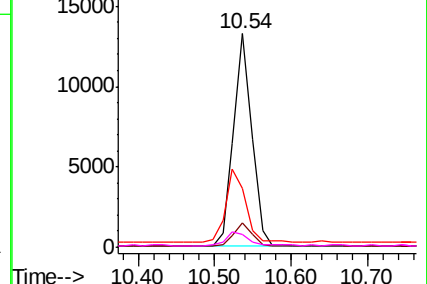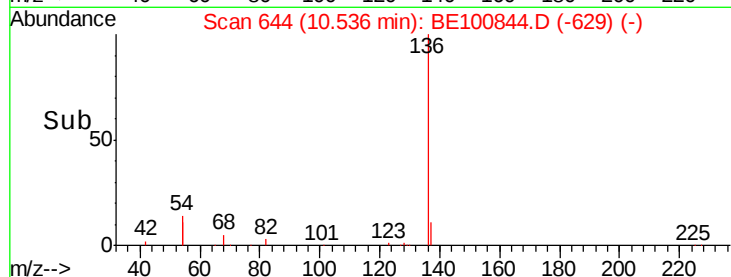

#8

Nitrobenzene-d5

Concen: 0.531 ng

RT: 8.90 min Scan# 518

Delta R.T. 0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08


Tgt Ion: 82 Resp: 5626

Ion Ratio Lower Upper

82 100

128 133.5 97.0 145.4

54 185.7 171.8 257.6


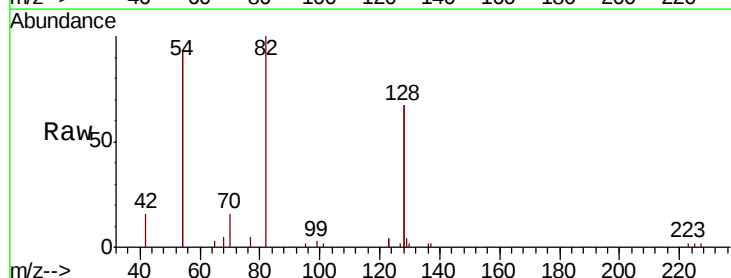


Abundance

Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE1

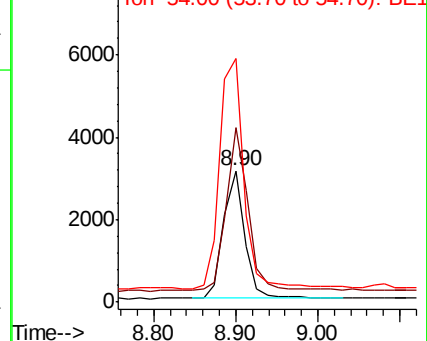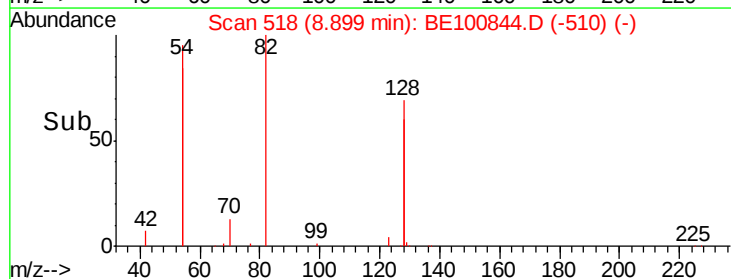



#11

2-Methylnaphthalene-d10

Concen: 0.442 ng

RT: 12.14 min Scan# 758

Delta R.T. -0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08

Instrument :

BNA_E

ClientSampleId :


RE131D2-20191205

Tot Ion:152 Resp: 14262

Ion Ratio Lower Upper

152 100

151 19.6 15.8 23.8

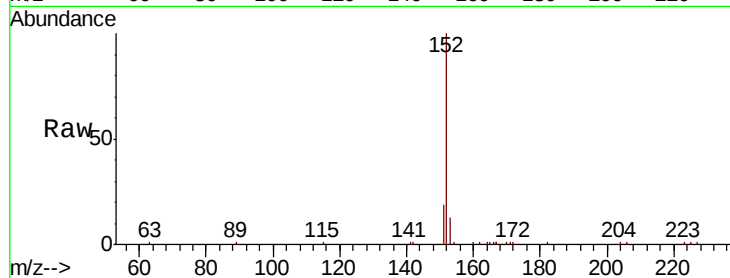

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

12.14

8000

6000



4000

2000

0

Time-->

12.00 12.10 12.20 12.30

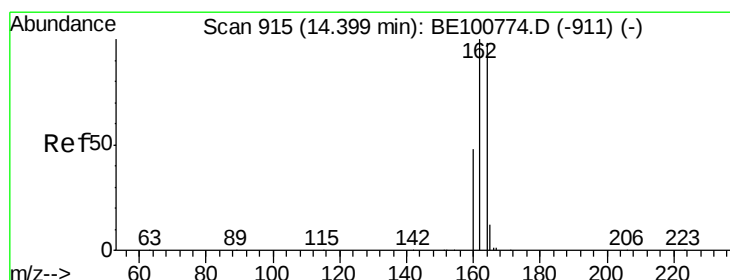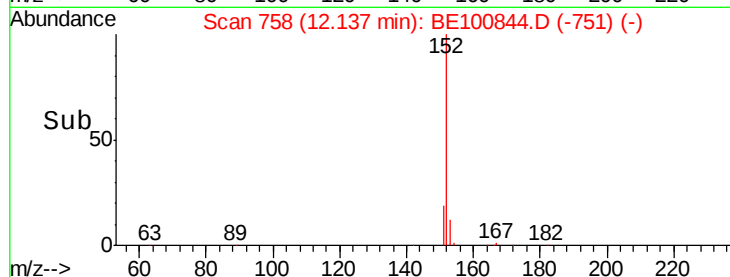

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.40 min Scan# 915

Delta R.T. -0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08


Tgt Ion:164 Resp: 12822

Ion Ratio Lower Upper

164 100

162 99.9 81.4 122.0

160 48.2 39.4 59.0

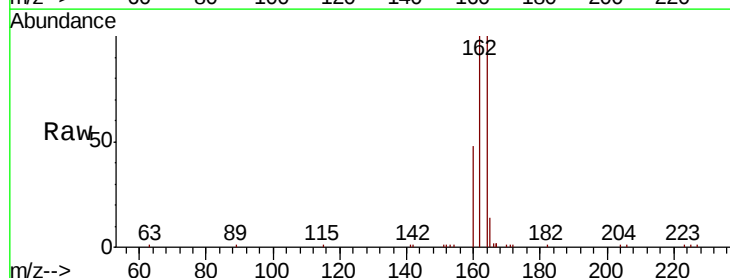

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.40

10000

8000

6000


4000


2000

0

Time-->

14.30 14.40 14.50




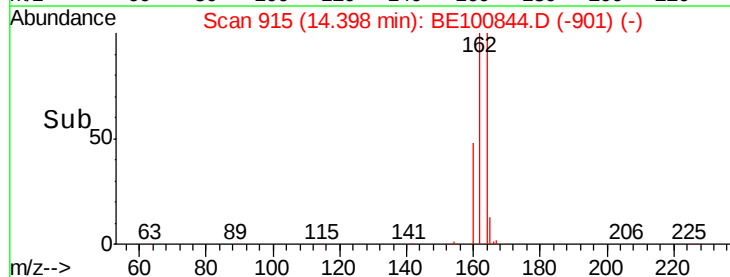


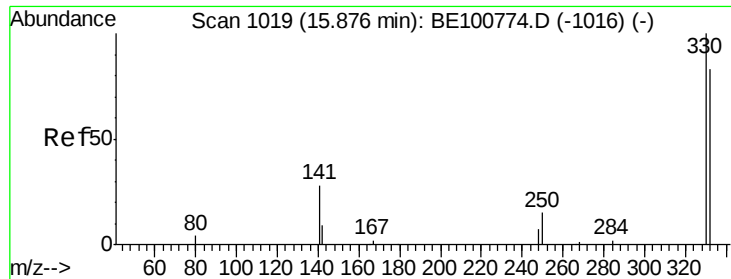

#14
 2,4,6-Tribromophenol
 Concen: 0.845 ng
 RT: 15.88 min Scan# 1019
 Delta R.T. -0.00 min
 Lab File: BE100844.D
 Acq: 11 Dec 2019 13:08




Instrument :
 BNA_E
 ClientSampleId :
 RE131D2-20191205


Tot Ion:330 Resp: 1205
 Ion Ratio Lower Upper
 330 100
 332 97.1 69.4 104.2
 141 55.0 51.1 76.7

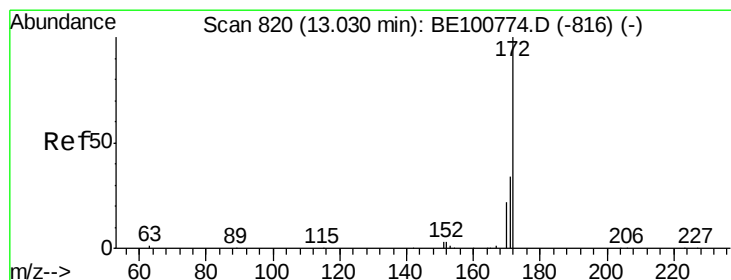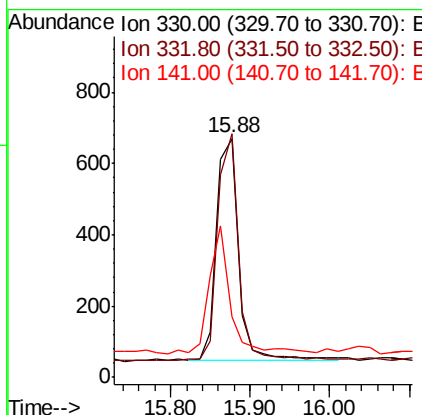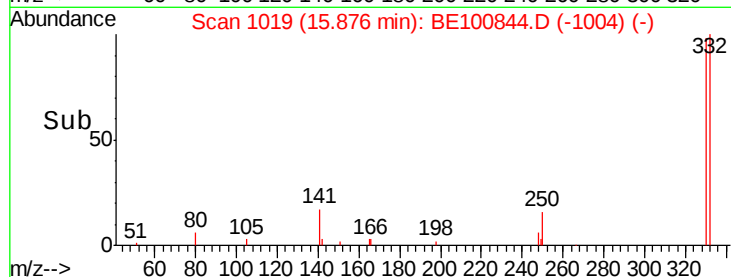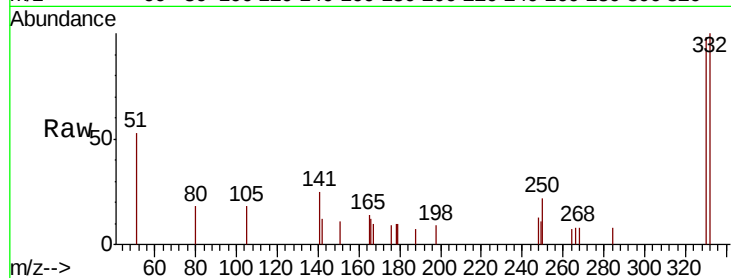

#15
 2-Fluorobiphenyl
 Concen: 0.420 ng
 RT: 13.02 min Scan# 819
 Delta R.T. -0.01 min
 Lab File: BE100844.D
 Acq: 11 Dec 2019 13:08

Tgt Ion:172 Resp: 21372
 Ion Ratio Lower Upper
 172 100
 171 36.0 27.2 40.8
 170 24.7 18.0 27.0

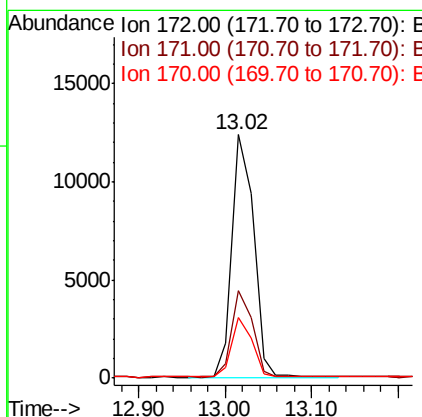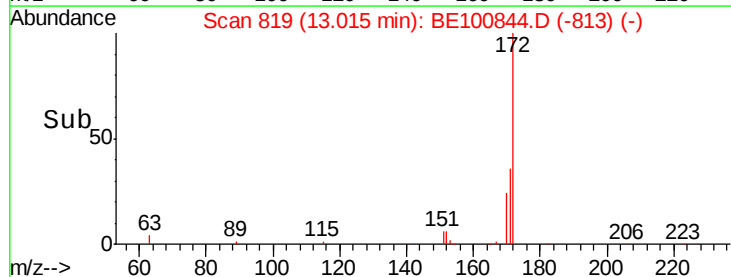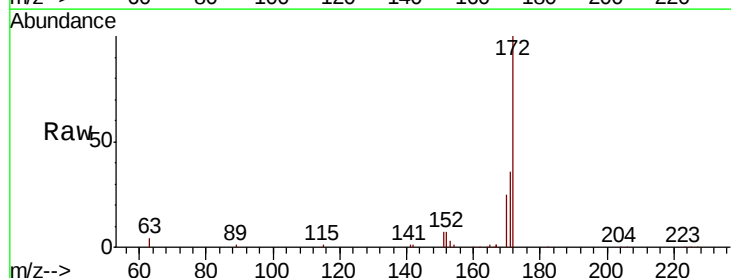

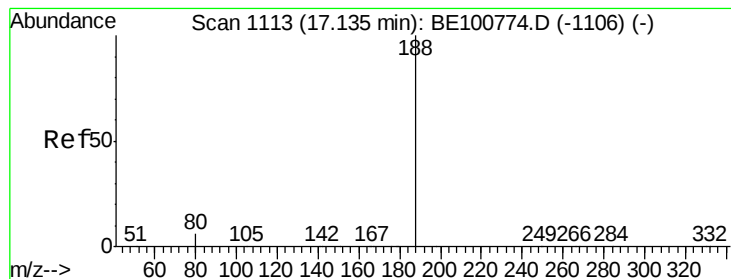

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.12 min Scan# 1112

Delta R.T. -0.01 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08

Instrument :

BNA_E

ClientSampleId :

RE131D2-20191205


Tot Ion:188 Resp: 33280

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 10.1 5.2 7.8#

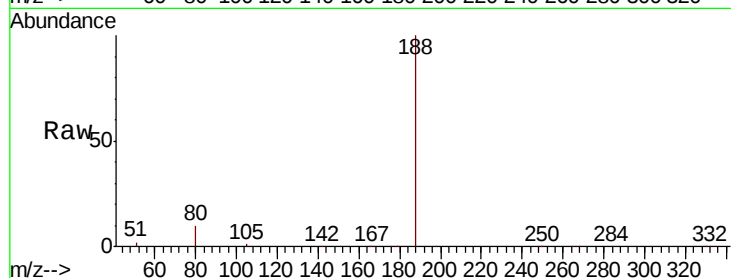

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE1

Ion 80.00 (79.70 to 80.70): BE1

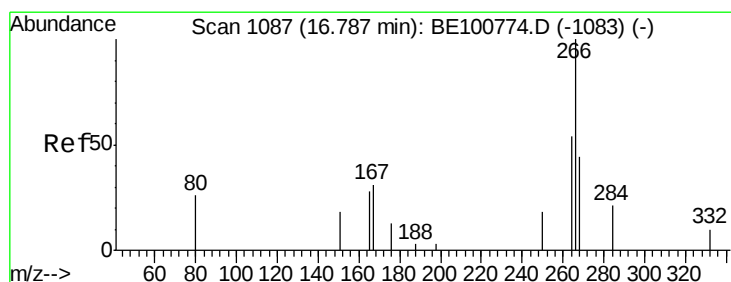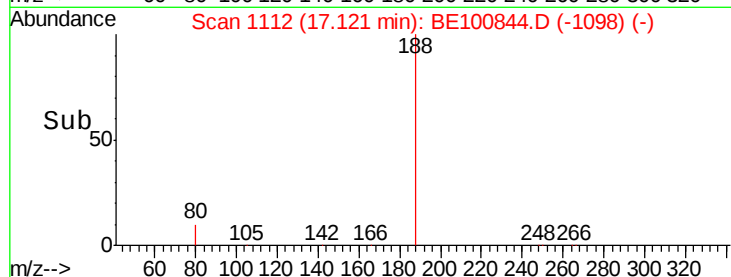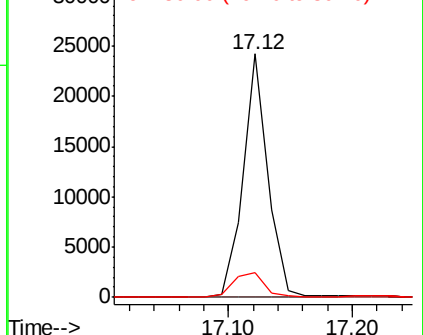

#22

Pentachlorophenol

Concen: 0.022 ng

RT: 16.79 min Scan# 1087

Delta R.T. -0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08


Tgt Ion:266 Resp: 27

Ion Ratio Lower Upper

266 100

264 89.1 63.4 95.0



268 101.6 65.8 98.8#

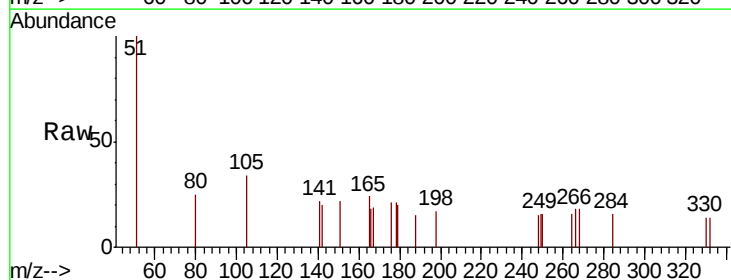


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

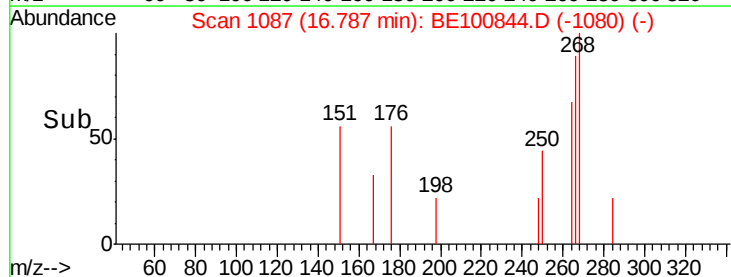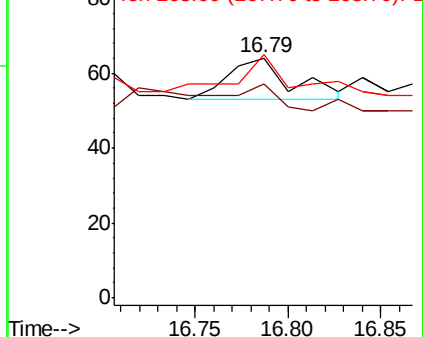

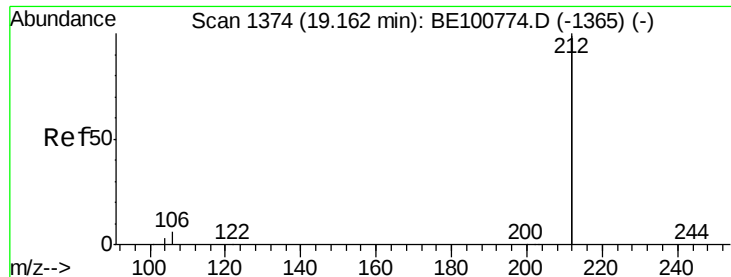

#25

Fluoranthene-d10

Concen: 0.403 ng

RT: 19.16 min Scan# 1373

Delta R.T. -0.01 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08

Instrument :

BNA_E

ClientSampleId :

RE131D2-20191205


Tot Ion:212 Resp: 158400

Ion Ratio Lower Upper

212 100

106 3.3 2.6 3.8




104 1.9 1.4 2.2

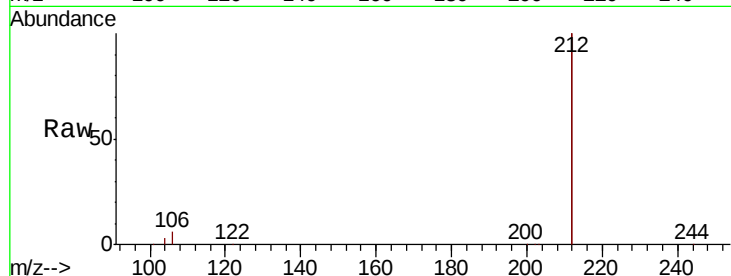

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

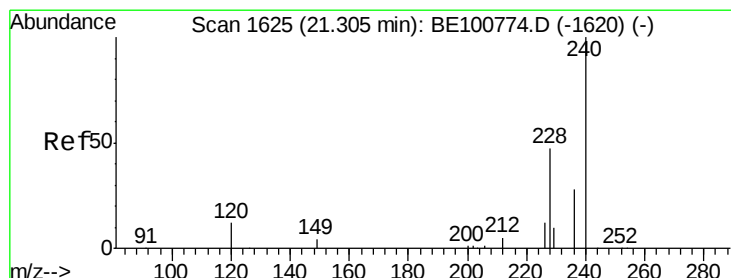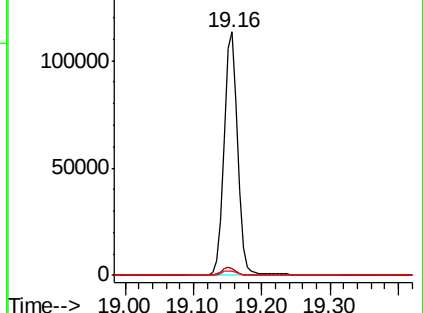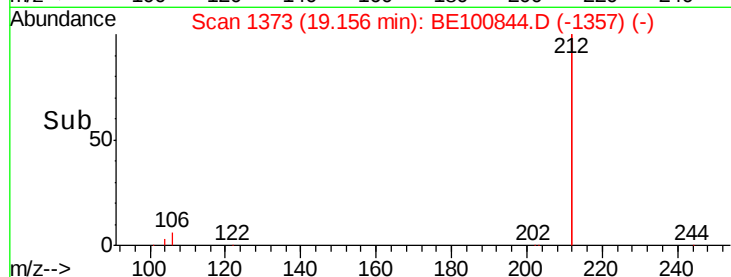

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.30 min Scan# 1624

Delta R.T. -0.00 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08


Tgt Ion:240 Resp: 28125

Ion Ratio Lower Upper

240 100

120 6.4 10.2 15.2#



236 27.8 22.3 33.5

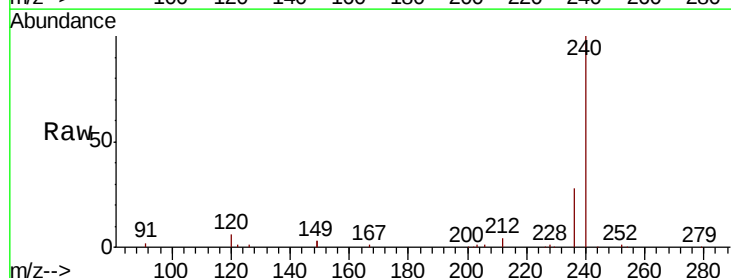


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

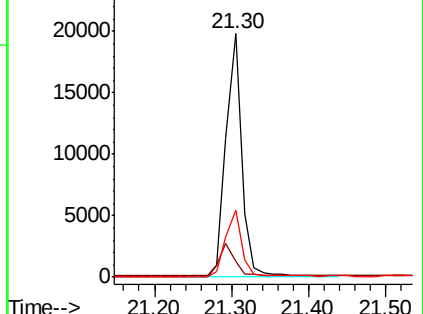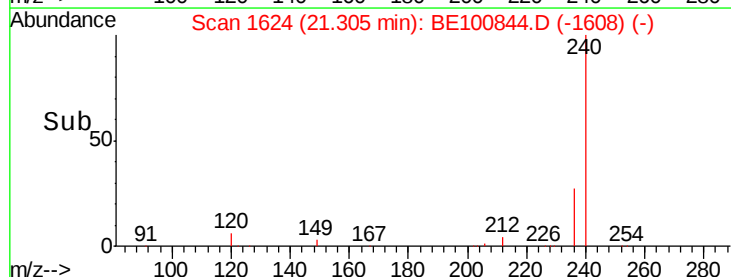

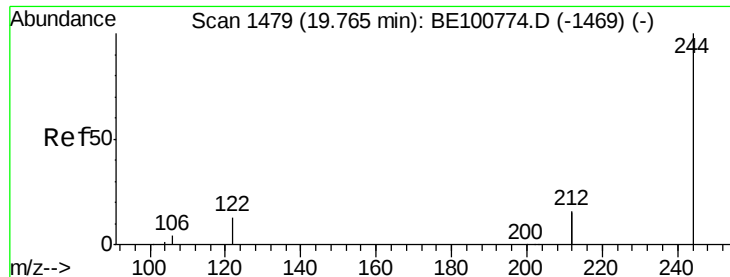

#29

Terphenyl-d14

Concen: 0.449 ng

RT: 19.76 min Scan# 1478

Delta R.T. -0.01 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08

Instrument :

BNA_E

ClientSampleId :

RE131D2-20191205


Tot Ion:244 Resp: 30241

Ion Ratio Lower Upper

244 100

212 31.1 26.2 39.4




122 10.7 10.2 15.4

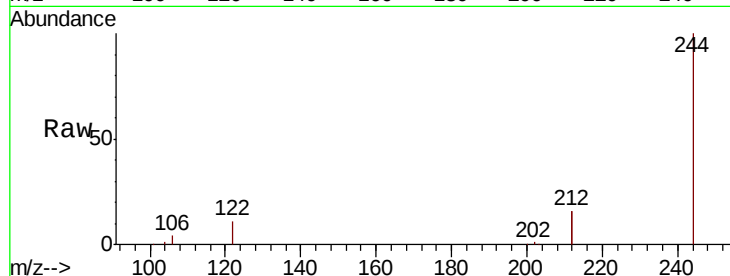

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

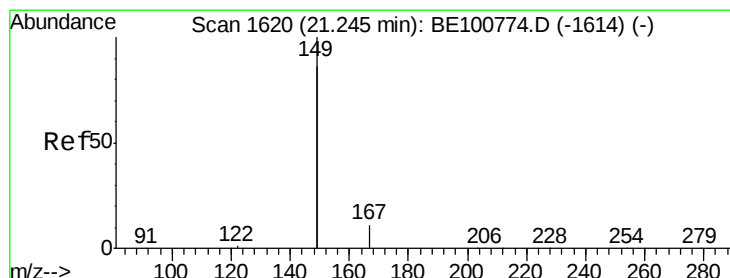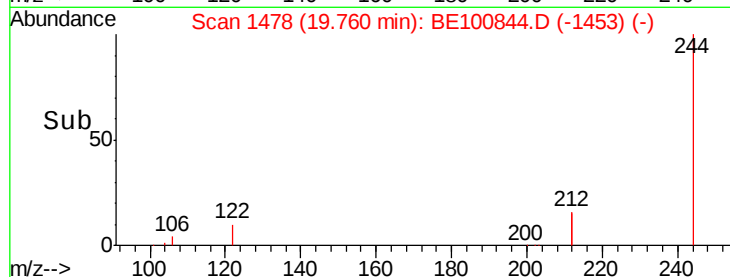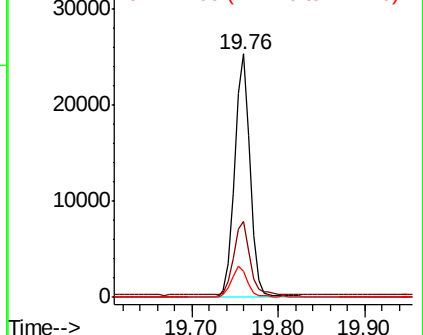

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.119 ng

RT: 21.23 min Scan# 1618

Delta R.T. -0.01 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08


Tgt Ion:149 Resp: 9236

Ion Ratio Lower Upper

149 100

167 7.4 5.0 7.6



279 0.9 0.7 1.1


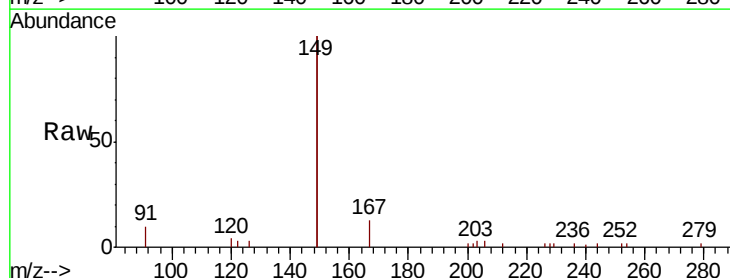


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

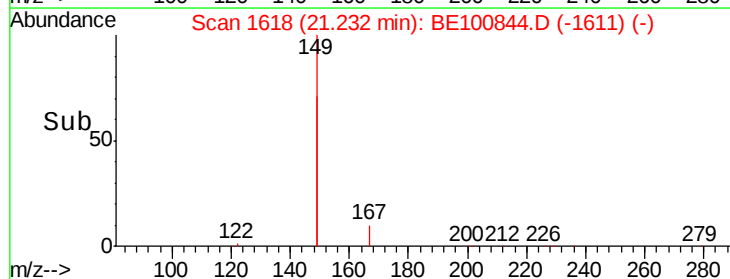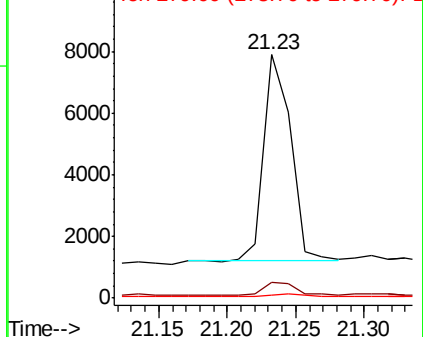

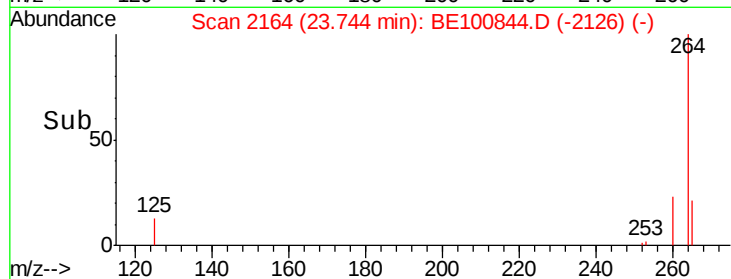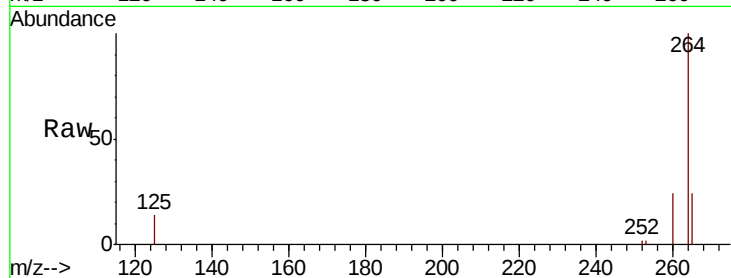

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.74 min Scan# 2164

Delta R.T. -0.01 min

Lab File: BE100844.D

Acq: 11 Dec 2019 13:08

Instrument :

BNA_E

ClientSampleId :

RE131D2-20191205

Tot Ion: 264 Resp: 36747

Ion Ratio Lower Upper

264 100

260 23.6 19.4 29.2

265 23.8 21.8 32.8

