


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121119\
 Data File : BE100856.D
 Acq On : 11 Dec 2019 21:49
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 04 17:18:11 2019

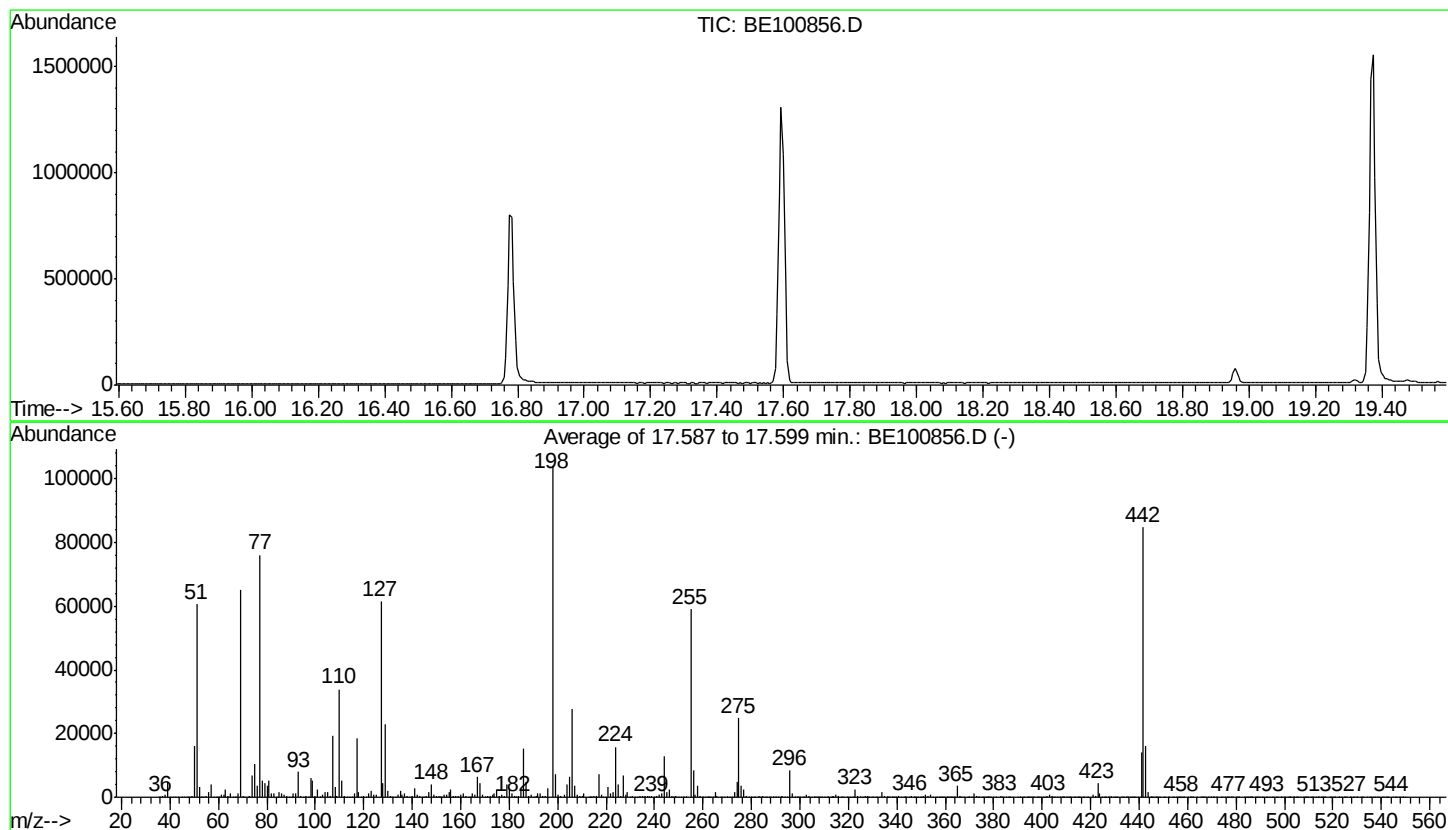

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	60592	PASS
68	69	0.00	2	1.6	1049	PASS
69	198	0.00	100	62.4	65014	PASS
70	69	0.00	2	0.4	244	PASS
127	198	10	80	58.9	61322	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	104142	PASS
199	198	5	9	6.8	7132	PASS
275	198	10	60	23.8	24810	PASS
365	198	1	100	3.4	3526	PASS
441	198	0.01	100	13.6	14156	PASS
442	198	50	100	81.4	84820	PASS
443	442	15	24	19.0	16138	PASS