

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121319\
 Data File : BE100881.D
 Acq On : 13 Dec 2019 11:34
 Operator : JU
 Sample : K6252-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE132D5-20191209

Quant Time: Dec 13 12:58:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 13 10:42:38 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	4744	0.40	ng	0.00
7) Naphthalene-d8	10.54	136	21544	0.40	ng	0.00
13) Acenaphthene-d10	14.39	164	13219	0.40	ng	0.00
19) Phenanthrene-d10	17.12	188	33635	0.40	ng	0.00
27) Chrysene-d12	21.29	240	33175	0.40	ng	-0.01
34) Perylene-d12	23.74	264	37117	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.36	112	975	0.09	ng	0.00
5) Phenol-d6	6.93	99	1039	0.06	ng	0.00
8) Nitrobenzene-d5	8.90	82	2762	0.27	ng	0.00
11) 2-Methylnaphthalene-d10	12.12	152	7267	0.23	ng	-0.01
14) 2,4,6-Tribromophenol	15.86	330	441	0.30	ng	-0.01
15) 2-Fluorobiphenyl	13.02	172	9655	0.18	ng	0.00
25) Fluoranthene-d10	19.15	212	91804	0.23	ng	0.00
29) Terphenyl-d14	19.75	244	17414	0.22	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.34	88	32094	3.711	ng	Qvalue # 87
6) bis(2-Chloroethyl)ether	7.18	93	628	0.038	ng	94
32) Bis(2-ethylhexyl)phthalate	21.23	149	136023	1.575	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121319\
Data File : BE100881.D
Acq On : 13 Dec 2019 11:34
Operator : JU
Sample : K6252-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE132D5-20191209

Quant Time: Dec 13 12:58:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 13 10:42:38 2019
Response via : Initial Calibration

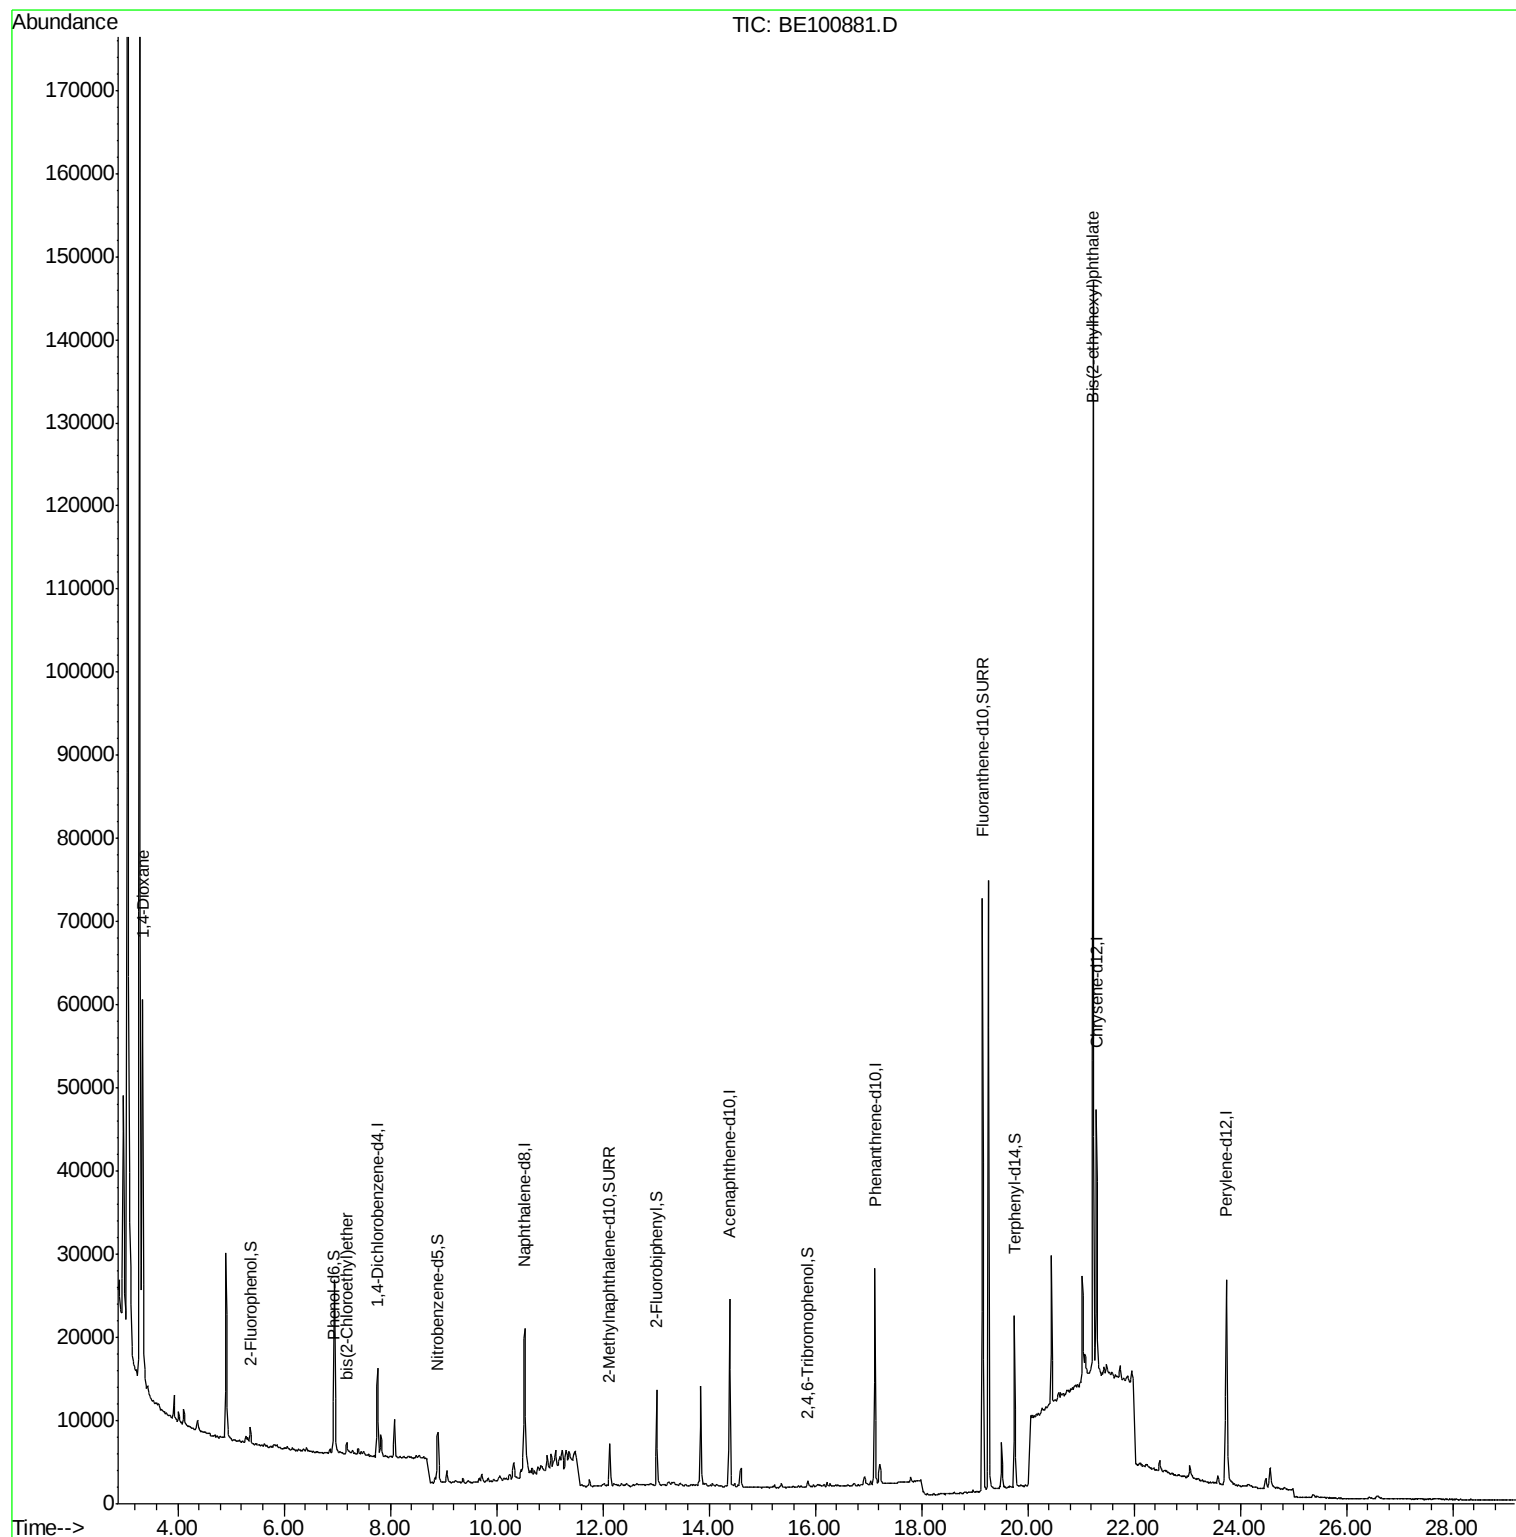

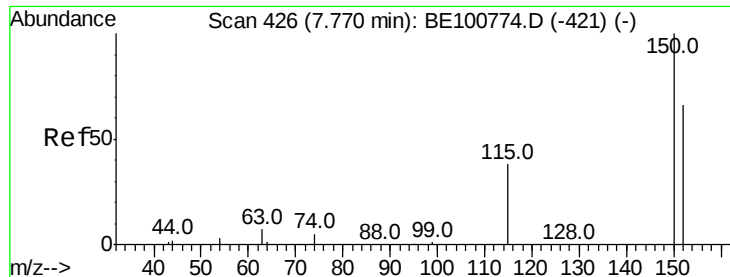

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.76 min Scan# 425

Delta R.T. 0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209


Tot Ion:152 Resp: 4744

Ion Ratio Lower Upper

152 100

150 151.9 125.5 188.3




115 63.9 55.7 83.5

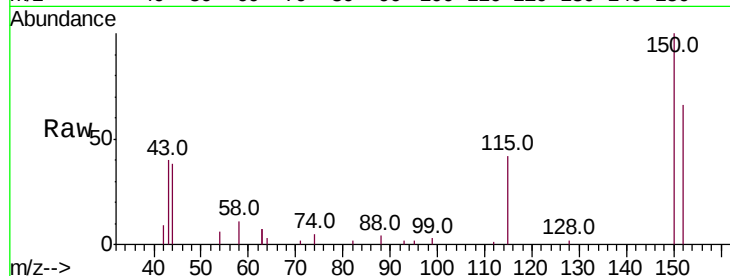

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

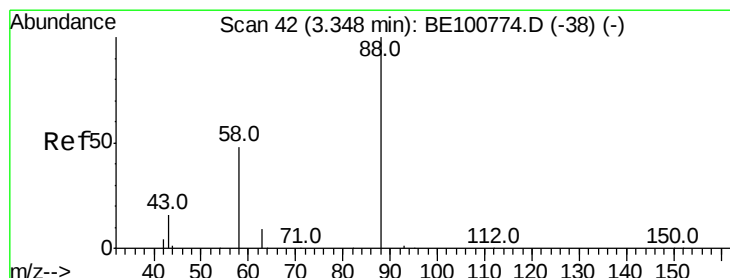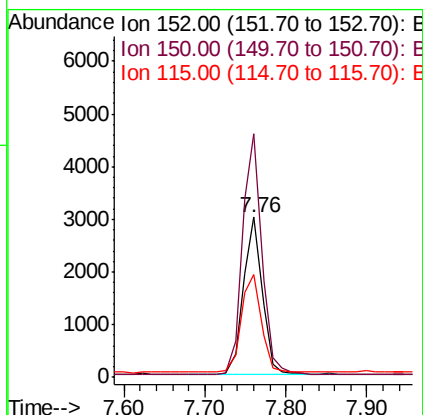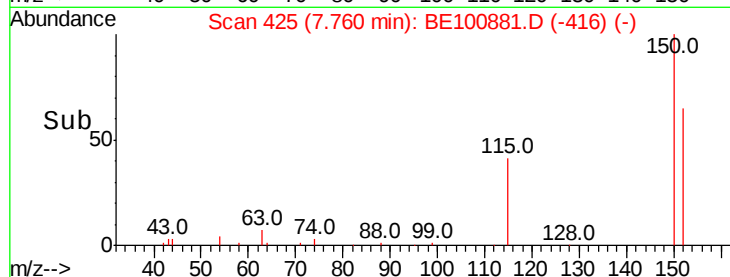

#2

1,4-Dioxane

Concen: 3.711 ng

RT: 3.34 min Scan# 41

Delta R.T. 0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34


Tgt Ion: 88 Resp: 32094

Ion Ratio Lower Upper

88 100

58 76.2 52.3 78.5



43 36.3 23.5 35.3#

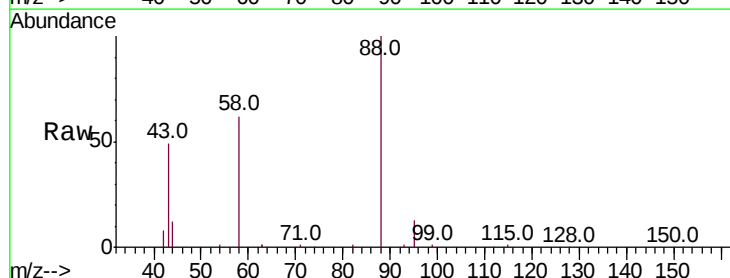


Abundance Ion 88.00 (87.70 to 88.70): BE1

Ion 58.00 (57.70 to 58.70): BE1

Ion 43.00 (42.70 to 43.70): BE1

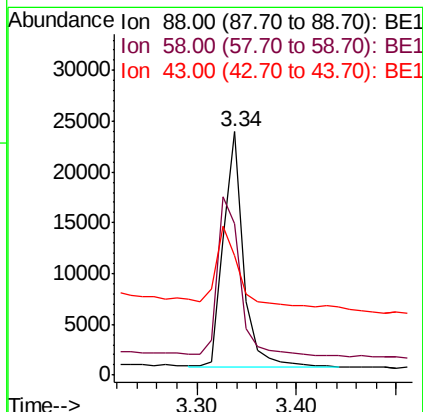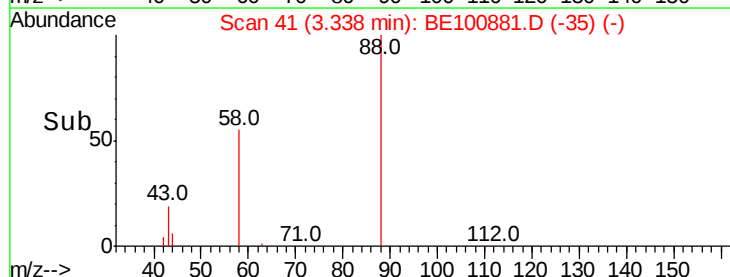

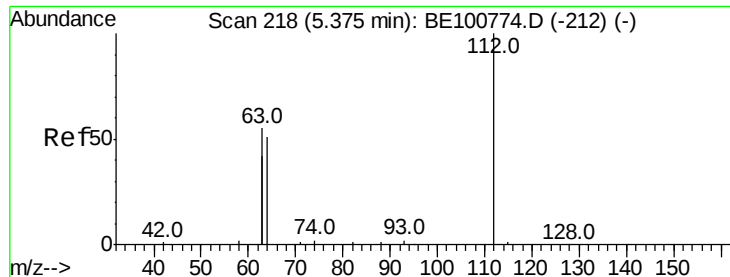

#4

2-Fluorophenol

Concen: 0.087 ng

RT: 5.36 min Scan# 217

Delta R.T. -0.01 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209


Tot Ion:112 Resp: 975

Ion Ratio Lower Upper

112 100

64 73.9 54.5 81.7




63 138.4 116.1 174.1

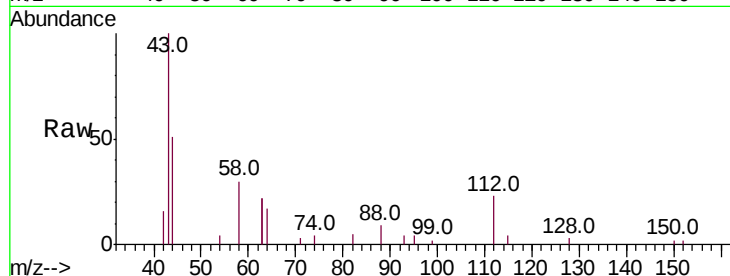

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

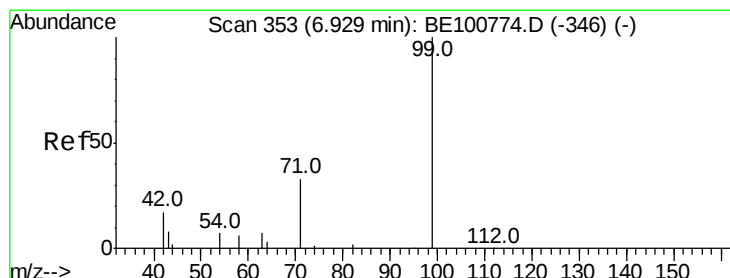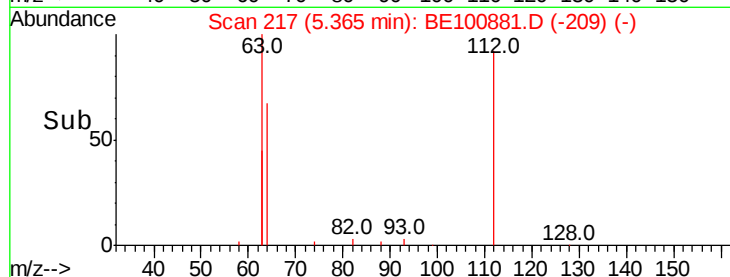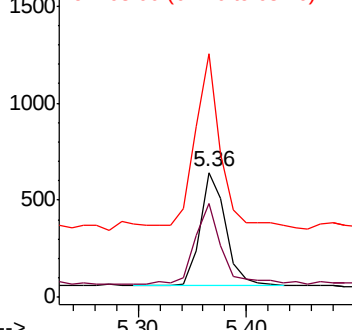

#5

Phenol-d6

Concen: 0.061 ng

RT: 6.93 min Scan# 353

Delta R.T. 0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34


Tgt Ion: 99 Resp: 1039

Ion Ratio Lower Upper

99 100

42 111.0 18.2 27.2#



71 0.0 29.1 43.7#

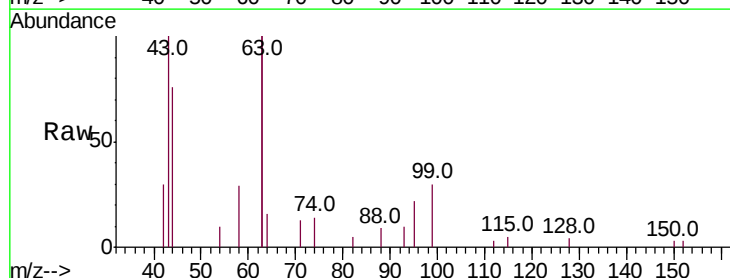


Abundance Ion 99.00 (98.70 to 99.70): BE1

Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

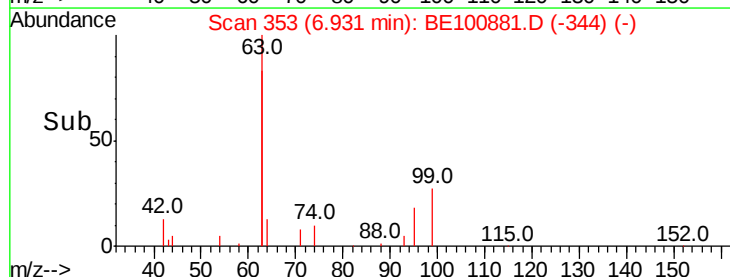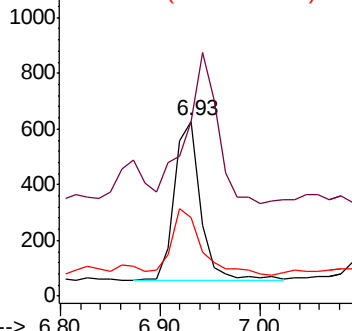

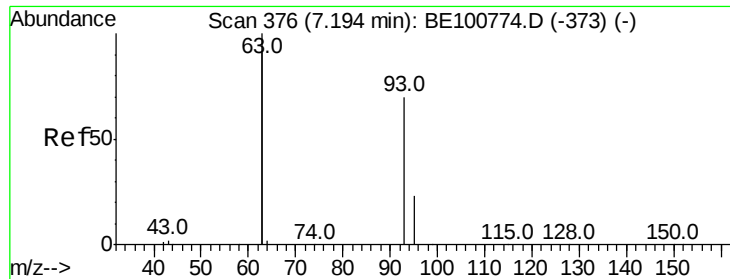

#6

bis(2-Chloroethyl)ether

Concen: 0.038 ng

RT: 7.18 min Scan# 375

Delta R.T. 0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209


Tot Ion: 93 Resp: 628

Ion Ratio Lower Upper

93 100

63 306.8 253.9 380.9




95 26.1 25.0 37.6

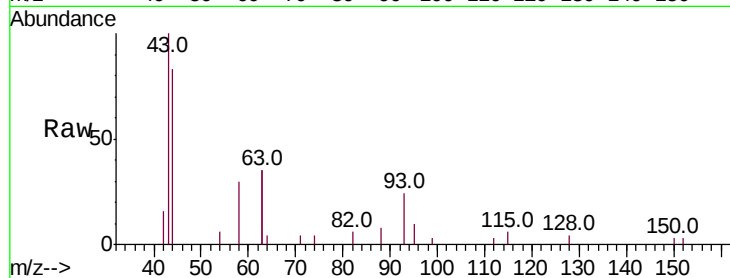

Abundance Ion 93.00 (92.70 to 93.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

Ion 95.00 (94.70 to 95.70): BE1

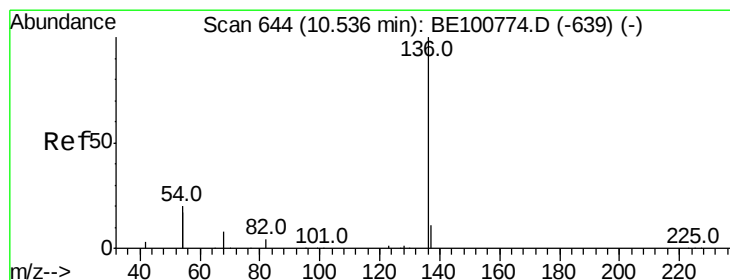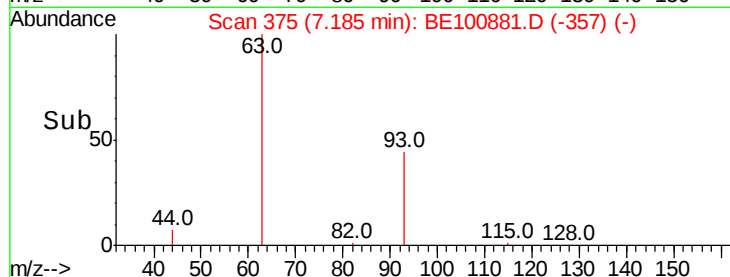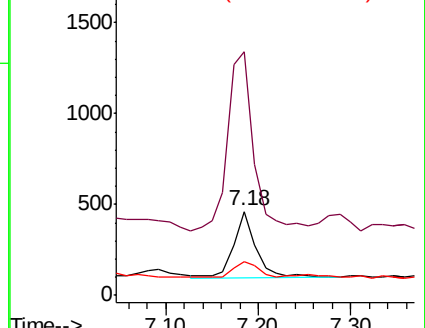

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.54 min Scan# 644

Delta R.T. -0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Tgt Ion: 136 Resp: 21544


Ion Ratio Lower Upper

136 100

137 11.4 9.1 13.7

54 26.6 18.9 28.3

68 6.2 4.6 6.8


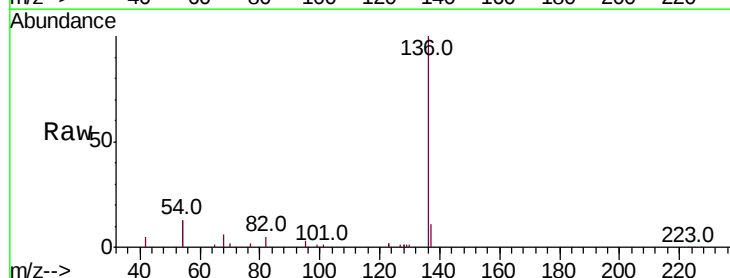



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

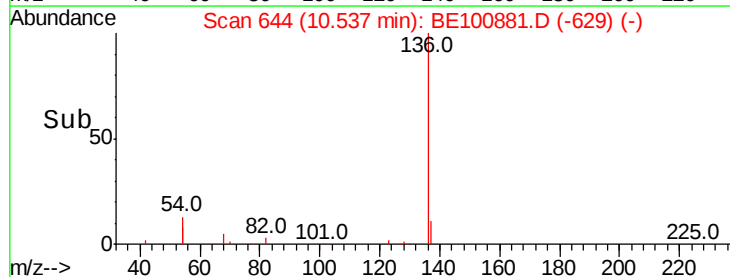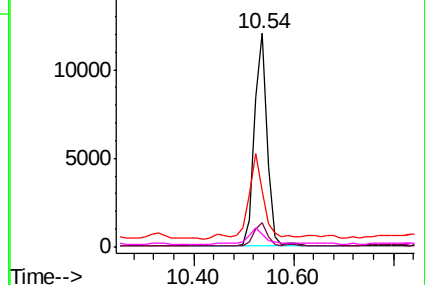



#8

Nitrobenzene-d5

Concen: 0.269 ng

RT: 8.90 min Scan# 518

Delta R.T. -0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209


Tot Ion: 82 Resp: 2762

Ion Ratio Lower Upper

82 100

128 148.7 113.5 170.3




54 184.6 138.9 208.3

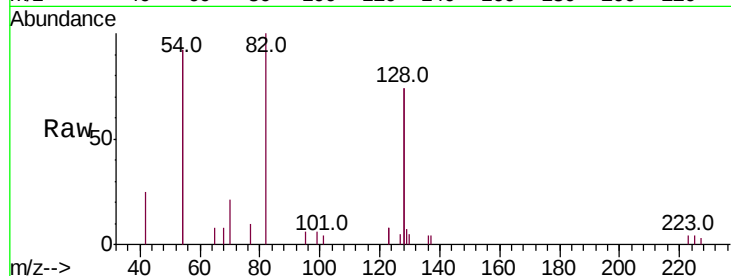

Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): BE1

Ion 54.00 (53.70 to 54.70): BE1

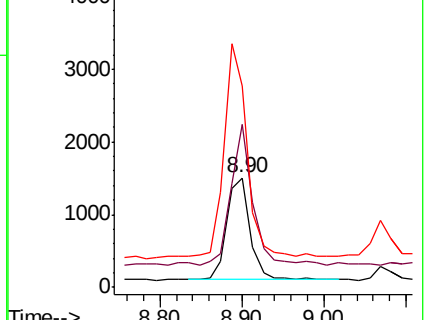

#11

2-Methylnaphthalene-d10

Concen: 0.233 ng

RT: 12.12 min Scan# 757

Delta R.T. -0.01 min

Lab File: BE100881.D


Acq: 13 Dec 2019 11:34

Tgt Ion: 152 Resp: 7267

Ion Ratio Lower Upper



152 100


151 29.0 15.1 22.7#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

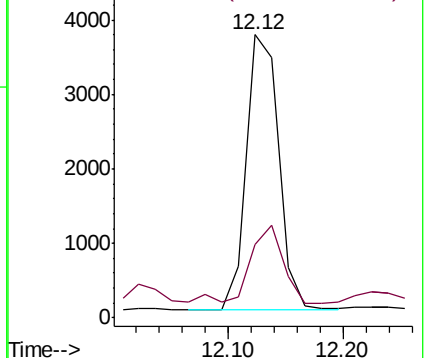







#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.39 min Scan# 914
Delta R.T. 0.00 min
Lab File: BE100881.D
Acq: 13 Dec 2019 11:34

Instrument :
BNA_E
ClientSampleId :
RE132D5-20191209

Tot Ion:164 Resp: 13219
Ion Ratio Lower Upper
164 100
162 106.6 86.0 129.0
160 50.8 42.3 63.5

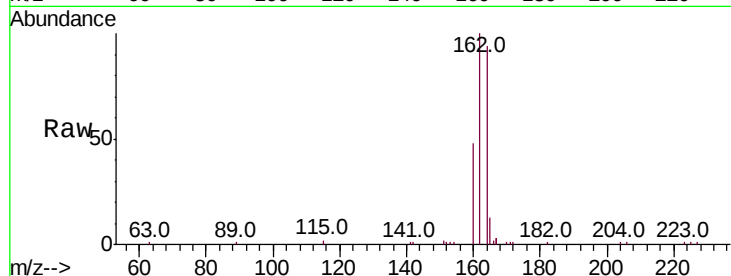


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


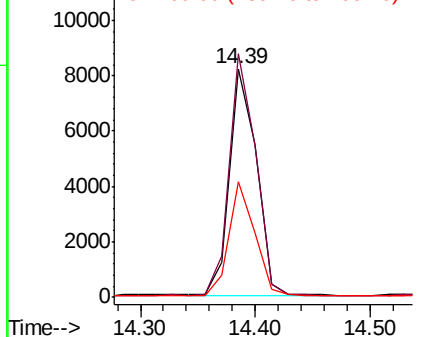



#14
2,4,6-Tribromophenol
Concen: 0.300 ng
RT: 15.86 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BE100881.D
Acq: 13 Dec 2019 11:34

Tgt Ion:330 Resp: 441
Ion Ratio Lower Upper
330 100
332 102.3 74.1 111.1
141 68.7 46.7 70.1



Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

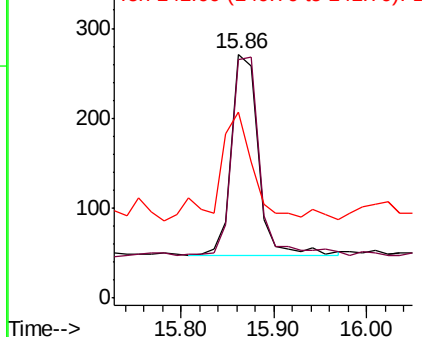

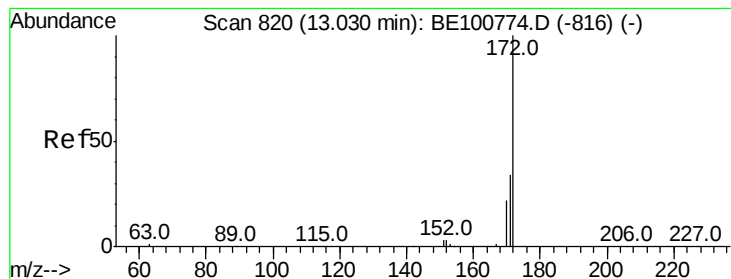

#15

2-Fluorobiphenyl

Concen: 0.184 ng

RT: 13.02 min Scan# 819

Delta R.T. 0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209


Tot Ion:172 Resp: 9655

Ion Ratio Lower Upper

172 100

171 35.7 28.2 42.4




170 24.8 19.4 29.0



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

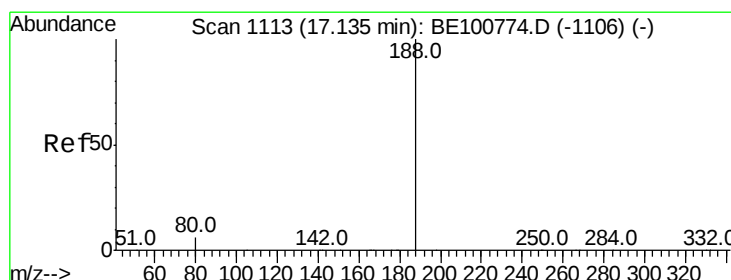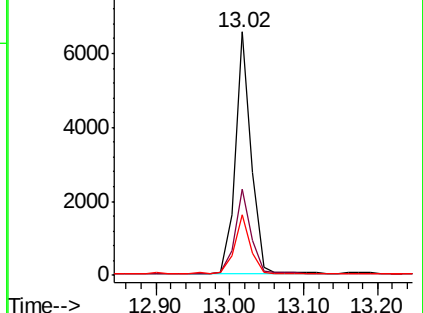

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.12 min Scan# 1112

Delta R.T. -0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34


Tgt Ion:188 Resp: 33635

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 10.1 7.9 11.9




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE1

Ion 80.00 (79.70 to 80.70): BE1

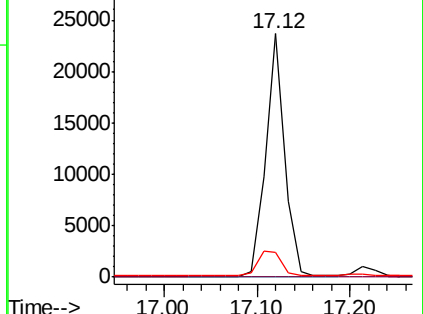



#25

Fluoranthene-d10

Concen: 0.231 ng

RT: 19.15 min Scan# 1372

Delta R.T. 0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209


Tot Ion:212 Resp: 91804

Ion Ratio Lower Upper

212 100

106 3.3 2.6 4.0




104 1.9 1.4 2.2

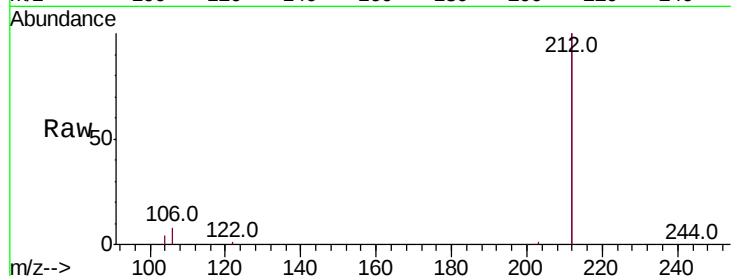

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

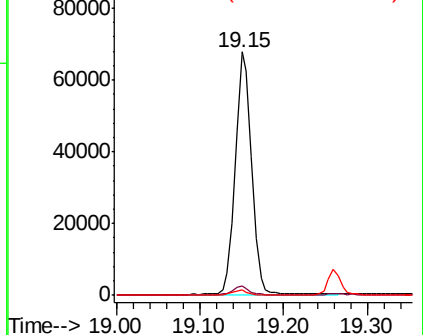

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.29 min Scan# 1624

Delta R.T. -0.01 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34


Tgt Ion:240 Resp: 33175

Ion Ratio Lower Upper

240 100

120 16.7 4.0 6.0#



236 29.0 21.6 32.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

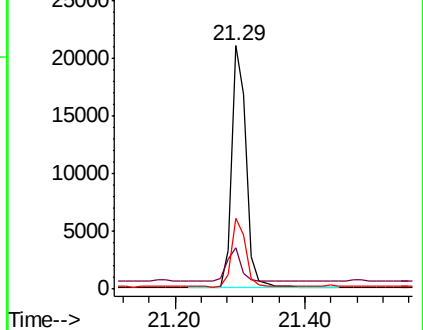



#29

Terphenyl-d14

Concen: 0.219 ng

RT: 19.75 min Scan# 1477

Delta R.T. -0.01 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209


Tot Ion:244 Resp: 17414

Ion Ratio Lower Upper

244 100

212 33.7 25.2 37.8




122 16.4 8.9 13.3#

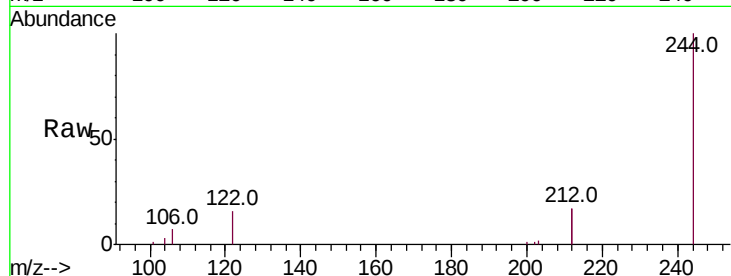

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

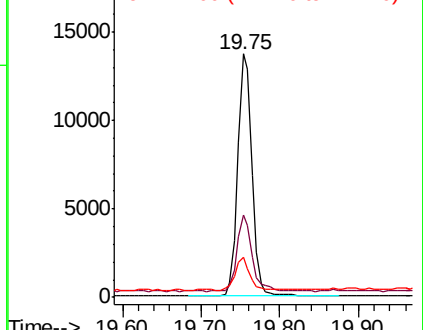

#32

Bis(2-ethylhexyl)phthalate

Concen: 1.575 ng

RT: 21.23 min Scan# 1619

Delta R.T. -0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34


Tgt Ion:149 Resp: 136023

Ion Ratio Lower Upper

149 100

167 6.6 5.0 7.4



279 0.8 0.6 1.0






Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

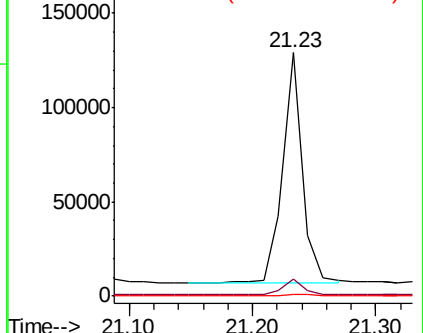

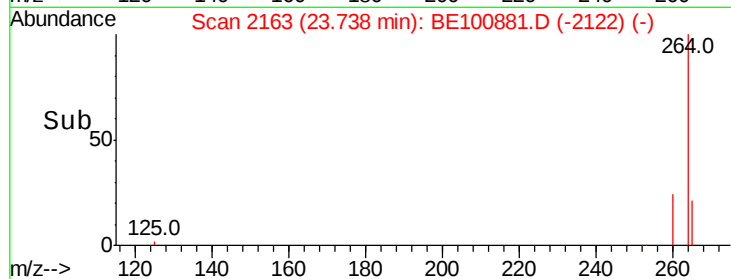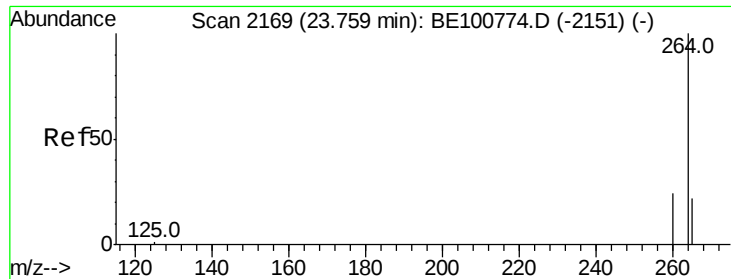

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.74 min Scan# 2163

Delta R.T. -0.00 min

Lab File: BE100881.D

Acq: 13 Dec 2019 11:34

Instrument :

BNA_E

ClientSampleId :

RE132D5-20191209

Tot Ion:264 Resp: 37117

Ion Ratio Lower Upper

264 100

260 24.3 19.4 29.0

265 23.8 20.1 30.1

