


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121319\
 Data File : BE100896.D
 Acq On : 13 Dec 2019 21:25
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 13 10:42:38 2019

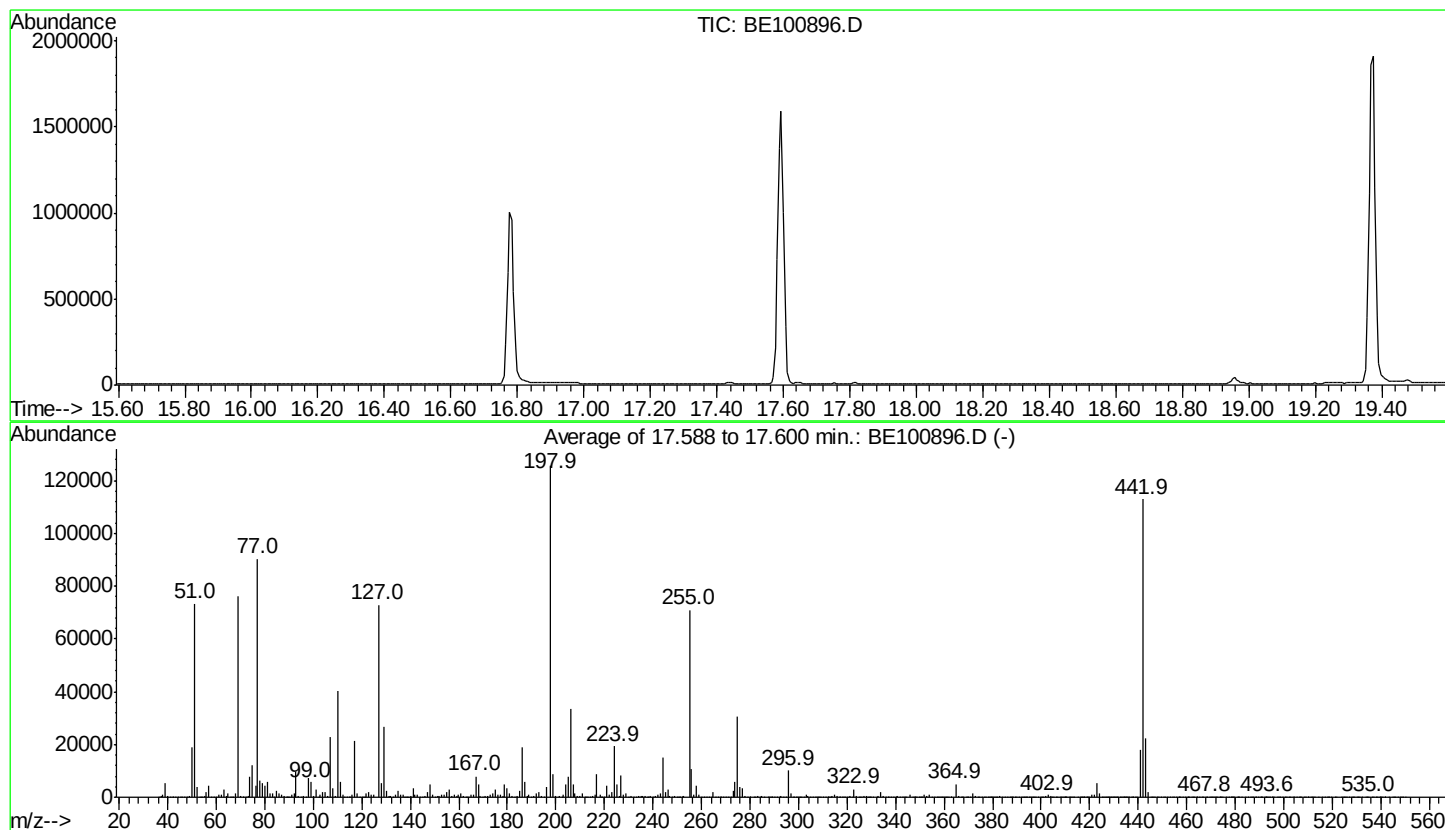

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.3	73286	PASS
68	69	0.00	2	1.7	1305	PASS
69	198	0.00	100	60.5	76080	PASS
70	69	0.00	2	0.5	362	PASS
127	198	10	80	58.1	73014	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125655	PASS
199	198	5	9	6.8	8551	PASS
275	198	10	60	24.2	30362	PASS
365	198	1	100	3.9	4874	PASS
441	198	0.01	100	14.4	18099	PASS
442	198	50	100	89.9	112989	PASS
443	442	15	24	19.6	22162	PASS