

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121418\
 Data File : BE098444.D
 Acq On : 14 Dec 2018 20:16
 Operator : SJ/JU
 Sample : J6343-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW310S-20181209

Quant Time: Dec 14 23:49:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	904	0.40	ng	0.00
7) Naphthalene-d8	10.65	136	3897	0.40	ng	-0.01
13) Acenaphthene-d10	14.53	164	2558	0.40	ng	0.00
19) Phenanthrene-d10	17.27	188	6388	0.40	ng	-0.01
27) Chrysene-d12	21.46	240	7965	0.40	ng	0.00
34) Perylene-d12	24.00	264	7213	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	500	0.24	ng	0.00
5) Phenol-d6	7.04	99	400	0.13	ng	0.00
8) Nitrobenzene-d5	9.03	82	1398	0.39	ng	0.01
11) 2-Methylnaphthalene-d10	12.27	152	2717	0.43	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	508	0.54	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	5532	0.51	ng	0.00
25) Fluoranthene-d10	19.30	212	39307	0.48	ng	0.00
29) Terphenyl-d14	19.90	244	7613	0.39	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.37	88	262	0.168	ng	# 67
32) Bis(2-ethylhexyl)phthalate	21.35	149	3593	0.078	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121418\
Data File : BE098444.D
Acq On : 14 Dec 2018 20:16
Operator : SJ/JU
Sample : J6343-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW310S-20181209

Quant Time: Dec 14 23:49:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

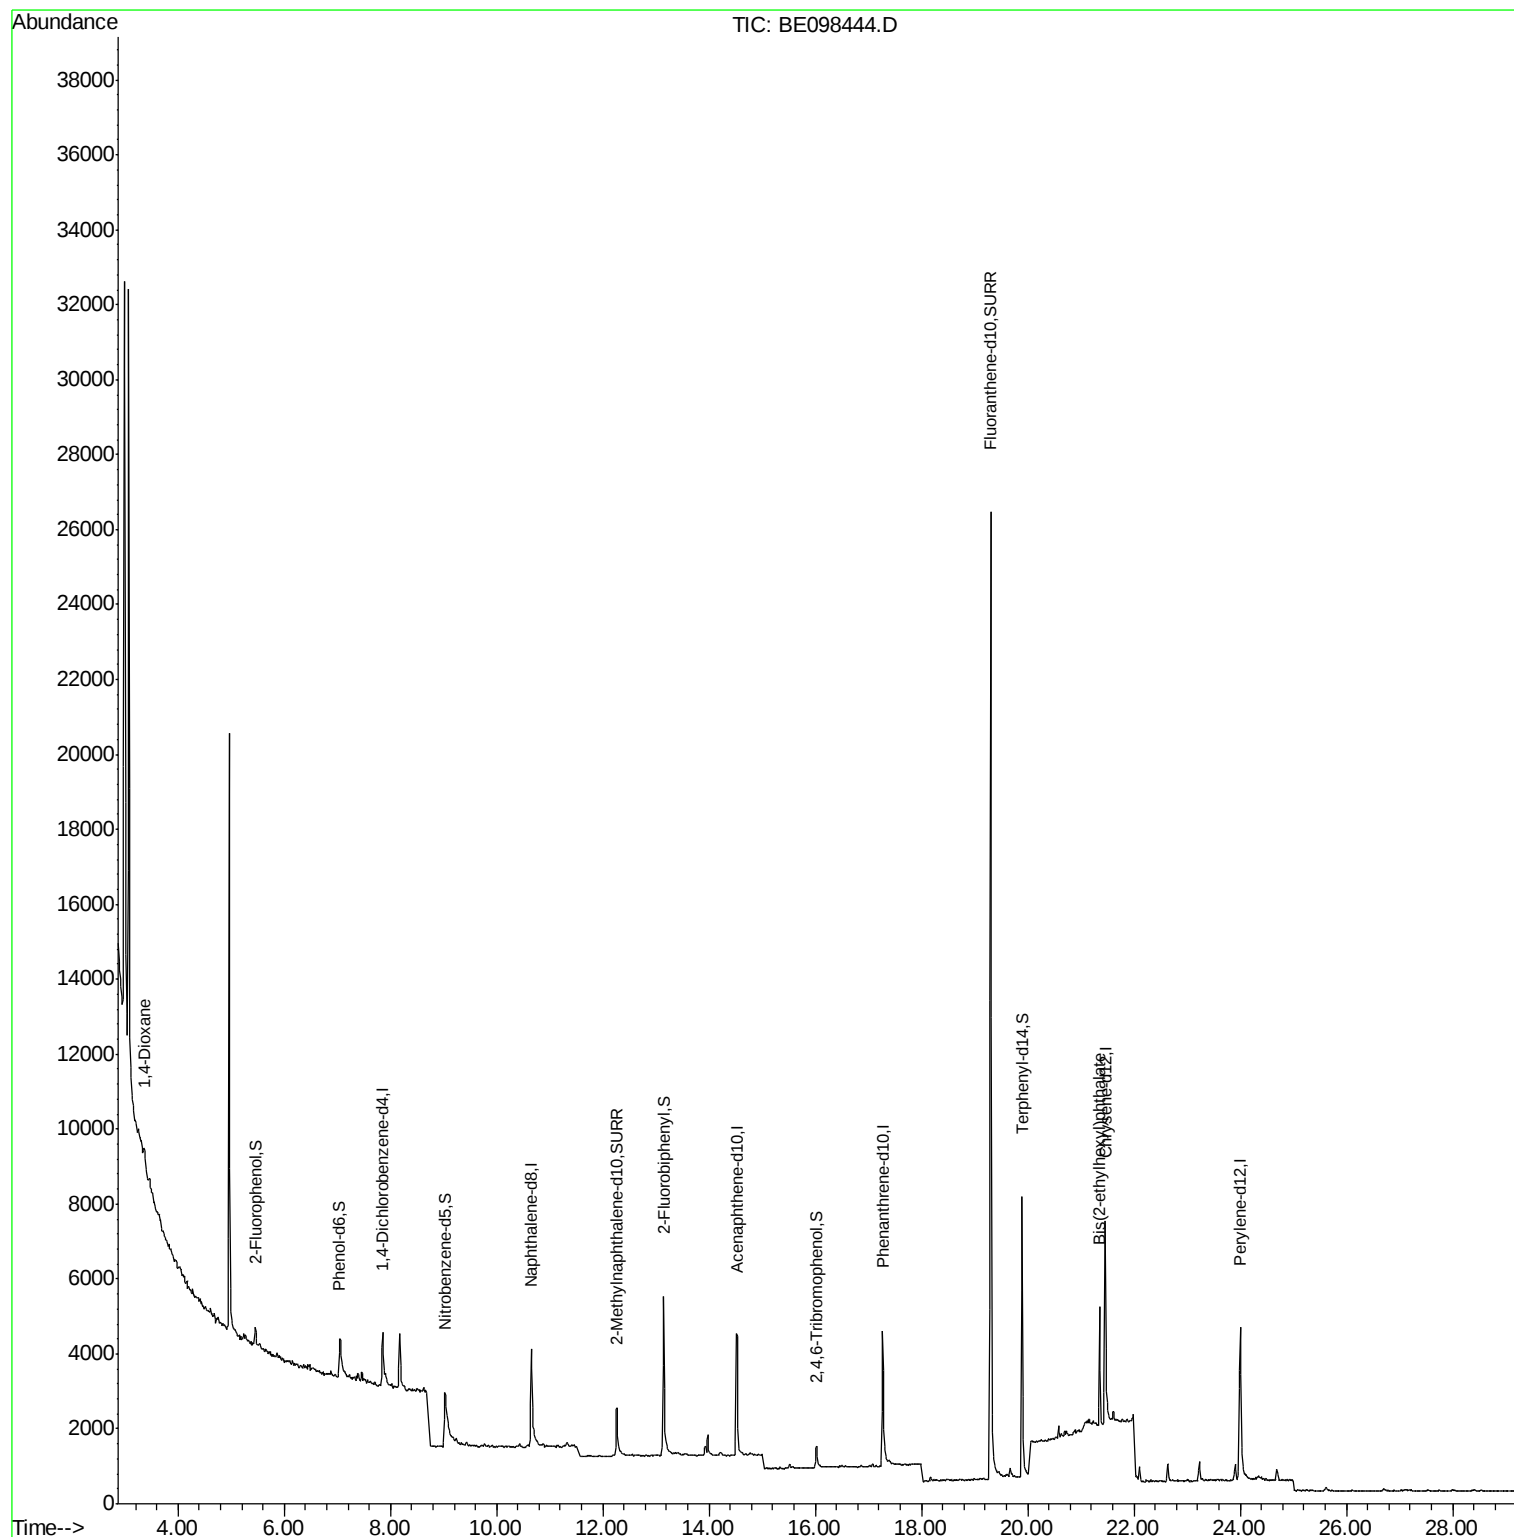



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.86 min Scan# 434

Delta R.T. -0.00 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW310S-20181209


Tot Ion:152 Resp: 904

Ion Ratio Lower Upper

152 100

150 142.2 124.2 186.4



115 71.7 53.9 80.9

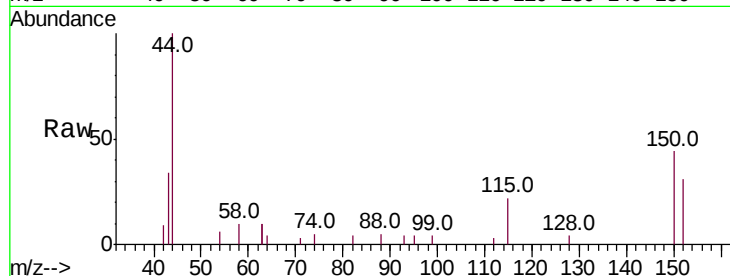

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

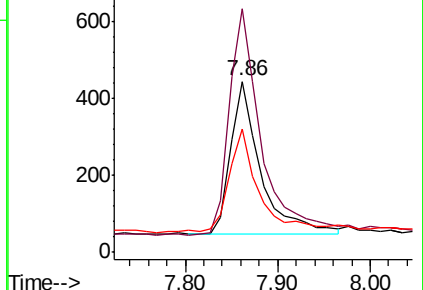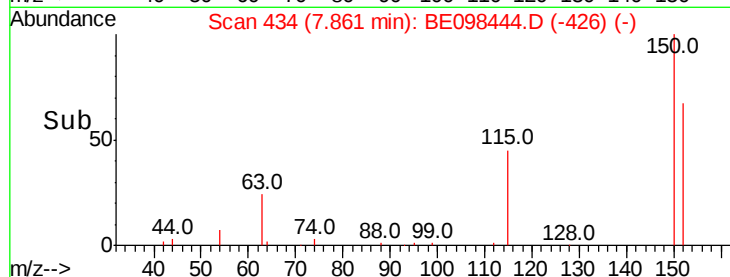

#2

1,4-Dioxane

Concen: 0.168 ng

RT: 3.37 min Scan# 44

Delta R.T. -0.00 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16


Tgt Ion: 88 Resp: 262

Ion Ratio Lower Upper

88 100

58 80.9 75.0 112.6



43 0.0 38.3 57.5#

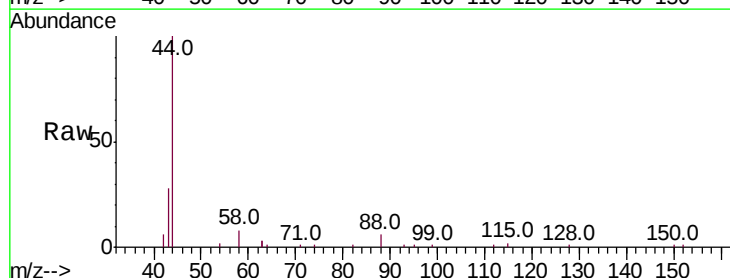

Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

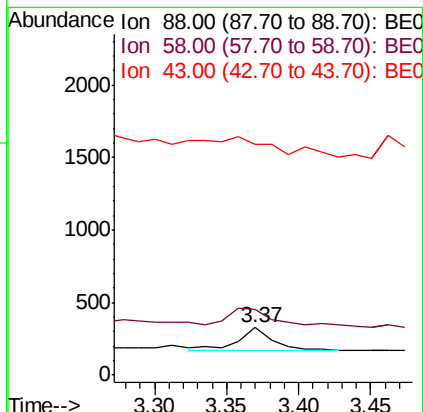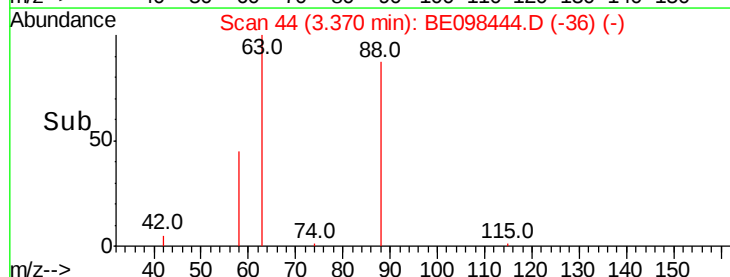



#4

2-Fluorophenol

Concen: 0.236 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW310S-20181209


Tot Ion: 112 Resp: 500

Ion Ratio Lower Upper

112 100

64 74.6 59.8 89.8




63 153.4 133.7 200.5

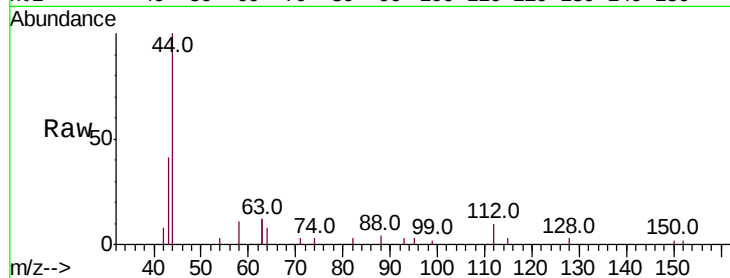

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

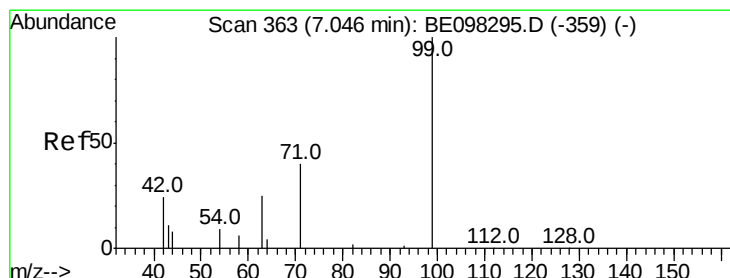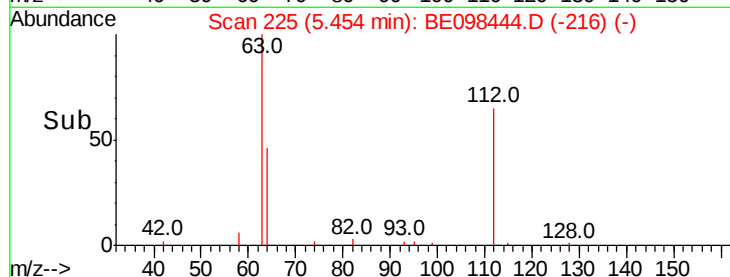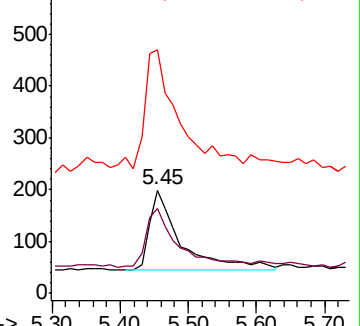

#5

Phenol-d6

Concen: 0.133 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16


Tgt Ion: 99 Resp: 400

Ion Ratio Lower Upper

99 100

42 58.0 26.3 39.5#



71 44.0 33.6 50.4

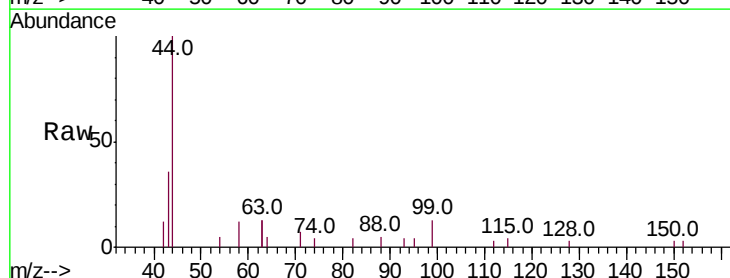


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

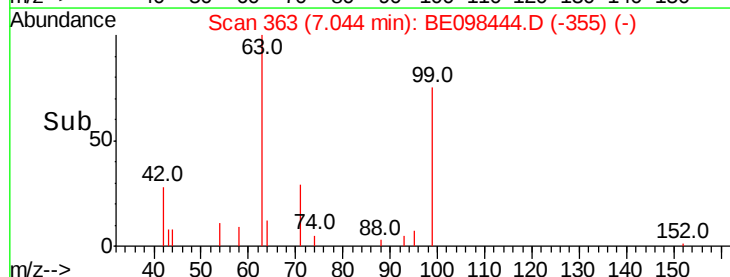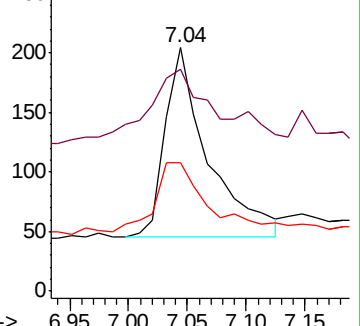

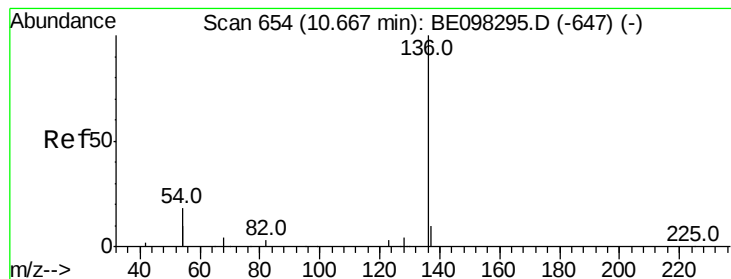

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.65 min Scan# 653

Delta R.T. -0.01 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW310S-20181209

Tot Ion:136 Resp: 3897





Ion Ratio Lower Upper

136 100

137 14.6 9.2 13.8#

54 68.1 28.4 42.6#

68 12.1 5.4 8.0#

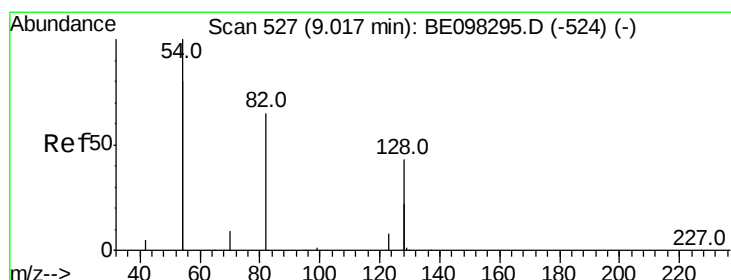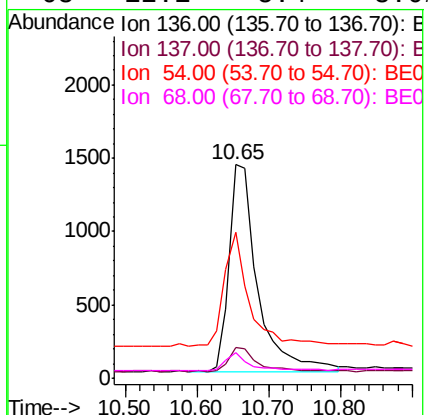

#8

Nitrobenzene-d5

Concen: 0.394 ng

RT: 9.03 min Scan# 528

Delta R.T. 0.01 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16




Tgt Ion: 82 Resp: 1398


Ion Ratio Lower Upper

82 100

128 157.7 102.4 153.6#

54 299.4 221.8 332.8


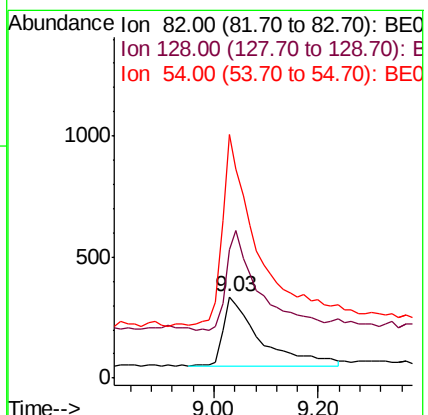




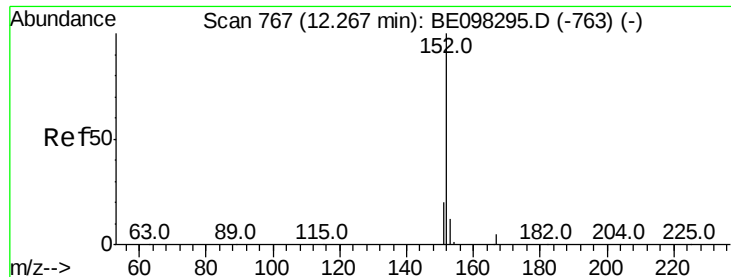

#11
2-Methylnaphthalene-d10
Concen: 0.429 ng
RT: 12.27 min Scan# 767
Delta R.T. -0.00 min
Lab File: BE098444.D
Acq: 14 Dec 2018 20:16




Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW310S-20181209

Tot Ion:152 Resp: 2717
Ion Ratio Lower Upper
152 100
151 18.2 16.2 24.4

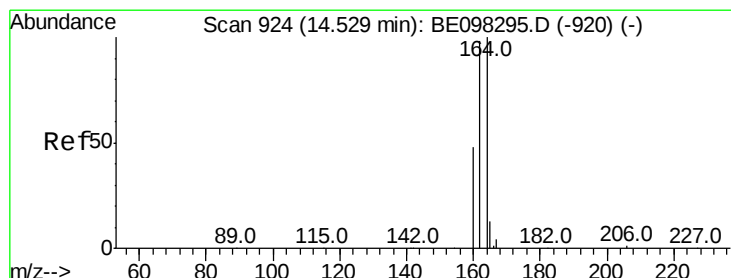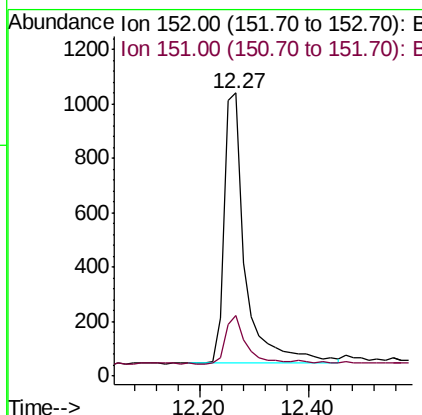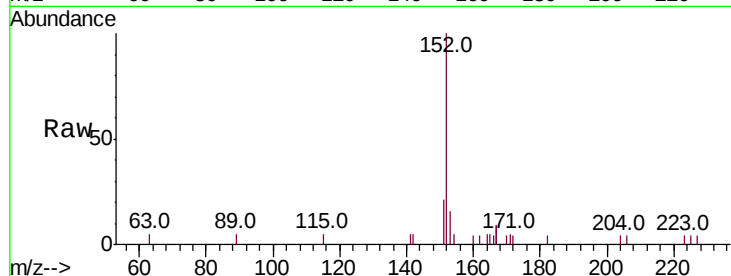

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.53 min Scan# 924
Delta R.T. -0.00 min
Lab File: BE098444.D
Acq: 14 Dec 2018 20:16

Tgt Ion:164 Resp: 2558
Ion Ratio Lower Upper
164 100
162 95.5 77.6 116.4
160 53.3 36.0 54.0

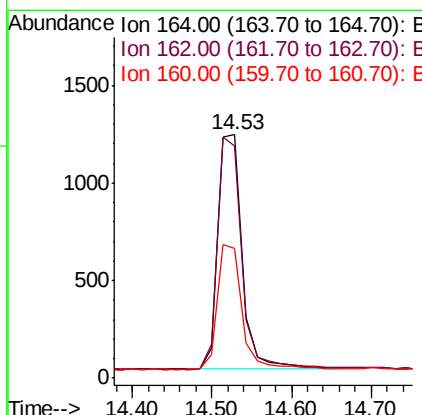







#14
 2,4,6-Tribromophenol
 Concen: 0.541 ng
 RT: 16.02 min Scan# 1041
 Delta R.T. -0.00 min
 Lab File: BE098444.D
 Acq: 14 Dec 2018 20:16

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW310S-20181209

Tot Ion:330 Resp: 508
 Ion Ratio Lower Upper
 330 100
 332 98.6 76.2 114.4
 141 47.8 39.0 58.4

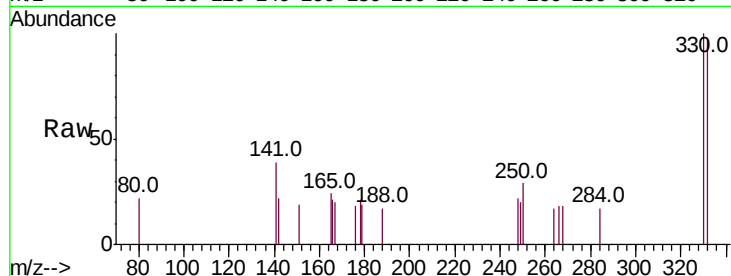


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

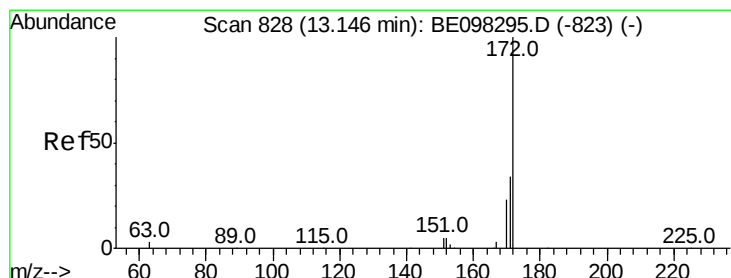
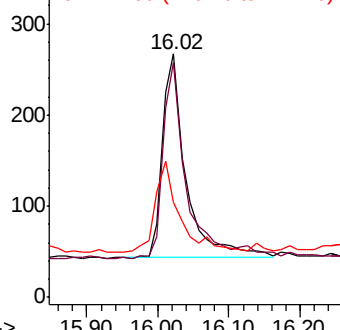



#15
 2-Fluorobiphenyl
 Concen: 0.513 ng
 RT: 13.15 min Scan# 828
 Delta R.T. -0.00 min
 Lab File: BE098444.D
 Acq: 14 Dec 2018 20:16

Tgt Ion:172 Resp: 5532
 Ion Ratio Lower Upper
 172 100
 171 33.2 27.5 41.3
 170 22.7 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

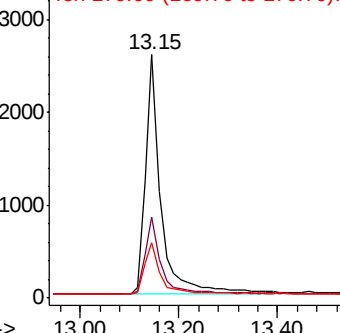

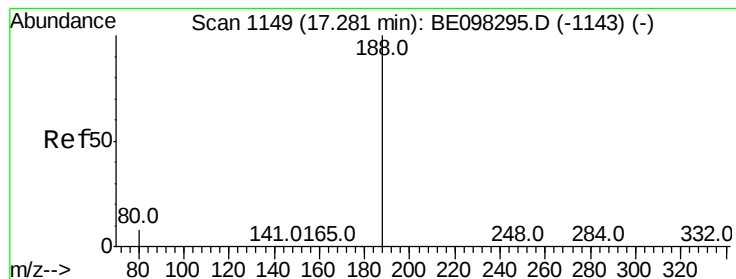

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.27 min Scan# 1148

Delta R.T. -0.01 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW310S-20181209


Tot Ion:188 Resp: 6388

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 11.7 7.2 10.8#

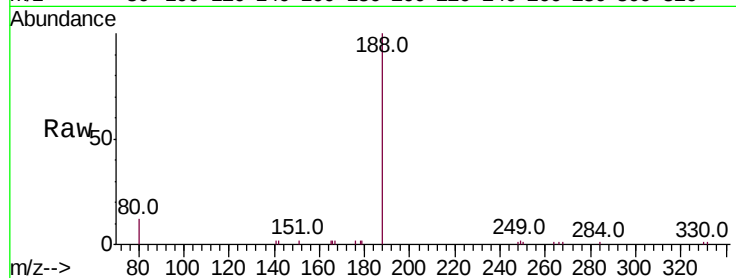

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

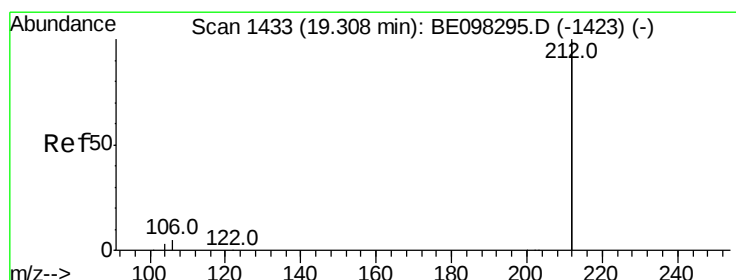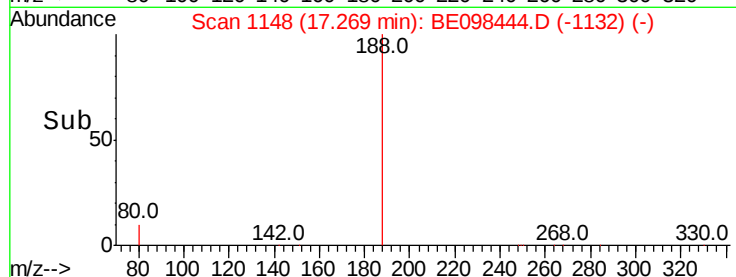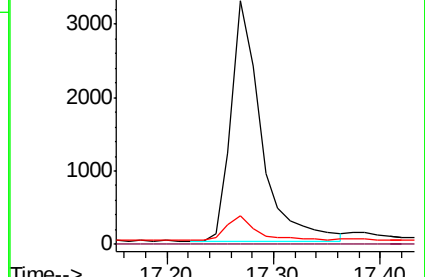

#25

Fluoranthene-d10

Concen: 0.480 ng

RT: 19.30 min Scan# 1432

Delta R.T. -0.01 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16


Tgt Ion:212 Resp: 39307

Ion Ratio Lower Upper

212 100

106 2.5 2.2 3.2



104 1.5 1.3 1.9

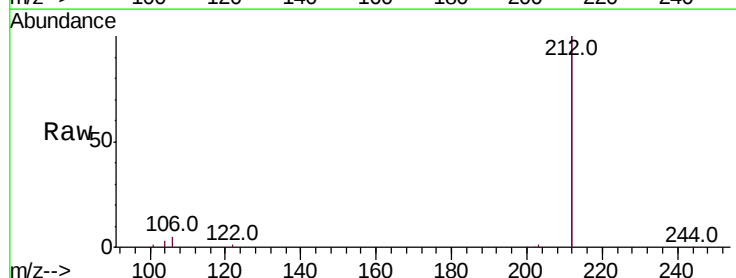

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

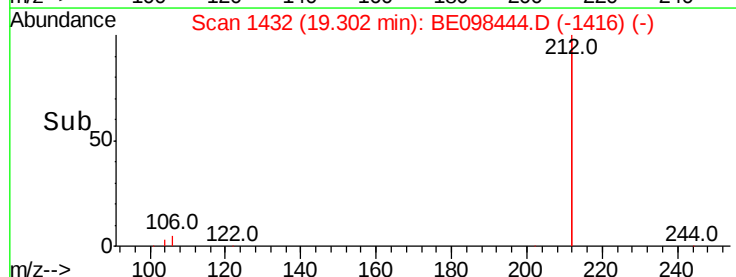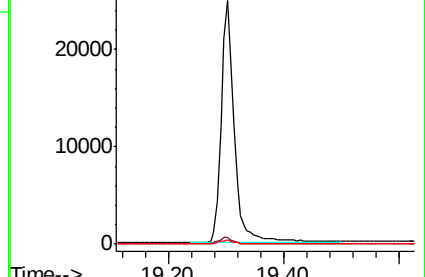



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.46 min Scan# 1671

Delta R.T. -0.00 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW310S-20181209


Tot Ion:240 Resp: 7965

Ion Ratio Lower Upper

240 100

120 7.9 9.5 14.3#




236 27.7 22.7 34.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

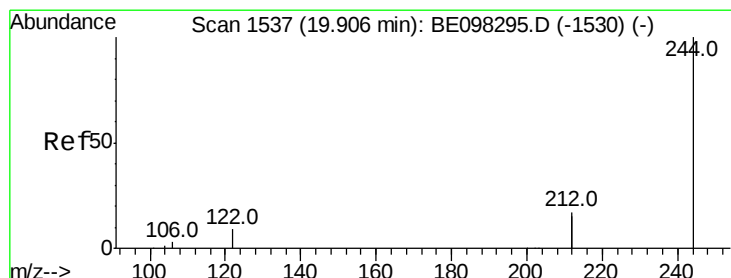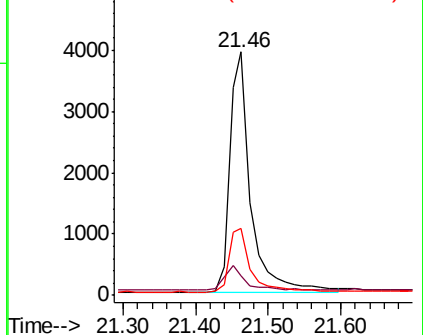

#29

Terphenyl-d14

Concen: 0.393 ng

RT: 19.90 min Scan# 1536

Delta R.T. -0.01 min

Lab File: BE098444.D

Acq: 14 Dec 2018 20:16


Tgt Ion:244 Resp: 7613

Ion Ratio Lower Upper

244 100

212 35.2 27.4 41.0



122 8.6 8.3 12.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




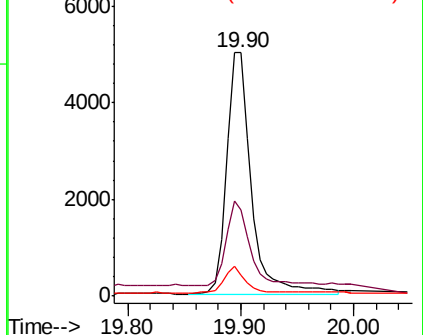


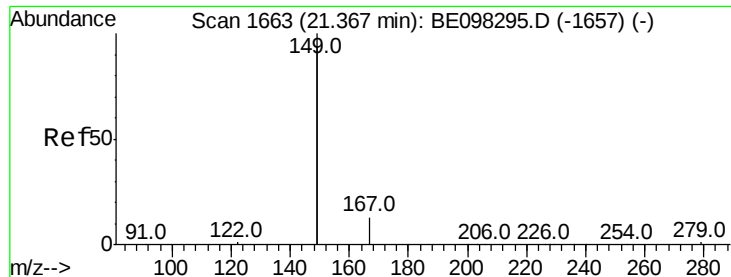

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.078 ng
 RT: 21.35 min Scan# 1662
 Delta R.T. -0.01 min
 Lab File: BE098444.D
 Acq: 14 Dec 2018 20:16

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW310S-20181209

Tot Ion:149 Resp: 3593
 Ion Ratio Lower Upper
 149 100
 167 7.5 5.7 8.5
 279 1.8 1.0 1.4#

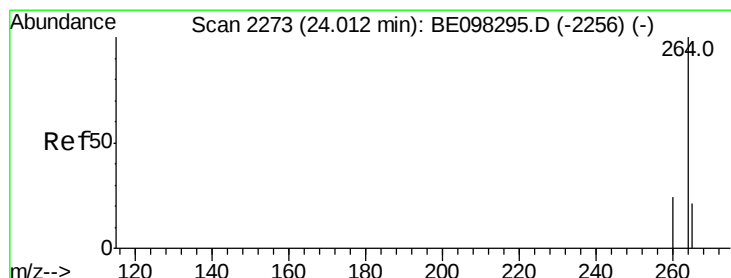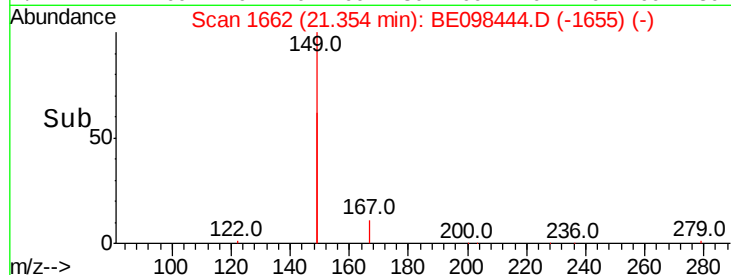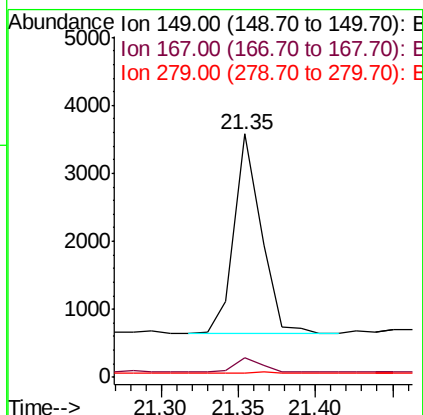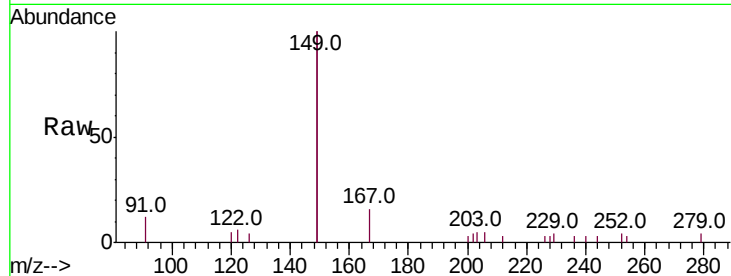

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.00 min Scan# 2269
 Delta R.T. -0.01 min
 Lab File: BE098444.D
 Acq: 14 Dec 2018 20:16

Tgt Ion:264 Resp: 7213
 Ion Ratio Lower Upper
 264 100
 260 27.3 20.2 30.2
 265 28.8 25.2 37.8

