


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121418\
 Data File : BE098434.D
 Acq On : 14 Dec 2018 14:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

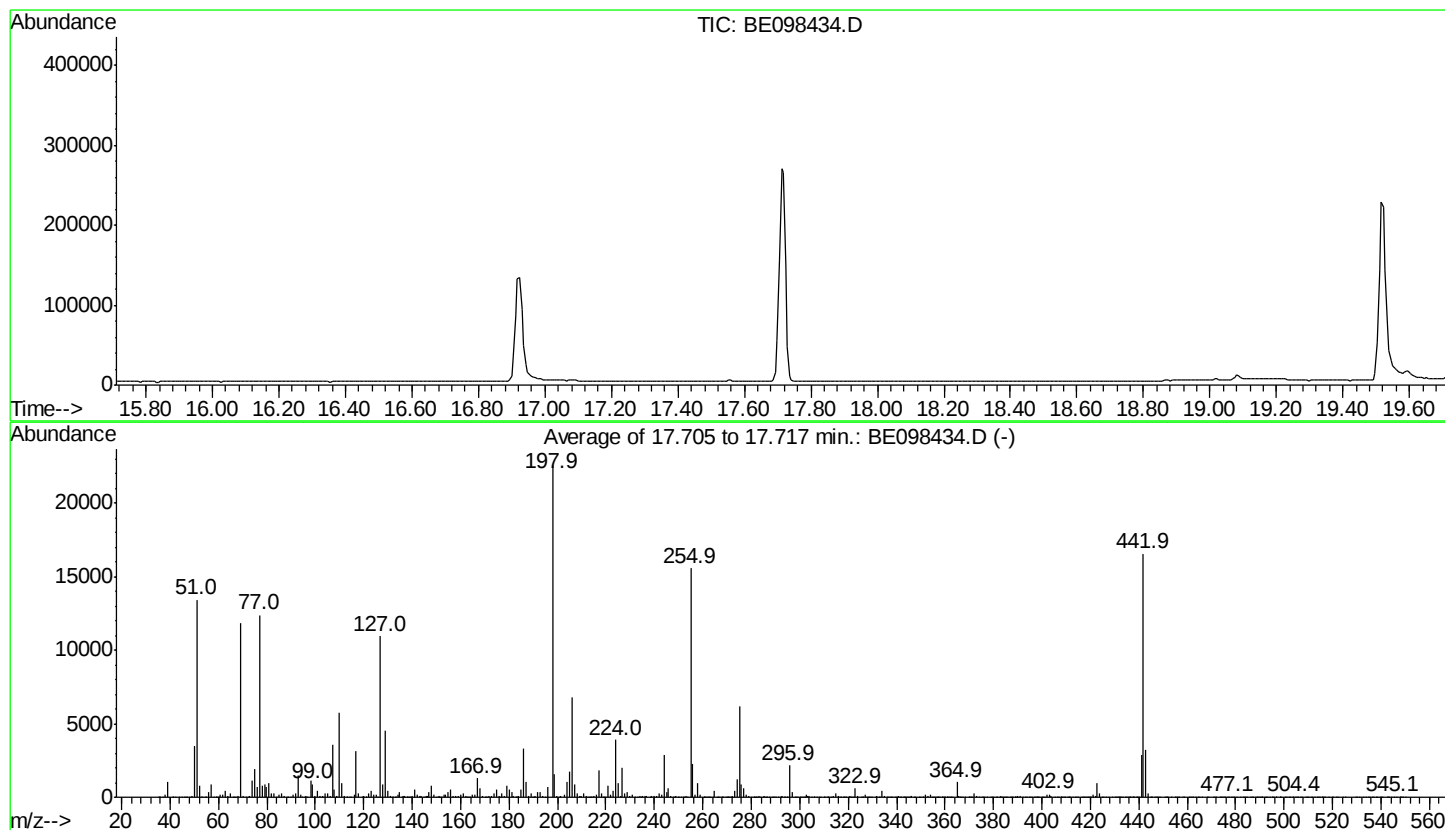

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.6	13438	PASS
68	69	0.00	2	1.0	123	PASS
69	198	0.00	100	52.7	11873	PASS
70	69	0.00	2	0.6	74	PASS
127	198	10	80	48.5	10925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22541	PASS
199	198	5	9	6.8	1543	PASS
275	198	10	60	27.3	6156	PASS
365	198	1	100	4.5	1017	PASS
441	198	0.01	100	12.6	2850	PASS
442	198	50	100	73.5	16566	PASS
443	442	15	24	19.2	3181	PASS