


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121418\
 Data File : BE098453.D
 Acq On : 15 Dec 2018 3:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

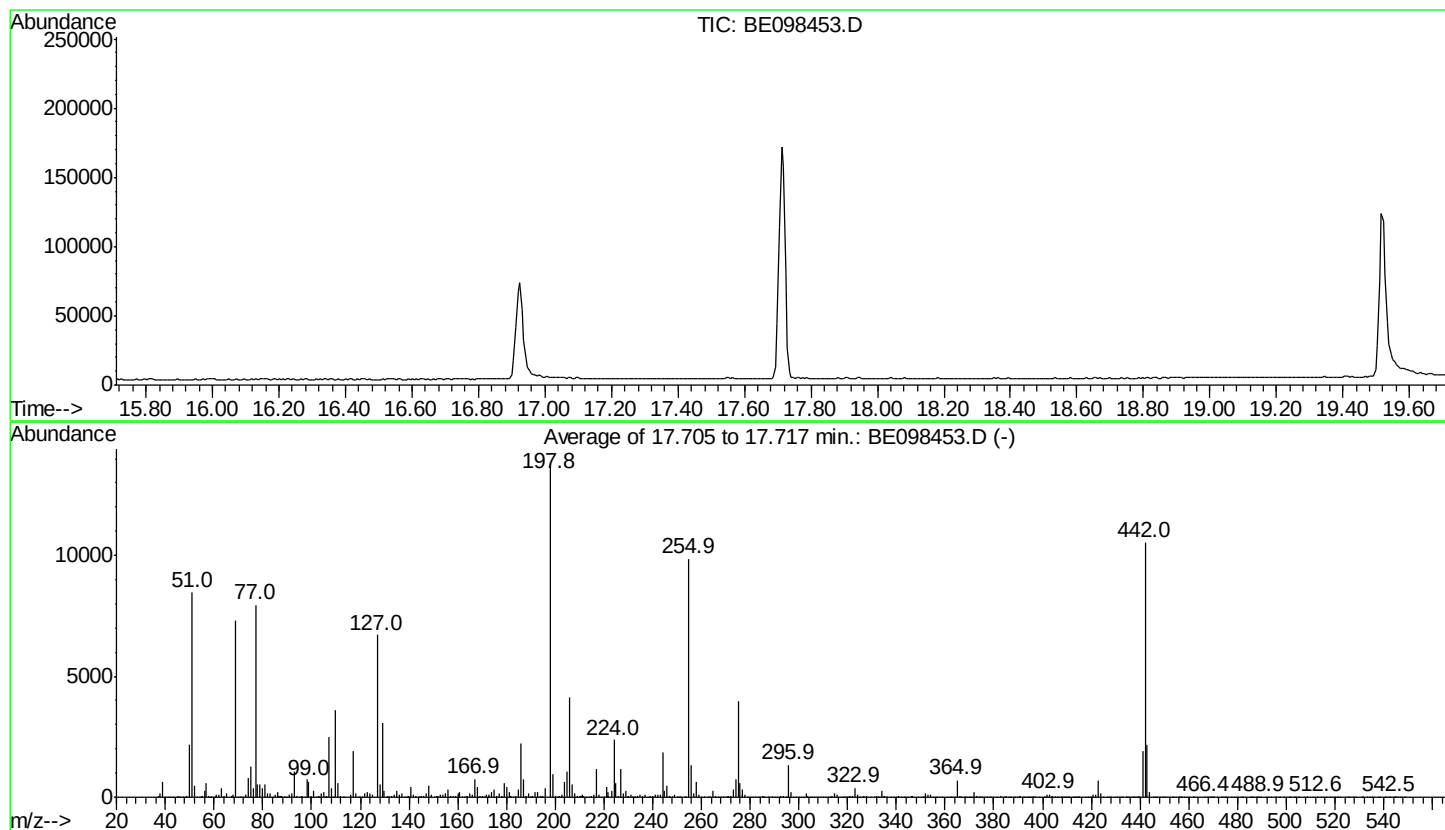

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.7	8462	PASS
68	69	0.00	2	1.2	85	PASS
69	198	0.00	100	53.2	7291	PASS
70	69	0.00	2	0.2	18	PASS
127	198	10	80	48.9	6713	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13715	PASS
199	198	5	9	6.9	950	PASS
275	198	10	60	29.0	3979	PASS
365	198	1	100	5.1	699	PASS
441	198	0.01	100	14.0	1921	PASS
442	198	50	100	76.8	10533	PASS
443	442	15	24	20.6	2172	PASS