

Data Path : U:\HPCHEM1\BNA E\DATA\BE121515\
 Data File : BE091343.D
 Acq On : 15 Dec 2015 4:10
 Operator : UM/SJ
 Sample : PB87220BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Dec 15 07:58:32 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 15 04:50:57 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	7760	0.40	ng/ul	-0.07
4) Naphthalene-d8	9.54	136	36922	0.40	ng/ul	-0.04
8) Acenaphthene-d10	13.36	164	10746	0.40	ng/ul	-0.01
12) Phenanthrene-d10	16.16	188	3802872	0.40	ng/ul	0.06
18) Chrysene-d12	20.23	240	14850	0.40	ng/ul	0.00
22) Perylene-d12	21.98	264	4040389	0.40	ng/ul	-0.13
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.90	96	52920	9.70	ng/uL	-0.05
6) 2-Methylnaphthalene-d10	11.08	152	6354	0.26	ng/ul	0.00
16) Fluoranthene-d10	18.06	212	13210	0.00	ng/ul	-0.01
Target Compounds						
19) Pyrene	18.45	202	35055	0.21	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA E\DATA\BE121515\
Data File : BE091343.D
Acq On : 15 Dec 2015 4:10
Operator : UM/SJ
Sample : PB87220BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Dec 15 07:58:32 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 04:50:57 2015
Response via : Initial Calibration

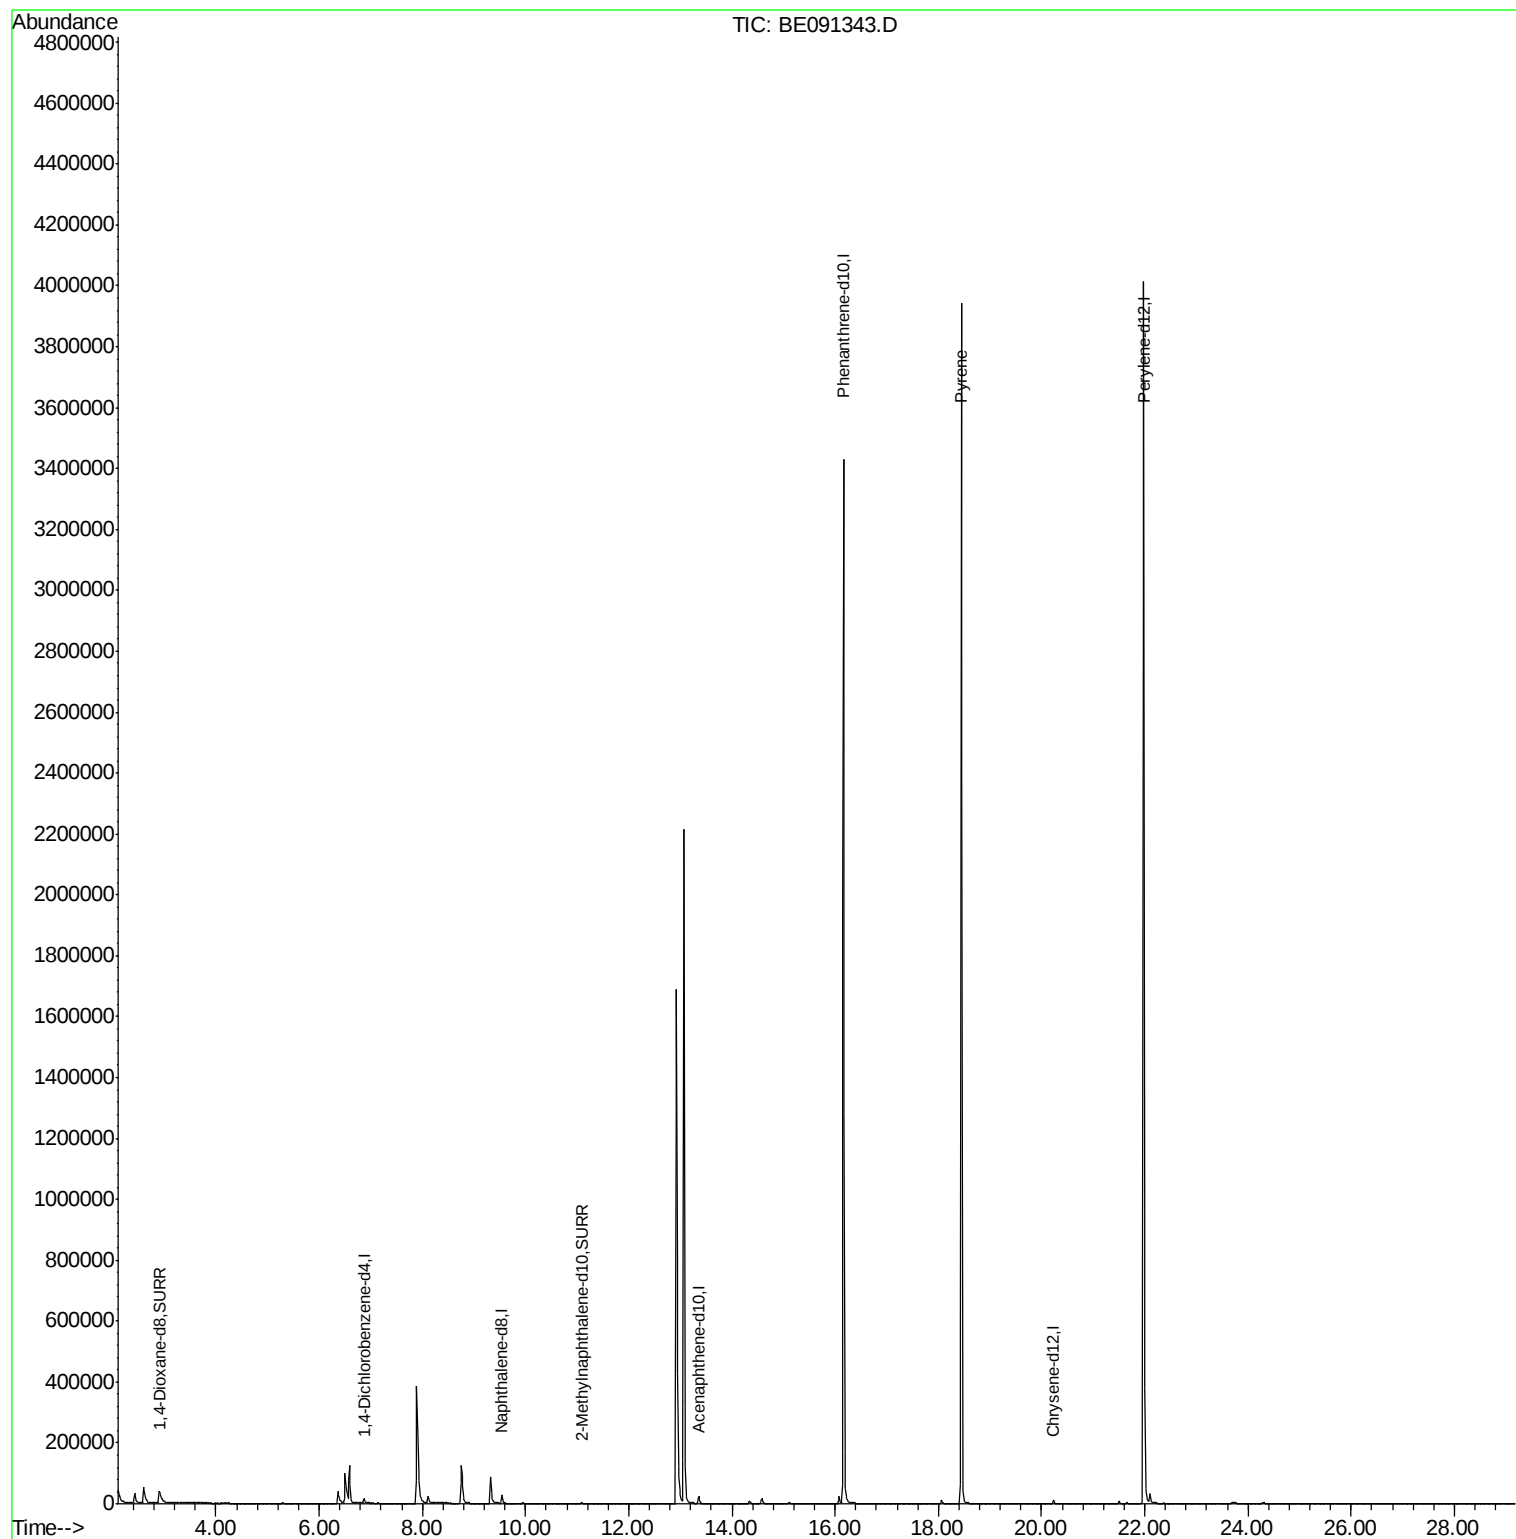

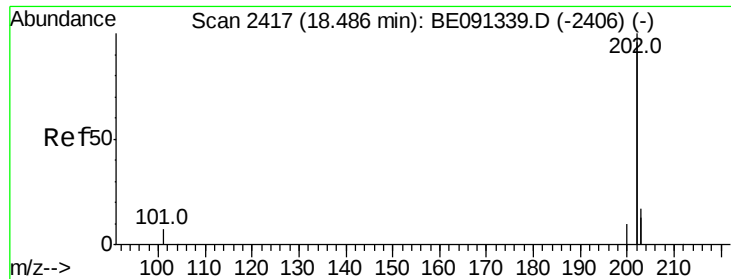

#19

Pvrene

Concen: 0.21 ng/ul

RT: 18.45 min Scan# 2411

Delta R.T. -0.04 min

Lab File: BE091343.D

Acq: 15 Dec 2015 4:10

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 35055

Ion Ratio Lower Upper

202 100

200 1.4 4.4 6.6#

203 213.4 13.8 20.8#

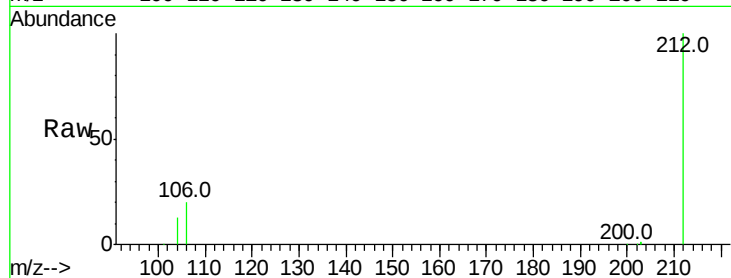

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

