

Data Path : U:\HPCHEM1\BNA E\DATA\BE121515\
 Data File : BE091344.D
 Acq On : 15 Dec 2015 4:52
 Operator : UM/SJ
 Sample : G4734-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Dec 15 07:58:38 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 15 04:50:57 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	8912	0.40	ng/ul	-0.07
4) Naphthalene-d8	9.54	136	43042	0.40	ng/ul	-0.04
8) Acenaphthene-d10	13.36	164	13233	0.40	ng/ul	-0.01
12) Phenanthrene-d10	16.16	188	3944326	0.40	ng/ul	0.06
18) Chrysene-d12	20.23	240	27644	0.40	ng/ul	0.00
22) Perylene-d12	21.98	264	4060423	0.40	ng/ul	-0.13
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.94	96	11361	1.81	ng/uL	-0.01
6) 2-Methylnaphthalene-d10	11.08	152	6720	0.23	ng/ul	0.00
16) Fluoranthene-d10	18.06	212	19627	0.00	ng/ul	-0.01
Target Compounds						
					Ovalue	
11) Fluorene	14.34	166	7673	0.13	ng/ul#	7
19) Pyrene	18.45	202	43562	0.14	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA E\DATA\BE121515\
Data File : BE091344.D
Acq On : 15 Dec 2015 4:52
Operator : UM/SJ
Sample : G4734-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Dec 15 07:58:38 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 04:50:57 2015
Response via : Initial Calibration




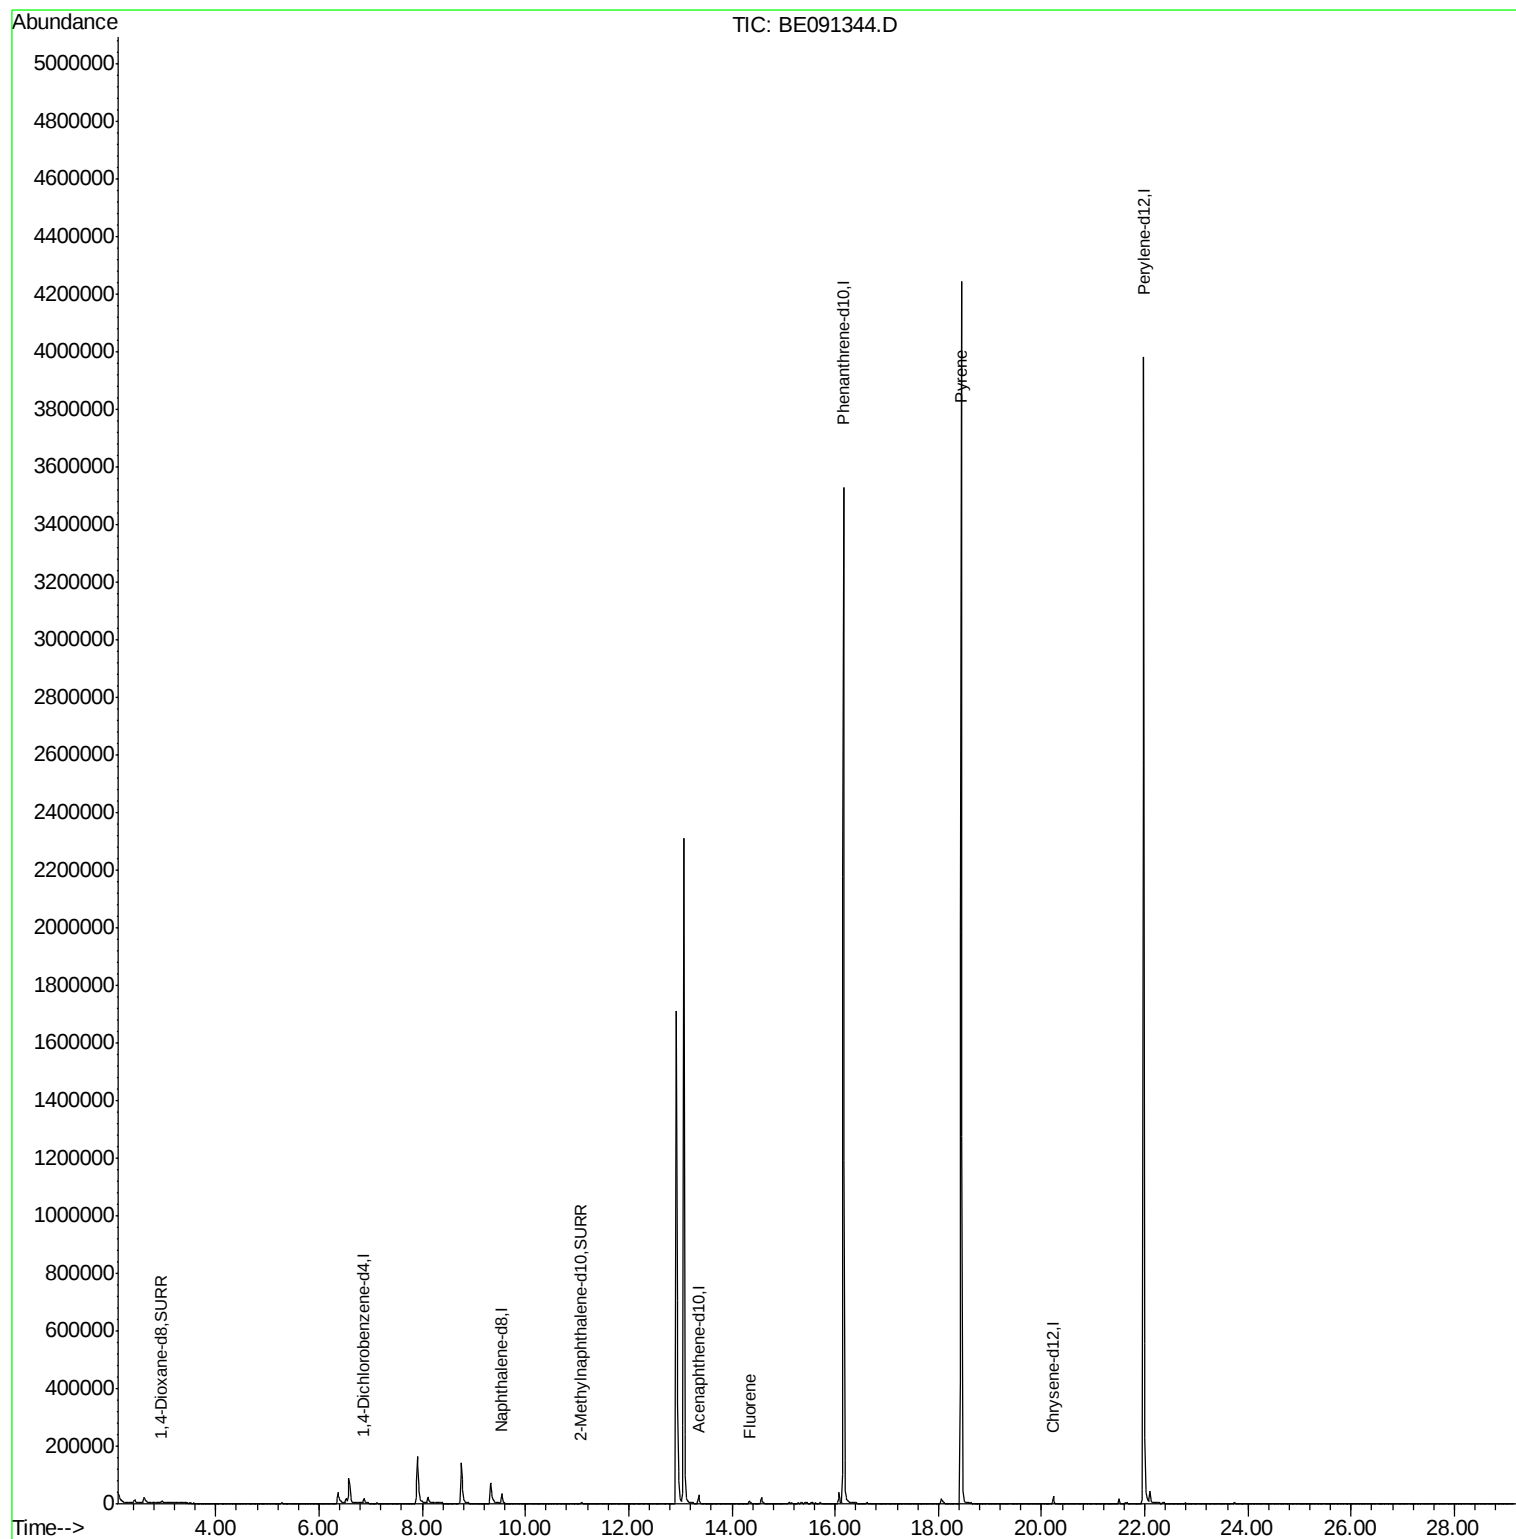


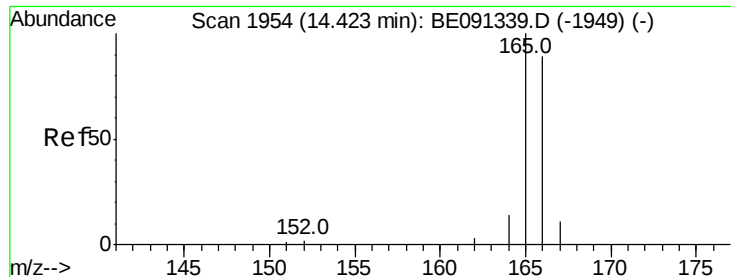

#11
Fluorene
 Concen: 0.13 ng/ul
 RT: 14.34 min Scan# 1943
 Delta R.T. -0.08 min
 Lab File: BE091344.D
 Acq: 15 Dec 2015 4:52

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 7673
 Ion Ratio Lower Upper
 166 100
 165 7.0 90.2 135.4#
 167 36.9 12.2 18.2#

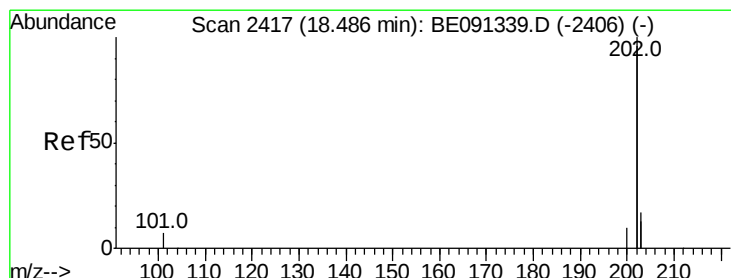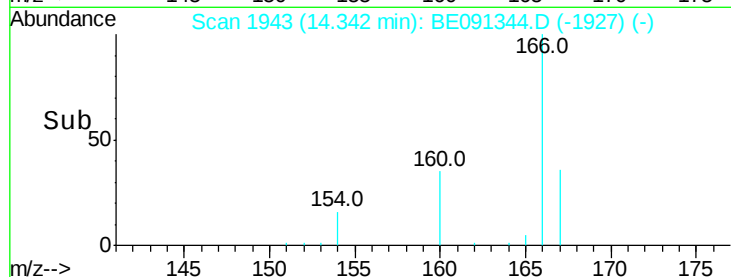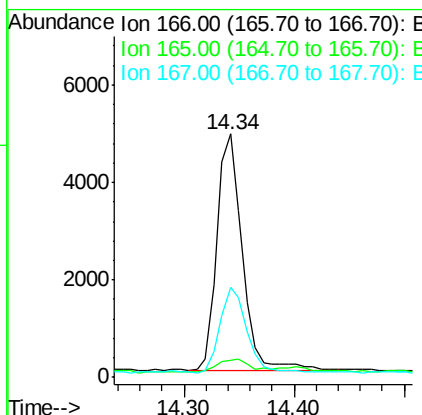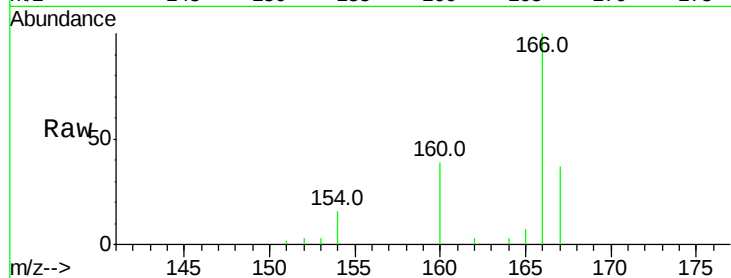

#19
Pyrene
 Concen: 0.14 ng/ul
 RT: 18.45 min Scan# 2411
 Delta R.T. -0.04 min
 Lab File: BE091344.D
 Acq: 15 Dec 2015 4:52

Tgt Ion:202 Resp: 43562
 Ion Ratio Lower Upper
 202 100
 200 1.6 4.4 6.6#
 203 185.2 13.8 20.8#

