

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE121515\
 Data File : BE091347.D
 Acq On : 15 Dec 2015 6:45
 Operator : UM/SJ
 Sample : G4734-04MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A4KW2MSD

Manual Integrations
 APPROVED

MMdadoda
 12/15/2015 6:15:23 PM

Quant Time: Dec 15 08:16:33 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 15 04:50:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	7930	0.40	ng/ul	-0.08
4) Naphthalene-d8	9.54	136	37195	0.40	ng/ul	-0.04
8) Acenaphthene-d10	13.35	164	14287	0.40	ng/ul	-0.02
12) Phenanthrene-d10	16.08	188	43576m	0.40	ng/ul	-0.02
18) Chrysene-d12	20.23	240	39447	0.40	ng/ul	0.00
22) Perylene-d12	22.10	264	64529m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	2.95	96	11923	2.14	ng/uL	0.00
6) 2-Methylnaphthalene-d10	11.07	152	8445	0.34	ng/ul	-0.02
16) Fluoranthene-d10	18.06	212	30568	0.41	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) 2-Methylnaphthalene	11.15	142	553351	19.20	ng/ul#	6
9) Acenaphthylene	13.09	152	2436	0.04	ng/ul#	94
10) Acenaphthene	13.40	153	2149943	41.27	ng/ul#	73
13) Pentachlorophenol	15.83	266	335474	107.77	ng/ul#	85
19) Pyrene	18.47	202	19305425	43.96	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE121515\
Data File : BE091347.D
Acq On : 15 Dec 2015 6:45
Operator : UM/SJ
Sample : G4734-04MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
A4KW2MSD

Manual Integrations
APPROVED

MMdadoda
12/15/2015 6:15:23 PM

Quant Time: Dec 15 08:16:33 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 04:50:57 2015
Response via : Initial Calibration

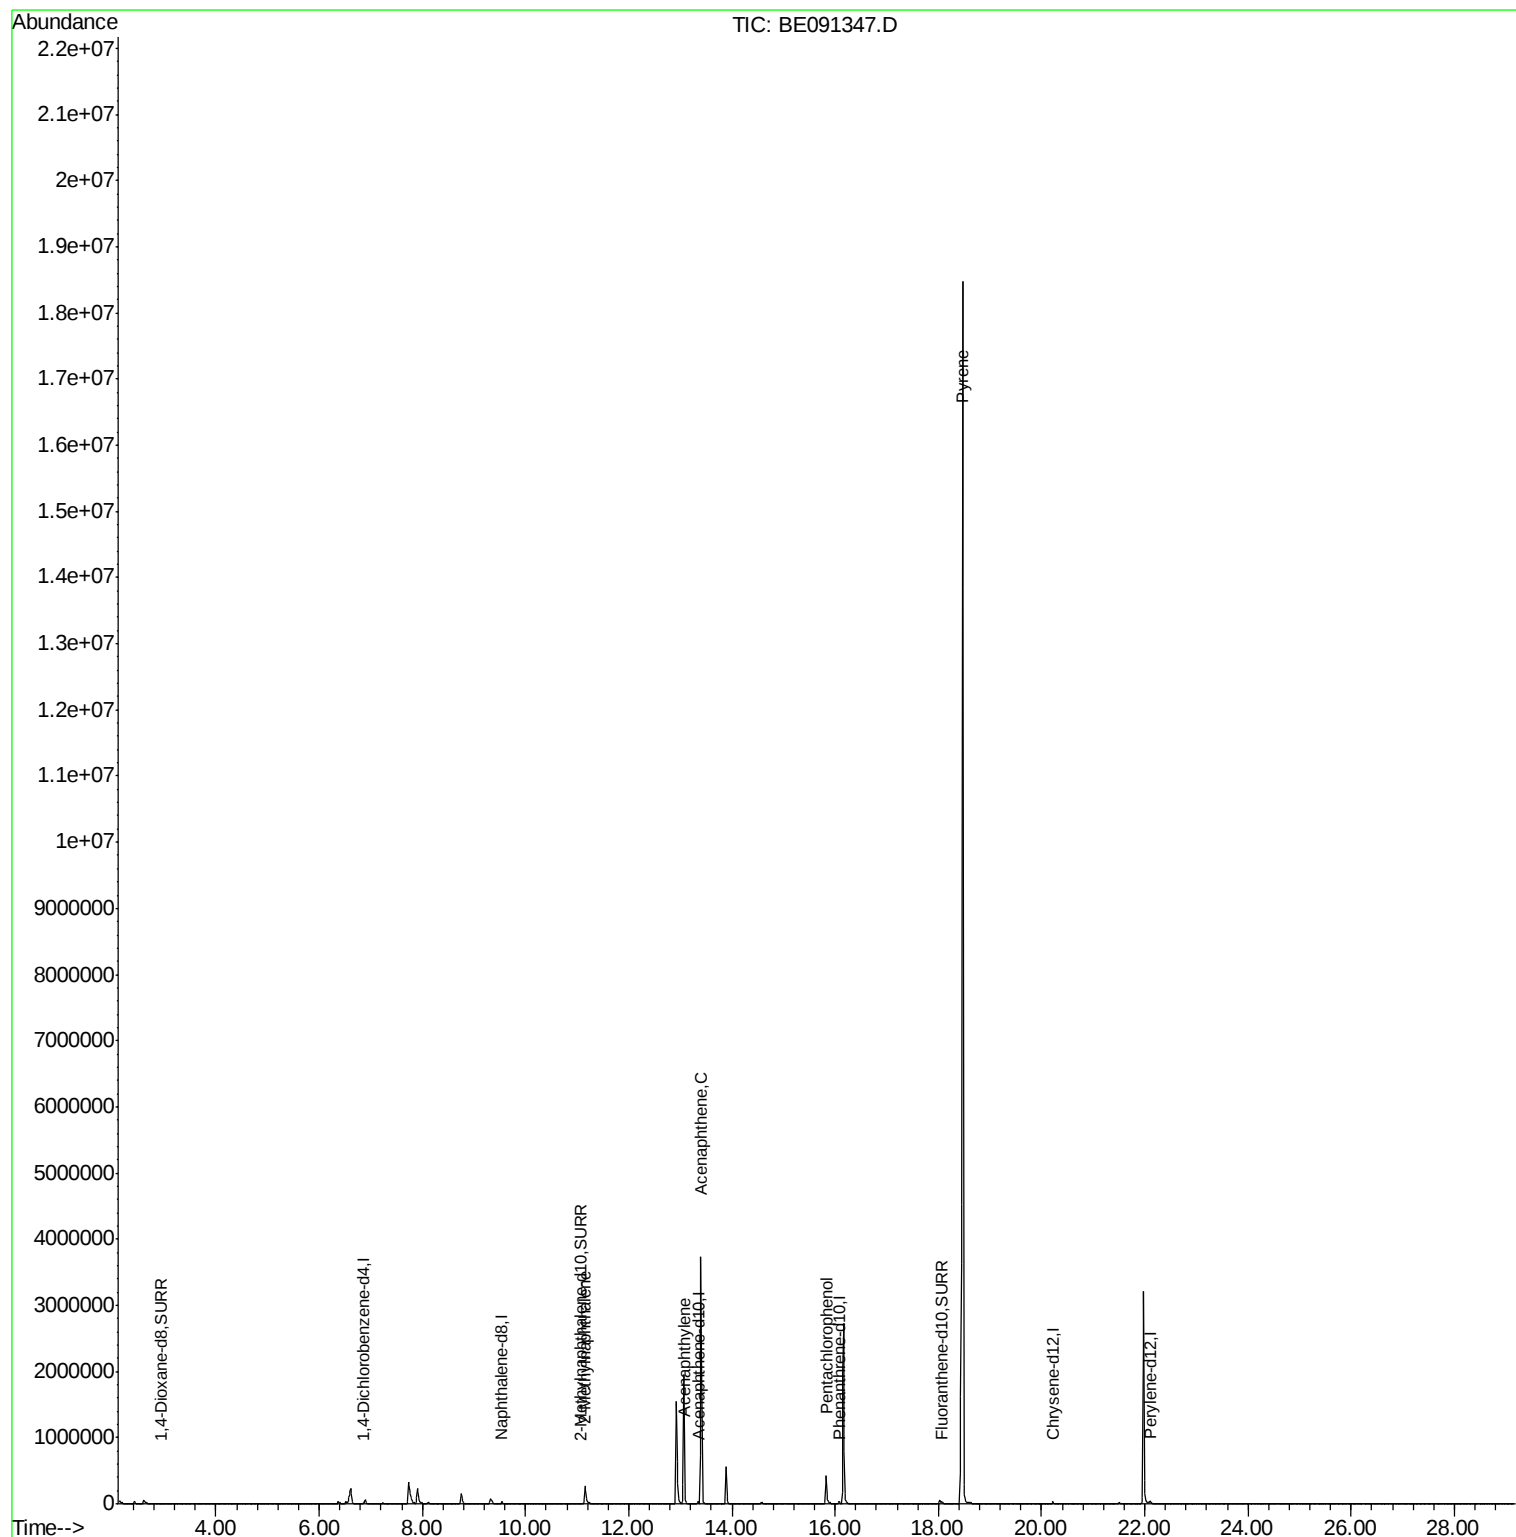

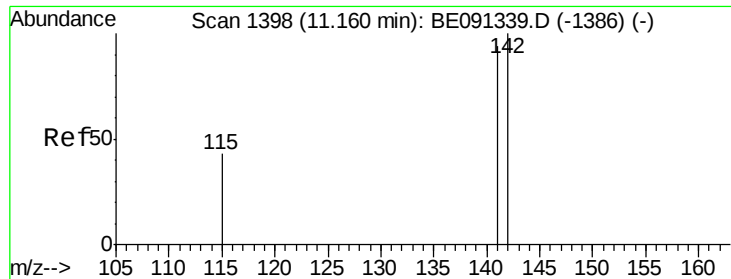

#7

2-Methylnaphthalene

Concen: 19.20 ng/ul

RT: 11.15 min Scan# 1396

Delta R.T. -0.01 min

Lab File: BE091347.D

Acq: 15 Dec 2015 6:45

Instrument :

BNA_E





ClientSampleId :

A4KW2MSD

Manual Integrations
APPROVED

MMdadoda
12/15/2015 6:15:23 PM

Tgt Ion:142 Resp: 553351
Ion Ratio Lower Upper
142 100
141 11.3 89.4 134.2#

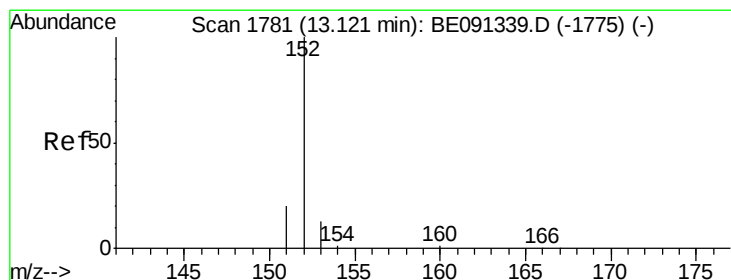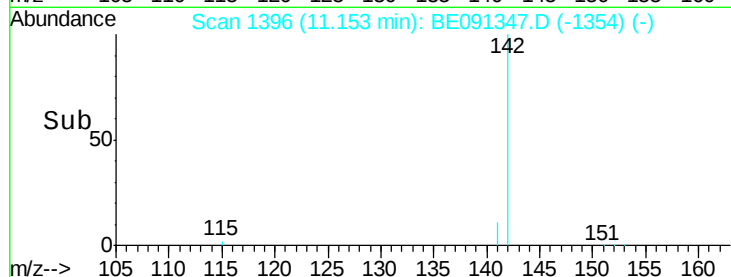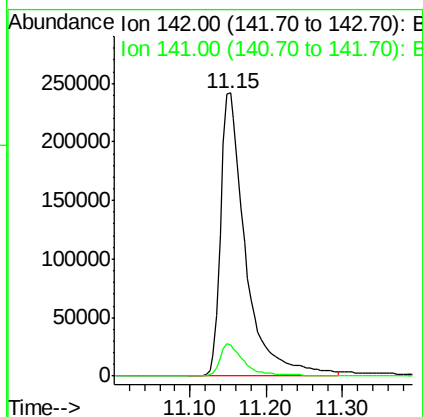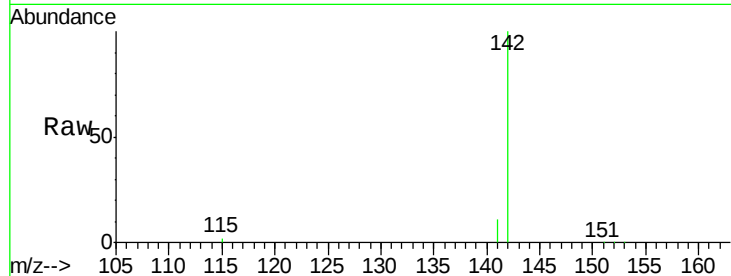

#9

Acenaphthylene

Concen: 0.04 ng/ul




RT: 13.09 min Scan# 1777


Delta R.T. -0.03 min

Lab File: BE091347.D

Acq: 15 Dec 2015 6:45

Tgt Ion:152 Resp: 2436
Ion Ratio Lower Upper
152 100
151 24.1 17.8 26.8
153 19.4 12.4 18.6#

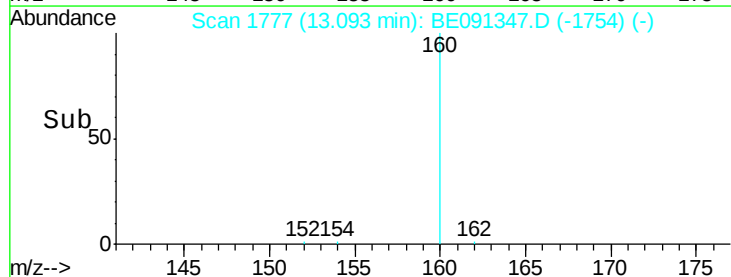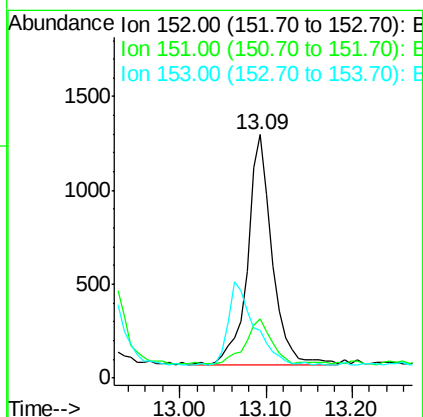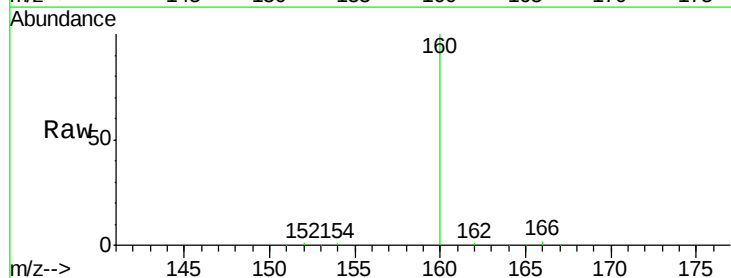

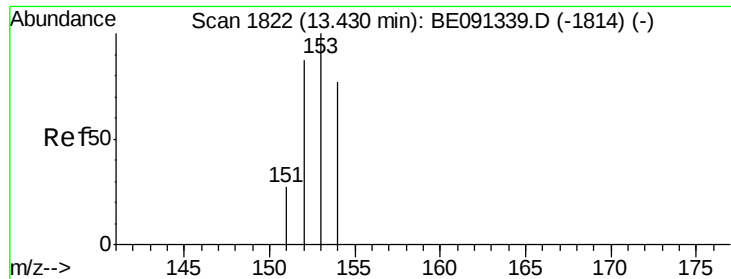

#10

Acenaphthene

Concen: 41.27 ng/ul

RT: 13.40 min Scan# 1818

Delta R.T. -0.03 min

Lab File: BE091347.D


Acq: 15 Dec 2015 6:45

Instrument :

BNA_E

ClientSampleId :

A4KW2MSD

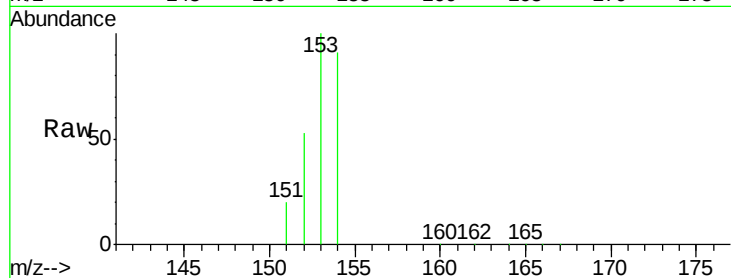

Tgt Ion:153 Resp: 2149943

Ion Ratio Lower Upper




153 100

152 53.4 70.5 105.7#

154 90.6 62.3 93.5

Manual Integrations
APPROVED

MMdadoda
12/15/2015 6:15:23 PM

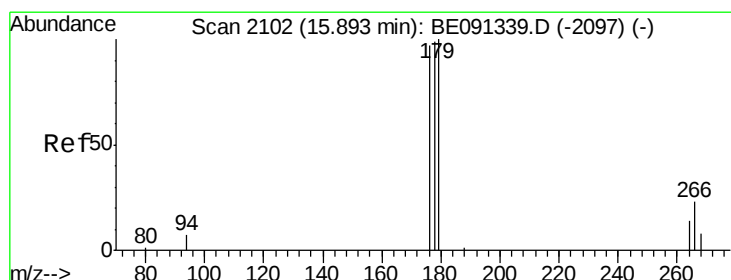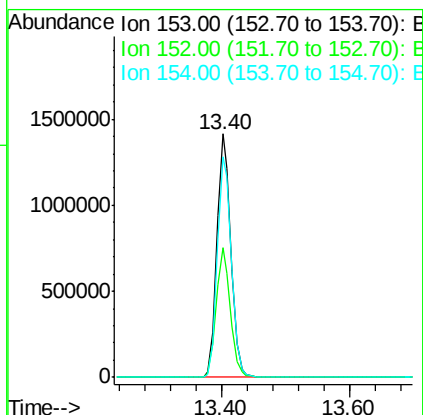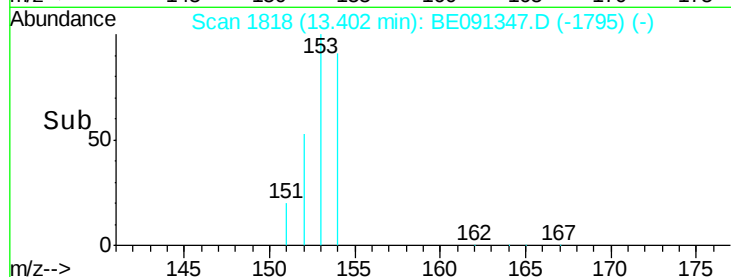

#13

Pentachlorophenol

Concen: 107.77 ng/ul

RT: 15.83 min Scan# 2097

Delta R.T. -0.06 min

Lab File: BE091347.D

Acq: 15 Dec 2015 6:45




Tgt Ion:266 Resp: 335474




Ion Ratio Lower Upper

266 100

264 63.2 54.7 82.1

268 63.8 36.2 54.2#

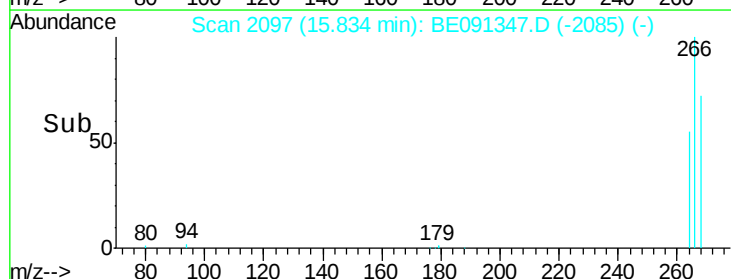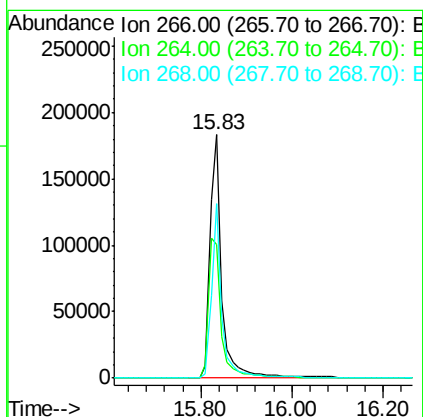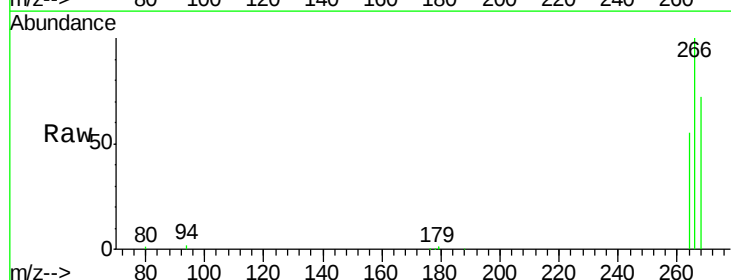

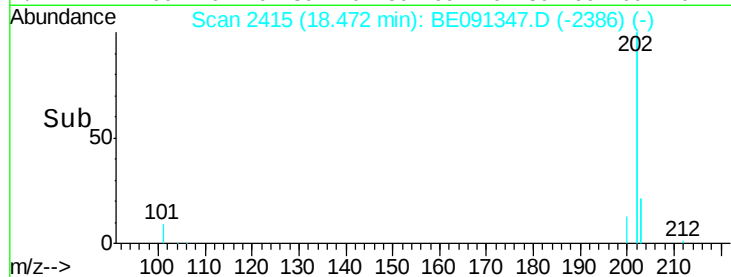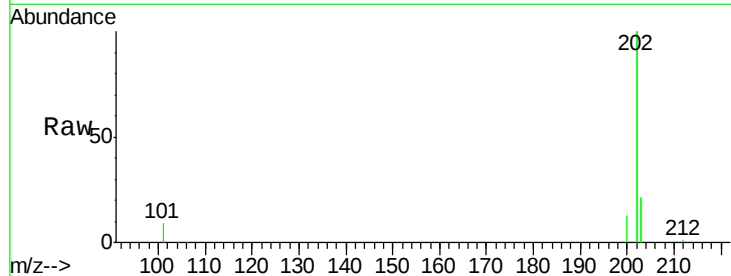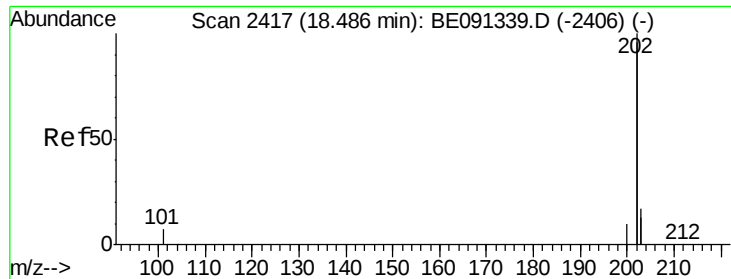

#19

Pyrene

Concen: 43.96 ng/ul

RT: 18.47 min Scan# 2415

Delta R.T. -0.01 min

Lab File: BE091347.D

Acq: 15 Dec 2015 6:45

Tgt Ion: 202 Resp: 19305425

Ion Ratio Lower Upper

202 100

200 6.5 4.4 6.6

203 21.2 13.8 20.8#

Instrument :

BNA_E

ClientSampleId :

A4KW2MSD

Manual Integrations
APPROVED

MMdadoda
12/15/2015 6:15:23 PM

