


Data Path : Z:\HPCHEM1\BNA_E\Data\BE121517\
 Data File : BE094994.D
 Acq On : 15 Dec 2017 9:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 14 18:42:53 2017

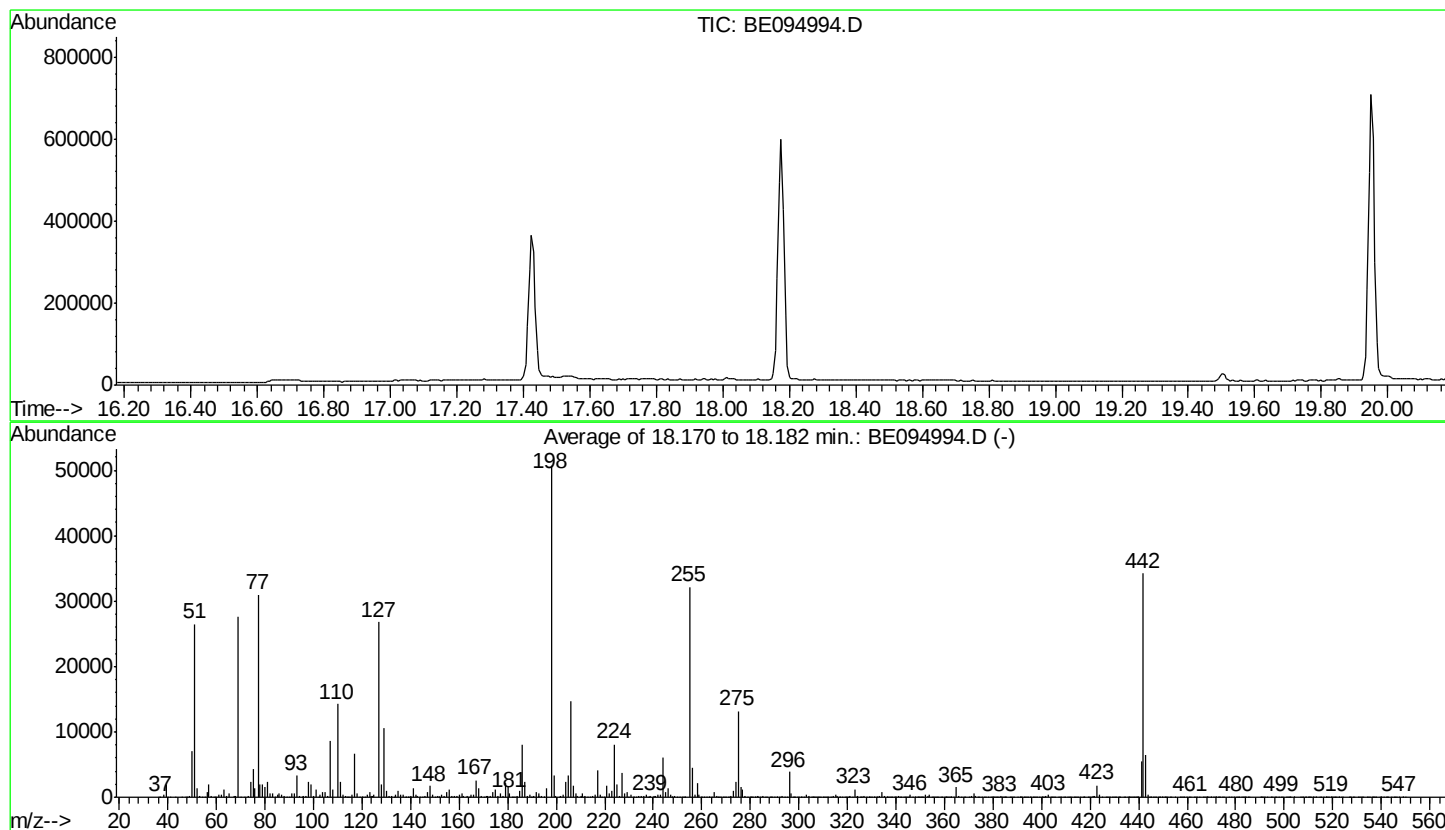

AutoFind: Scans 2652, 2653, 2654; Background Corrected with Scan 2643

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.2	26452	PASS
68	69	0.00	2	0.9	257	PASS
69	198	0.00	100	54.4	27590	PASS
70	69	0.00	2	0.3	90	PASS
127	198	10	80	52.8	26797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50706	PASS
199	198	5	9	6.7	3412	PASS
275	198	10	60	26.0	13206	PASS
365	198	1	100	3.0	1514	PASS
441	442	0.01	24	16.3	5565	PASS
442	198	50	100	67.4	34176	PASS
443	442	15	24	18.8	6414	PASS