

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121518\
 Data File : BE098471.D
 Acq On : 15 Dec 2018 14:23
 Operator : SJ/JU
 Sample : PB115682BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB115682BL

Quant Time: Dec 16 02:33:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	706	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	2656	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	1679	0.40	ng	0.00
19) Phenanthrene-d10	17.28	188	4780	0.40	ng	0.00
27) Chrysene-d12	21.46	240	5853	0.40	ng	0.00
34) Perylene-d12	24.00	264	5440	0.40	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.46	112	651	0.39	ng	0.01
5) Phenol-d6	7.07	99	802	0.34	ng	0.02
8) Nitrobenzene-d5	9.07	82	673	0.28	ng	0.05
11) 2-Methylnaphthalene-d10	12.28	152	1410	0.33	ng	0.01
14) 2,4,6-Tribromophenol	16.05	330	200	0.32	ng	0.02
15) 2-Fluorobiphenyl	13.16	172	2282	0.32	ng	0.01
25) Fluoranthene-d10	19.31	212	24005	0.39	ng	0.00
29) Terphenyl-d14	19.91	244	4392	0.31	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) n-Nitrosodimethylamine	3.74	42	70	0.064	ng	# 100
22) Pentachlorophenol	16.90	266	8	0.035	ng	# 73
32) Bis(2-ethylhexyl)phthalate	21.35	149	718	0.021	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121518\
Data File : BE098471.D
Acq On : 15 Dec 2018 14:23
Operator : SJ/JU
Sample : PB115682BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB115682BL

Quant Time: Dec 16 02:33:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

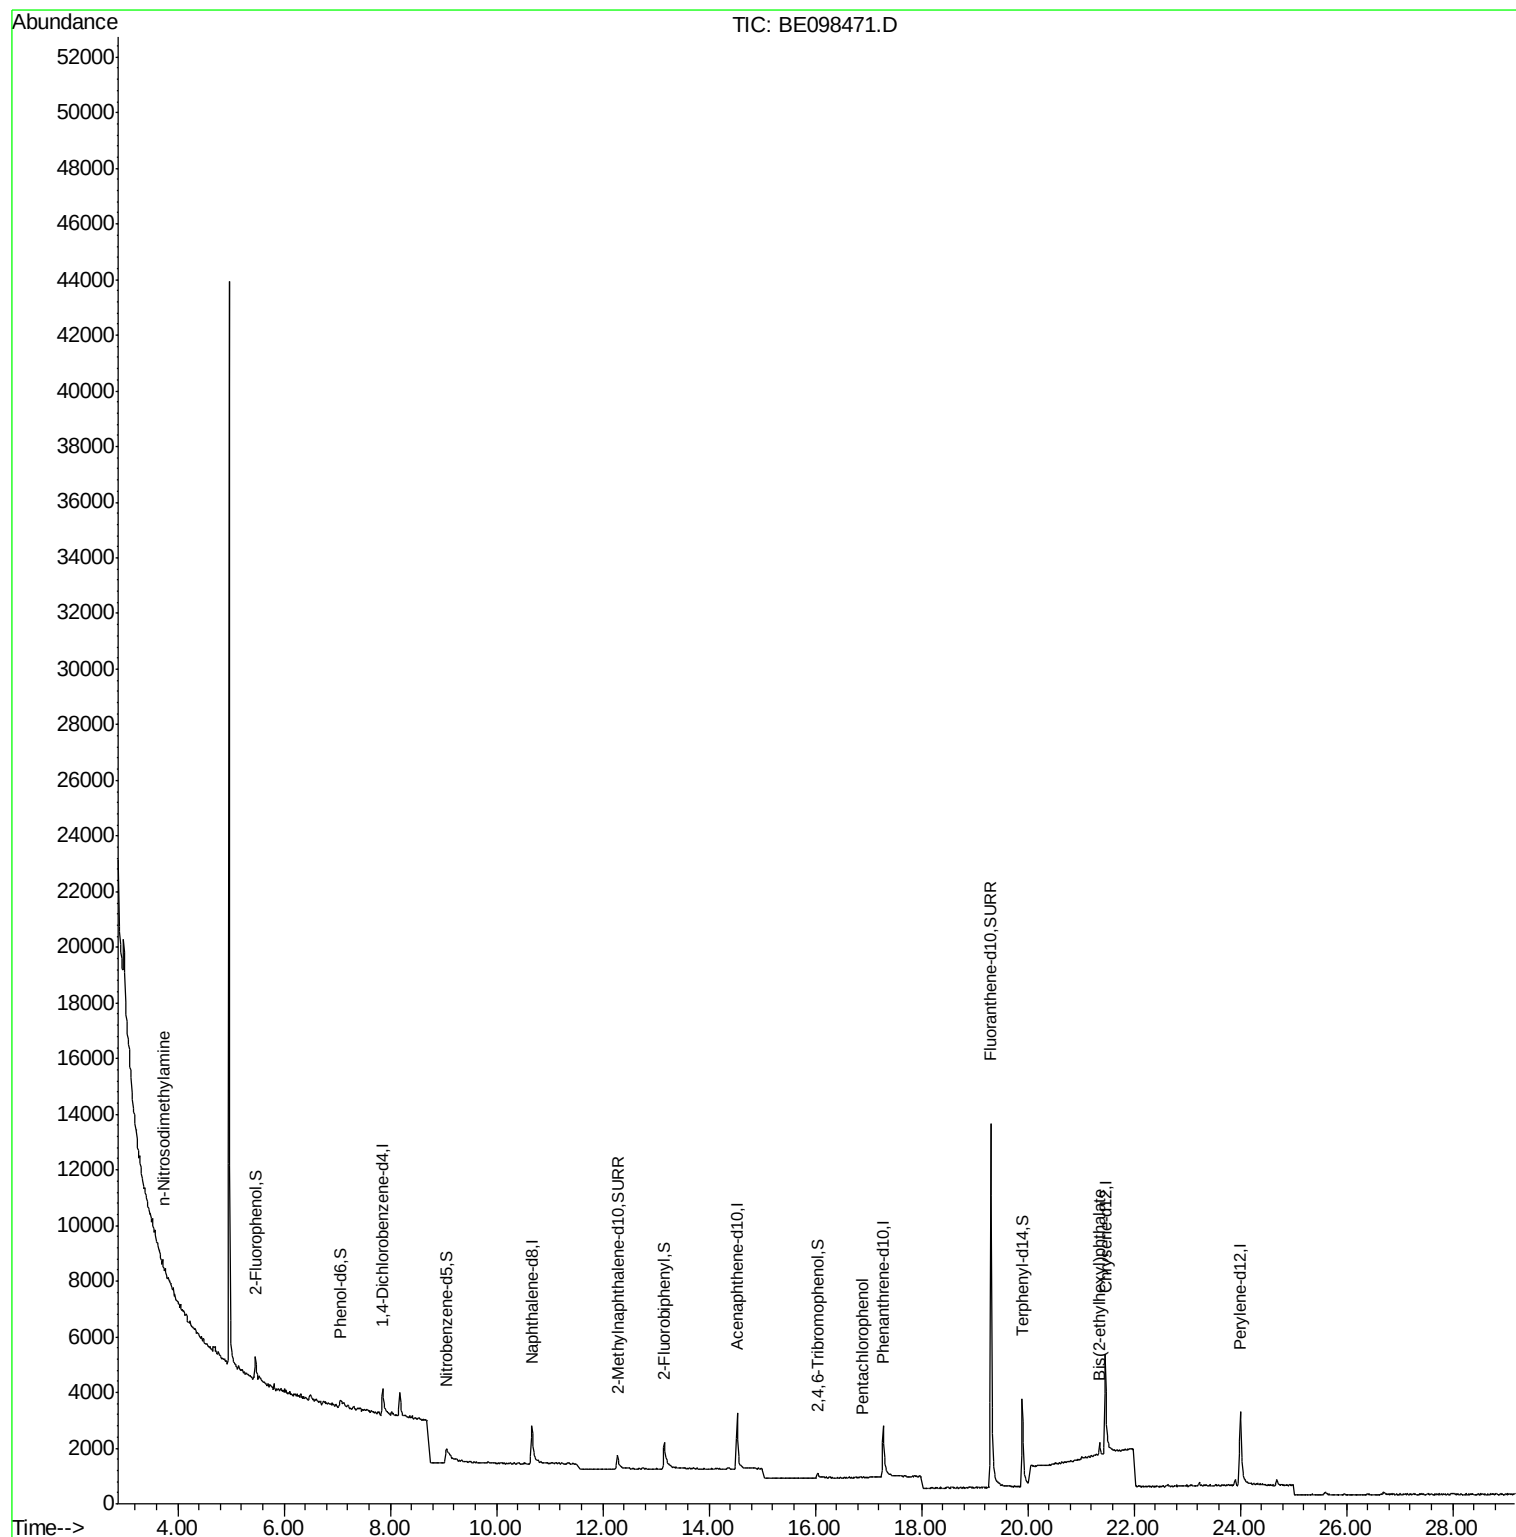

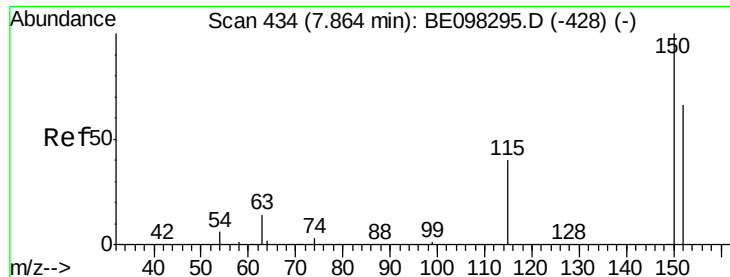


#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 434
Delta R.T. 0.00 min
Lab File: BE098471.D
Acq: 15 Dec 2018 14:23

Instrument :
BNA_E
ClientSampleId :
PB115682BL

Tgt Ion	Ratio	Lower	Upper
152	100		
150	136.1	124.2	186.4
115	67.3	53.9	80.9



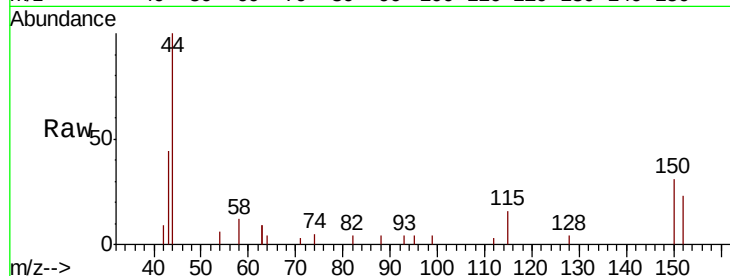


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

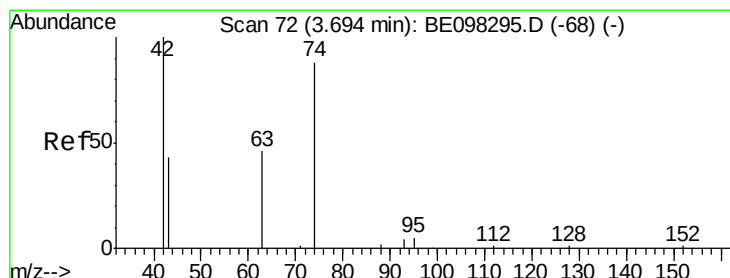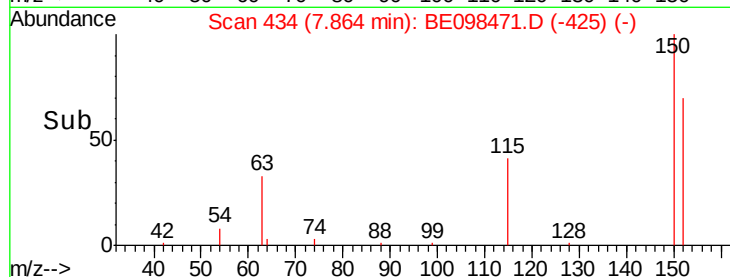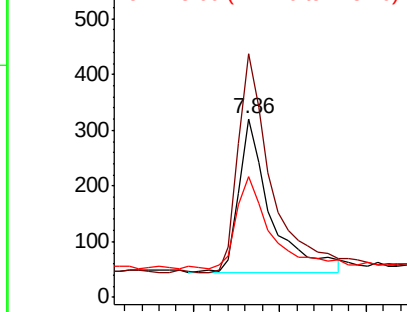

#3

n-Nitrosodimethylamine
Concen: 0.064 ng
RT: 3.74 min Scan# 76
Delta R.T. 0.05 min
Lab File: BE098471.D
Acq: 15 Dec 2018 14:23

Tgt Ion	Ratio	Lower	Upper
42	100		
74	4.3	0.0	0.0#
44	0.0	0.0	0.0


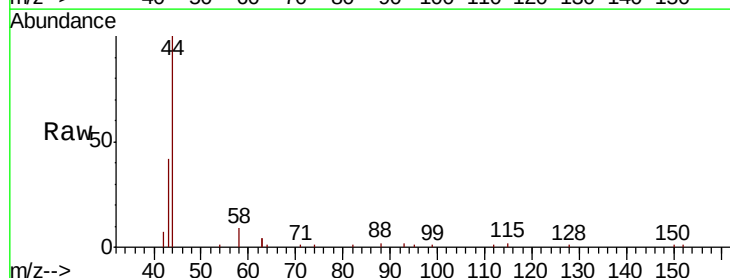



Abundance

Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

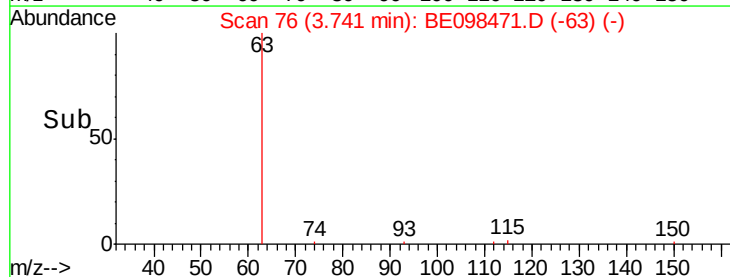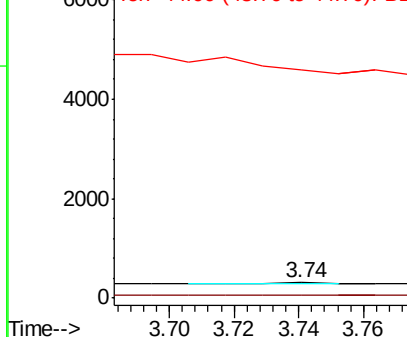

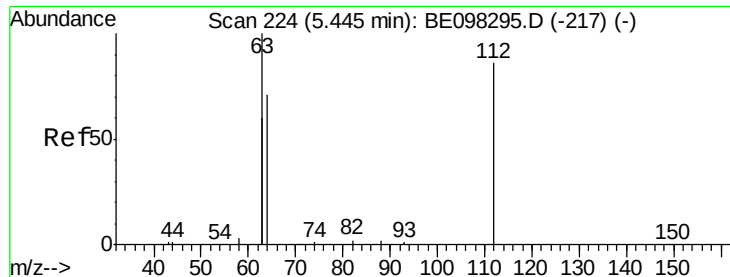

#4

2-Fluorophenol

Concen: 0.394 ng

RT: 5.46 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098471.D

Acq: 15 Dec 2018 14:23

Instrument :

BNA_E

ClientSampleId :

PB115682BL


Tgt Ion: 112 Resp: 651

Ion Ratio Lower Upper

112 100

64 79.6 59.8 89.8

63 169.6 133.7 200.5



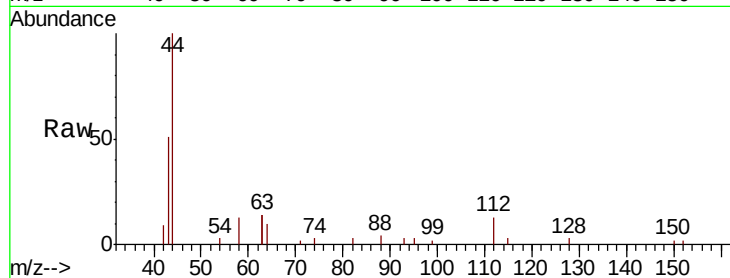


Abundance Ion 112.00 (111.70 to 112.70): BE098471.D (-215) (-)

Ion 64.00 (63.70 to 64.70): BE098471.D (-215) (-)

Ion 63.00 (62.70 to 63.70): BE098471.D (-215) (-)

Time-->

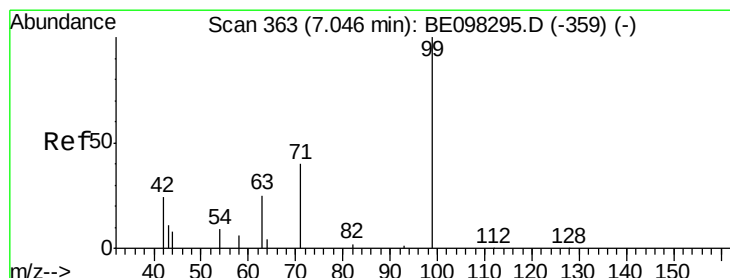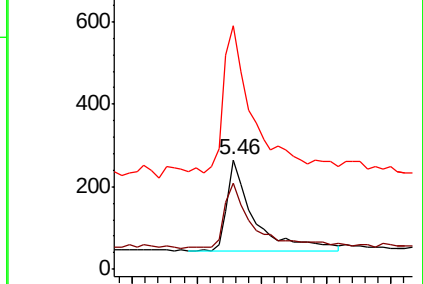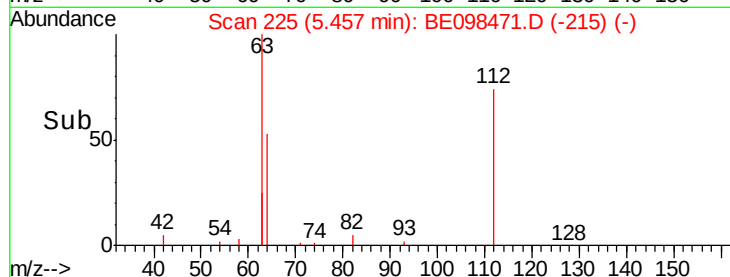

#5

Phenol-d6

Concen: 0.343 ng

RT: 7.07 min Scan# 365

Delta R.T. 0.02 min

Lab File: BE098471.D

Acq: 15 Dec 2018 14:23


Tgt Ion: 99 Resp: 802

Ion Ratio Lower Upper

99 100

42 21.7 26.3 39.5#

71 29.7 33.6 50.4#


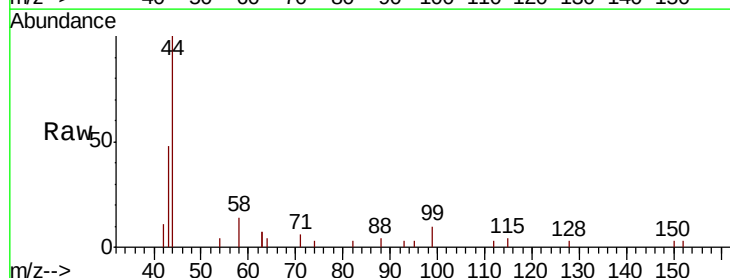



Abundance Ion 99.00 (98.70 to 99.70): BE098471.D (-354) (-)

Ion 42.00 (41.70 to 42.70): BE098471.D (-354) (-)

Ion 71.00 (70.70 to 71.70): BE098471.D (-354) (-)

Time-->

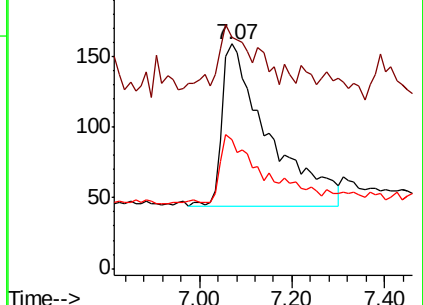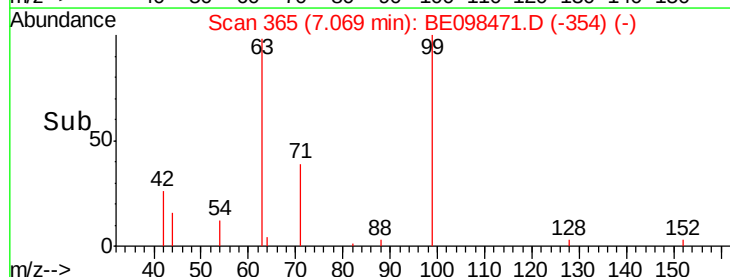



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098471.D

Acq: 15 Dec 2018 14:23

Instrument :

BNA_E

ClientSampleId :

PB115682BL

Tgt Ion: 136 Resp: 2656


Ion Ratio Lower Upper

136 100

137 14.9 9.2 13.8#

54 66.4 28.4 42.6#

68 11.6 5.4 8.0#



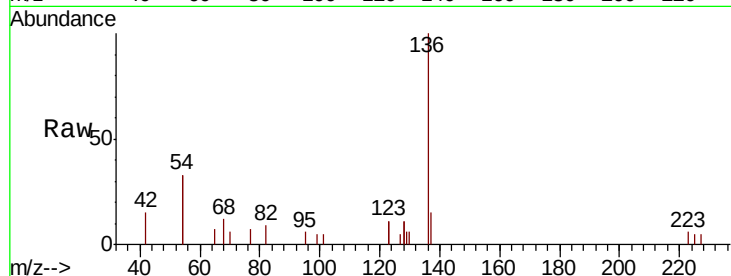


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

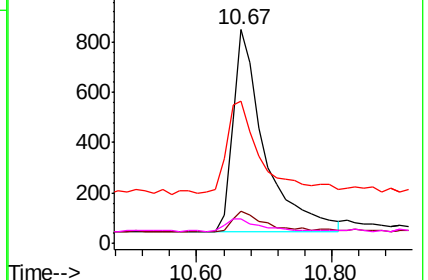

#8

Nitrobenzene-d5

Concen: 0.278 ng

RT: 9.07 min Scan# 531

Delta R.T. 0.05 min

Lab File: BE098471.D

Acq: 15 Dec 2018 14:23


Tgt Ion: 82 Resp: 673

Ion Ratio Lower Upper

82 100

128 216.6 102.4 153.6#



54 314.5 221.8 332.8




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



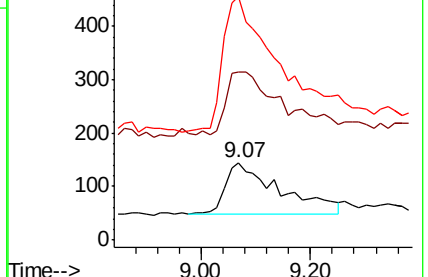





#11
 2-Methylnaphthalene-d10
 Concen: 0.326 ng
 RT: 12.28 min Scan# 768
 Delta R.T. 0.01 min
 Lab File: BE098471.D
 Acq: 15 Dec 2018 14:23




Instrument :
 BNA_E
 ClientSampleId :
 PB115682BL


Tgt Ion:152 Resp: 1410
 Ion Ratio Lower Upper
 152 100
 151 18.7 16.2 24.4

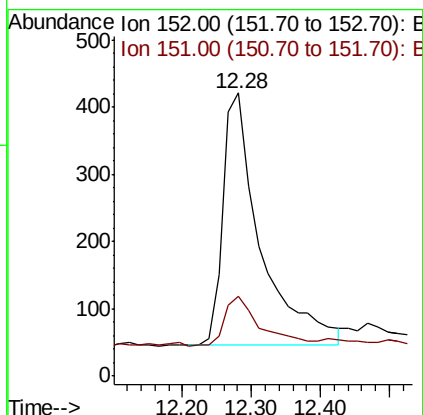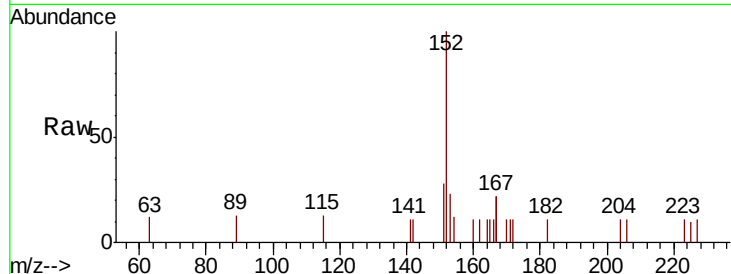

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.53 min Scan# 924
 Delta R.T. 0.00 min
 Lab File: BE098471.D
 Acq: 15 Dec 2018 14:23

Tgt Ion:164 Resp: 1679
 Ion Ratio Lower Upper
 164 100
 162 106.9 77.6 116.4
 160 59.2 36.0 54.0#



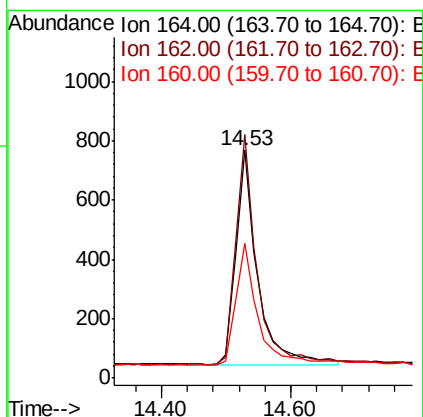
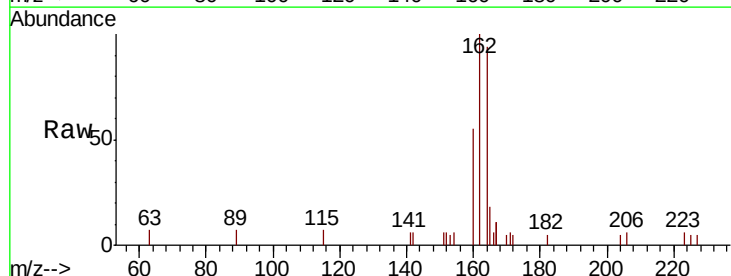




#14
 2,4,6-Tribromophenol
 Concen: 0.324 ng
 RT: 16.05 min Scan# 1043
 Delta R.T. 0.02 min
 Lab File: BE098471.D
 Acq: 15 Dec 2018 14:23




Instrument :
 BNA_E
 ClientSampleId :
 PB115682BL


Tgt Ion: 330 Resp: 200
 Ion Ratio Lower Upper
 330 100
 332 103.0 76.2 114.4
 141 0.0 39.0 58.4#

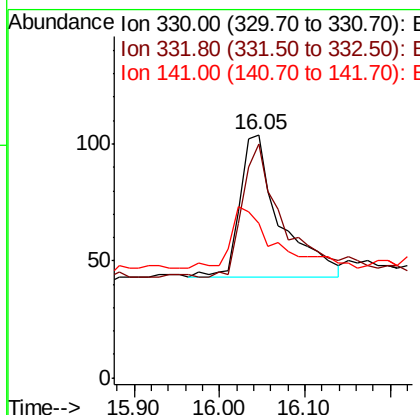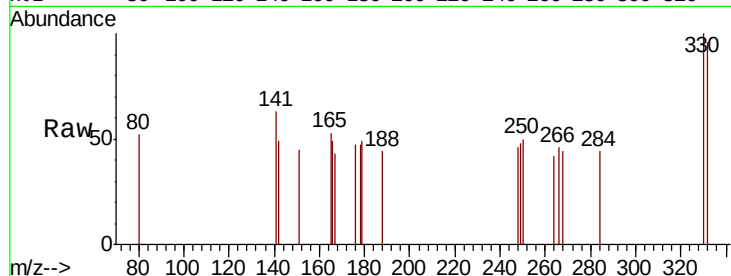

#15
 2-Fluorobiphenyl
 Concen: 0.322 ng
 RT: 13.16 min Scan# 829
 Delta R.T. 0.01 min
 Lab File: BE098471.D
 Acq: 15 Dec 2018 14:23

Tgt Ion: 172 Resp: 2282
 Ion Ratio Lower Upper
 172 100
 171 37.7 27.5 41.3
 170 26.9 19.6 29.4

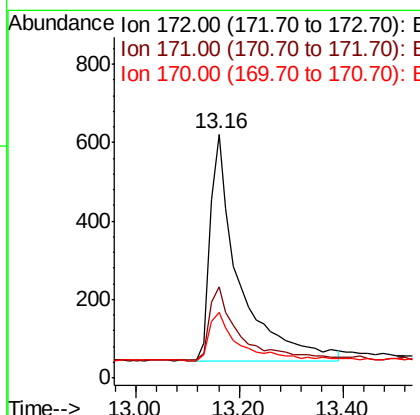



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.28 min Scan# 1149

Delta R.T. 0.00 min

Lab File: BE098471.D

Acq: 15 Dec 2018 14:23

Instrument :

BNA_E

ClientSampleId :

PB115682BL


Tgt Ion:188 Resp: 4780

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 11.6 7.2 10.8#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

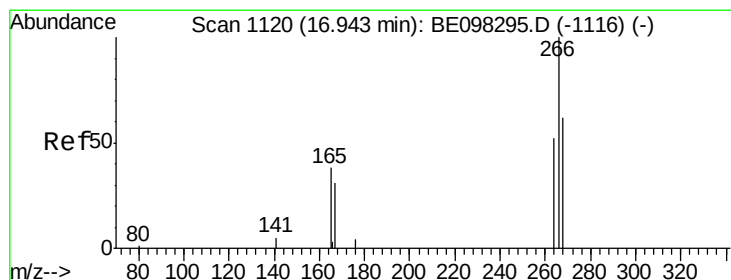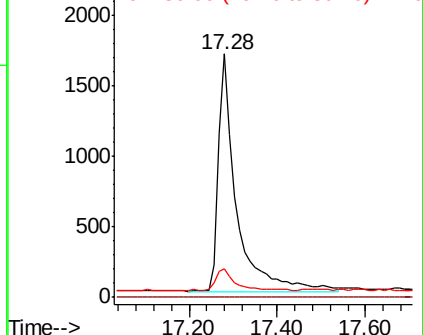

#22

Pentachlorophenol

Concen: 0.035 ng

RT: 16.90 min Scan# 1116

Delta R.T. -0.05 min

Lab File: BE098471.D

Acq: 15 Dec 2018 14:23


Tgt Ion:266 Resp: 8

Ion Ratio Lower Upper

266 100

264 91.5 59.0 88.4#



268 95.7 55.1 82.7#




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E




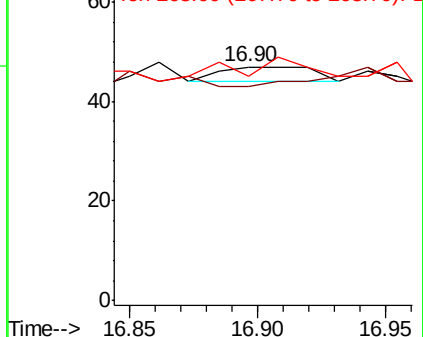


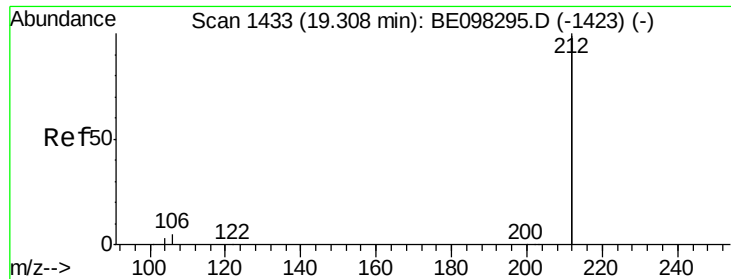

#25
 Fluoranthene-d10
 Concen: 0.391 ng
 RT: 19.31 min Scan# 1433
 Delta R.T. 0.00 min
 Lab File: BE098471.D
 Acq: 15 Dec 2018 14:23




Instrument :
 BNA_E
 ClientSampleId :
 PB115682BL


Tgt Ion:212 Resp: 24005
 Ion Ratio Lower Upper
 212 100
 106 2.4 2.2 3.2
 104 1.3 1.3 1.9

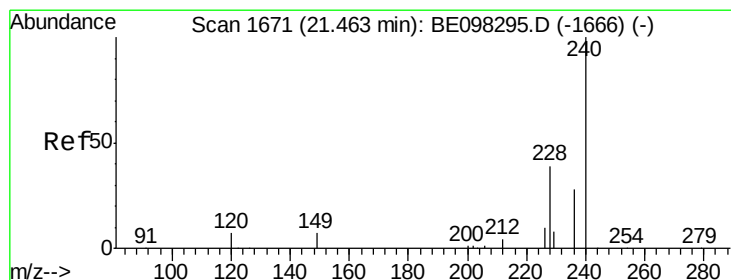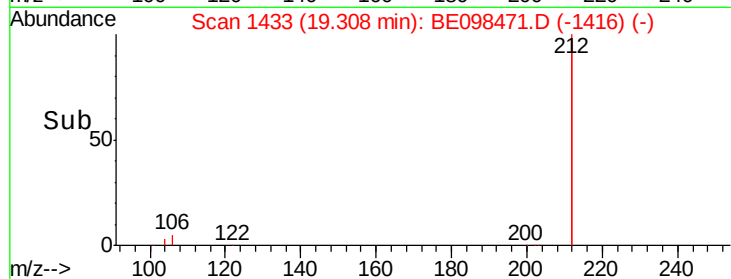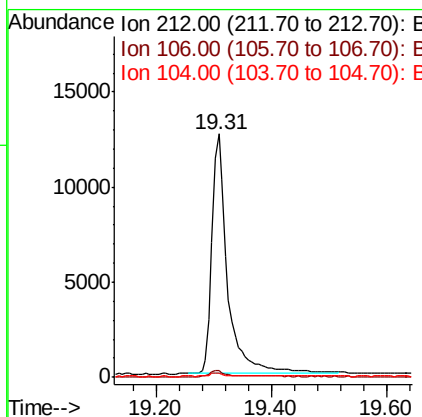

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.46 min Scan# 1671
 Delta R.T. -0.00 min
 Lab File: BE098471.D
 Acq: 15 Dec 2018 14:23

Tgt Ion:240 Resp: 5853
 Ion Ratio Lower Upper
 240 100
 120 10.2 9.5 14.3
 236 29.4 22.7 34.1

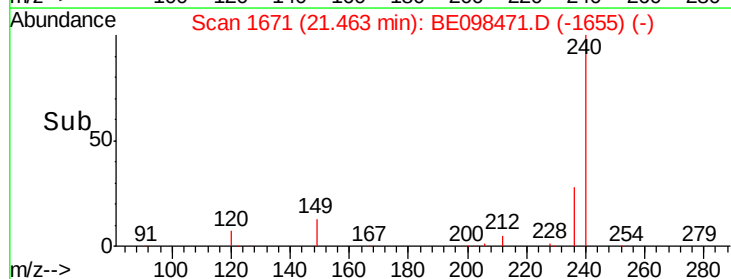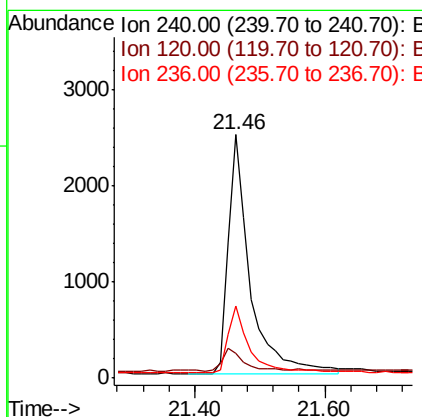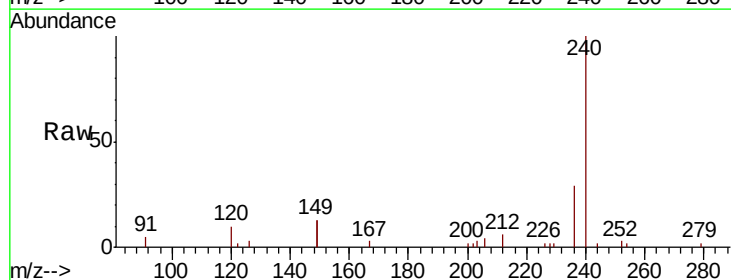

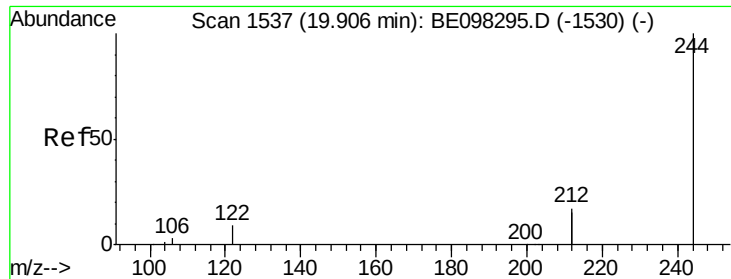

#29

Terphenyl-d14

Concen: 0.309 ng

RT: 19.91 min Scan# 1537

Delta R.T. 0.00 min

Lab File: BE098471.D

Acq: 15 Dec 2018 14:23


Instrument :

BNA_E




ClientSampleId :

PB115682BL

Tgt Ion:	244	Resp:	4392
Ion	Ratio	Lower	Upper
244	100		
212	43.2	27.4	41.0#
122	10.9	8.3	12.5



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

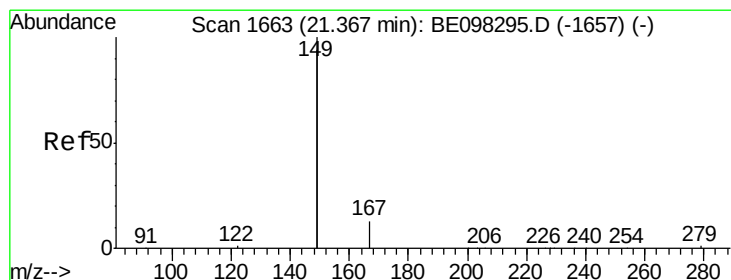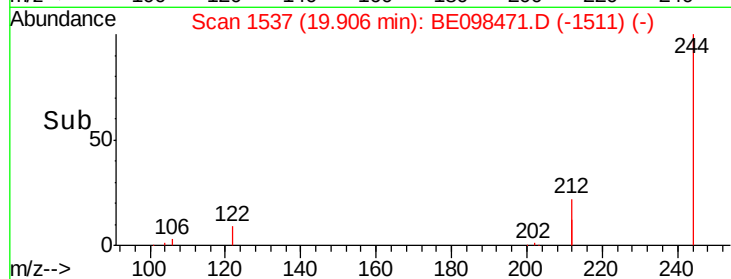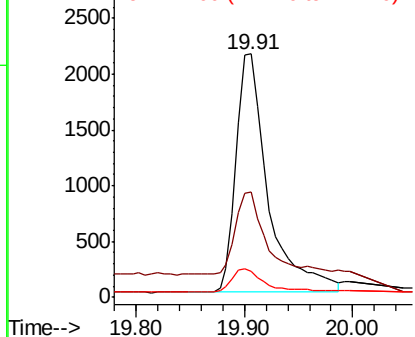

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.021 ng


RT: 21.35 min Scan# 1662

Delta R.T. -0.01 min



Lab File: BE098471.D


Acq: 15 Dec 2018 14:23

Tgt Ion:	149	Resp:	718
Ion	Ratio	Lower	Upper
149	100		
167	9.2	5.7	8.5#
279	0.0	1.0	1.4#

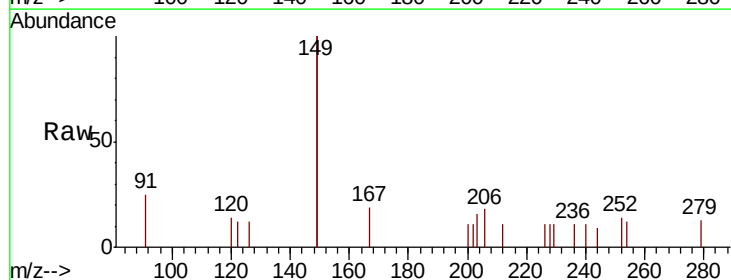

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

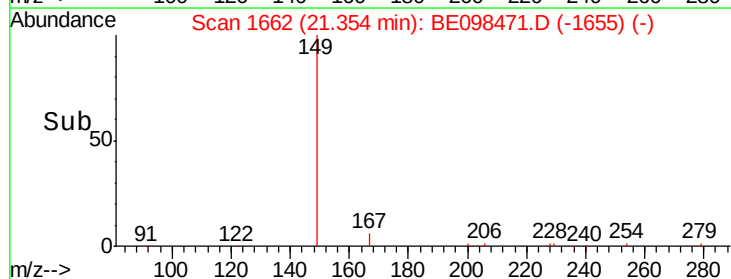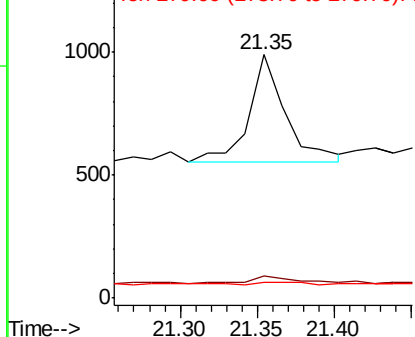


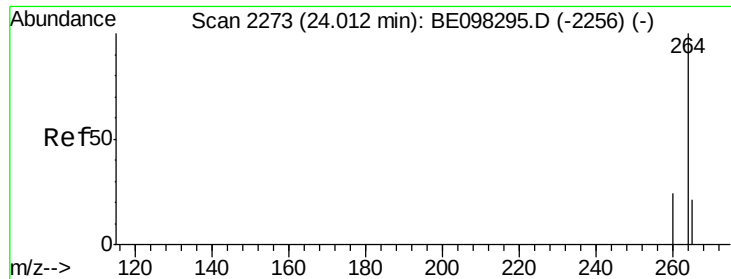

#34
Perylene-d12
Concen: 0.400 ng
RT: 24.00 min Scan# 2270
Delta R.T. -0.01 min
Lab File: BE098471.D
Acq: 15 Dec 2018 14:23

Instrument :
BNA_E
ClientSampleId :
PB115682BL

Tgt Ion: 264 Resp: 5440
Ion Ratio Lower Upper
264 100
260 27.8 20.2 30.2
265 35.5 25.2 37.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

